
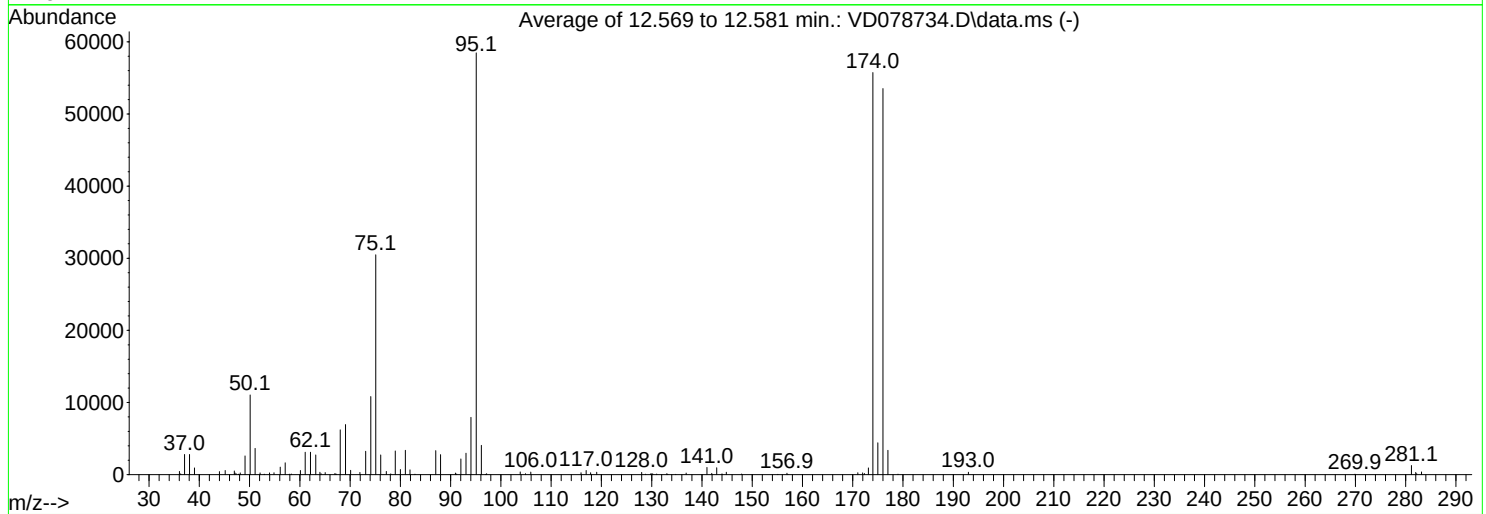


Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD032224\
Data File : VD078734.D
Acq On : 22 Mar 2024 08:43
Operator : RP/MD
Sample : BFB
Misc : 5.00G/5ml/MSVOA_D/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D031424S.M
Title : SW846 8260
Last Update : Fri Mar 15 05:38:03 2024

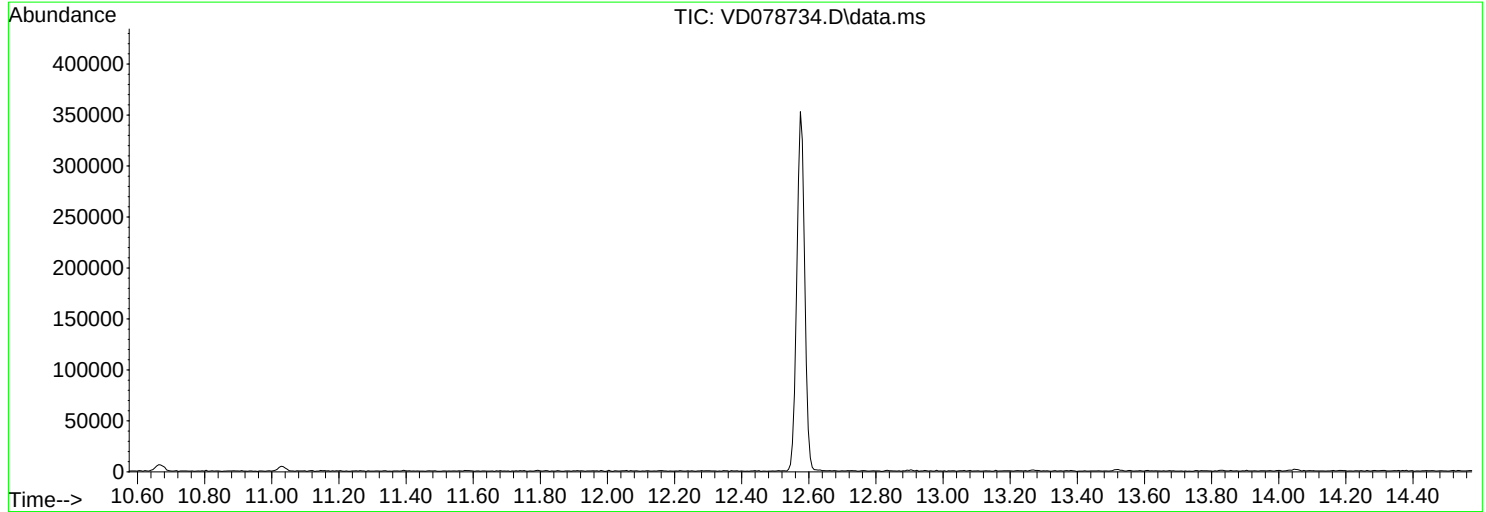

AutoFind: Scans 1867, 1868, 1869; Background Corrected with Scan 1858

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.9	11044	PASS
75	95	30	60	52.1	30469	PASS
95	95	100	100	100.0	58475	PASS
96	95	5	9	6.9	4064	PASS
173	174	0.00	2	1.7	923	PASS
174	95	50	100	95.3	55733	PASS
175	174	5	9	7.9	4414	PASS
176	174	95	101	96.1	53533	PASS
177	176	5	9	6.3	3373	PASS