

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD032323\
 Data File : VD075526.D
 Acq On : 23 Mar 2023 11:22
 Operator : KP/SY
 Sample : VD0323SBL01
 Misc : 5.00G/10.00ml/MSVOA_D/SOIL
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 VBLK112

Quant Time: Mar 24 01:27:46 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\SFAMDLM030123SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Mar 24 01:27:17 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.775	114	294062	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.587	117	263441	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.522	152	117859	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.275	65	124823	17.096	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	68.400%
7) Chloroethane-d5	2.805	69	133148	21.072	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	84.280%
11) 1,1-Dichloroethene-d2	3.922	63	89413	13.110	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	52.440%
21) 2-Butanone-d5	6.987	46	34298	50.690	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	101.380%
24) Chloroform-d	7.569	84	183855	23.857	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	95.440%
26) 1,2-Dichloroethane-d4	8.234	65	76656	22.961	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	91.840%
32) Benzene-d6	8.204	84	339048	21.671	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	86.680%
36) 1,2-Dichloropropane-d6	9.210	67	103846	23.484	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	93.920%
41) Toluene-d8	10.269	98	305126	21.378	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	85.520%
43) trans-1,3-Dichloroprop...	10.528	79	40489	22.407	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	89.640%
47) 2-Hexanone-d5	10.881	63	30262	47.439	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	94.880%
56) 1,1,2,2-Tetrachloroeth...	12.651	84	93108	25.172	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	100.680%
66) 1,2-Dichlorobenzene-d4	13.816	152	108879	26.410	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	105.640%
Target Compounds						Qvalue
16) Methylene chloride	4.799	84	17554	2.826	ug/L	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD032323\
Data File : VD075526.D
Acq On : 23 Mar 2023 11:22
Operator : KP/SY
Sample : VD0323SBL01
Misc : 5.00G/10.00ml/MSVOA_D/SOIL
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
VBLK112


Quant Time: Mar 24 01:27:46 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\SFAMDLM030123SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Mar 24 01:27:17 2023
Response via : Initial Calibration

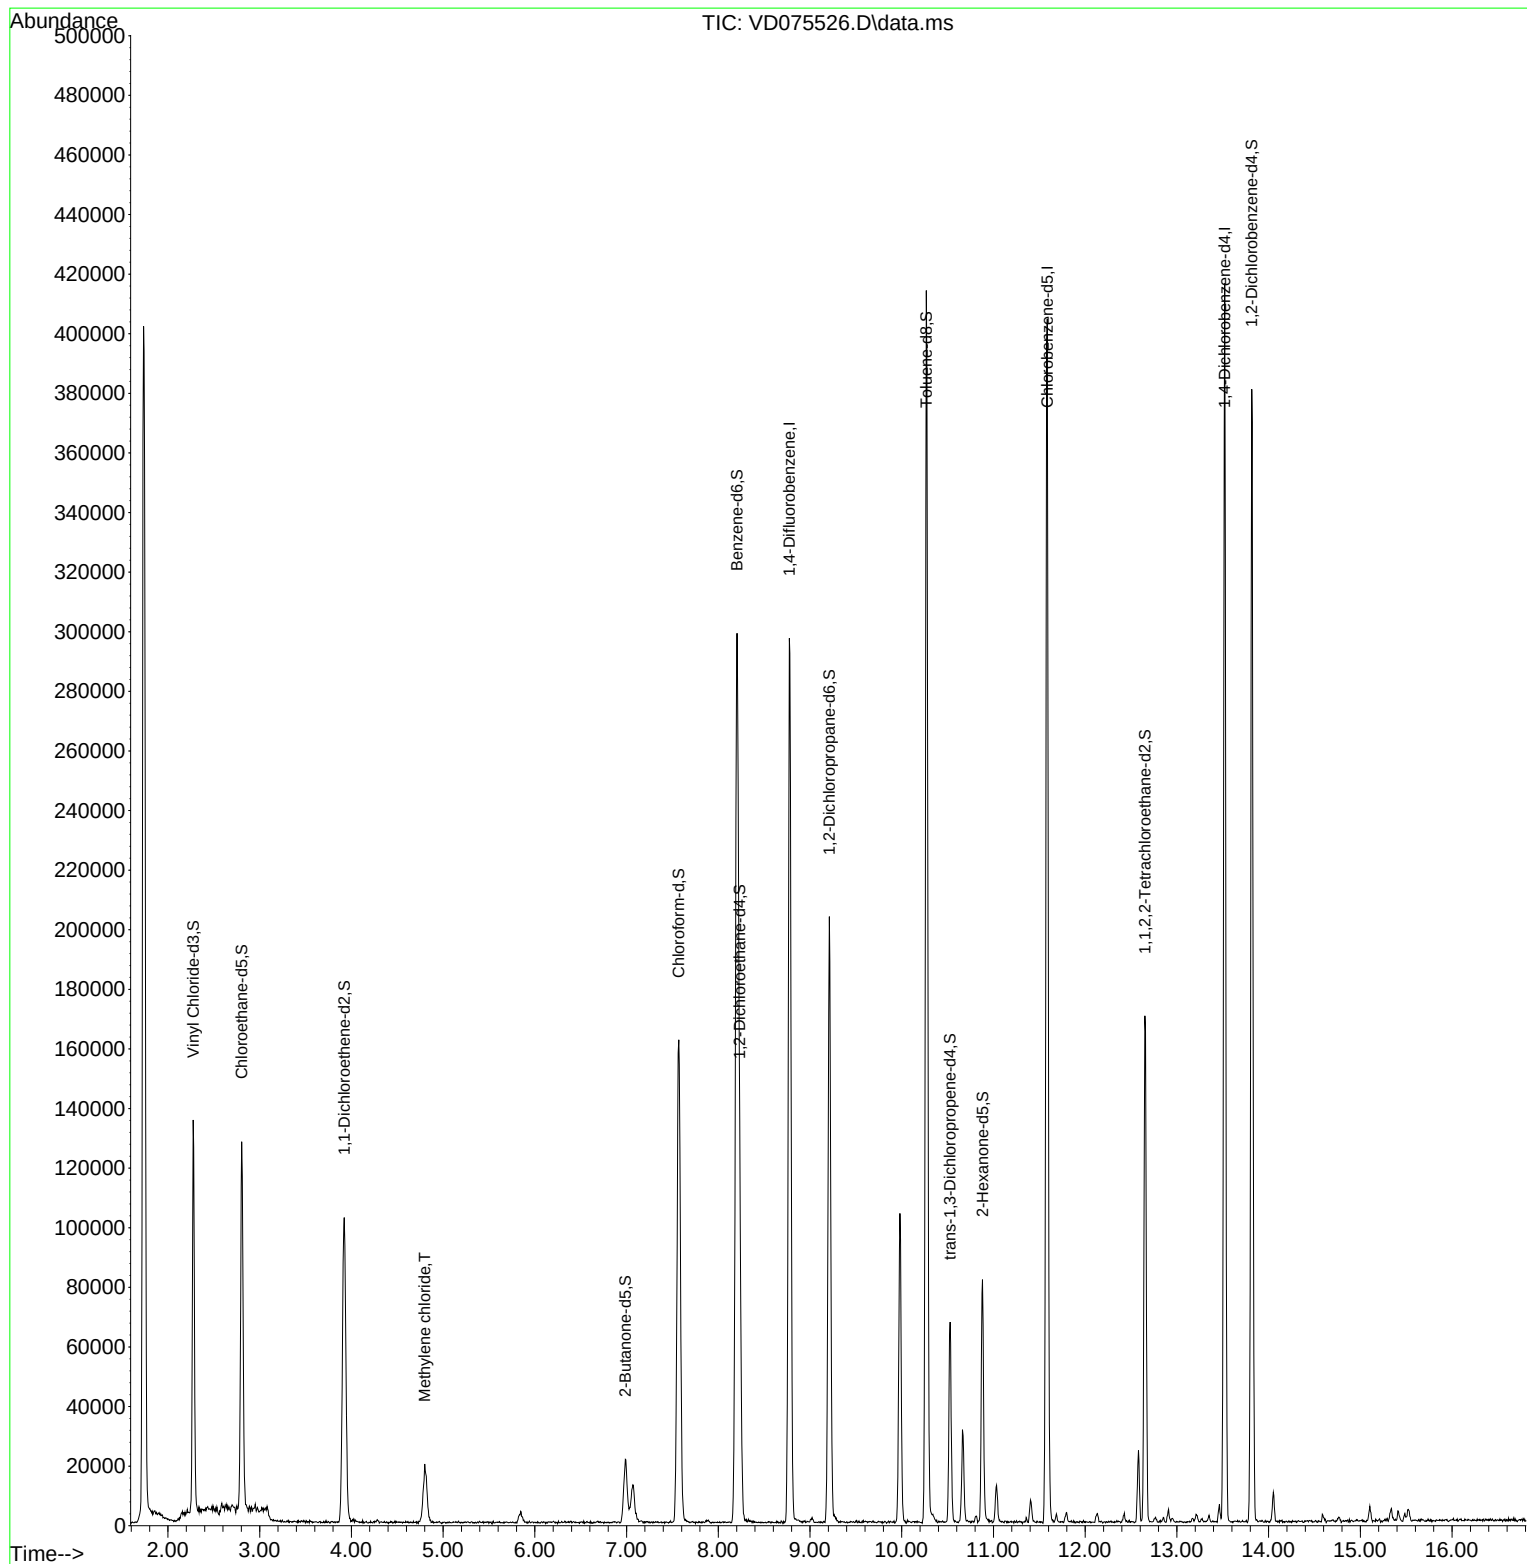

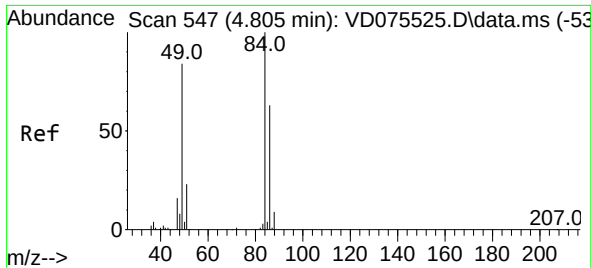

#16
Methylene chloride
Concen: 2.826 ug/L
RT: 4.799 min Scan# 54
Delta R.T. -0.006 min
Lab File: VD075526.D
Acq: 23 Mar 2023 11:22

Instrument :
MSVOA_D
ClientSampleId :
VBLK112

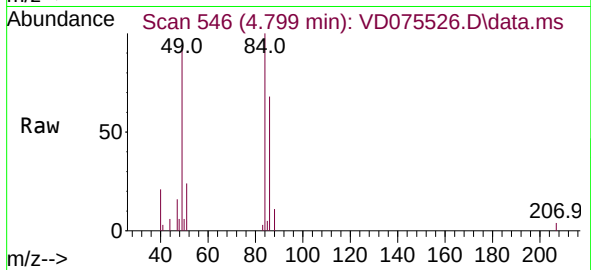

Tgt Ion:	84	Resp:	17554
Ion	Ratio	Lower	Upper
84	100		
86	68.2	44.2	82.2
49	93.2	63.6	118.2

