

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD032323\
 Data File : VD075526.D
 Acq On : 23 Mar 2023 11:22
 Operator : KP/SY
 Sample : VD0323SBL01
 Misc : 5.00G/10.00ml/MSVOA_D/SOIL
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 VBLK112

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\SFAMDLM030123SMA.M
 Title : SFAM01.0

Signal : TIC: VD075526.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.734	19	25	40	rVB	398103	819740	92.97%	10.660%
2	2.275	112	117	126	rVB	131259	196816	22.32%	2.559%
3	2.805	200	207	215	rBV	123130	228955	25.97%	2.977%
4	3.246	280	282	285	rBV	704	482	0.05%	0.006%
5	3.511	325	327	328	rBV2	777	497	0.06%	0.006%
6	3.546	332	333	338	rBV2	890	1035	0.12%	0.013%
7	3.746	366	367	370	rVB2	595	487	0.06%	0.006%
8	3.787	370	374	378	rBV2	609	1092	0.12%	0.014%
9	3.922	387	397	409	rBV	102191	271263	30.76%	3.527%
10	4.246	450	452	453	rVV	526	402	0.05%	0.005%
11	4.281	456	458	462	rVB2	1163	1564	0.18%	0.020%
12	4.328	462	466	467	rBV2	487	640	0.07%	0.008%
13	4.463	487	489	490	rBV	459	355	0.04%	0.005%
14	4.593	510	511	514	rVV	584	457	0.05%	0.006%
15	4.734	534	535	537	rBV	818	790	0.09%	0.010%
16	4.799	537	546	558	rVB3	19823	56572	6.42%	0.736%
17	5.169	606	609	610	rVB	537	353	0.04%	0.005%
18	5.311	630	633	635	rVB2	421	466	0.05%	0.006%
19	5.399	646	648	652	rVV	617	733	0.08%	0.010%
20	5.546	671	673	676	rBV	1060	1041	0.12%	0.014%
21	5.834	717	722	723	rBV3	2838	4196	0.48%	0.055%
22	5.940	737	740	742	rBV	751	659	0.07%	0.009%
23	6.075	760	763	765	rBV2	539	583	0.07%	0.008%
24	6.134	770	773	774	rBV	487	469	0.05%	0.006%
25	6.152	774	776	778	rBV	440	464	0.05%	0.006%
26	6.258	792	794	795	rBV	927	540	0.06%	0.007%
27	6.293	798	800	802	rVV2	448	367	0.04%	0.005%
28	6.387	814	816	819	rVB2	571	635	0.07%	0.008%
29	6.422	819	822	825	rBV	490	547	0.06%	0.007%
30	6.493	833	834	836	rBV	549	500	0.06%	0.007%
31	6.569	845	847	849	rVV	627	558	0.06%	0.007%
32	6.987	909	918	925	rBV	21145	57434	6.51%	0.747%
33	7.269	964	966	969	rVB2	409	430	0.05%	0.006%
34	7.569	1007	1017	1032	rBV	161728	416093	47.19%	5.411%
35	7.834	1060	1062	1065	rBV	465	461	0.05%	0.006%
36	7.875	1065	1069	1070	rBV	888	955	0.11%	0.012%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD032323\
 Data File : VD075526.D
 Acq On : 23 Mar 2023 11:22
 Operator : KP/SY
 Sample : VD0323SBL01
 Misc : 5.00G/10.00ml/MSVOA_D/SOIL
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 VBLK112

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\SFAMDLM030123SMA.M
 Title : SFAM01.0

37	8.204	1115	1125	1139	rBV2	298463	881727	100.00%	11.466%
38	8.328	1144	1146	1148	rBV2	912	543	0.06%	0.007%
39	8.381	1153	1155	1156	rBV	626	437	0.05%	0.006%
40	8.640	1198	1199	1202	rVB2	656	480	0.05%	0.006%
41	8.687	1206	1207	1210	rVB2	773	570	0.06%	0.007%
42	8.775	1214	1222	1232	rBV	296638	607815	68.93%	7.904%
43	8.934	1247	1249	1250	rBV2	616	531	0.06%	0.007%
44	9.010	1259	1262	1263	rBV2	971	999	0.11%	0.013%
45	9.151	1284	1286	1288	rBV2	577	502	0.06%	0.007%
46	9.210	1288	1296	1310	rVV	203336	411784	46.70%	5.355%
47	9.510	1343	1347	1349	rVB2	734	694	0.08%	0.009%
48	9.534	1349	1351	1352	rBV	628	352	0.04%	0.005%
49	9.569	1355	1357	1358	rBV	623	381	0.04%	0.005%
50	9.687	1375	1377	1379	rBV2	620	425	0.05%	0.006%
51	9.857	1402	1406	1407	rBV2	768	734	0.08%	0.010%
52	9.875	1407	1409	1411	rVV	656	586	0.07%	0.008%
53	9.916	1414	1416	1417	rVB2	752	400	0.05%	0.005%
54	9.981	1417	1427	1435	rBV2	103931	192591	21.84%	2.504%
55	10.063	1439	1441	1442	rBV2	1090	710	0.08%	0.009%
56	10.269	1468	1476	1487	rBV	413684	740817	84.02%	9.634%
57	10.404	1497	1499	1500	rBV	615	400	0.05%	0.005%
58	10.528	1513	1520	1528	rVB2	67049	118063	13.39%	1.535%
59	10.663	1535	1543	1550	rBV	31159	54151	6.14%	0.704%
60	10.810	1564	1568	1571	rVB3	2155	3274	0.37%	0.043%
61	10.881	1574	1580	1590	rVV	80927	138871	15.75%	1.806%
62	11.034	1600	1606	1615	rVB2	12401	21866	2.48%	0.284%
63	11.122	1620	1621	1622	rBV	605	397	0.05%	0.005%
64	11.228	1638	1639	1642	rBV2	759	612	0.07%	0.008%
65	11.328	1654	1656	1658	rBV2	549	711	0.08%	0.009%
66	11.357	1660	1661	1665	rVB	1724	1277	0.14%	0.017%
67	11.404	1665	1669	1674	rBV	7573	12514	1.42%	0.163%
68	11.475	1680	1681	1685	rBV	540	479	0.05%	0.006%
69	11.587	1692	1700	1709	rBV	404131	712090	80.76%	9.260%
70	11.687	1713	1717	1723	rVB3	2787	3581	0.41%	0.047%
71	11.798	1730	1736	1742	rBV2	3379	5895	0.67%	0.077%
72	11.910	1753	1755	1756	rBV	487	364	0.04%	0.005%
73	11.940	1759	1760	1766	rBV2	615	904	0.10%	0.012%
74	11.981	1766	1767	1769	rBV	732	436	0.05%	0.006%
75	12.134	1788	1793	1796	rBV5	2965	5105	0.58%	0.066%
76	12.428	1838	1843	1846	rBV2	3037	3963	0.45%	0.052%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD032323\
 Data File : VD075526.D
 Acq On : 23 Mar 2023 11:22
 Operator : KP/SY
 Sample : VD0323SBL01
 Misc : 5.00G/10.00ml/MSVOA_D/SOIL
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 VBLK112

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\SFAMDLM030123SMA.M
 Title : SFAM01.0

77	12.481	1850	1852	1853	rBV2	736	449	0.05%	0.006%
78	12.581	1861	1869	1874	rBV2	24304	37154	4.21%	0.483%
79	12.651	1875	1881	1890	rVB	169862	290630	32.96%	3.779%
80	12.769	1896	1901	1906	rVB2	1716	2850	0.32%	0.037%
81	12.910	1920	1925	1929	rBV2	4367	6134	0.70%	0.080%
82	13.169	1966	1969	1972	rBV4	1131	1506	0.17%	0.020%
83	13.275	1983	1987	1990	rBV3	1189	1500	0.17%	0.020%
84	13.463	2015	2019	2022	rBV2	6058	8007	0.91%	0.104%
85	13.522	2022	2029	2041	rVB	415673	655600	74.35%	8.525%
86	13.816	2072	2079	2087	rBV	379888	634205	71.93%	8.247%
87	14.051	2114	2119	2124	rVB2	9771	14259	1.62%	0.185%
88	14.263	2153	2155	2158	rBV	674	725	0.08%	0.009%
89	14.545	2201	2203	2206	rBV2	736	860	0.10%	0.011%
90	14.586	2208	2210	2214	rBV3	2575	3220	0.37%	0.042%
91	14.763	2236	2240	2245	rVB4	1864	3622	0.41%	0.047%
92	14.881	2258	2260	2261	rBV	945	379	0.04%	0.005%
93	15.104	2294	2298	2303	rVB5	5238	7907	0.90%	0.103%
94	15.169	2308	2309	2312	rBV3	859	657	0.07%	0.009%
95	15.339	2333	2338	2344	rVB2	4051	6591	0.75%	0.086%
96	15.410	2347	2350	2359	rVB4	3532	5448	0.62%	0.071%
97	15.486	2359	2363	2365	rBV2	2614	3521	0.40%	0.046%
98	15.522	2366	2369	2376	rVB5	3982	7081	0.80%	0.092%
99	15.769	2409	2411	2413	rVB2	897	605	0.07%	0.008%
100	16.616	2554	2555	2556	rBV	1037	425	0.05%	0.006%




Sum of corrected areas: 7689997

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD032323\
Data File : VD075526.D
Acq On : 23 Mar 2023 11:22
Operator : KP/SY
Sample : VD0323SBL01
Misc : 5.00G/10.00ml/MSVOA_D/SOIL
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
VBLK112

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\SFAMDLM030123SMA.M
Quant Title : SFAM01.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

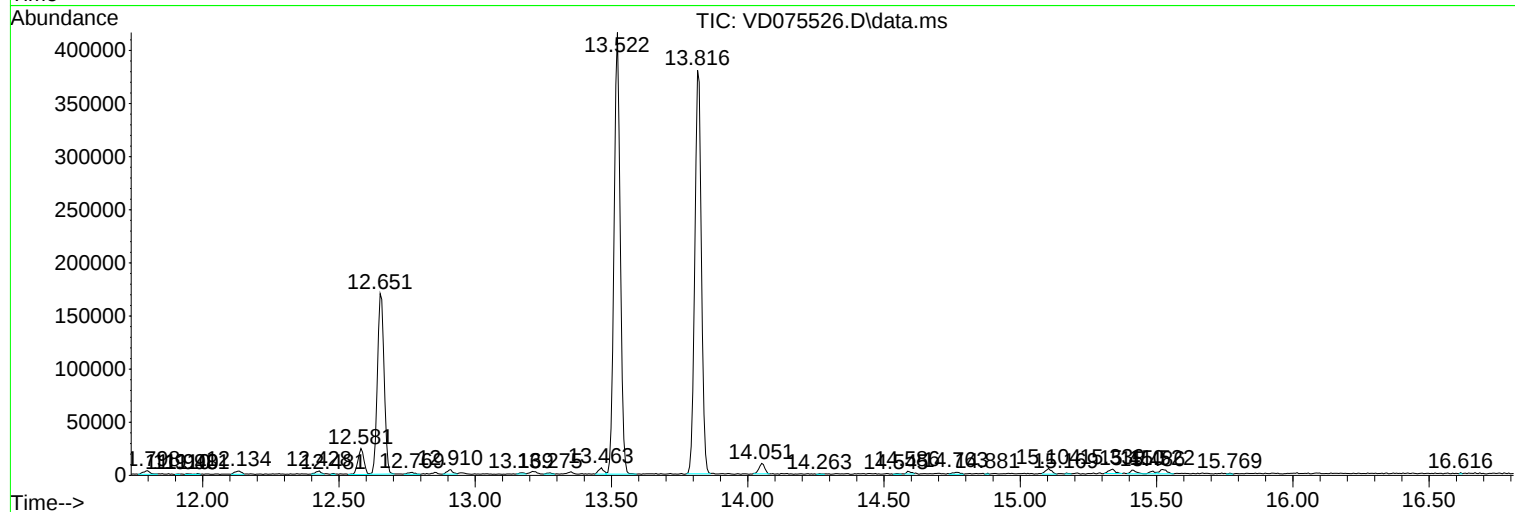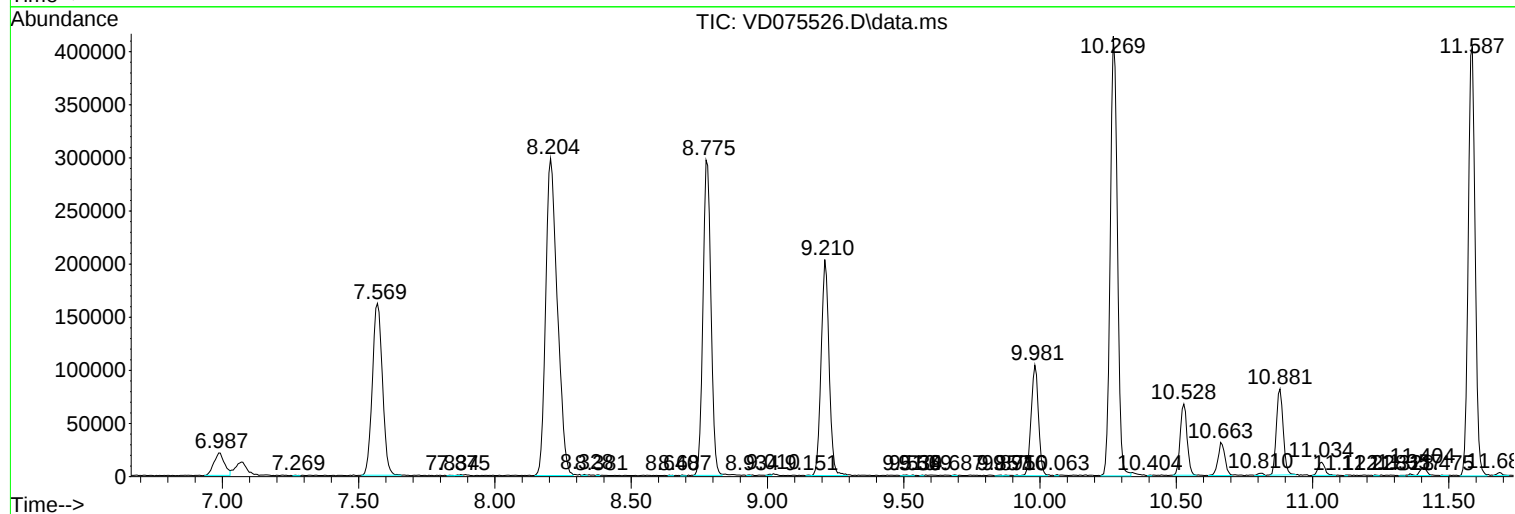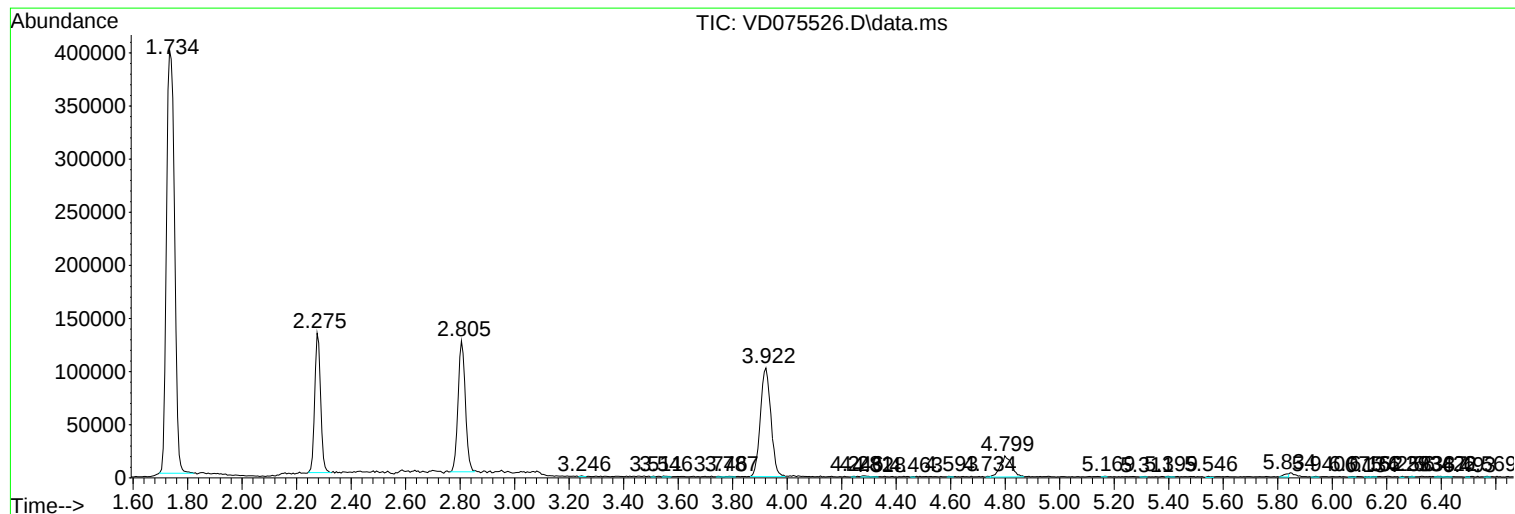

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD032323\
Data File : VD075526.D
Acq On : 23 Mar 2023 11:22
Operator : KP/SY
Sample : VD0323SBL01
Misc : 5.00G/10.00ml/MSVOA_D/SOIL
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
VBLK112

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\SFAMDLM030123SMA.M
Quant Title : SFAM01.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD032323\
Data File : VD075526.D
Acq On : 23 Mar 2023 11:22
Operator : KP/SY
Sample : VD0323SBL01
Misc : 5.00G/10.00ml/MSVOA_D/SOIL
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
VBLK112

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\SFAMDLM030123SMA.M
Quant Title : SFAM01.0

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------