
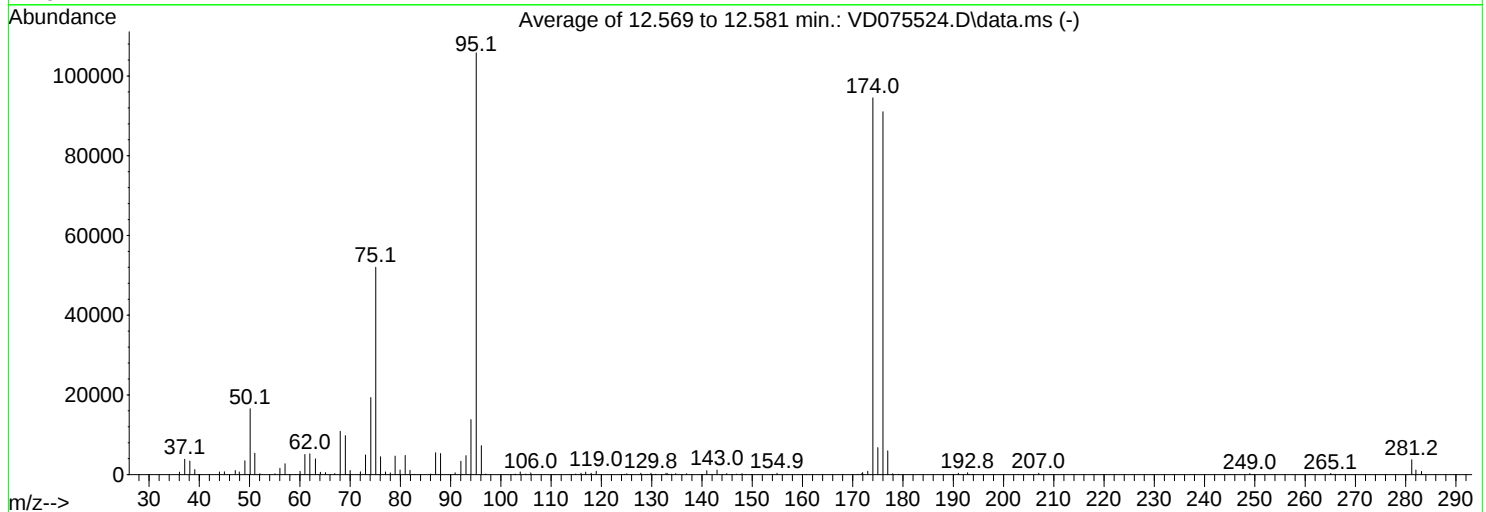


Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD032323\
Data File : VD075524.D
Acq On : 23 Mar 2023 09:28
Operator : KP/SY
Sample : BFB108
Misc : 5.00G/10.00ml/MSVOA_D/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB108

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\SFAMDLM030123SMA.M
Title : SFAM01.0
Last Update : Fri Mar 24 01:27:17 2023

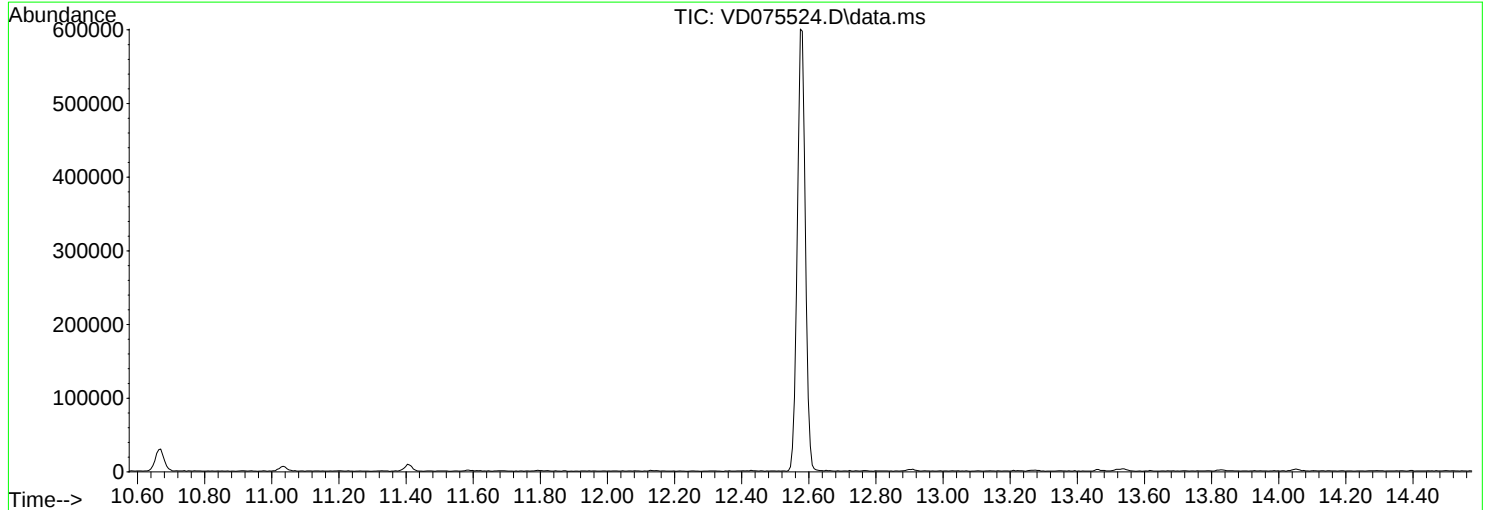

AutoFind: Scans 1867, 1868, 1869; Background Corrected with Scan 1860

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	15.6	16550	PASS
75	95	30	80	49.2	52019	PASS
95	95	100	100	100.0	105811	PASS
96	95	5	9	6.9	7261	PASS
173	174	0.00	2	0.9	858	PASS
174	95	50	120	89.3	94536	PASS
175	174	5	9	7.2	6794	PASS
176	174	95	105	96.3	91048	PASS
177	176	5	10	6.6	5970	PASS

Scan 1860 (12.528 min): VD075524.D\data.ms
BFB108

m/z	Abundance
39.90	1032.0
44.00	350.0

Instrument :
MSVOA_D
ClientSampleId :
BFB108

m/z	Abundance
36.10	536.0
37.10	2887.0
38.10	2932.0
39.20	1312.0
40.00	1084.0
44.00	874.0
44.90	665.0
47.10	1013.0
48.00	474.0
49.10	2680.0
50.10	13819.0
51.00	4290.0
52.10	246.0
55.10	213.0
56.10	1303.0
57.10	2297.0
60.10	678.0
61.00	4074.0
62.00	4960.0
63.10	3596.0
64.20	824.0
65.10	527.0
67.10	240.0
68.00	9282.0
69.00	8213.0
70.00	1140.0
72.00	433.0
73.00	4039.0
74.10	15537.0
75.10	42928.0
76.00	3594.0
77.10	700.0
78.00	411.0
78.90	3659.0
80.00	1058.0
80.90	3819.0
81.90	707.0
86.00	218.0
87.00	4504.0
88.00	4285.0
90.90	275.0
92.10	2579.0
93.10	3639.0
94.10	11266.0
95.10	84032.0
96.10	5756.0
103.80	397.0
106.00	366.0
116.00	233.0
117.00	412.0
118.00	322.0
118.90	675.0
125.10	337.0
127.80	244.0
129.80	320.0
132.80	357.0
133.40	246.0
134.80	229.0
136.90	209.0
140.90	889.0
143.10	1114.0
144.90	281.0
147.70	225.0
155.10	249.0
171.80	673.0
173.00	626.0
174.00	72696.0
175.00	5086.0
176.00	67736.0
176.90	4183.0
178.00	177.0
190.90	158.0
192.80	498.0
207.10	176.0
265.10	322.0
281.20	2709.0
282.10	823.0
283.10	502.0

Instrument :
MSVOA_D
ClientSampleId :
BFB108

m/z	Abundance
36.00	594.0
37.10	4357.0
38.10	3910.0
39.00	1285.0
40.00	1195.0
44.10	1382.0
45.00	660.0
47.20	1015.0
47.90	924.0
49.00	3831.0
50.10	18904.0
51.10	6491.0
52.00	225.0
55.00	284.0
56.10	2009.0
57.00	3008.0
58.20	172.0
59.20	180.0
60.10	929.0
61.00	5870.0
62.00	5493.0
63.10	4480.0
64.00	642.0
65.10	607.0
66.90	364.0
68.10	11830.0
69.10	11793.0
70.00	930.0
72.00	752.0
73.10	5607.0
74.10	21728.0
75.10	56448.0
76.10	4723.0
77.00	758.0
77.90	471.0
79.00	5509.0
79.90	1410.0
81.00	5547.0
81.90	1161.0
87.00	5654.0
88.00	6150.0
90.90	605.0
92.00	3750.0
93.00	5631.0
94.00	14966.0
95.10	118456.0
96.10	7712.0
97.00	175.0
102.70	152.0
103.90	856.0
105.00	197.0
105.90	493.0
110.70	178.0
114.90	225.0
115.90	471.0
116.80	623.0
117.90	384.0
119.00	1019.0
124.60	200.0
125.10	163.0
127.90	338.0
129.10	193.0
129.80	244.0
130.80	206.0
132.90	700.0
134.90	346.0
136.90	307.0
140.90	1036.0
143.00	1121.0
145.00	256.0
145.90	185.0
147.00	274.0
148.00	270.0
148.70	185.0
154.90	455.0
156.90	222.0
170.90	209.0
172.00	868.0
173.00	952.0
174.00	105032.0
175.00	8037.0
176.00	100048.0
177.00	6333.0
177.90	360.0
191.00	540.0
193.10	306.0
207.00	354.0
208.00	166.0
249.00	362.0
265.10	190.0
281.20	3758.0
282.10	1081.0

Instrument :
MSVOA_D
ClientSampleId :
BFB108

283.10

687.0

Instrument :
MSVOA_D
ClientSampleId :
BFB108

m/z	Abundance
36.10	808.0
37.10	4284.0
38.10	3370.0
39.10	1252.0
40.10	883.0
44.00	821.0
45.10	895.0
47.10	1091.0
47.90	612.0
49.10	3940.0
50.10	16928.0
51.10	5311.0
52.00	233.0
55.10	222.0
56.00	1559.0
57.10	2898.0
60.00	992.0
61.00	5242.0
62.00	5207.0
63.10	3843.0
64.00	388.0
65.10	441.0
66.90	293.0
68.10	11488.0
69.10	9432.0
70.00	1129.0
72.10	964.0
73.00	5171.0
74.10	20760.0
75.10	56680.0
76.10	5172.0
77.00	558.0
78.10	427.0
78.90	4834.0
80.00	995.0
81.00	5129.0
81.90	1390.0
82.80	192.0
86.10	225.0
87.00	6388.0
88.00	5431.0
90.90	557.0
92.00	3842.0
93.00	5104.0
94.10	15260.0
95.10	114944.0
96.10	8314.0
97.00	366.0
102.90	376.0
103.90	817.0
104.90	277.0
105.90	524.0
114.90	253.0
116.00	441.0
116.80	899.0
117.90	393.0
118.90	825.0
125.00	259.0
125.90	177.0
127.90	545.0
128.80	190.0
129.90	486.0
130.80	208.0
133.10	866.0
133.90	323.0
134.70	260.0
137.00	241.0
141.00	1148.0
142.90	1222.0
144.90	281.0
146.90	194.0
147.90	478.0
149.80	166.0
154.90	339.0
160.80	248.0
171.90	666.0
173.00	995.0
174.00	105880.0
175.00	7259.0
176.00	105360.0
177.00	7395.0
177.90	185.0
179.10	209.0
191.00	415.0
192.90	902.0
193.90	164.0
203.00	202.0
205.00	161.0
206.90	502.0
249.00	461.0
249.90	172.0
265.10	418.0

Instrument :
MSVOA_D
ClientSampleId :
BFB108

266.00	223.0
267.00	196.0
281.20	4781.0
282.00	1618.0
283.20	1177.0

Instrument :
MSVOA_D
ClientSampleId :
BFB108