


Data Path : Z:\VOASRV\HPCHEM1\MSVOA D\DATA\VD032519\
Data File : VD061314.D
Acq On : 25 Mar 2019 22:16
Operator : VA/AP
Sample : BFB
Misc : 5.00µl/5ml/MSVOA D/SOIL
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D032519S.M
Title : SW846 8260
Last Update : Tue Mar 26 03:31:57 2019

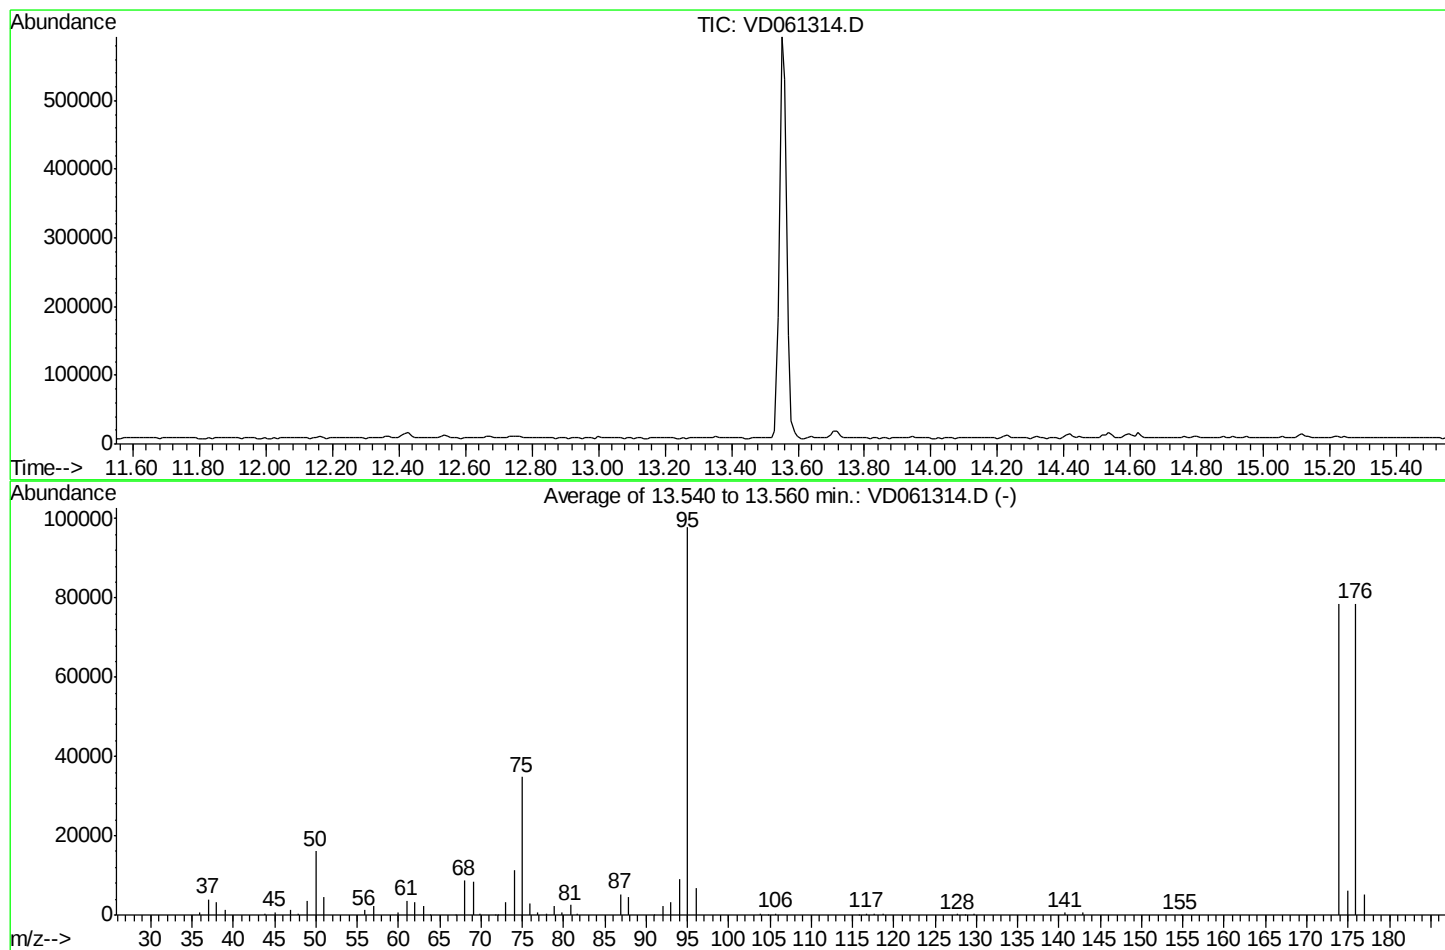

AutoFind: Scans 1231, 1232, 1233; Background Corrected with Scan 1227

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.5	16117	PASS
75	95	30	60	35.6	34792	PASS
95	95	100	100	100.0	97829	PASS
96	95	5	9	6.9	6707	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	80.2	78466	PASS
175	174	5	9	7.7	6016	PASS
176	174	95	101	100.1	78549	PASS
177	176	5	9	6.5	5121	PASS