


Data Path : Z:\voasrv\HPCHEM1\MSVOA D\Data\VD032619\
 Data File : VD061332.D
 Acq On : 26 Mar 2019 12:54
 Operator : VA/AP
 Sample : BFB
 Misc : 5.00g/5ml/MSVOA D/SOIL
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D032519S.M
 Title : SW846 8260
 Last Update : Tue Mar 26 03:31:57 2019

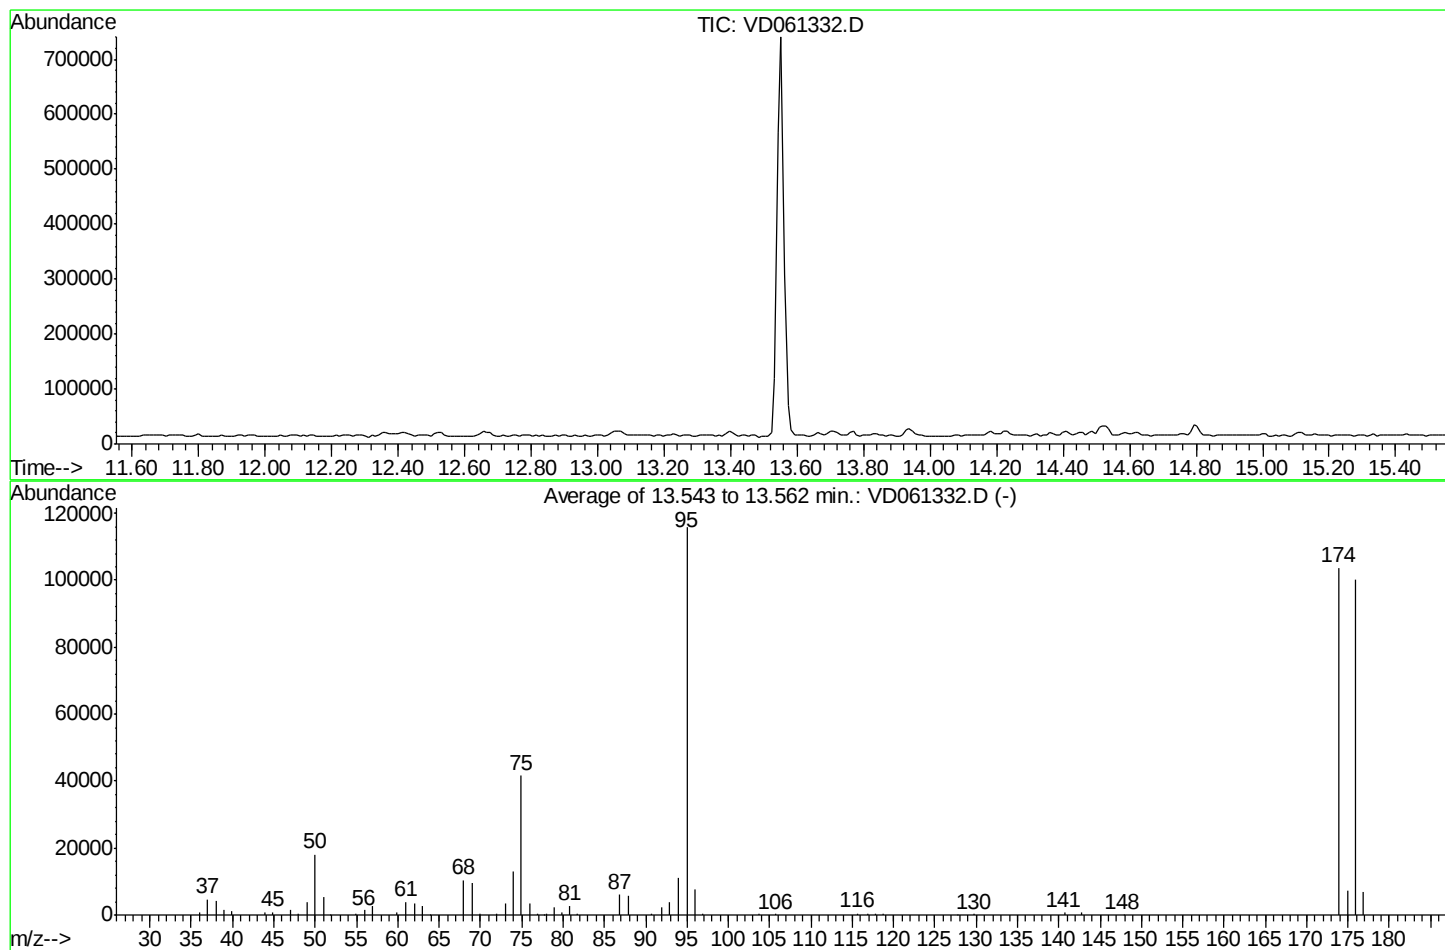

AutoFind: Scans 1231, 1232, 1233; Background Corrected with Scan 1226

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	15.6	18069	PASS
75	95	30	60	35.9	41565	PASS
95	95	100	100	100.0	115784	PASS
96	95	5	9	6.6	7619	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	89.5	103648	PASS
175	174	5	9	7.1	7329	PASS
176	174	95	101	96.6	100146	PASS
177	176	5	9	6.8	6797	PASS