




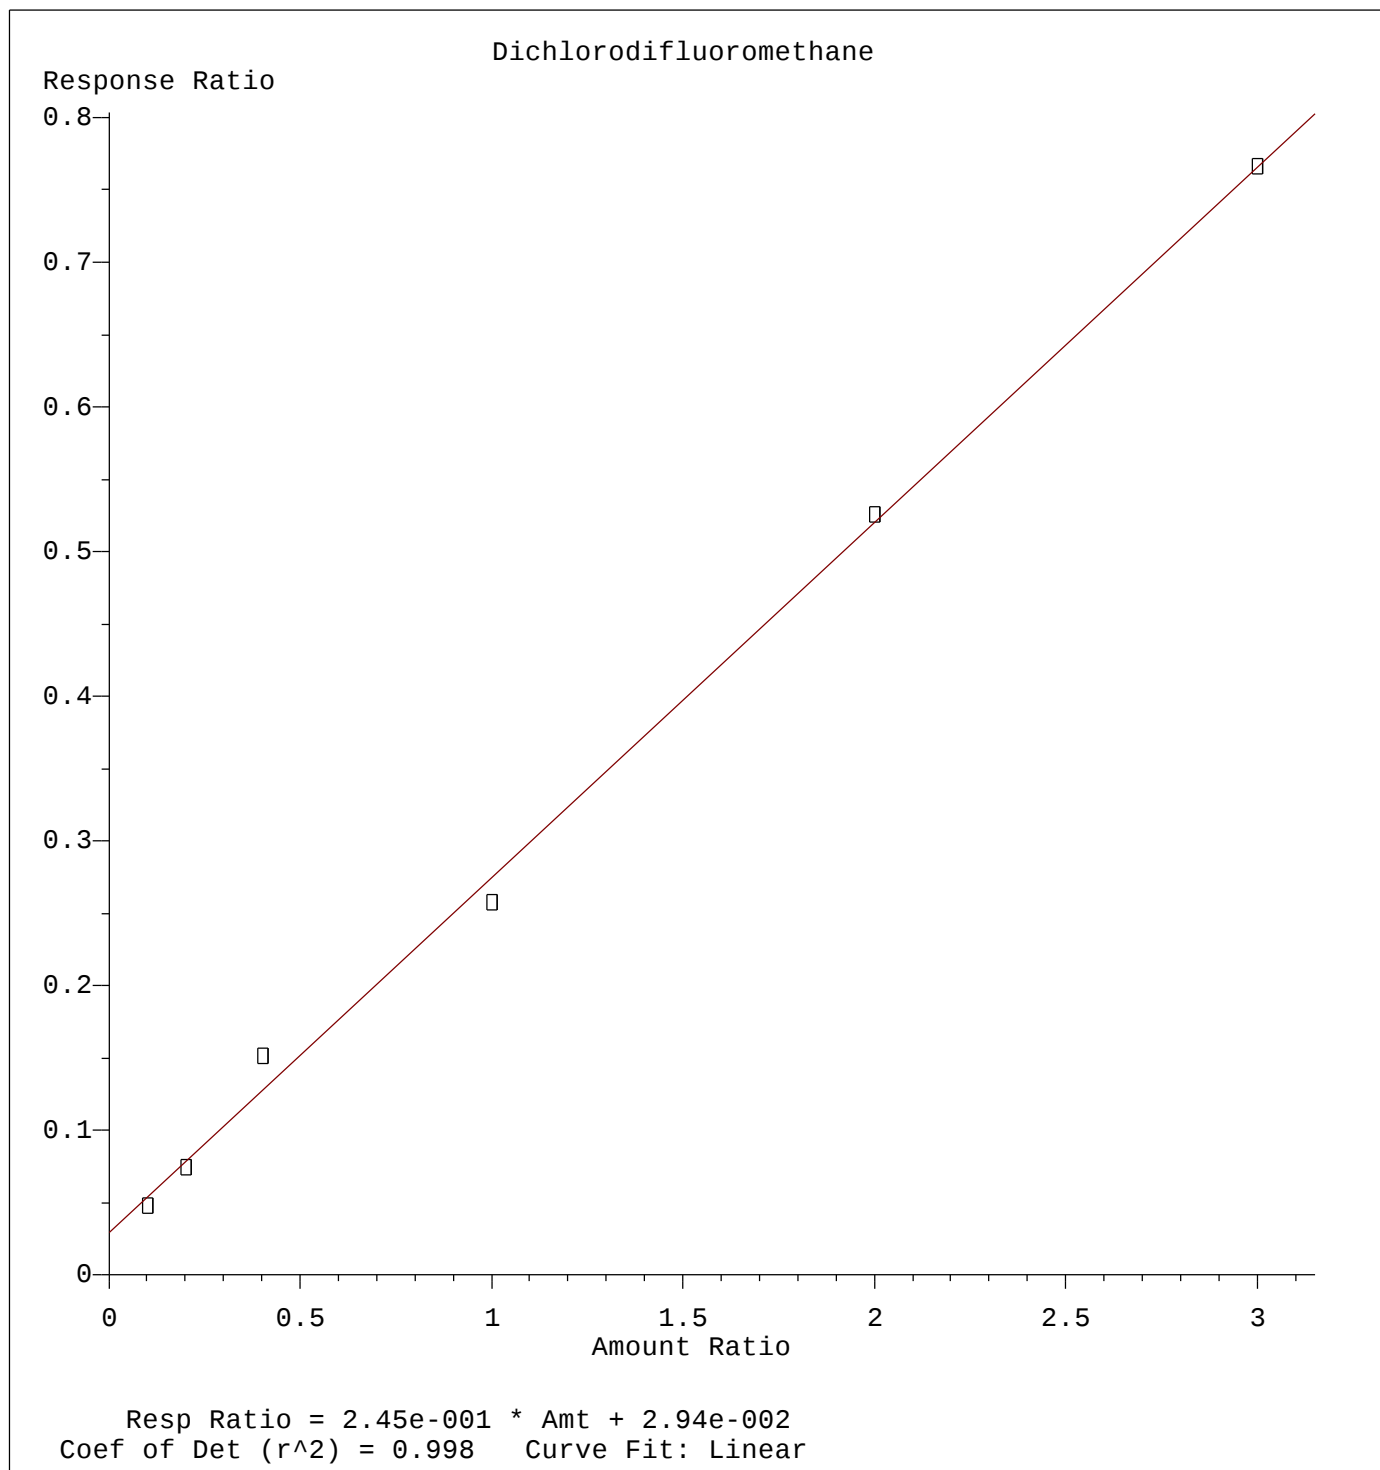

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D032620S.M
Calibration Table Last Updated: Fri Mar 27 01:47:48 2020

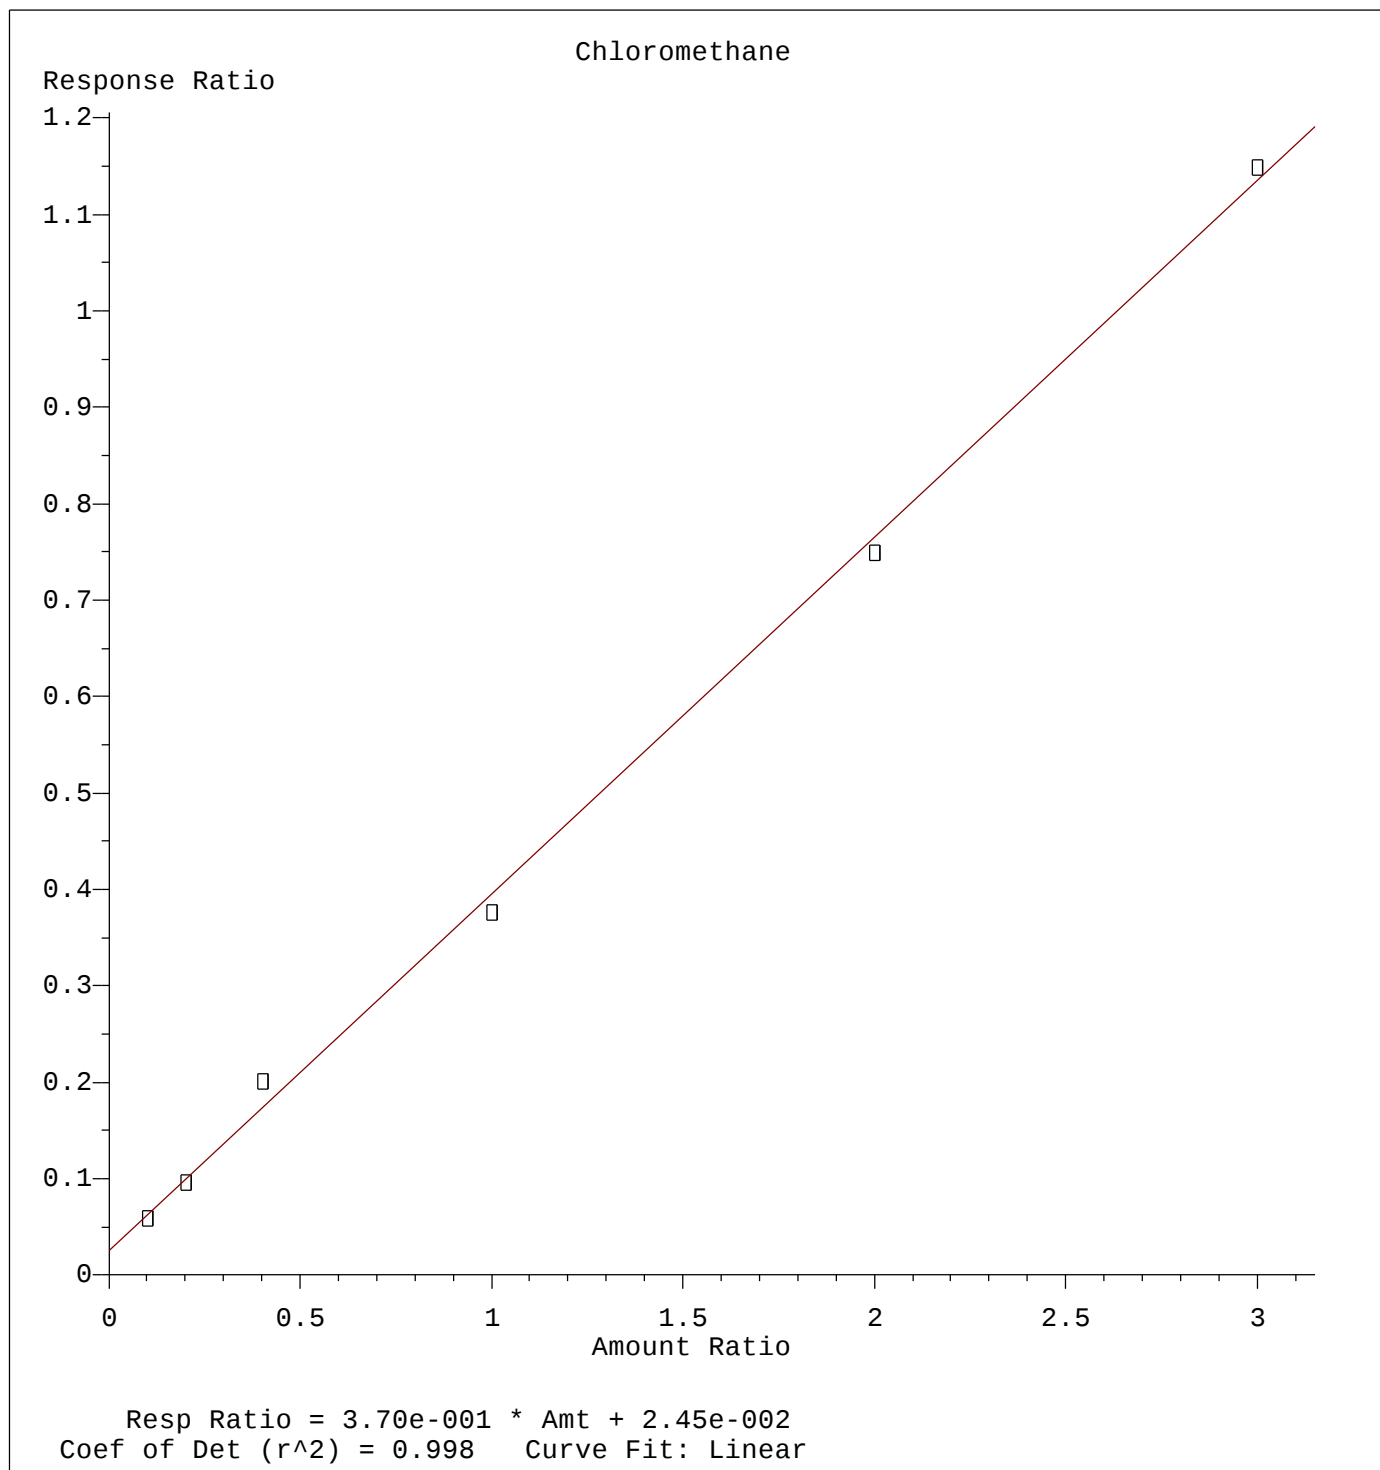


Method Name: Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D032620S.M
Calibration Table Last Updated: Fri Mar 27 01:47:48 2020

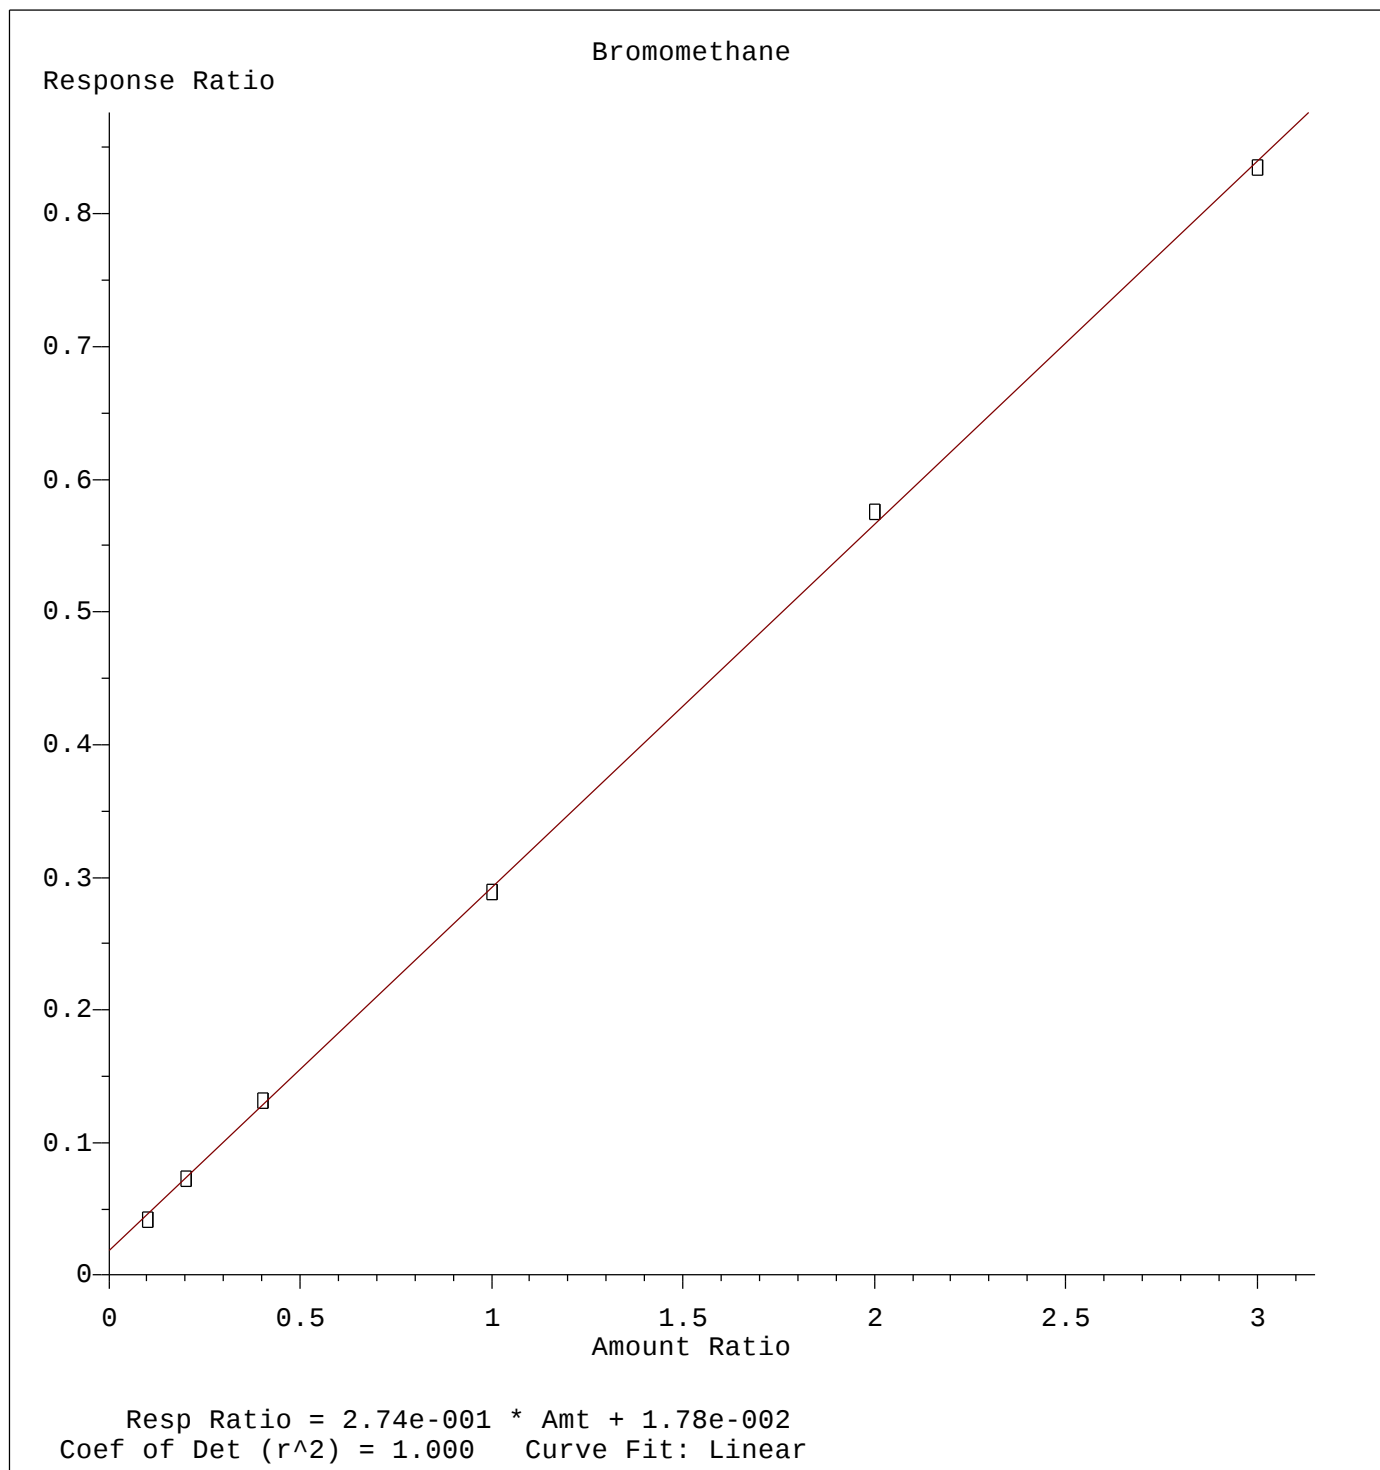

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D032620S.M
Calibration Table Last Updated: Fri Mar 27 01:47:48 2020

Methylene Chloride

Response Ratio

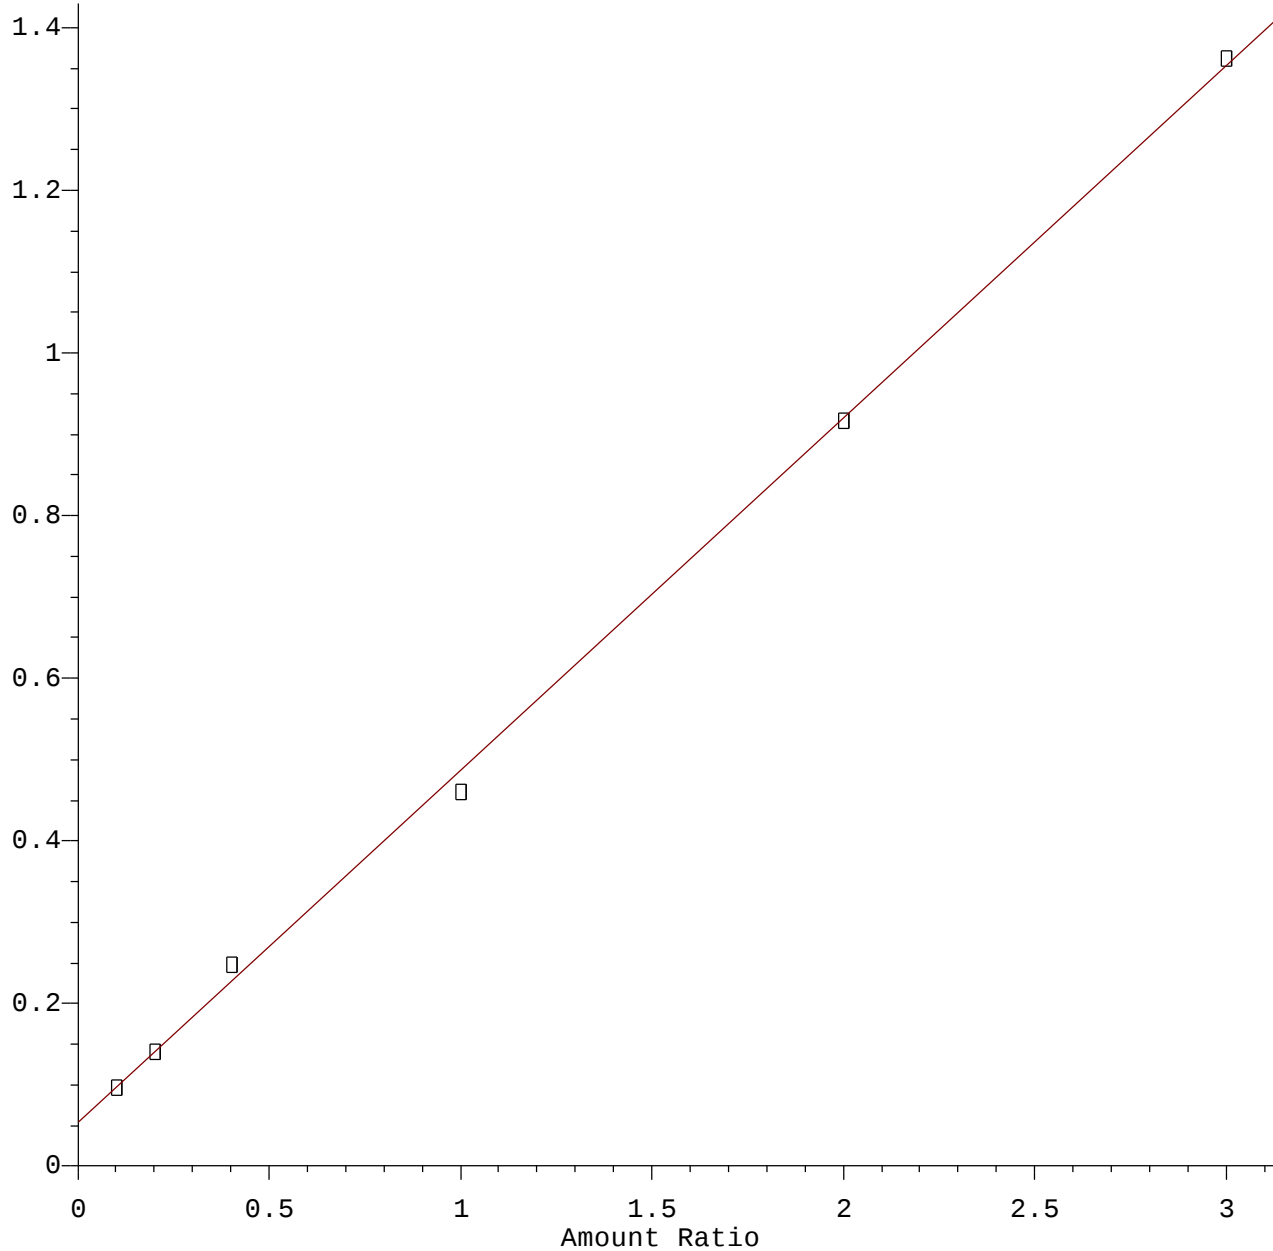


Resp Ratio = $4.33\text{e-}001 \times \text{Amt} + 5.29\text{e-}002$
Coef of Det (r^2) = 0.999 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D032620S.M
Calibration Table Last Updated: Fri Mar 27 01:47:48 2020


Naphthalene

Response Ratio

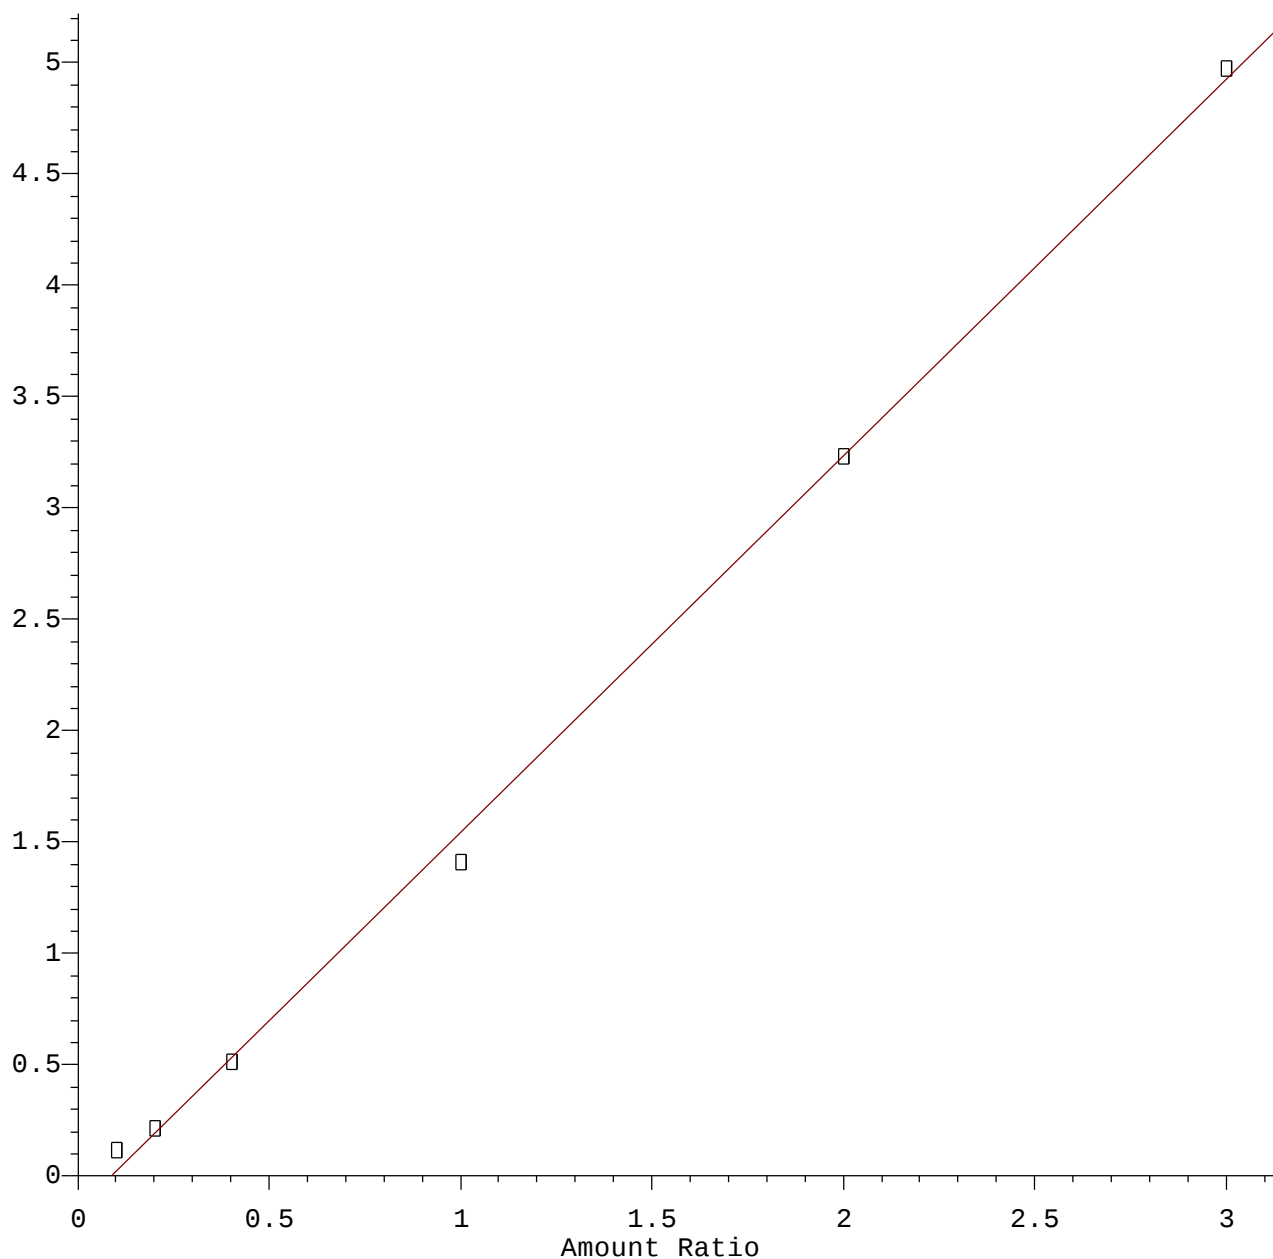


Resp Ratio = 1.69e+000 * Amt - 1.46e-001
Coef of Det (r^2) = 0.998 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D032620S.M
Calibration Table Last Updated: Fri Mar 27 01:47:48 2020

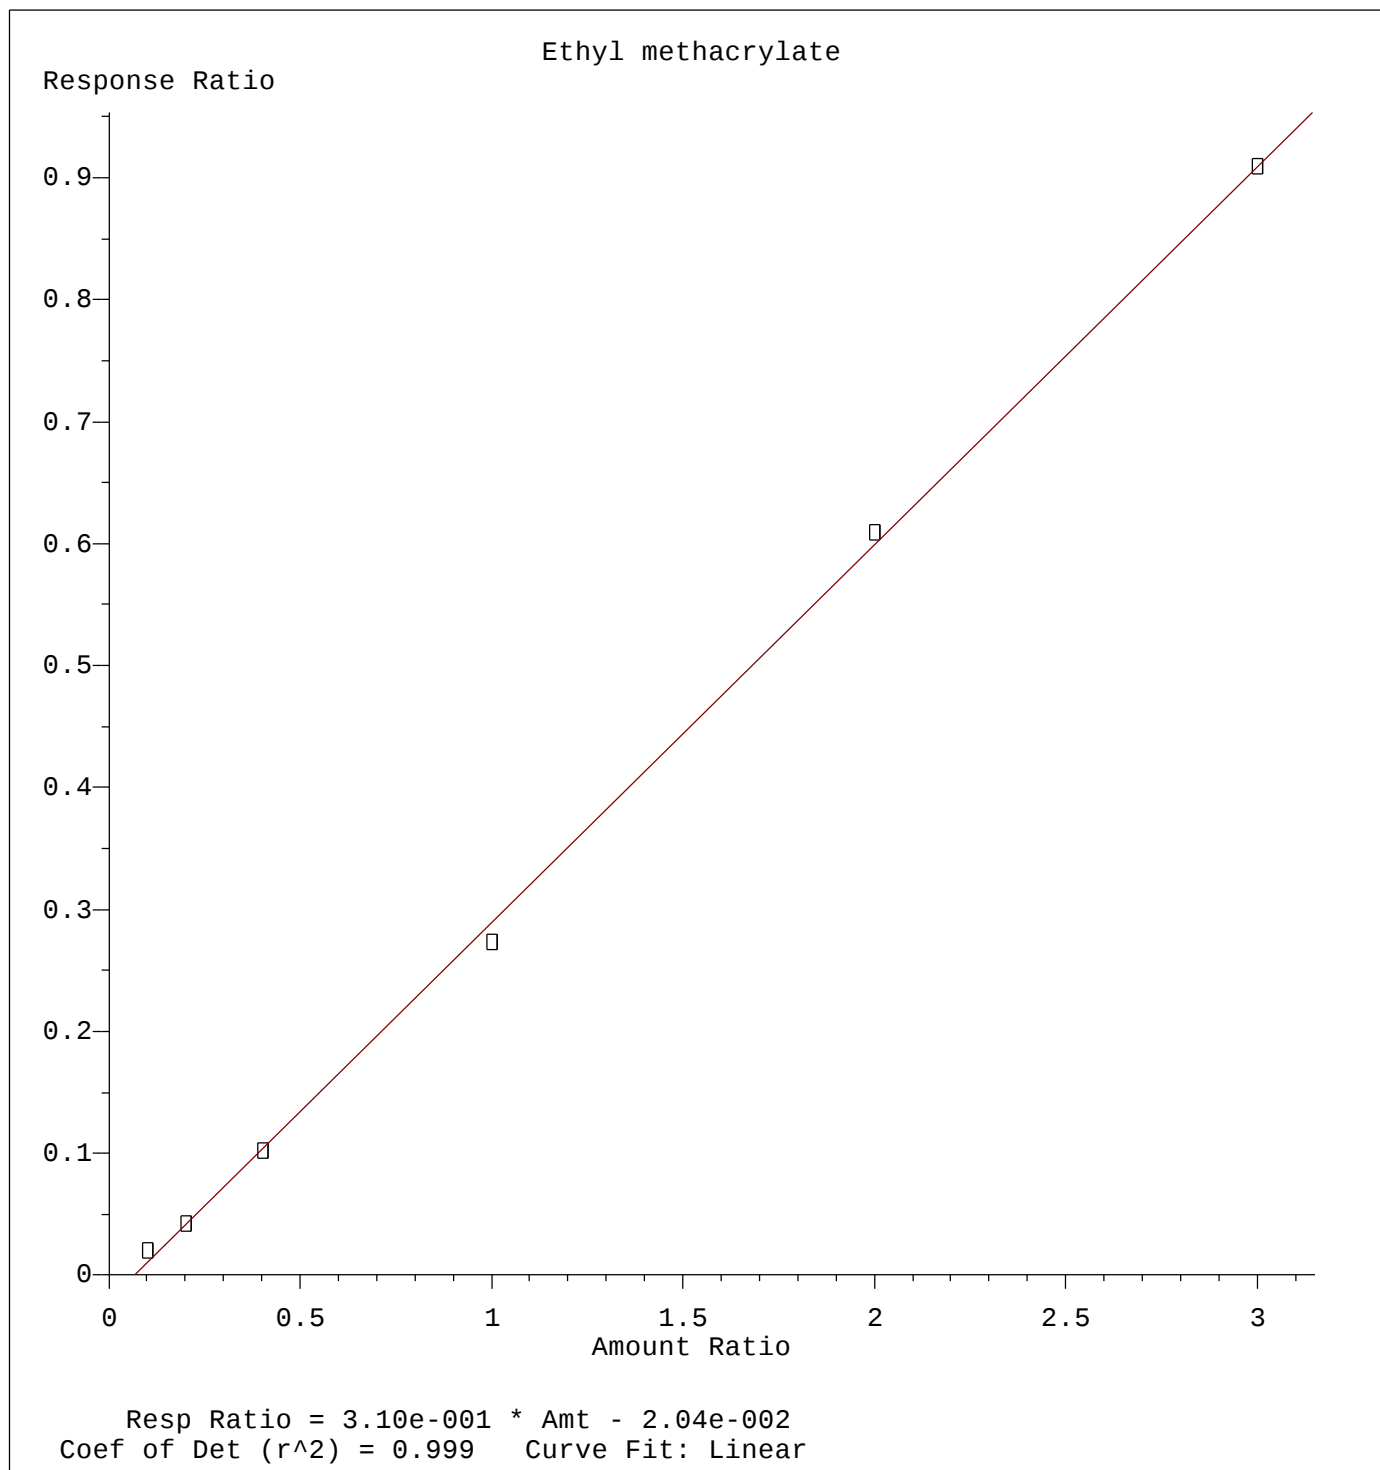

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D032620S.M
Calibration Table Last Updated: Fri Mar 27 01:47:48 2020

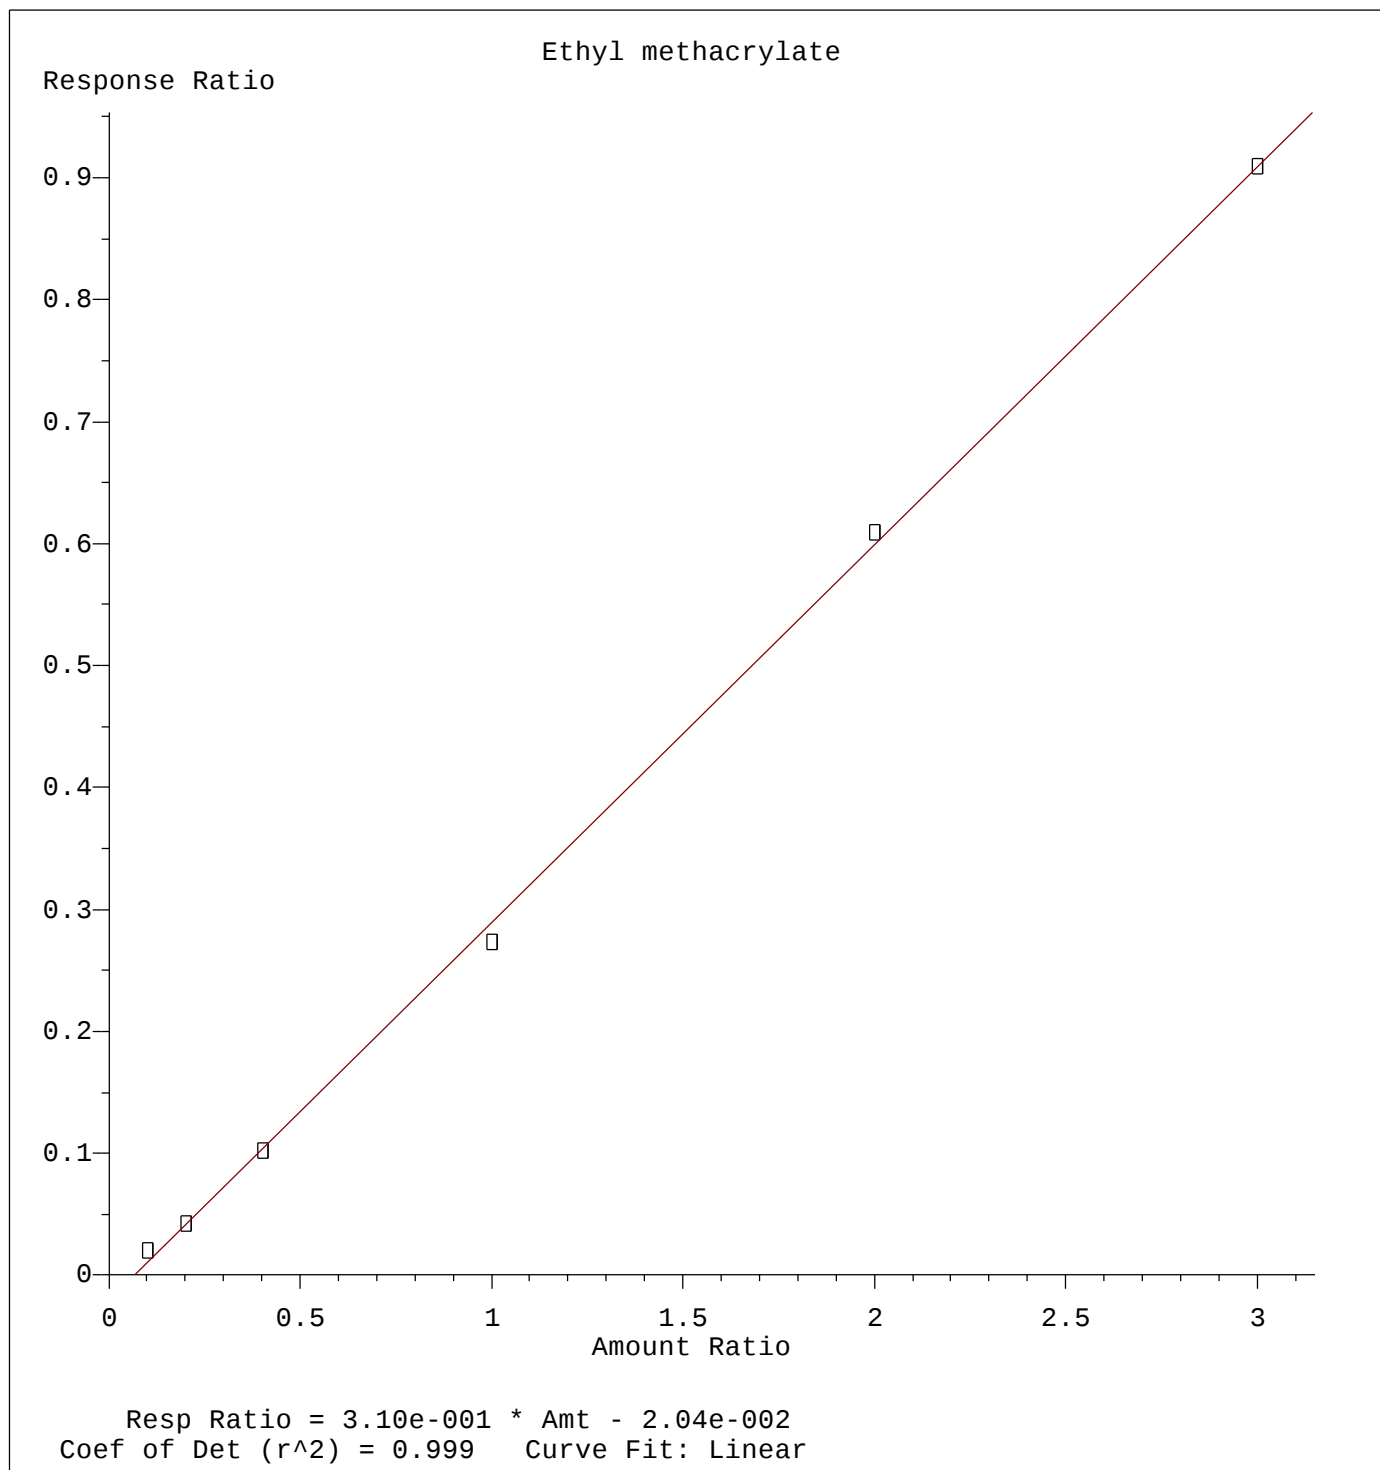

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D032620S.M
Calibration Table Last Updated: Fri Mar 27 01:47:48 2020