


Data Path : Z:\voasrv\HPCHEM1\MSVOA D\Data\VD032620\
Data File : VD065524.D
Acq On : 26 Mar 2020 13:14
Operator : VA/SY
Sample : BFB
Misc : 5.00G/5.00ml/MSVOA D/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D032620S.M
Title : SW846 8260
Last Update : Fri Mar 27 01:47:48 2020

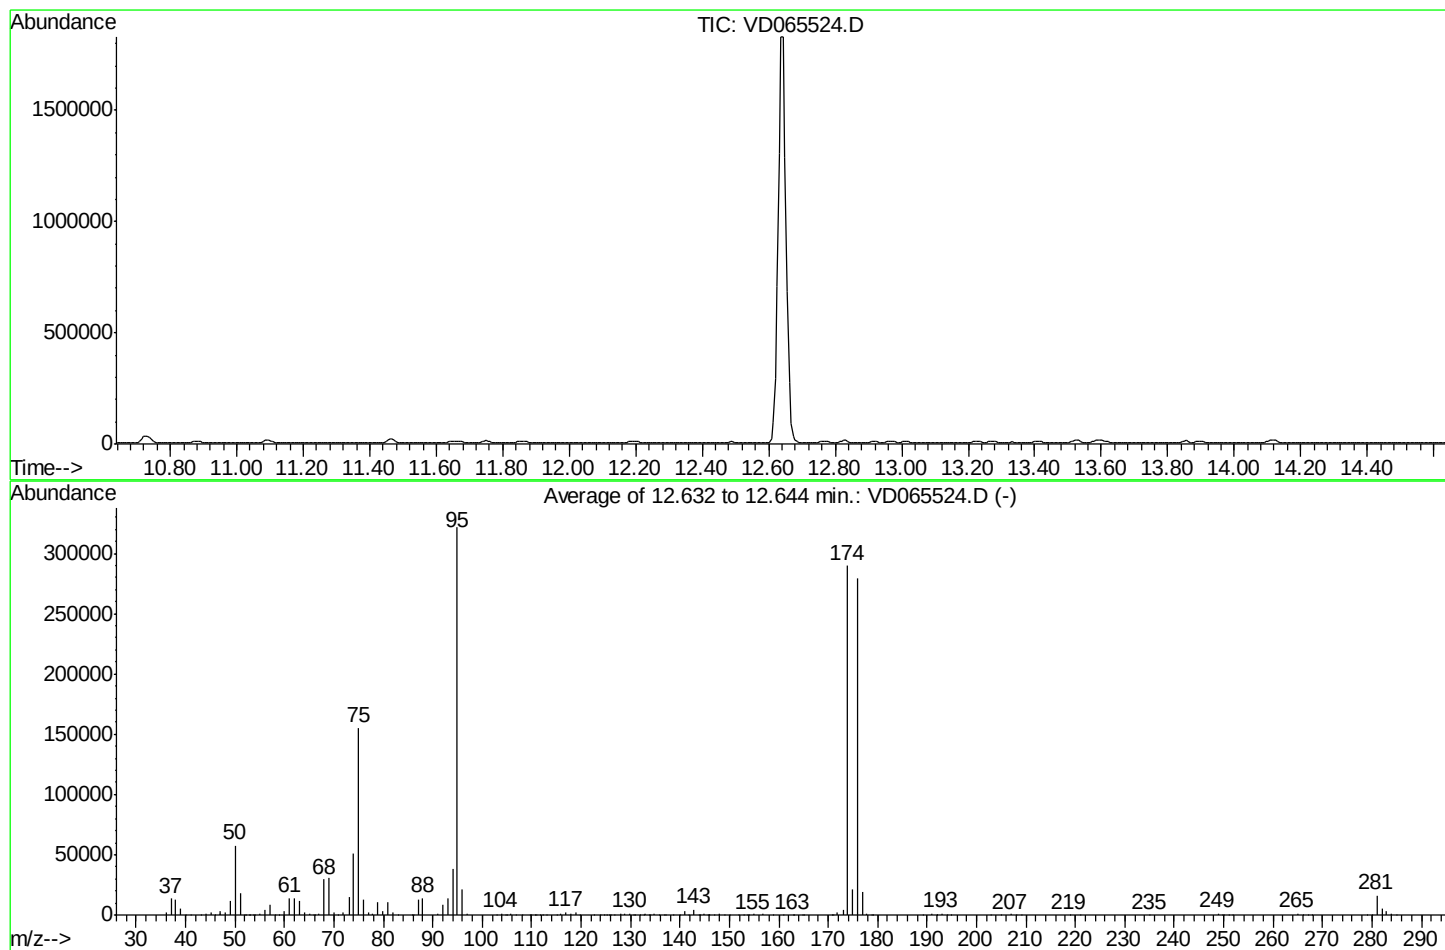

AutoFind: Scans 1821, 1822, 1823; Background Corrected with Scan 1813

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.9	57602	PASS
75	95	30	60	48.3	155221	PASS
95	95	100	100	100.0	321664	PASS
96	95	5	9	6.8	21781	PASS
173	174	0.00	2	1.3	3906	PASS
174	95	50	100	90.0	289578	PASS
175	174	5	9	7.4	21317	PASS
176	174	95	101	96.4	279253	PASS
177	176	5	9	6.8	18869	PASS