
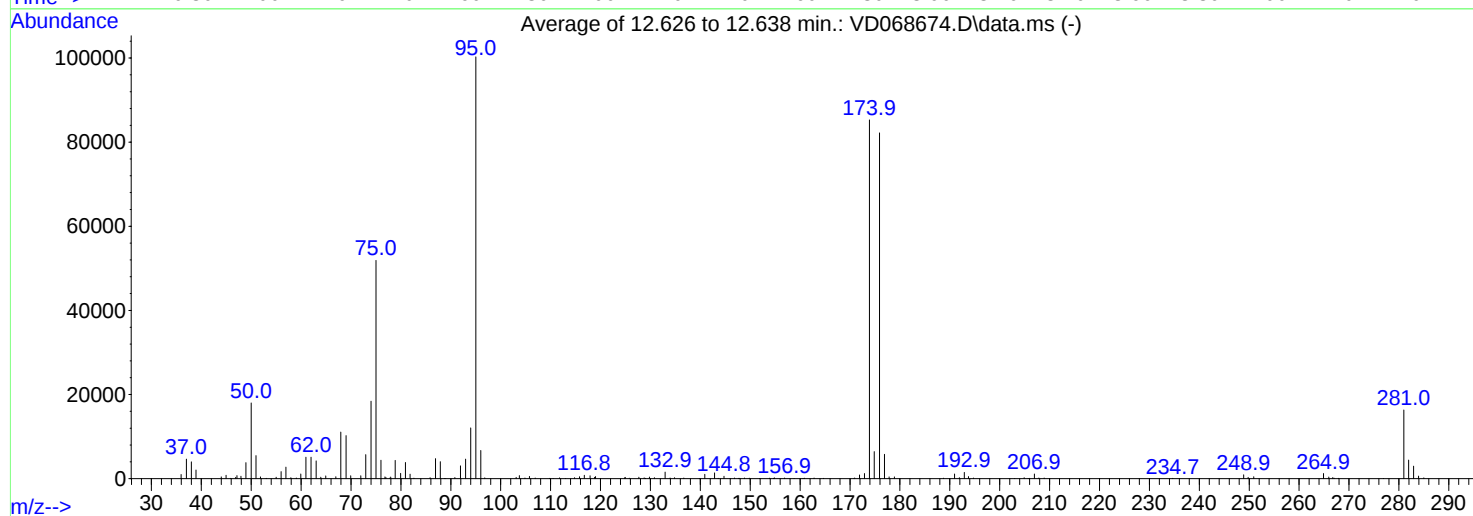


Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD032621\
 Data File : VD068674.D
 Acq On : 26 Mar 2021 09:20
 Operator : VA/SY
 Sample : BFB
 Misc : 5.00G/5.00ml/MSVOA_D/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D031921S.M
 Title : SW846 8260
 Last Update : Sat Mar 20 02:00:55 2021

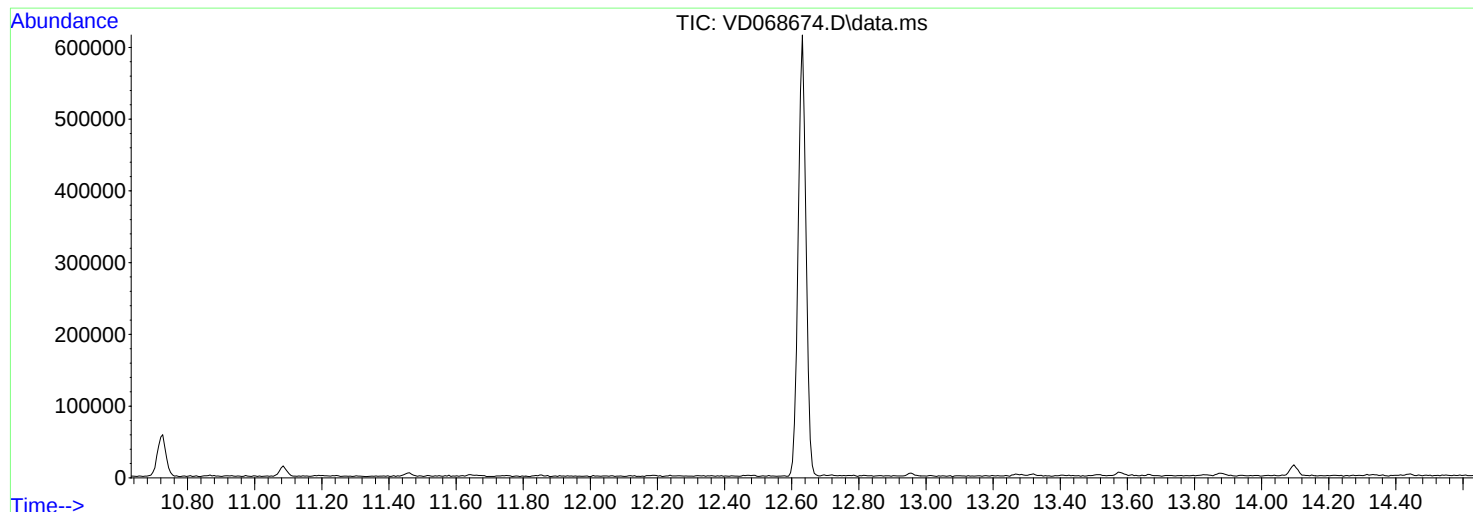

AutoFind: Scans 1820, 1821, 1822; Background Corrected with Scan 1812

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.0	18006	PASS
75	95	30	60	51.7	51896	PASS
95	95	100	100	100.0	100285	PASS
96	95	5	9	6.7	6681	PASS
173	174	0.00	2	1.4	1224	PASS
174	95	50	100	85.1	85301	PASS
175	174	5	9	7.5	6416	PASS
176	174	95	101	96.4	82213	PASS
177	176	5	9	7.1	5802	PASS