


Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD032719\
Data File : VD061346.D
Acq On : 27 Mar 2019 10:00
Operator : VA/AP
Sample : BFB
Misc : 5.00g/5ml/MSVOA_D/SOIL
ALS Vial : 2 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D032719S.M
Title : SW846 8260
Last Update : Thu Mar 28 09:22:37 2019

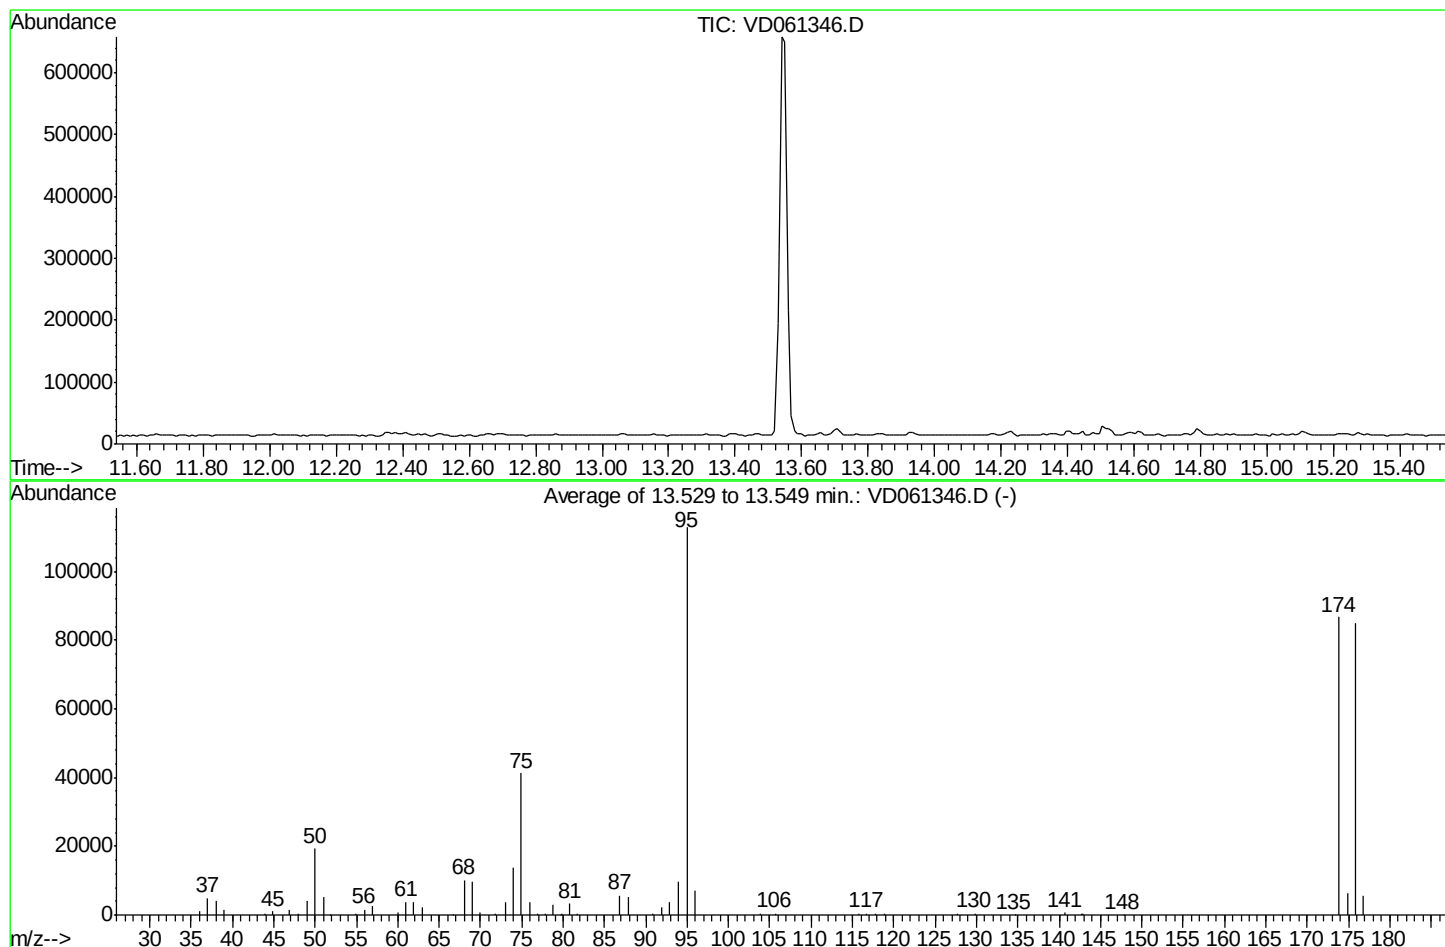

AutoFind: Scans 1230, 1231, 1232; Background Corrected with Scan 1226

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.2	19369	PASS
75	95	30	60	36.5	41194	PASS
95	95	100	100	100.0	112840	PASS
96	95	5	9	6.4	7271	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	76.9	86738	PASS
175	174	5	9	7.2	6210	PASS
176	174	95	101	97.7	84781	PASS
177	176	5	9	6.6	5584	PASS