


Data Path : Z:\VOASRV\HPCHEM1\MSVOA_D\DATA\VD032719\
Data File : VD061366.D
Acq On : 27 Mar 2019 22:33
Operator : VA/AP
Sample : BFB
Misc : 5.00g/5ml/MSVOA_D/SOIL
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D032719S.M
Title : SW846 8260
Last Update : Thu Mar 28 09:22:37 2019

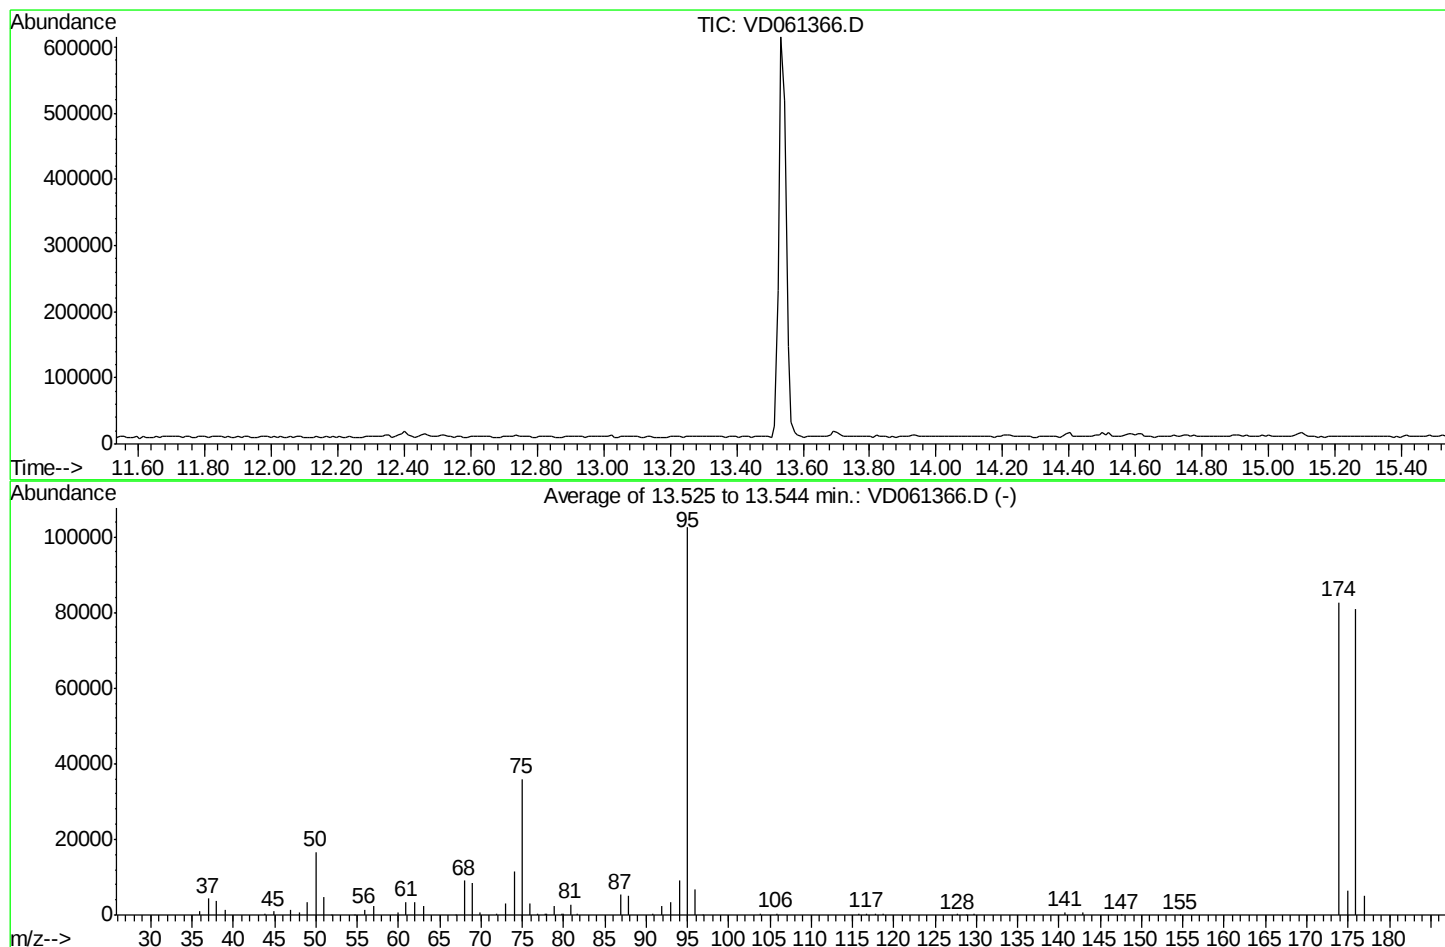

AutoFind: Scans 1229, 1230, 1231; Background Corrected with Scan 1225

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.2	16646	PASS
75	95	30	60	35.0	35888	PASS
95	95	100	100	100.0	102501	PASS
96	95	5	9	6.7	6904	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	80.6	82642	PASS
175	174	5	9	7.6	6304	PASS
176	174	95	101	97.9	80890	PASS
177	176	5	9	6.3	5069	PASS