


Data Path : Z:\VOASRV\HPCHEM1\MSVOA D\DATA\VD032819\
 Data File : VD061388.D
 Acq On : 28 Mar 2019 12:42
 Operator : VA/AP
 Sample : BFB
 Misc : 5.00g/5ml/MSVOA D/SOIL
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D032719S.M
 Title : SW846 8260
 Last Update : Thu Mar 28 09:22:37 2019

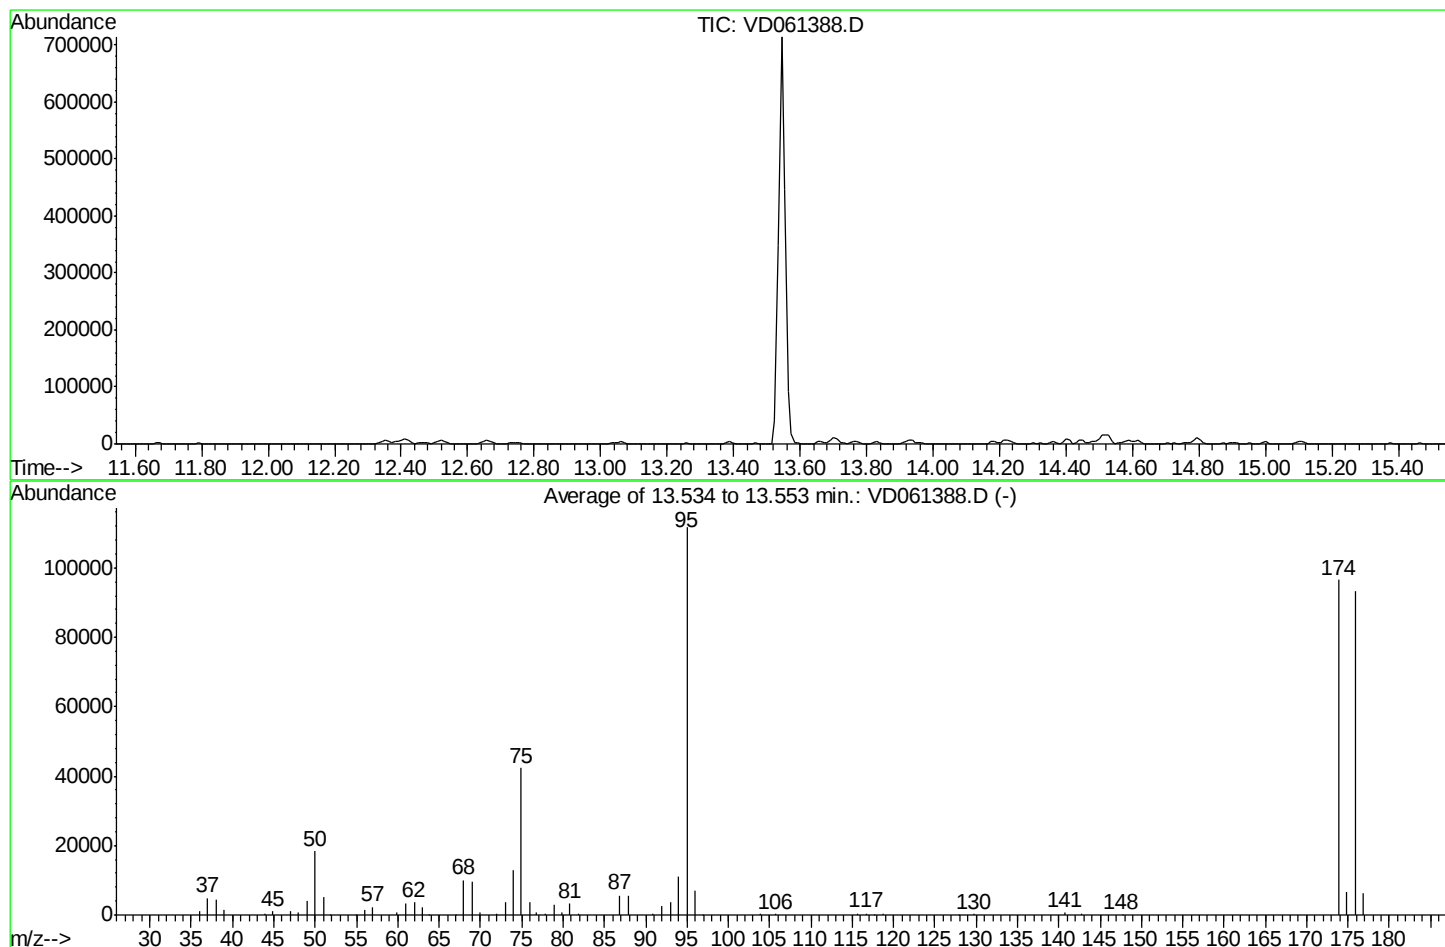

AutoFind: Scans 1230, 1231, 1232; Background Corrected with Scan 1226

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.5	18374	PASS
75	95	30	60	37.9	42357	PASS
95	95	100	100	100.0	111664	PASS
96	95	5	9	6.4	7143	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	86.4	96442	PASS
175	174	5	9	6.9	6702	PASS
176	174	95	101	96.8	93338	PASS
177	176	5	9	6.7	6223	PASS