

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD032824\
 Data File : VD078774.D
 Acq On : 28 Mar 2024 15:07
 Operator : RP/MD
 Sample : P1894-06
 Misc : 5.08G/5ml/MSVOA_D/SOIL/B
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 RT3414

Quant Time: Mar 29 01:35:04 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D031424S.M
 Quant Title : SW846 8260
 QLast Update : Fri Mar 15 05:38:03 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	7.881	168	137759	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.781	114	265477	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.581	117	235407	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.516	152	96353	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.234	65	59879	46.381	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	=	92.760%
35) Dibromofluoromethane	7.810	113	82491	48.261	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	=	96.520%
50) Toluene-d8	10.269	98	323559	51.471	ug/l	0.00
Spiked Amount	50.000	Range	58 - 134	Recovery	=	102.940%
62) 4-Bromofluorobenzene	12.575	95	80714	43.889	ug/l	0.00
Spiked Amount	50.000	Range	30 - 143	Recovery	=	87.780%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD032824\
Data File : VD078774.D
Acq On : 28 Mar 2024 15:07
Operator : RP/MD
Sample : P1894-06
Misc : 5.08G/5ml/MSVOA_D/SOIL/B
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
RT3414

Quant Time: Mar 29 01:35:04 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D031424S.M
Quant Title : SW846 8260
QLast Update : Fri Mar 15 05:38:03 2024
Response via : Initial Calibration




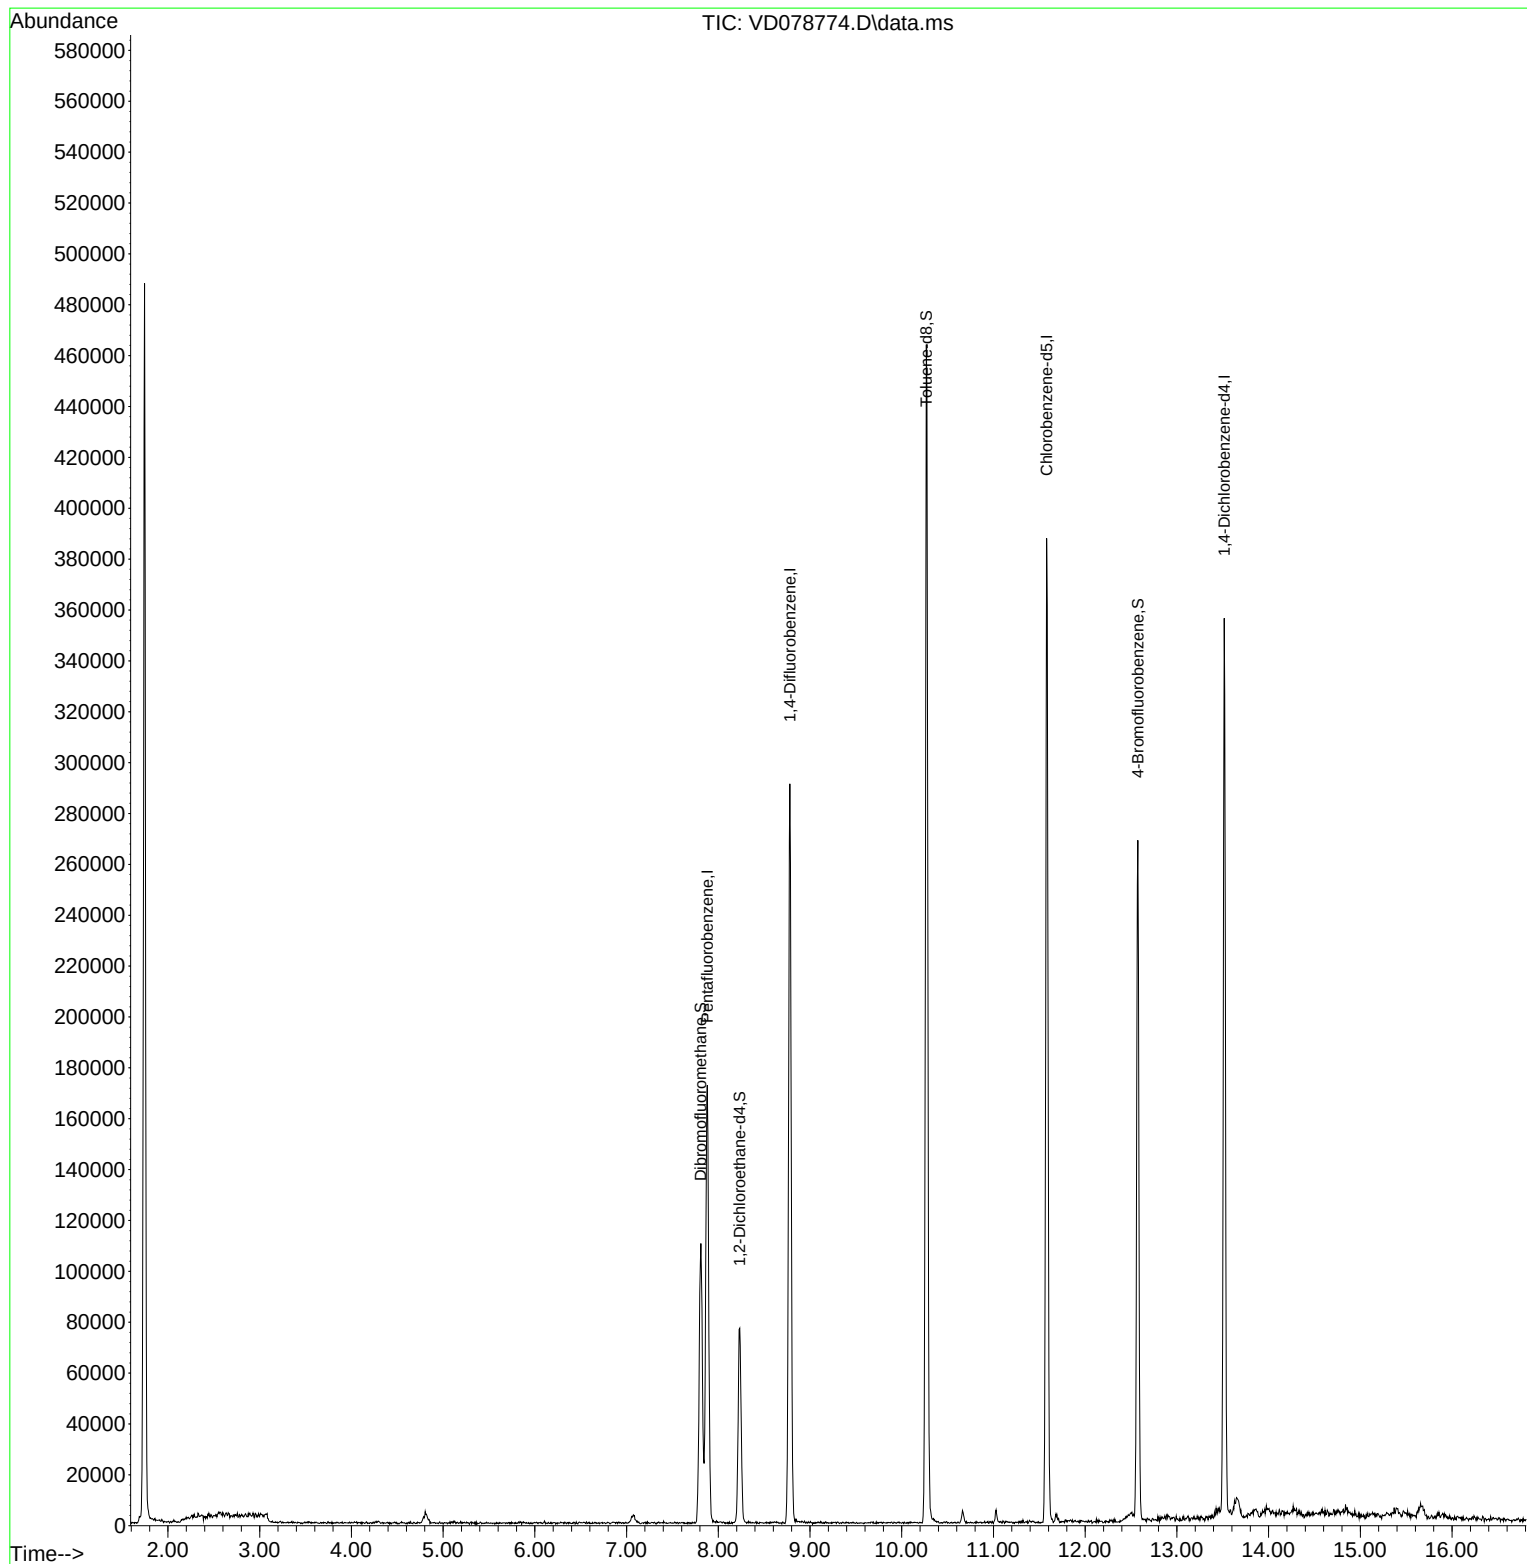


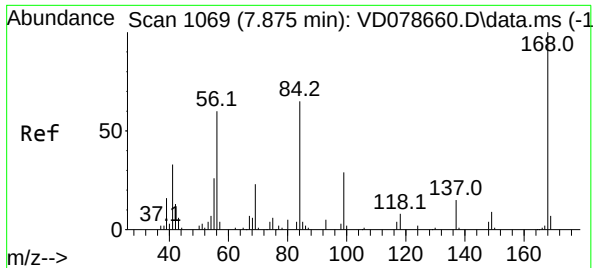

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.881 min Scan# 1069
Delta R.T. 0.006 min
Lab File: VD078774.D
Acq: 28 Mar 2024 15:07




Instrument :
MSVOA_D
ClientSampleId :
RT3414


Tgt Ion:168 Resp: 137759
Ion Ratio Lower Upper
168 100
99 50.1 38.8 58.2

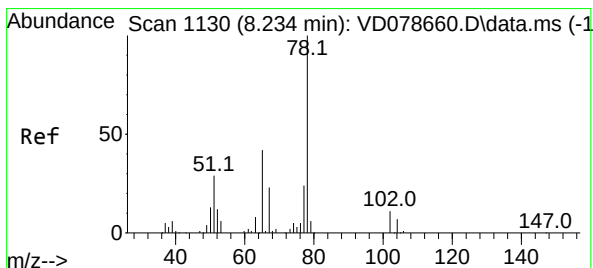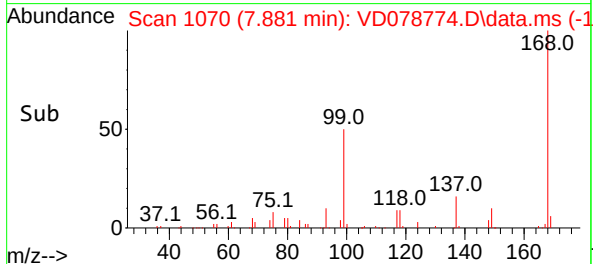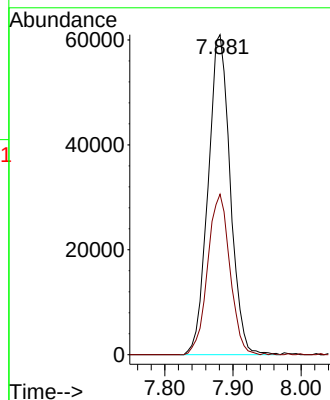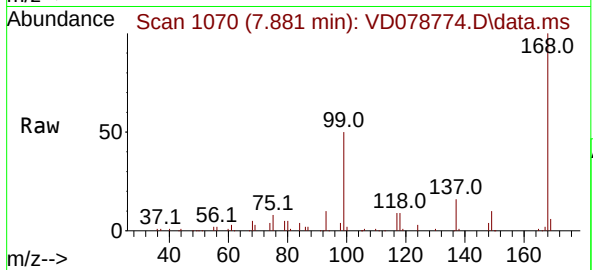

#33
1,2-Dichloroethane-d4
Concen: 46.381 ug/l
RT: 8.234 min Scan# 1130
Delta R.T. -0.000 min
Lab File: VD078774.D
Acq: 28 Mar 2024 15:07

Tgt Ion: 65 Resp: 59879
Ion Ratio Lower Upper
65 100
67 53.5 0.0 110.2

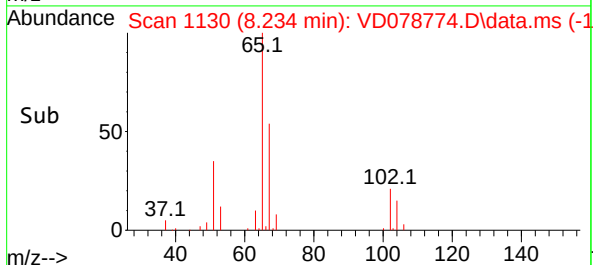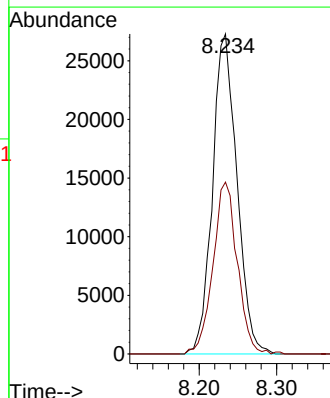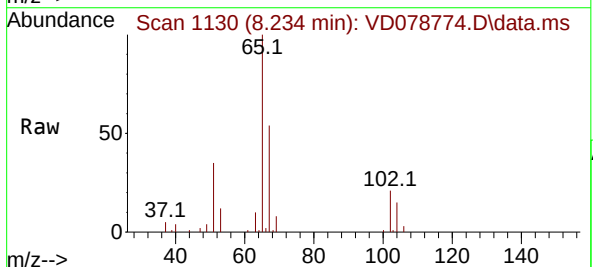

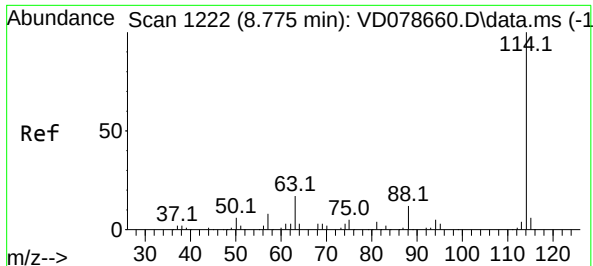

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.781 min Scan# 11

Delta R.T. 0.006 min

Lab File: VD078774.D

Acq: 28 Mar 2024 15:07

Instrument :

MSVOA_D

ClientSampleId :

RT3414





Tgt Ion:114 Resp: 265477

Ion Ratio Lower Upper

114 100

63 17.0 0.0 33.4

88 14.1 0.0 24.6

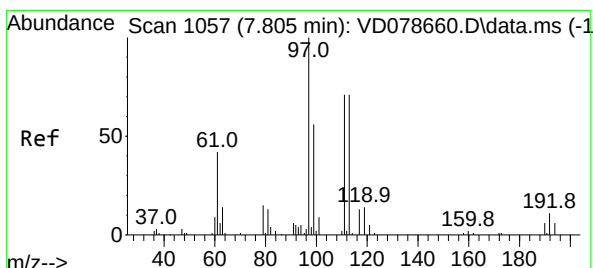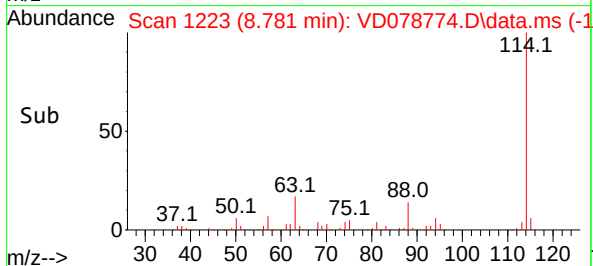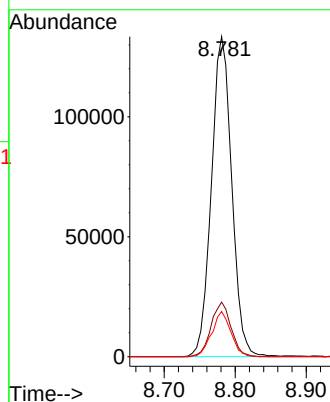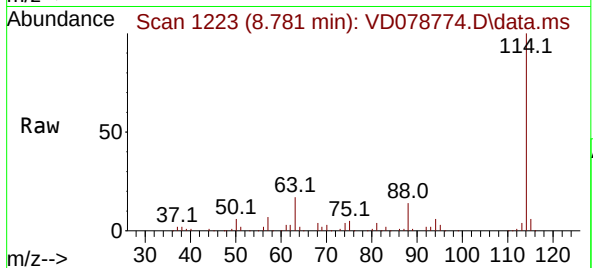

#35

Dibromofluoromethane

Concen: 48.261 ug/l

RT: 7.810 min Scan# 1058

Delta R.T. 0.006 min

Lab File: VD078774.D

Acq: 28 Mar 2024 15:07




Tgt Ion:113 Resp: 82491


Ion Ratio Lower Upper

113 100

111 101.2 81.9 122.9

192 18.5 15.4 23.0


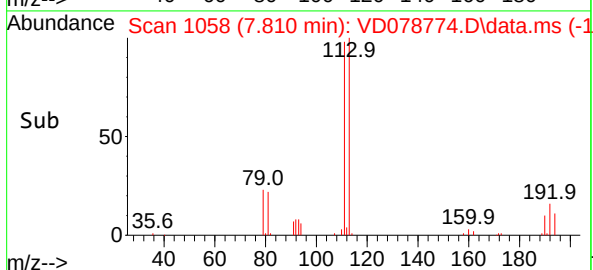
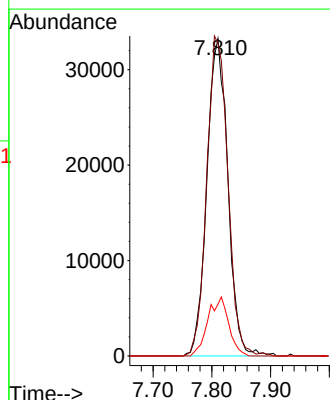
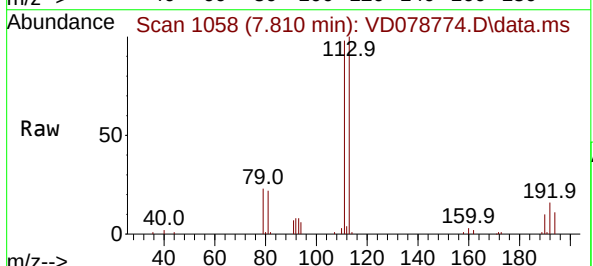


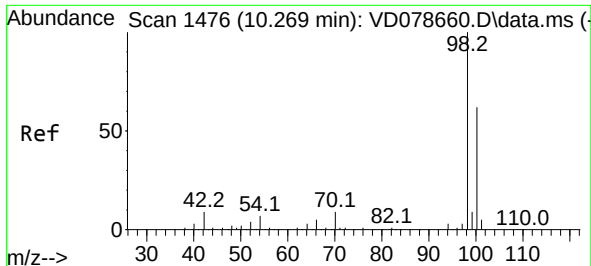

#50
Toluene-d8
Concen: 51.471 ug/l
RT: 10.269 min Scan# 1476
Delta R.T. -0.000 min
Lab File: VD078774.D
Acq: 28 Mar 2024 15:07




Instrument :
MSVOA_D
ClientSampleId :
RT3414


Tgt Ion: 98 Resp: 323559
Ion Ratio Lower Upper
98 100
100 65.0 50.5 75.7

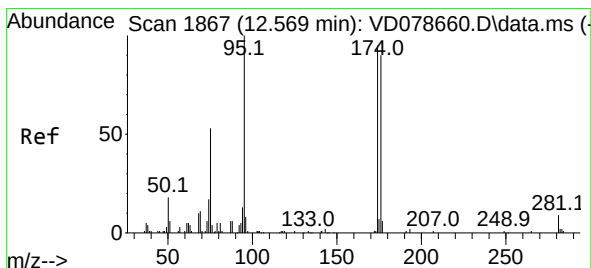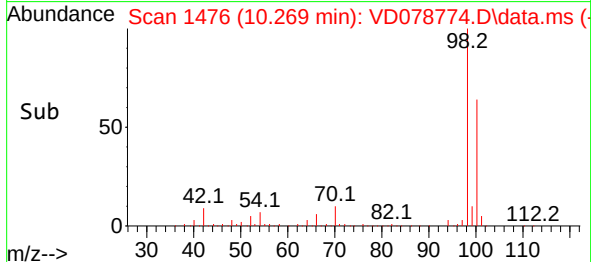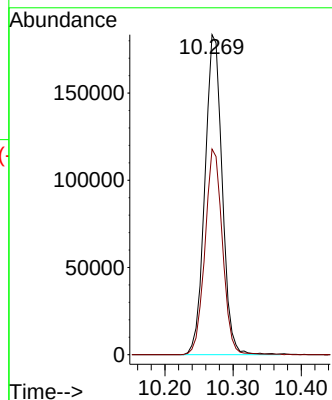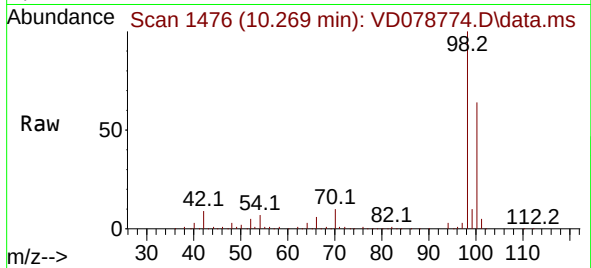

#62
4-Bromofluorobenzene
Concen: 43.889 ug/l
RT: 12.575 min Scan# 1868
Delta R.T. 0.006 min
Lab File: VD078774.D
Acq: 28 Mar 2024 15:07

Tgt Ion: 95 Resp: 80714
Ion Ratio Lower Upper
95 100
174 95.3 0.0 195.2
176 92.7 0.0 188.2


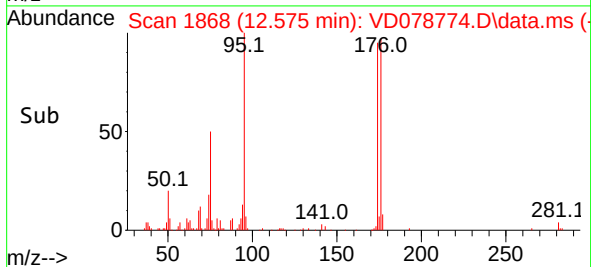
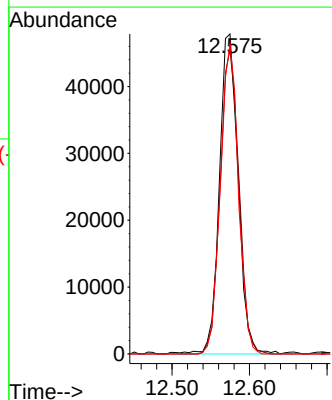
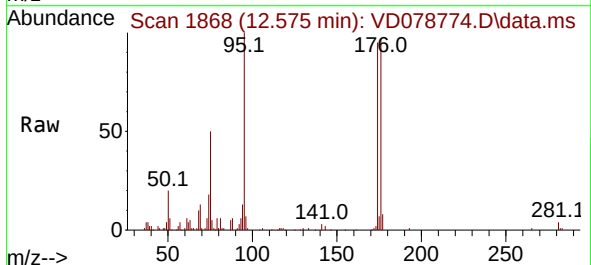


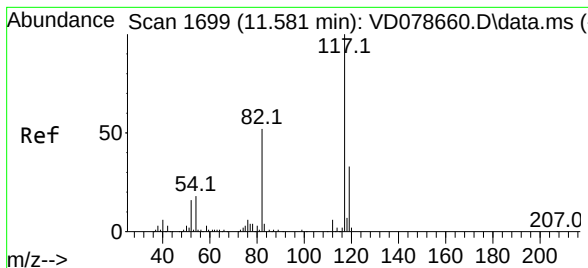

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.581 min Scan# 1
Delta R.T. -0.000 min
Lab File: VD078774.D
Acq: 28 Mar 2024 15:07

Instrument :
MSVOA_D
ClientSampleId :
RT3414

Tgt Ion:117 Resp: 235407
Ion Ratio Lower Upper
117 100
82 48.8 41.4 62.2
119 31.6 26.5 39.7

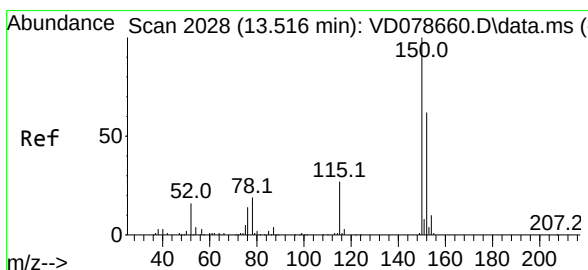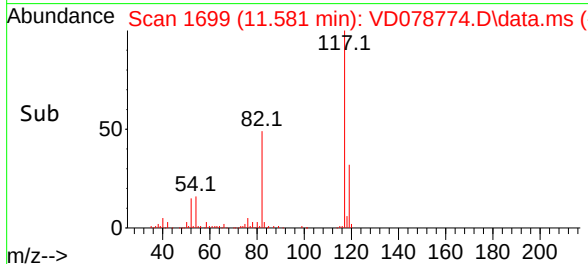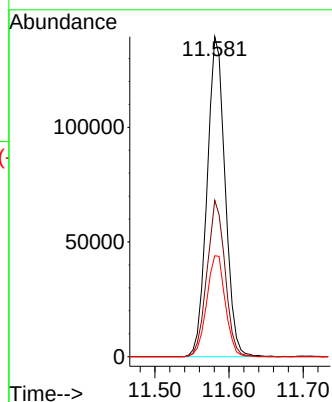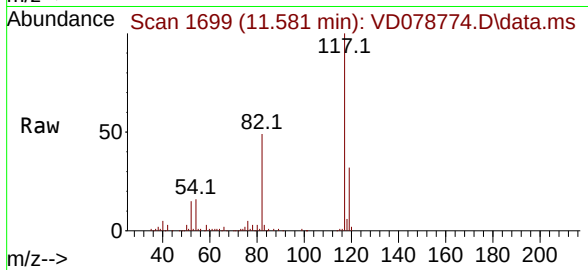

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.516 min Scan# 2028
Delta R.T. -0.000 min
Lab File: VD078774.D
Acq: 28 Mar 2024 15:07

Tgt Ion:152 Resp: 96353
Ion Ratio Lower Upper
152 100
115 54.4 27.1 81.2
150 156.9 0.0 350.2

