
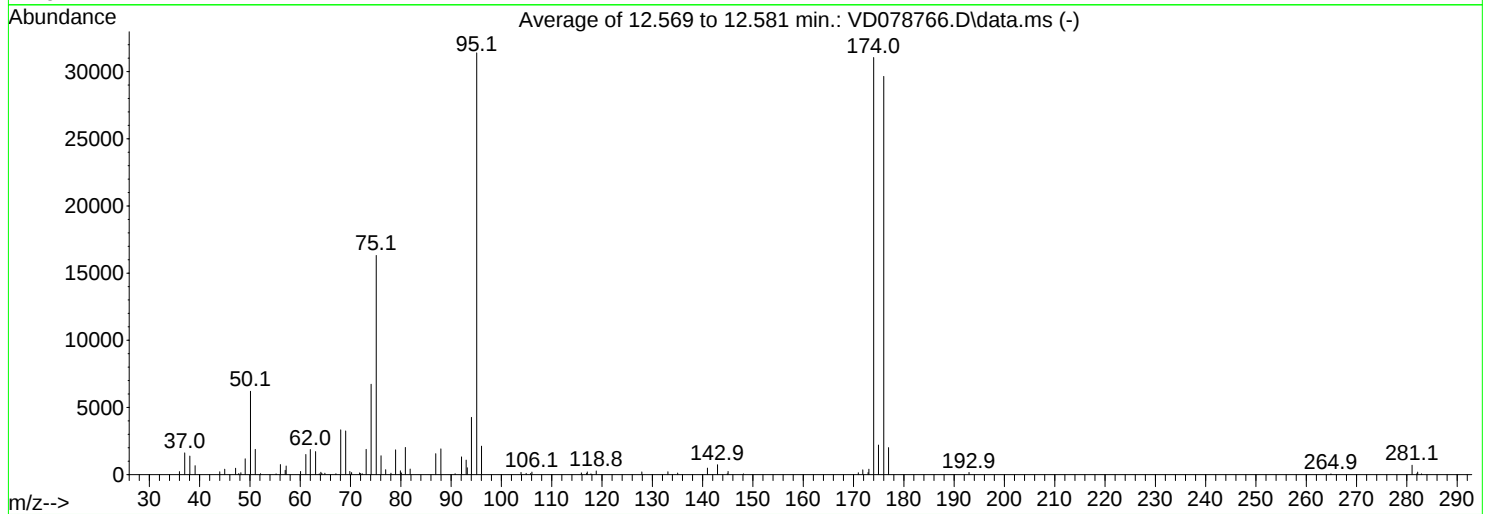


Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD032824\
Data File : VD078766.D
Acq On : 28 Mar 2024 10:07
Operator : RP/MD
Sample : BFB
Misc : 5.00G/5ml/MSVOA_D/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D031424S.M
Title : SW846 8260
Last Update : Fri Mar 15 05:38:03 2024

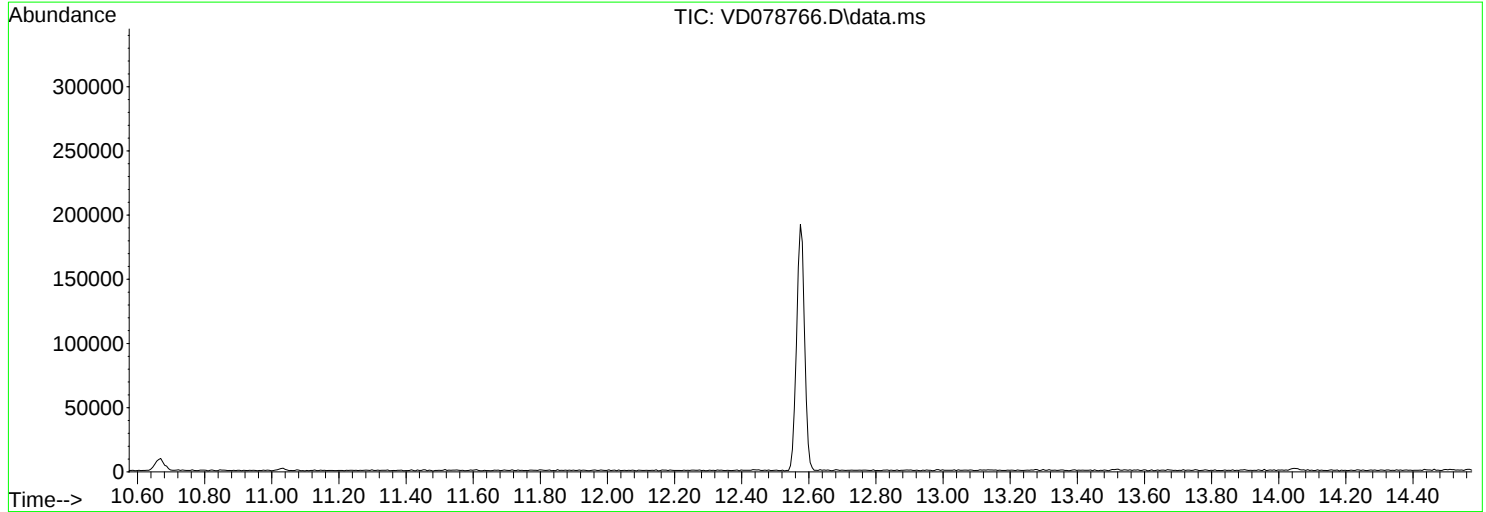

AutoFind: Scans 1867, 1868, 1869; Background Corrected with Scan 1859

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	19.8	6204	PASS
75	95	30	60	52.0	16320	PASS
95	95	100	100	100.0	31397	PASS
96	95	5	9	6.8	2126	PASS
173	174	0.00	2	1.3	409	PASS
174	95	50	100	98.9	31048	PASS
175	174	5	9	7.1	2200	PASS
176	174	95	101	95.5	29645	PASS
177	176	5	9	6.8	2019	PASS