


Data Path : Z:\VOASRV\HPCHEM1\MSVOA D\DATA\VD032919\
 Data File : VD061421.D
 Acq On : 29 Mar 2019 9:18
 Operator : VA/AP
 Sample : BFB
 Misc : 5.00µl/5ml/MSVOA D/SOIL
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D032719S.M
 Title : SW846 8260
 Last Update : Thu Mar 28 09:22:37 2019

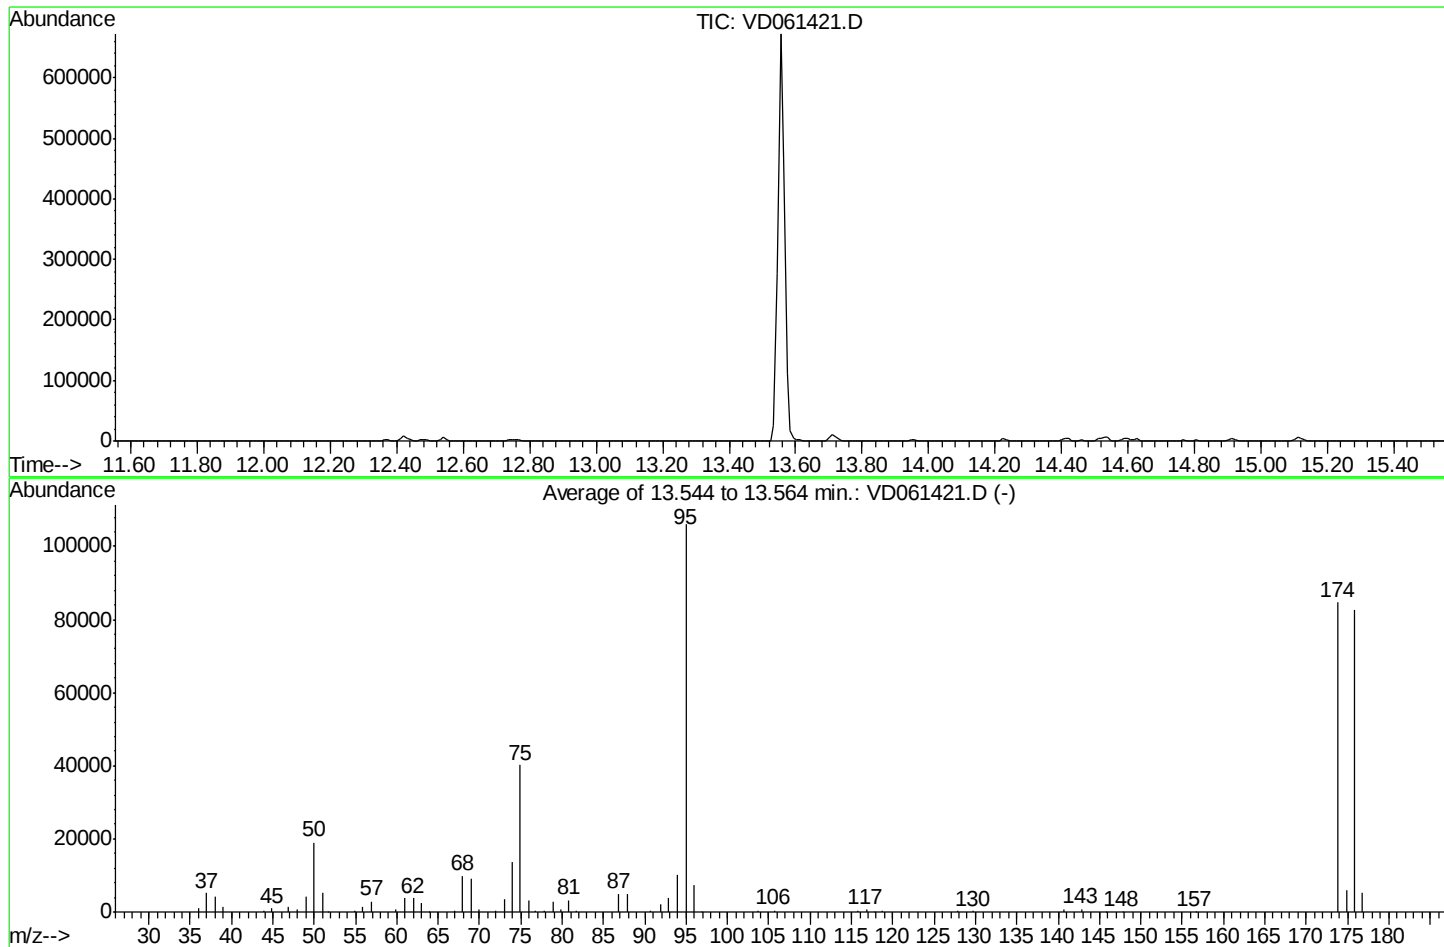

AutoFind: Scans 1231, 1232, 1233; Background Corrected with Scan 1227

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.9	19022	PASS
75	95	30	60	37.8	40122	PASS
95	95	100	100	100.0	106048	PASS
96	95	5	9	7.0	7381	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	79.9	84712	PASS
175	174	5	9	7.1	5997	PASS
176	174	95	101	97.5	82552	PASS
177	176	5	9	6.4	5308	PASS