


Vinyl Chloride

Response Ratio

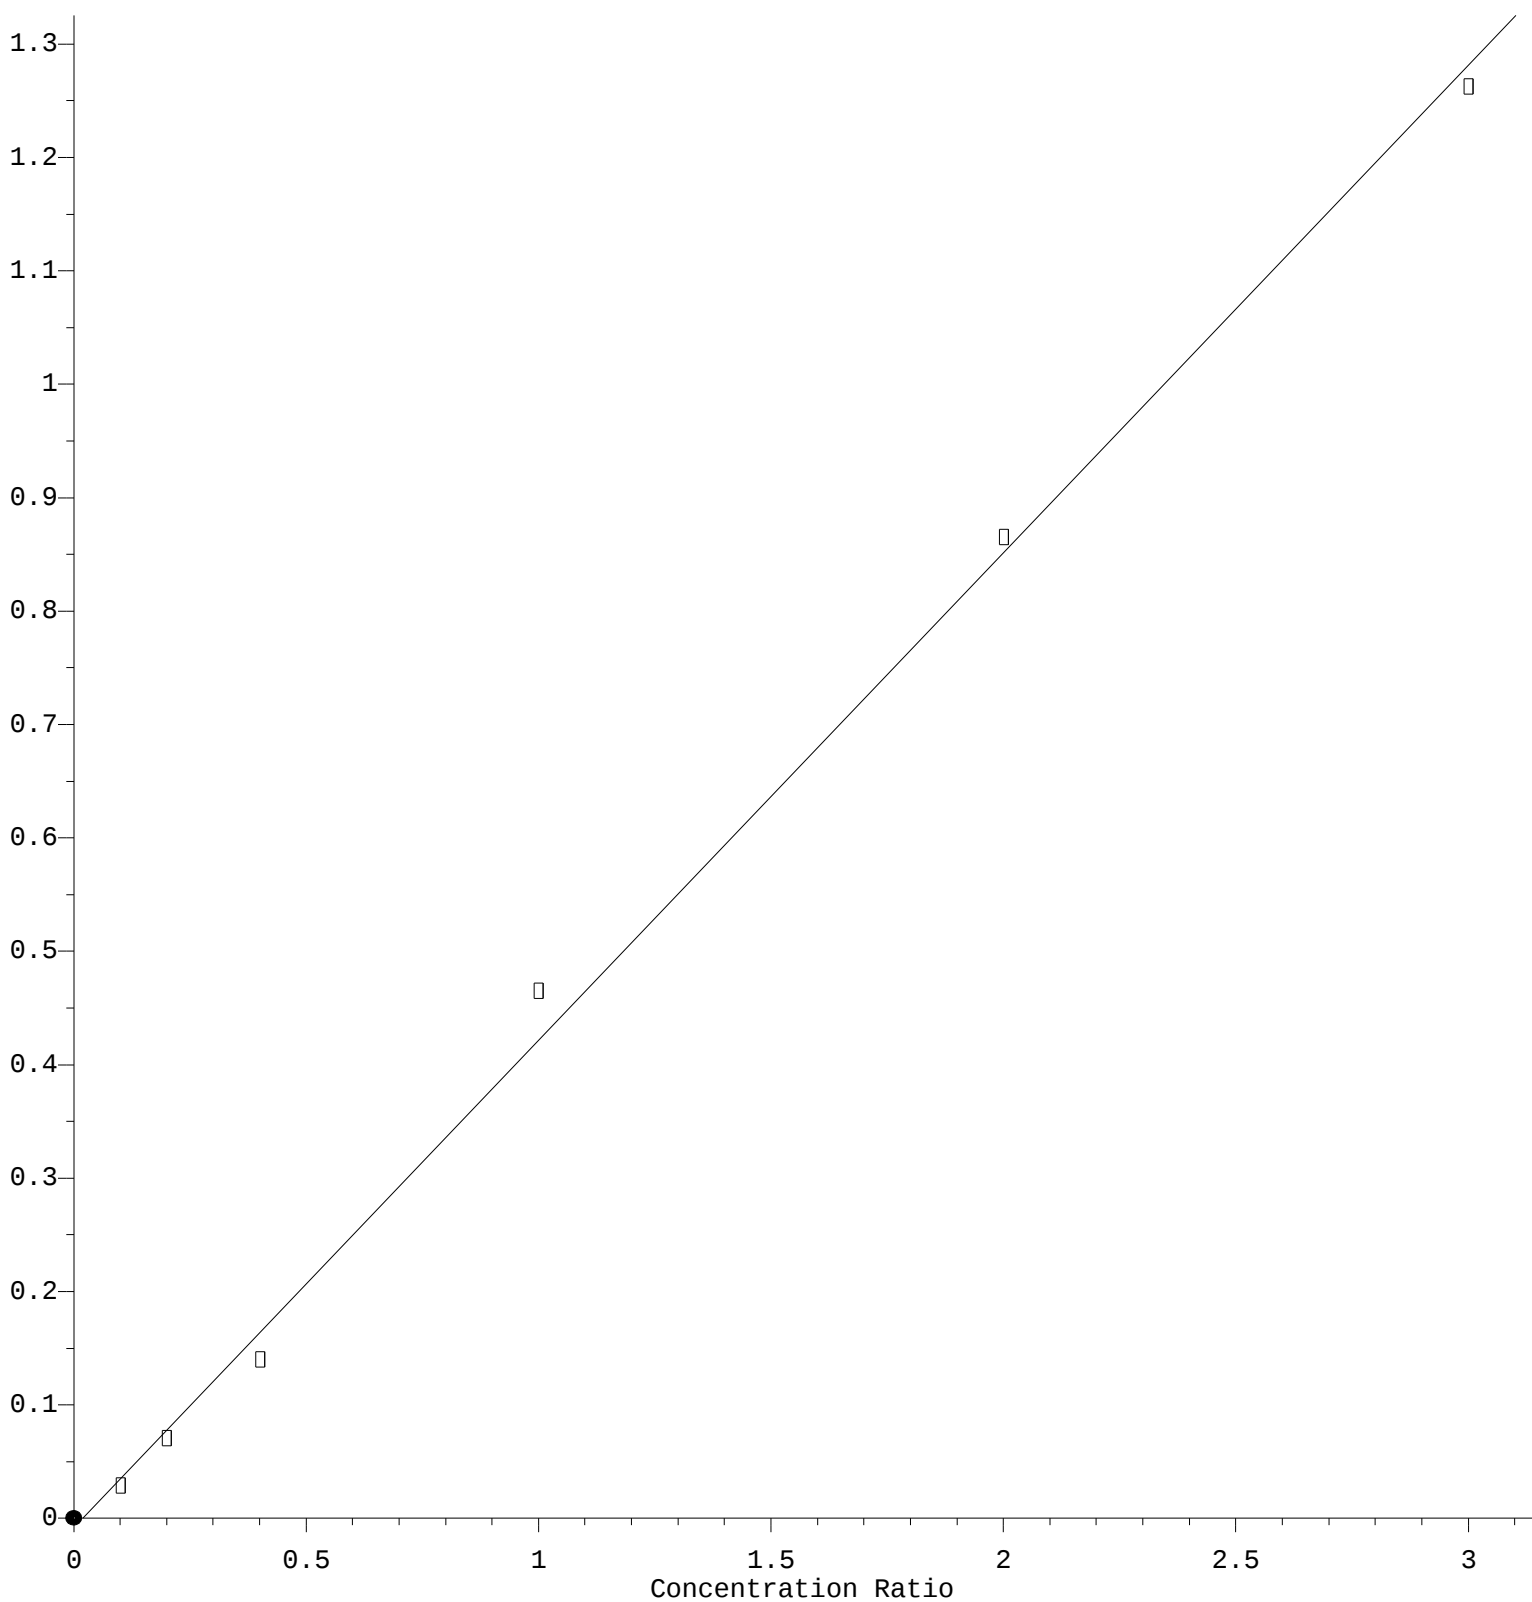

$$\text{Response} = 4.300\text{e-}001 * \text{Amt} - 8.172\text{e-}003$$


Coef of Det (r^2) = 0.997522 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D032922S.M

Calibration Table Last Updated: Wed Mar 30 02:44:36 2022

Methyl Iodide

Response Ratio

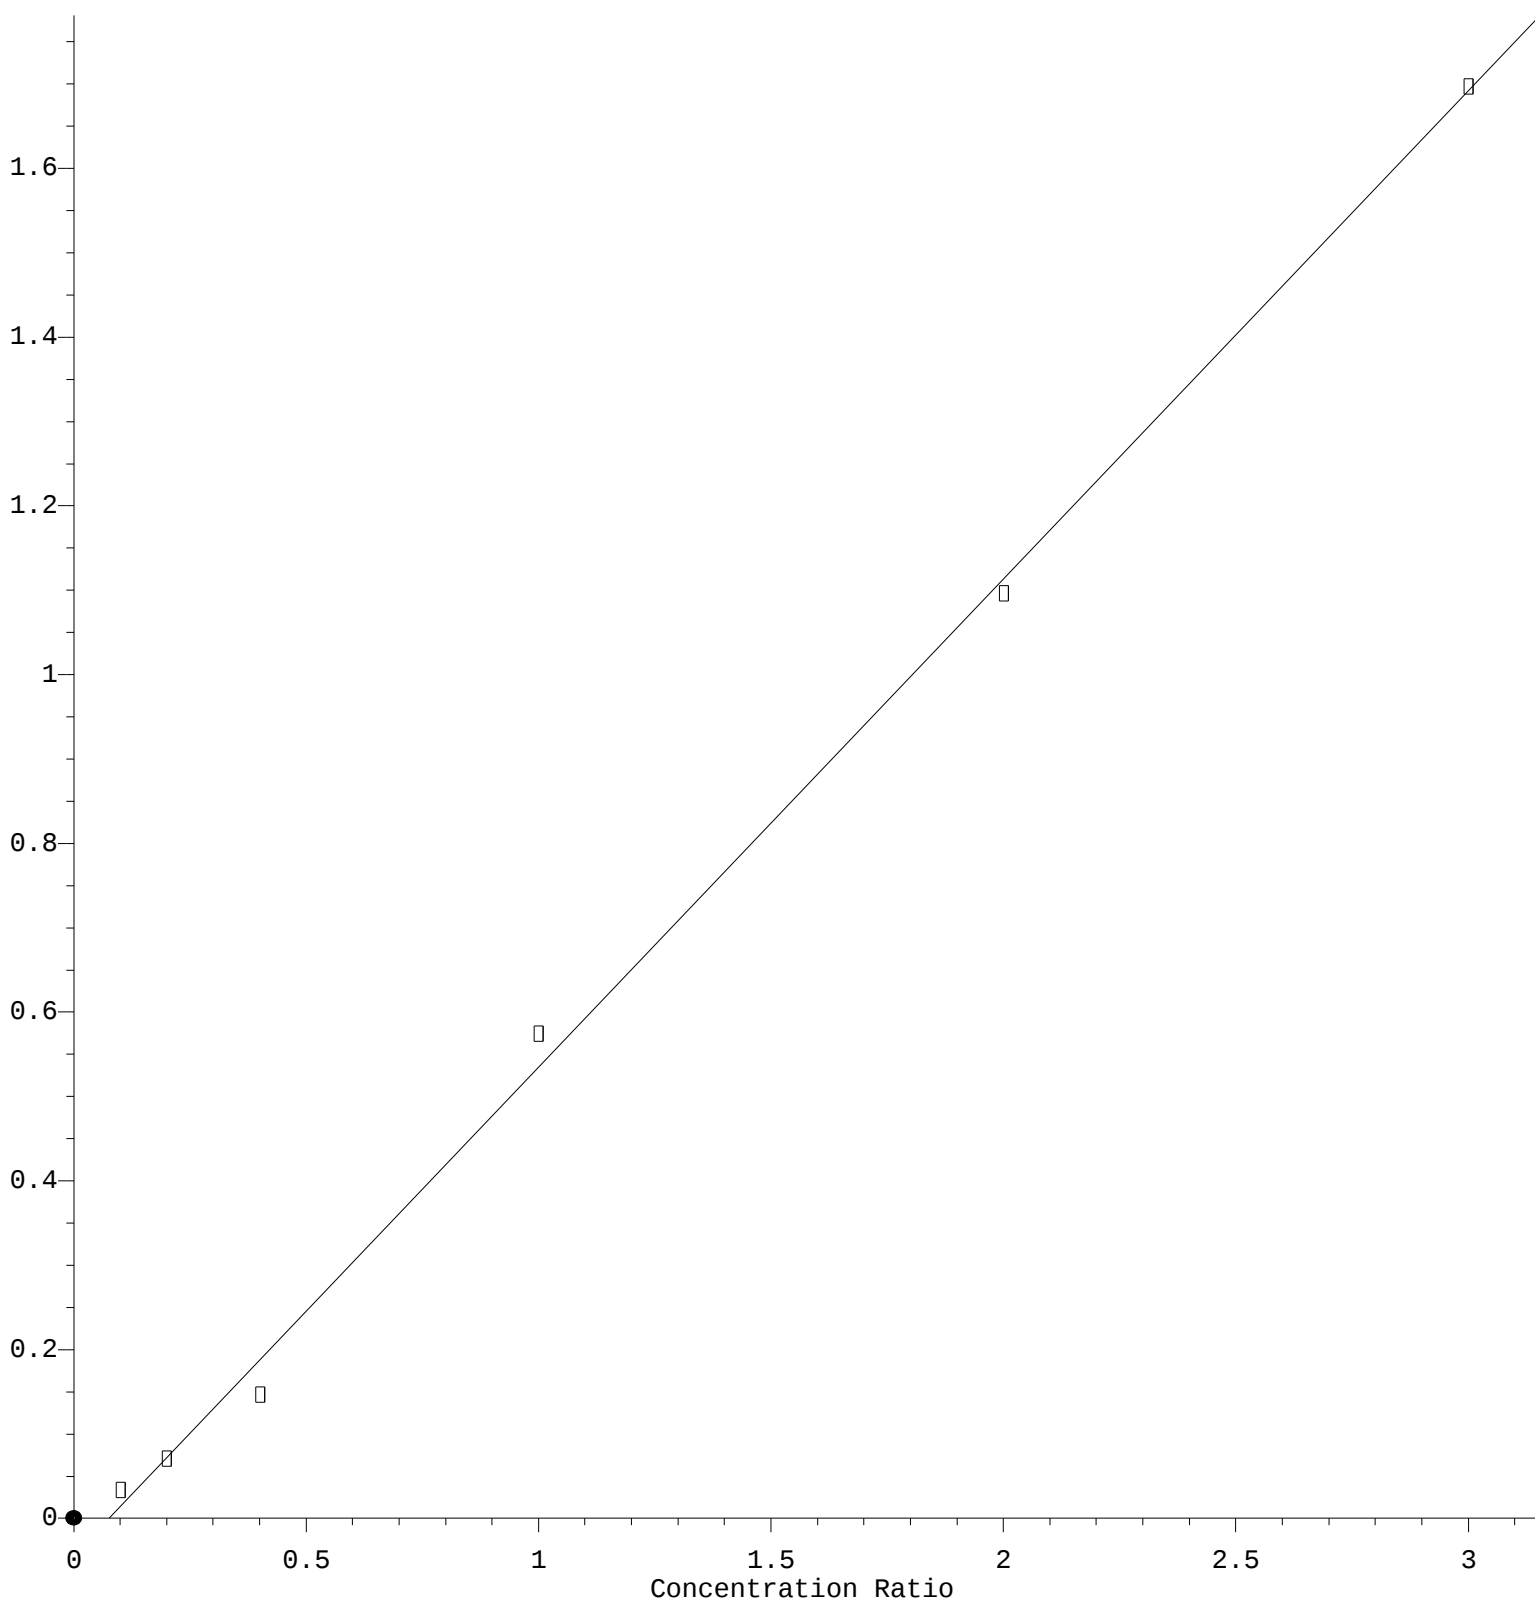

$$\text{Response} = 5.786\text{e-}001 * \text{Amt} - 4.318\text{e-}002$$


Coef of Det (r^2) = 0.998248 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D032922S.M

Calibration Table Last Updated: Wed Mar 30 02:44:36 2022

Allyl chloride

Response Ratio

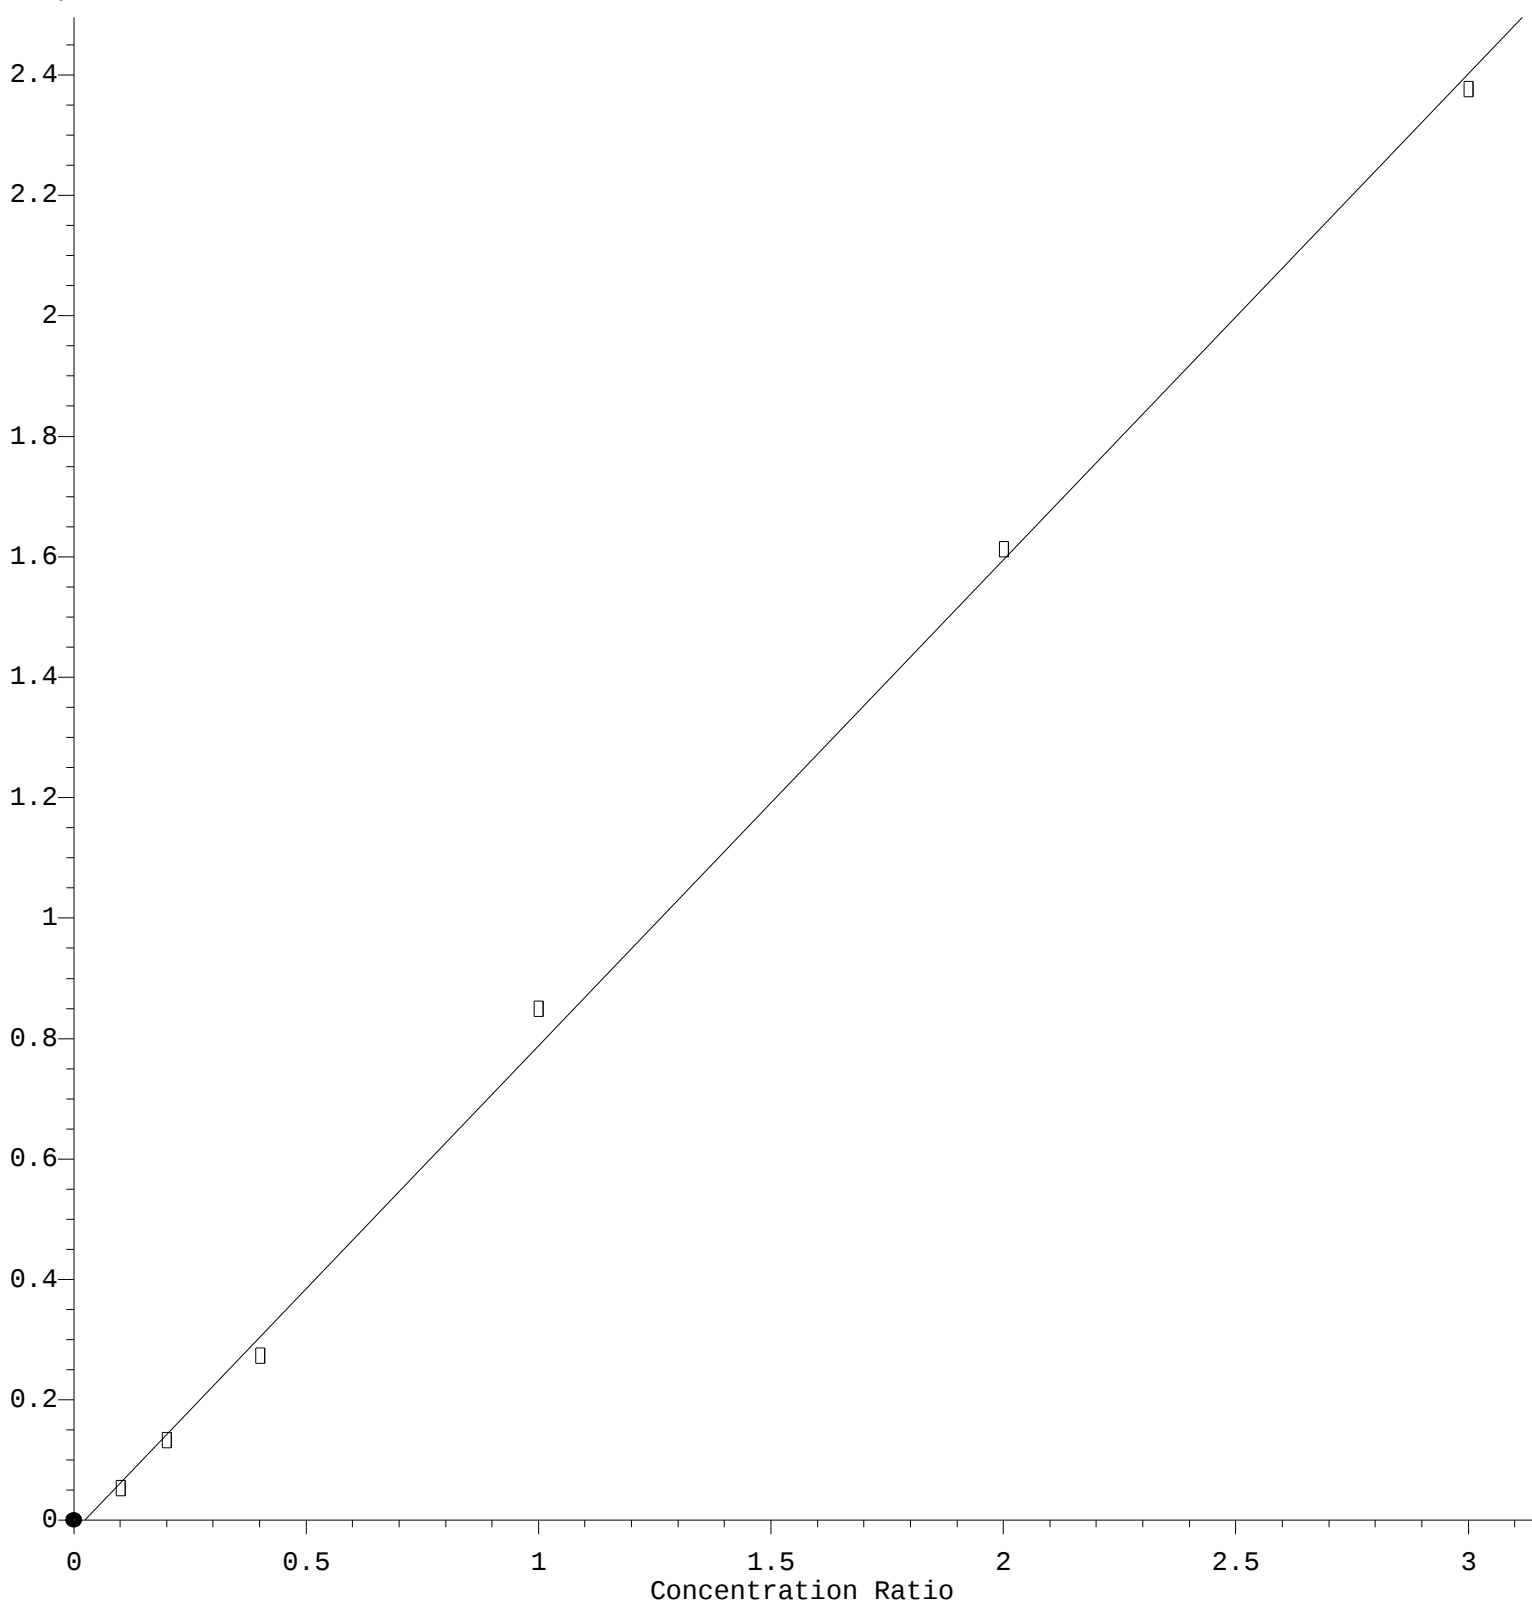

$$\text{Response} = 8.068\text{e-}001 * \text{Amt} - 1.818\text{e-}002$$


Coef of Det (r^2) = 0.998676 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D032922S.M

Calibration Table Last Updated: Wed Mar 30 02:44:36 2022

Carbon Disulfide

Response Ratio

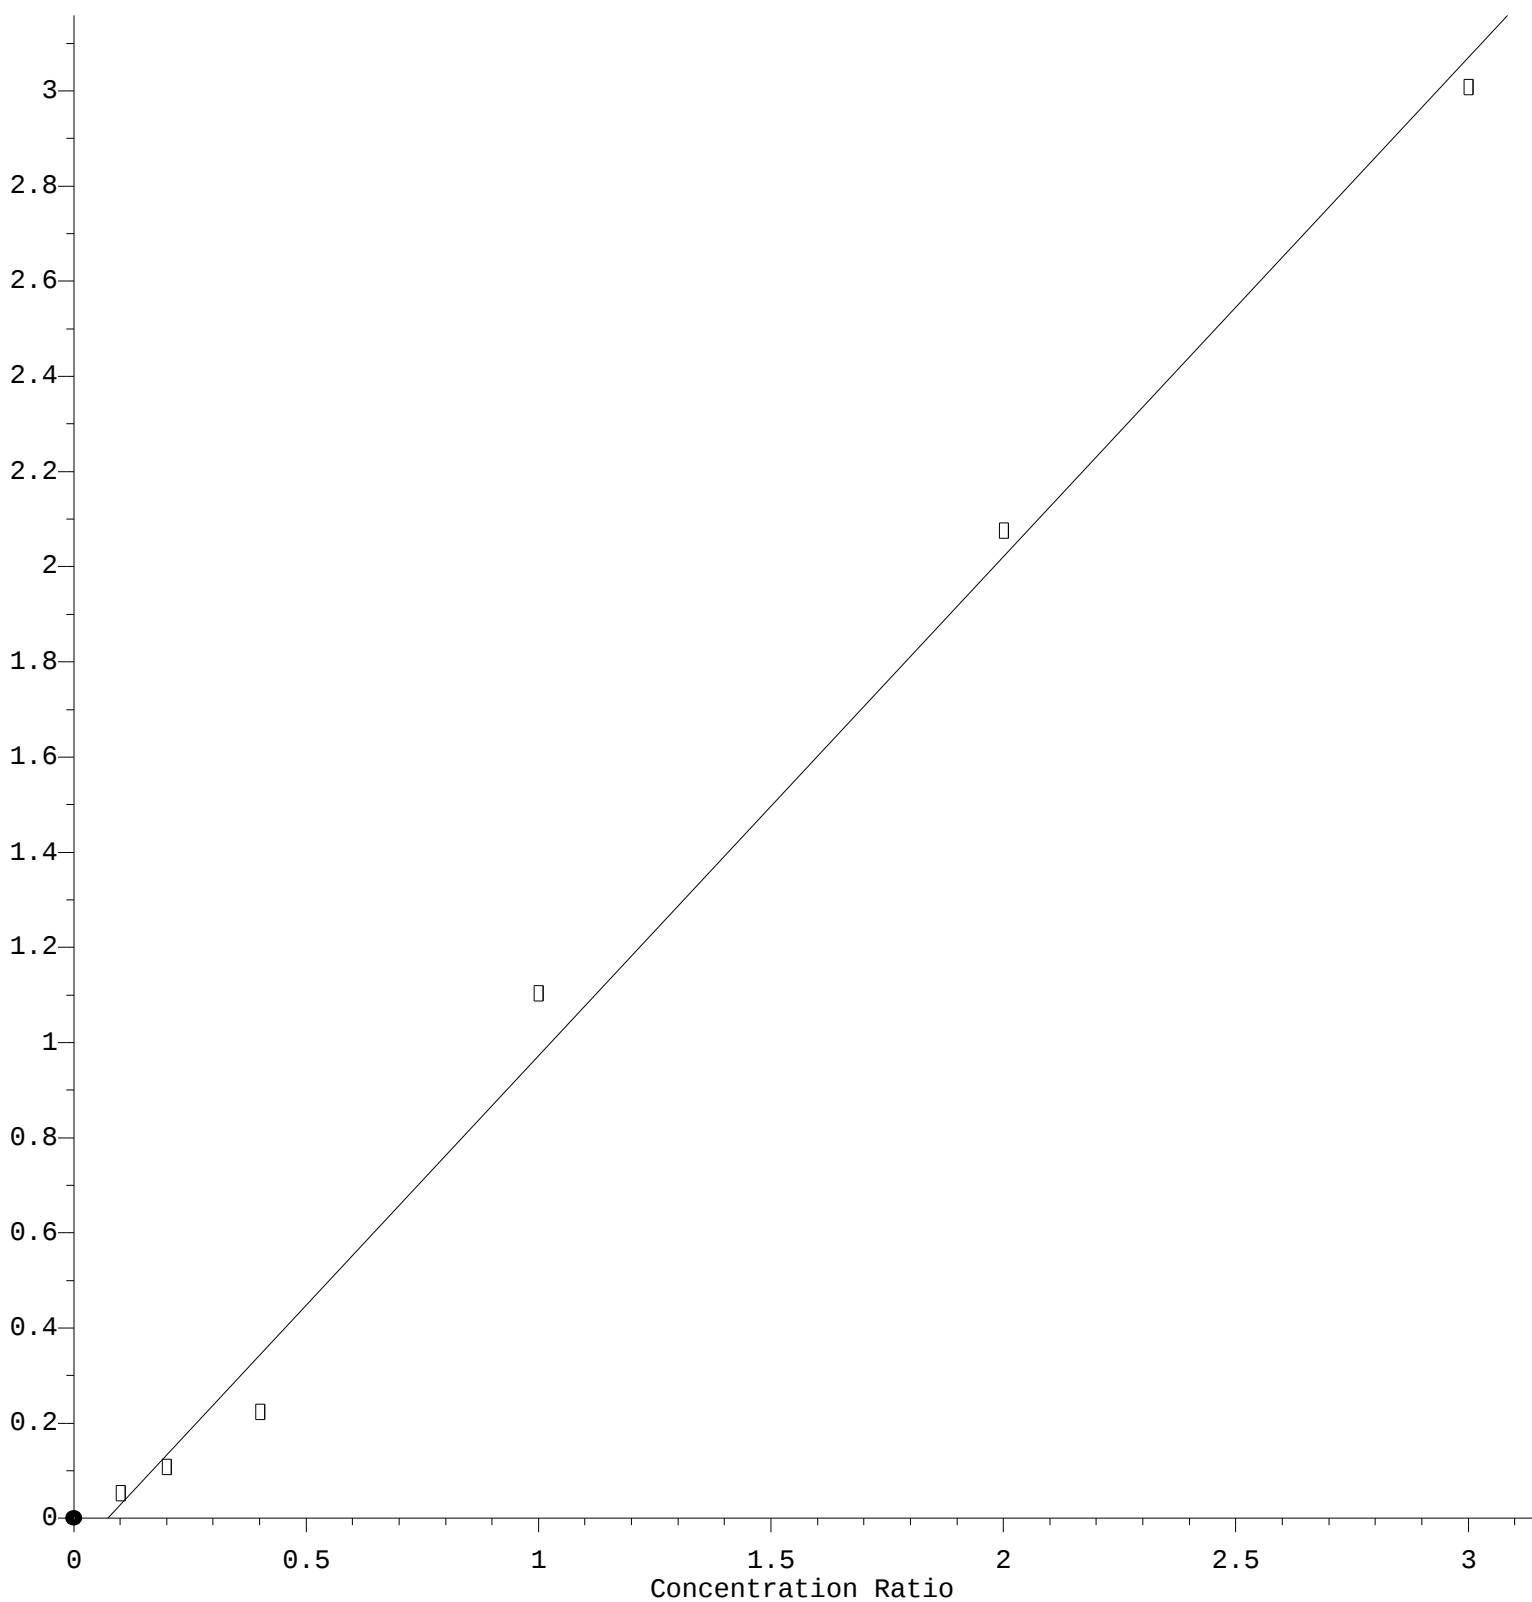

$$\text{Response} = 1.049\text{e}+000 * \text{Amt} - 7.605\text{e}-002$$


Coef of Det (r^2) = 0.994720 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D032922S.M

Calibration Table Last Updated: Wed Mar 30 02:44:36 2022

trans-1,2-Dichloroethene

Response Ratio

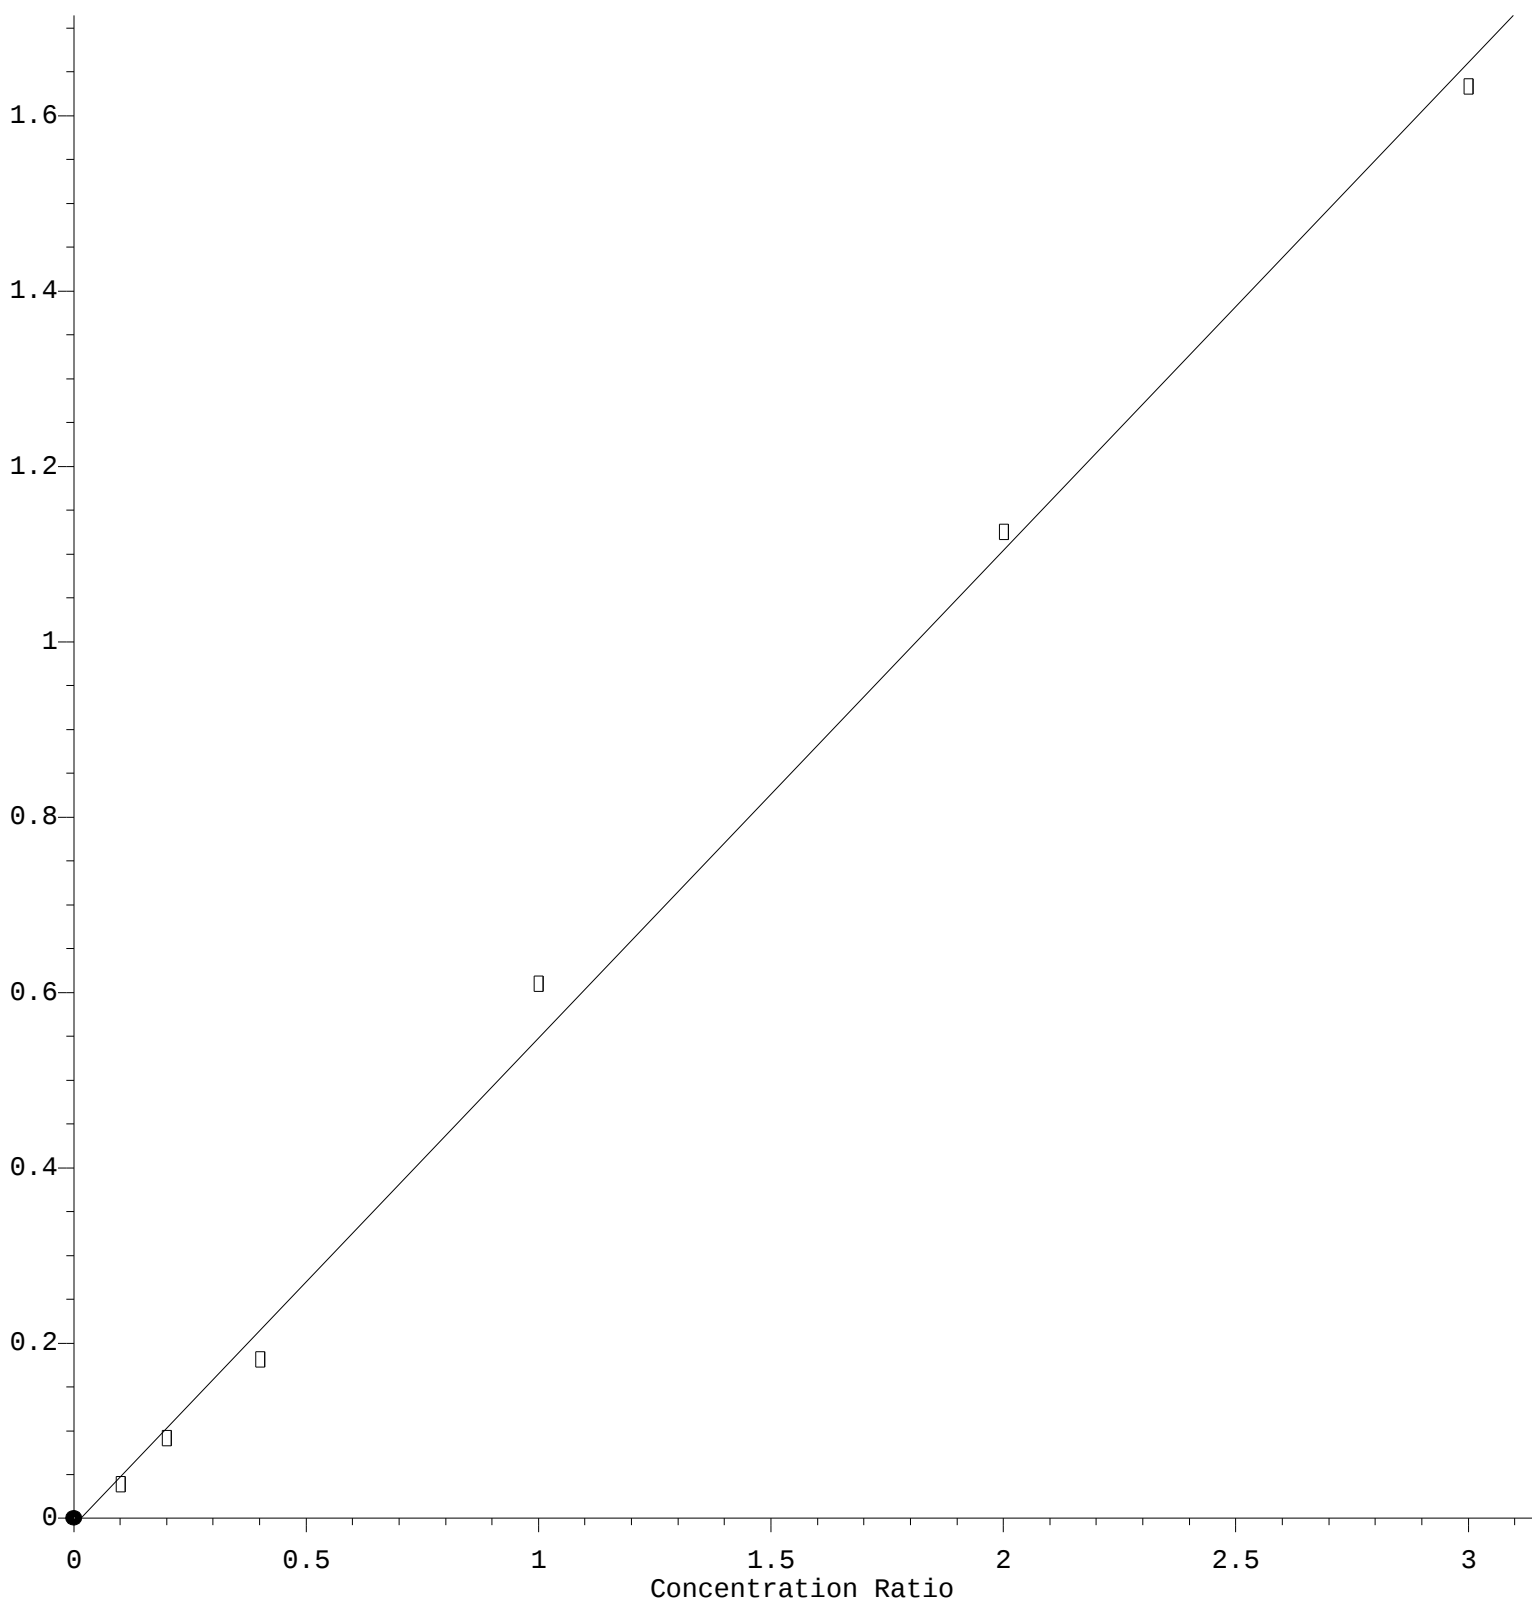

$$\text{Response} = 5.565\text{e-}001 * \text{Amt} - 8.394\text{e-}003$$


Coef of Det (r^2) = 0.996990 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D032922S.M

Calibration Table Last Updated: Wed Mar 30 02:44:36 2022

Vinyl Acetate

Response Ratio

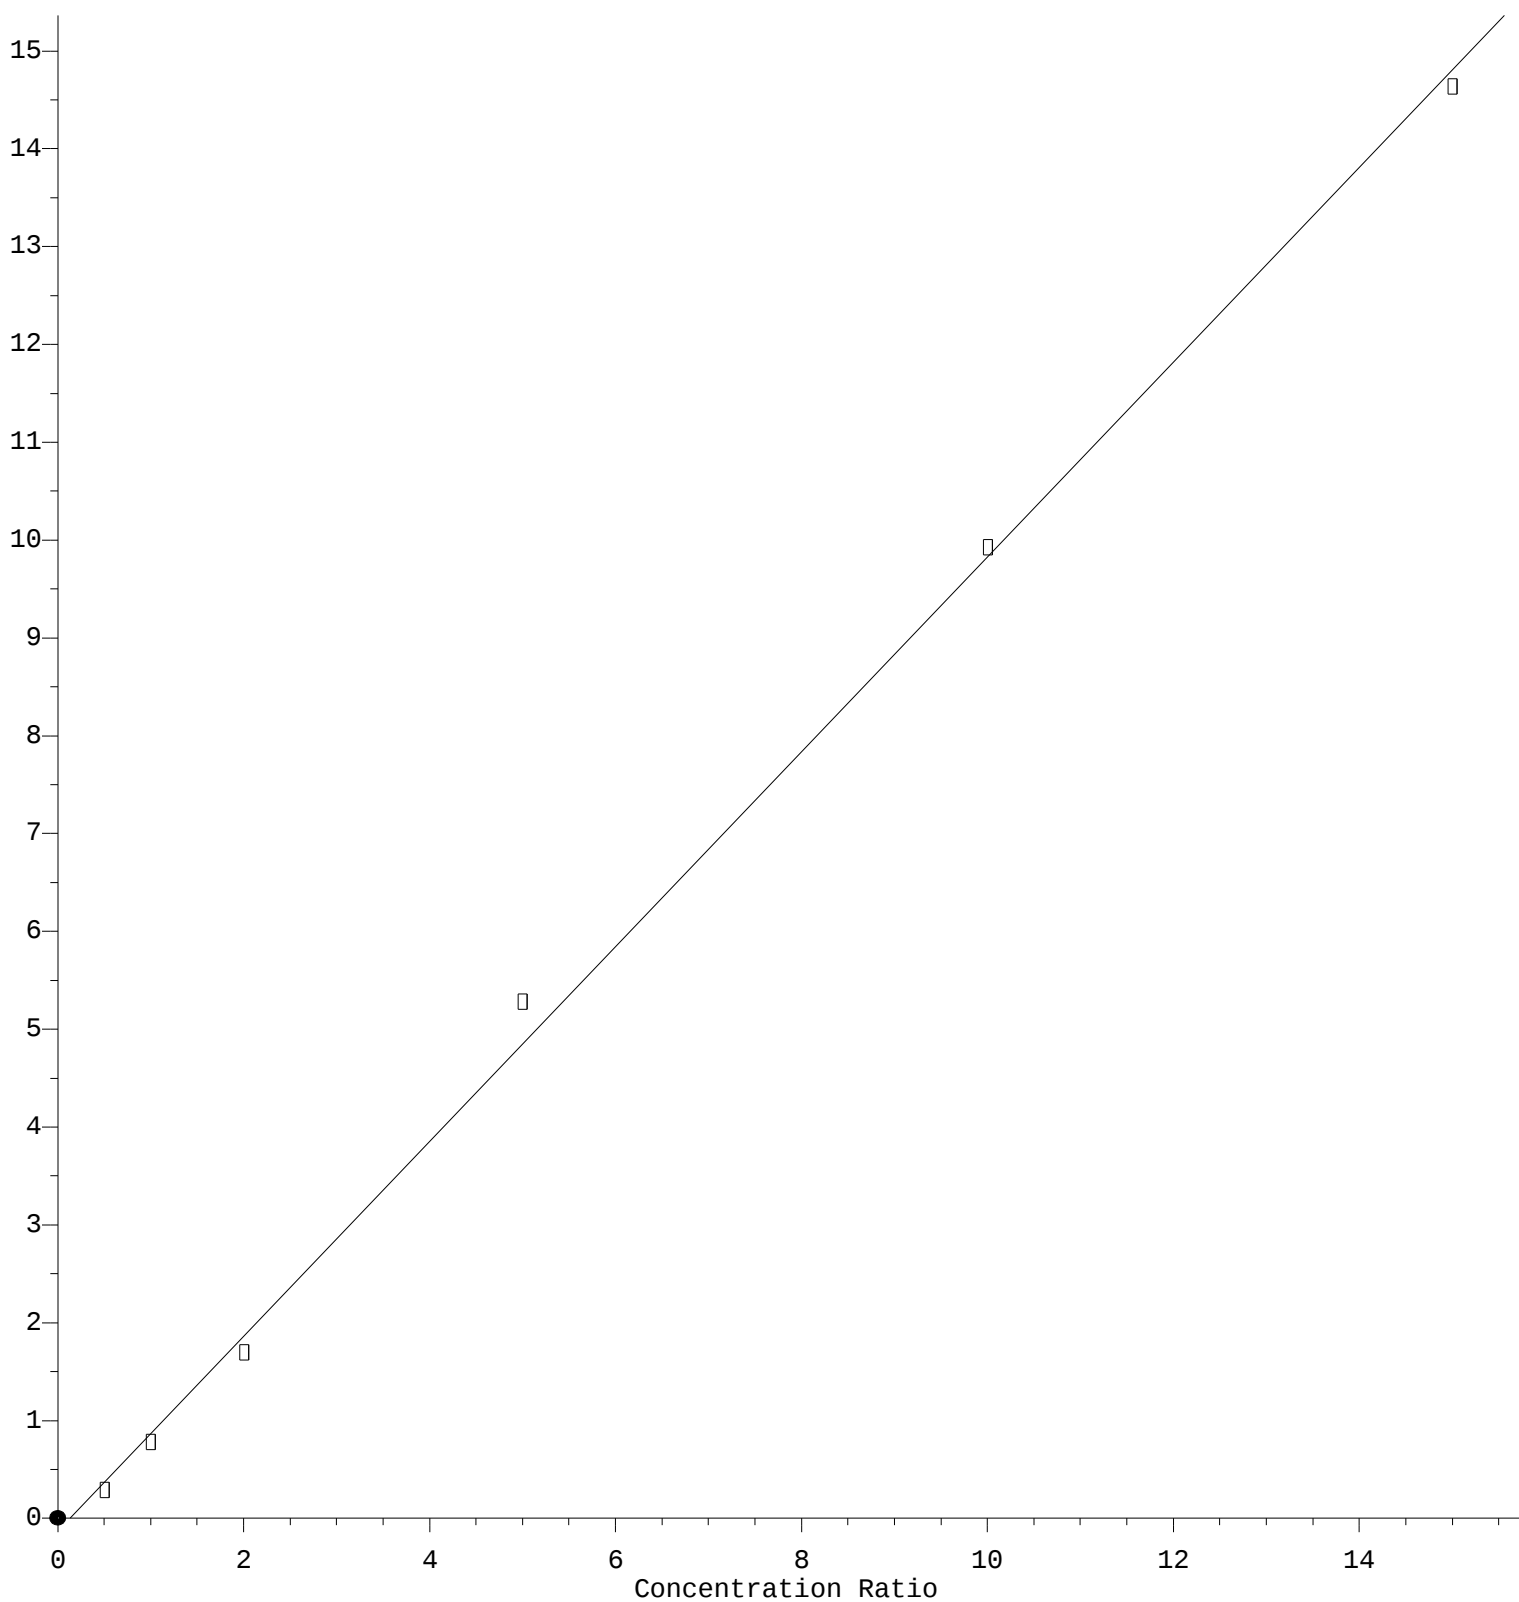

$$\text{Response} = 9.955\text{e-}001 * \text{Amt} - 1.252\text{e-}001$$


Coef of Det (r^2) = 0.998414 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D032922S.M

Calibration Table Last Updated: Wed Mar 30 02:44:36 2022

1,1-Dichloropropene

Response Ratio

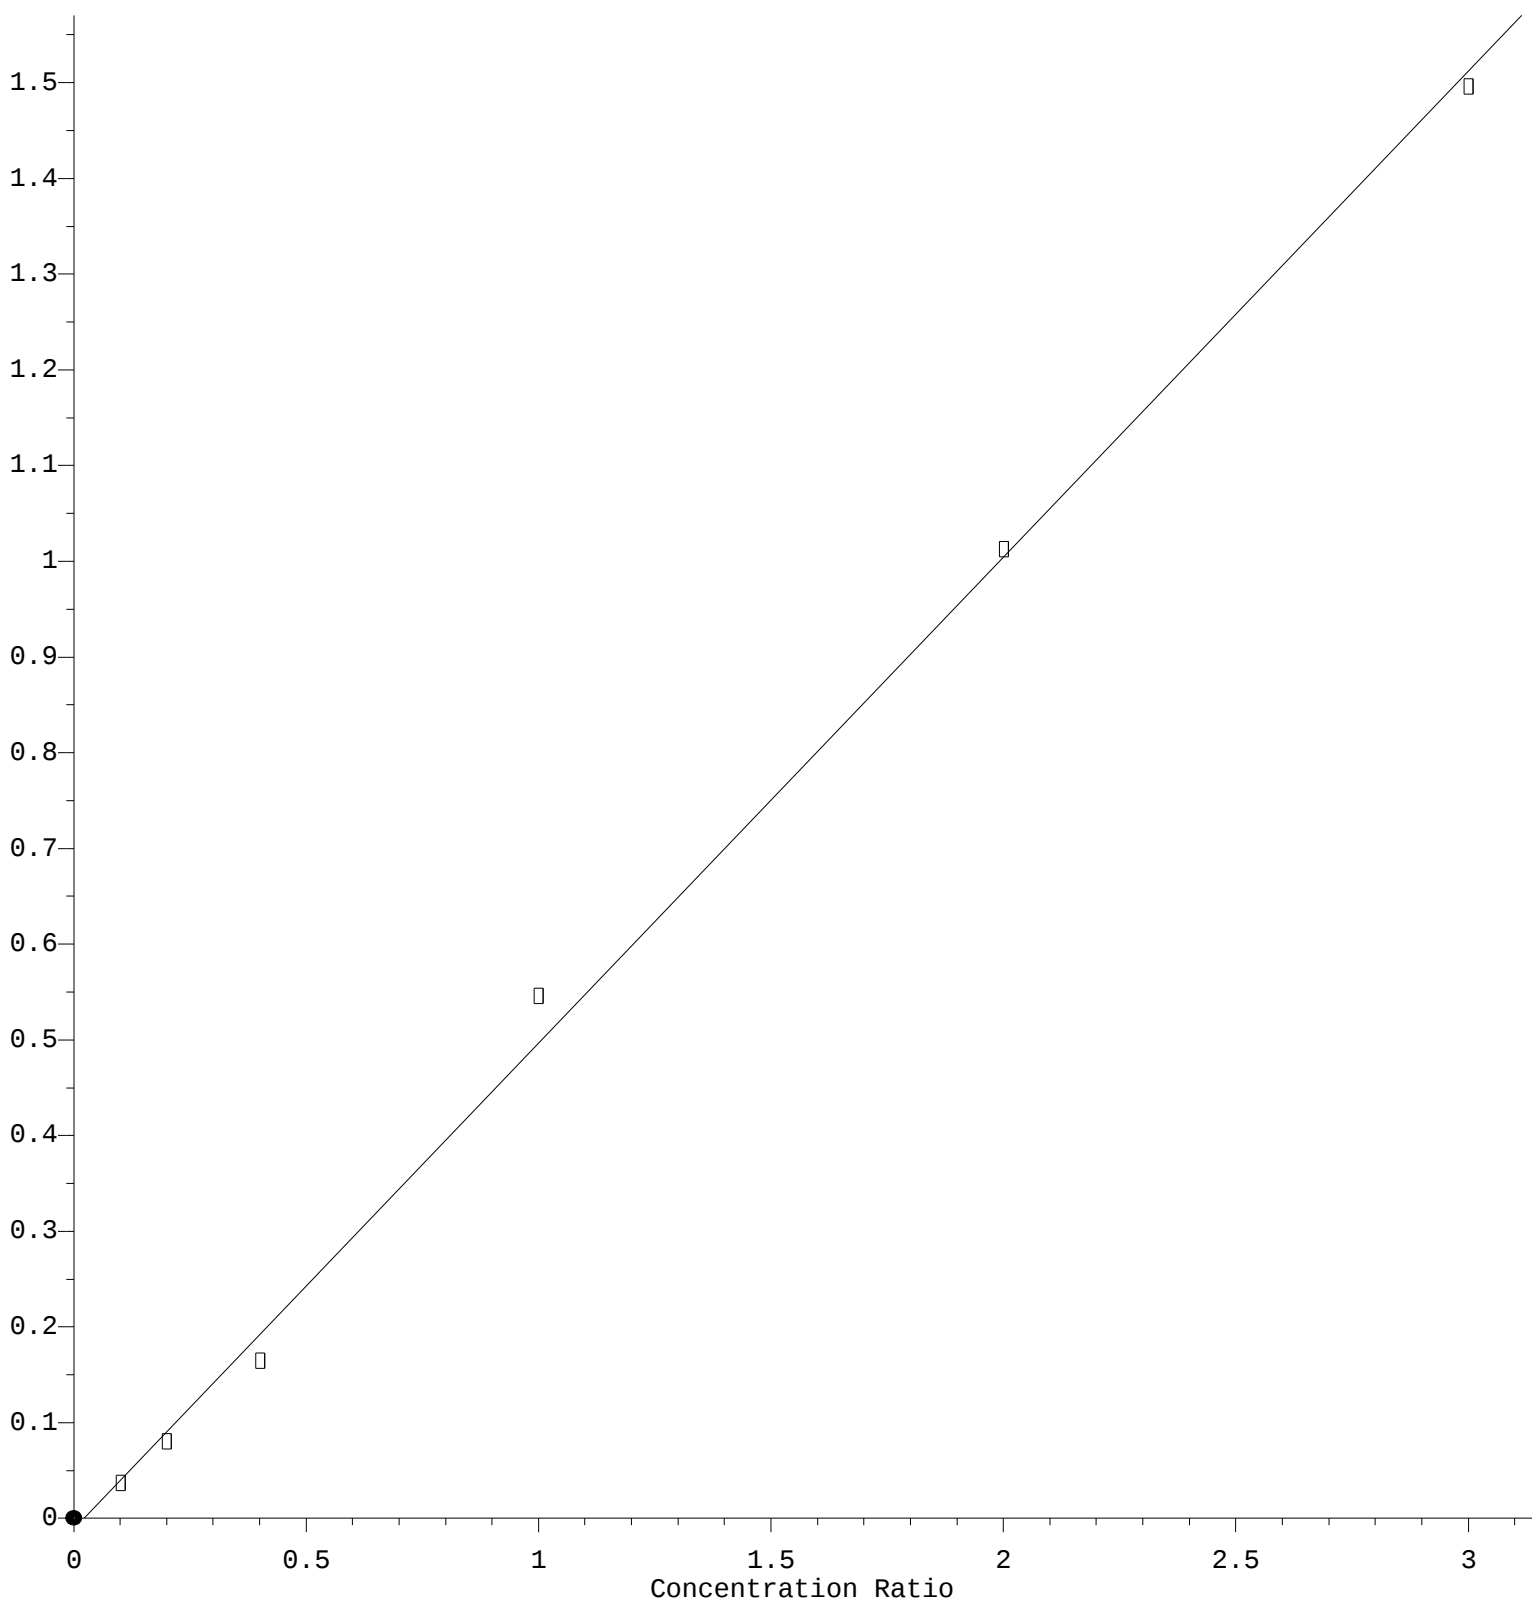

$$\text{Response} = 5.080\text{e-}001 * \text{Amt} - 1.142\text{e-}002$$


Coef of Det (r^2) = 0.997954 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D032922S.M

Calibration Table Last Updated: Wed Mar 30 02:44:36 2022

Methylcyclohexane

Response Ratio

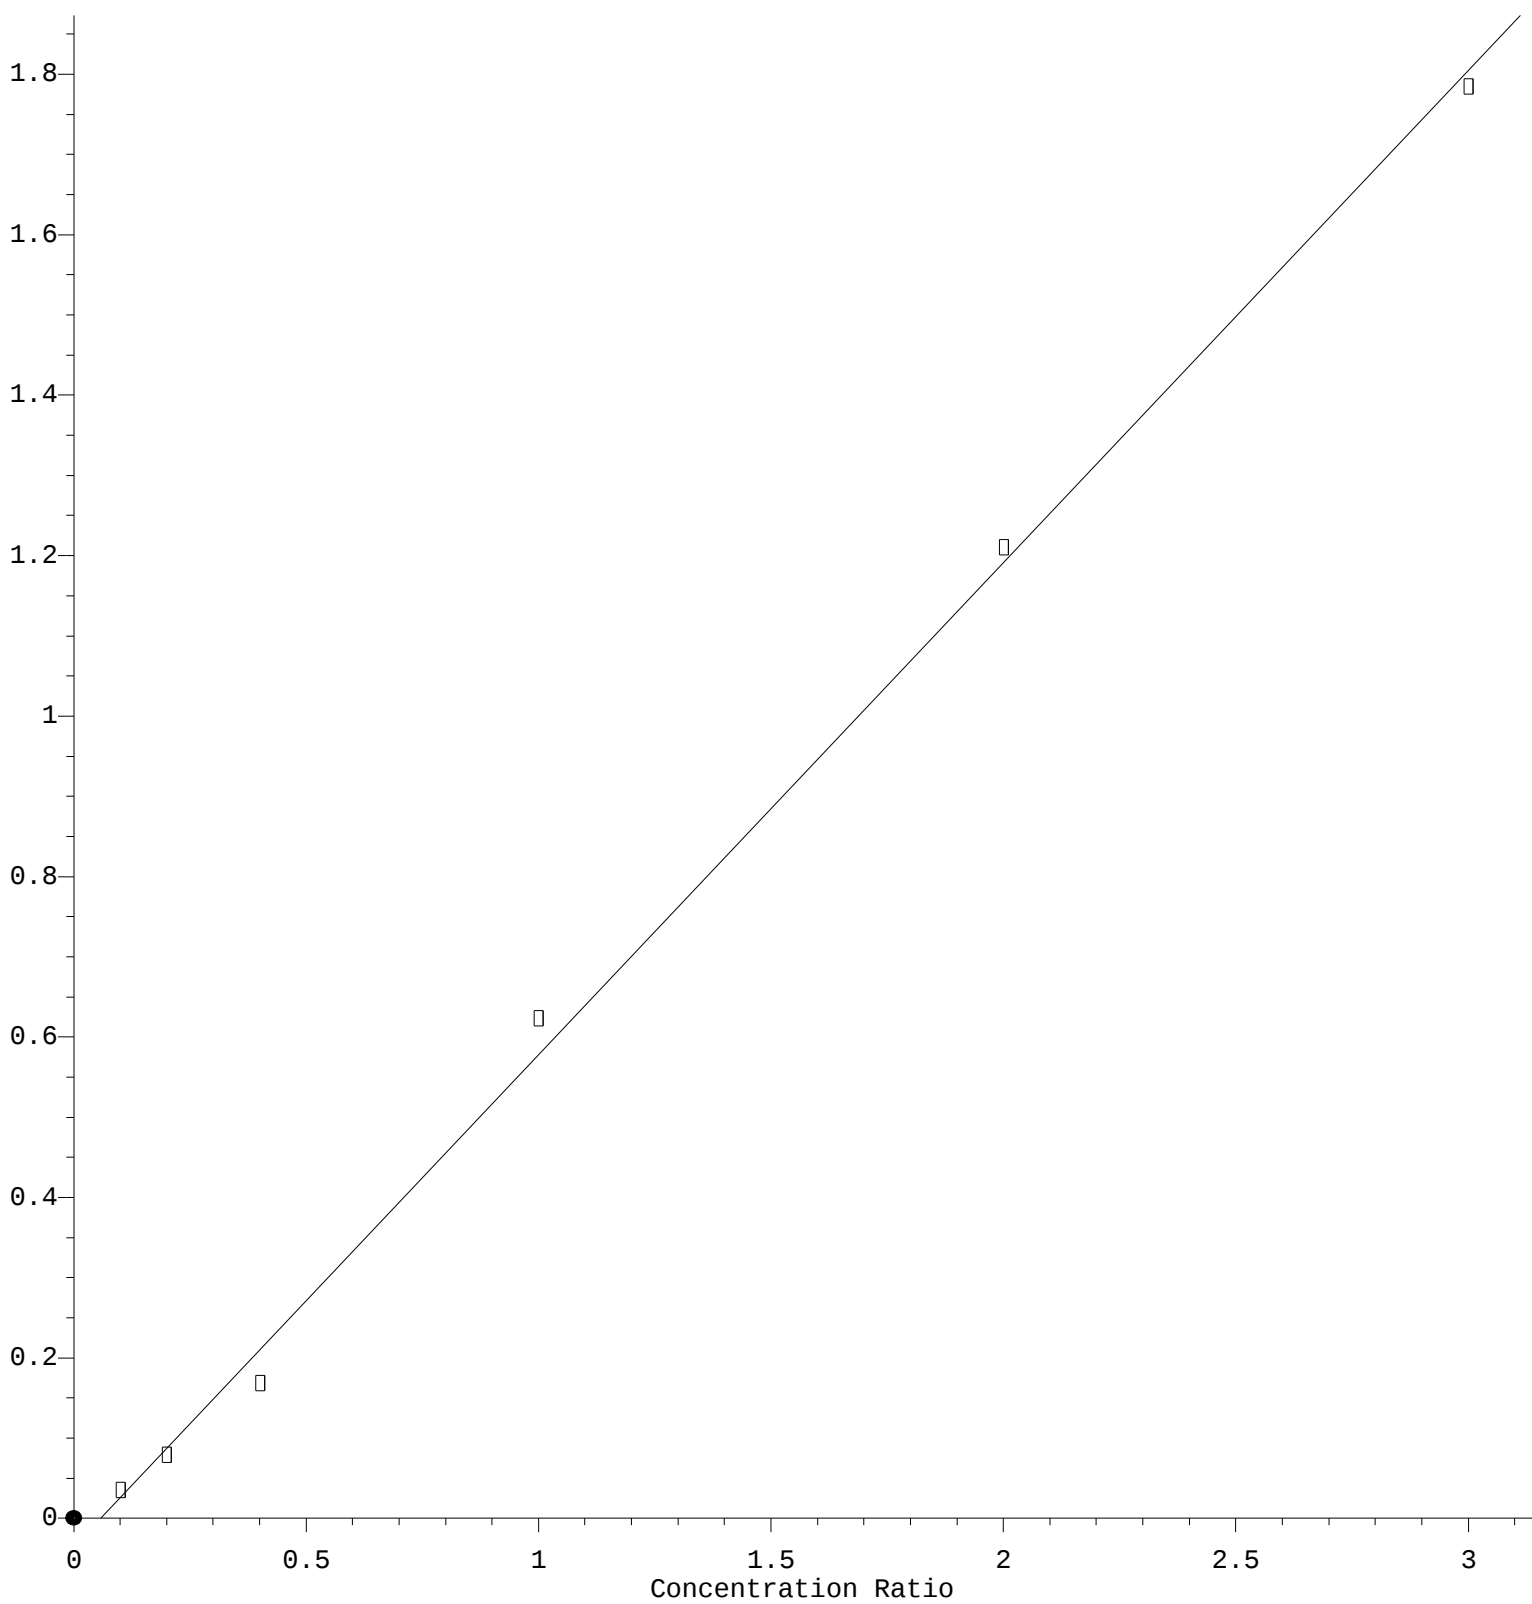


$$\text{Response} = 6.136\text{e-}001 * \text{Amt} - 3.530\text{e-}002$$

Coef of Det (r^2) = 0.998160 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D032922S.M

Calibration Table Last Updated: Wed Mar 30 02:44:36 2022


Methacrylonitrile

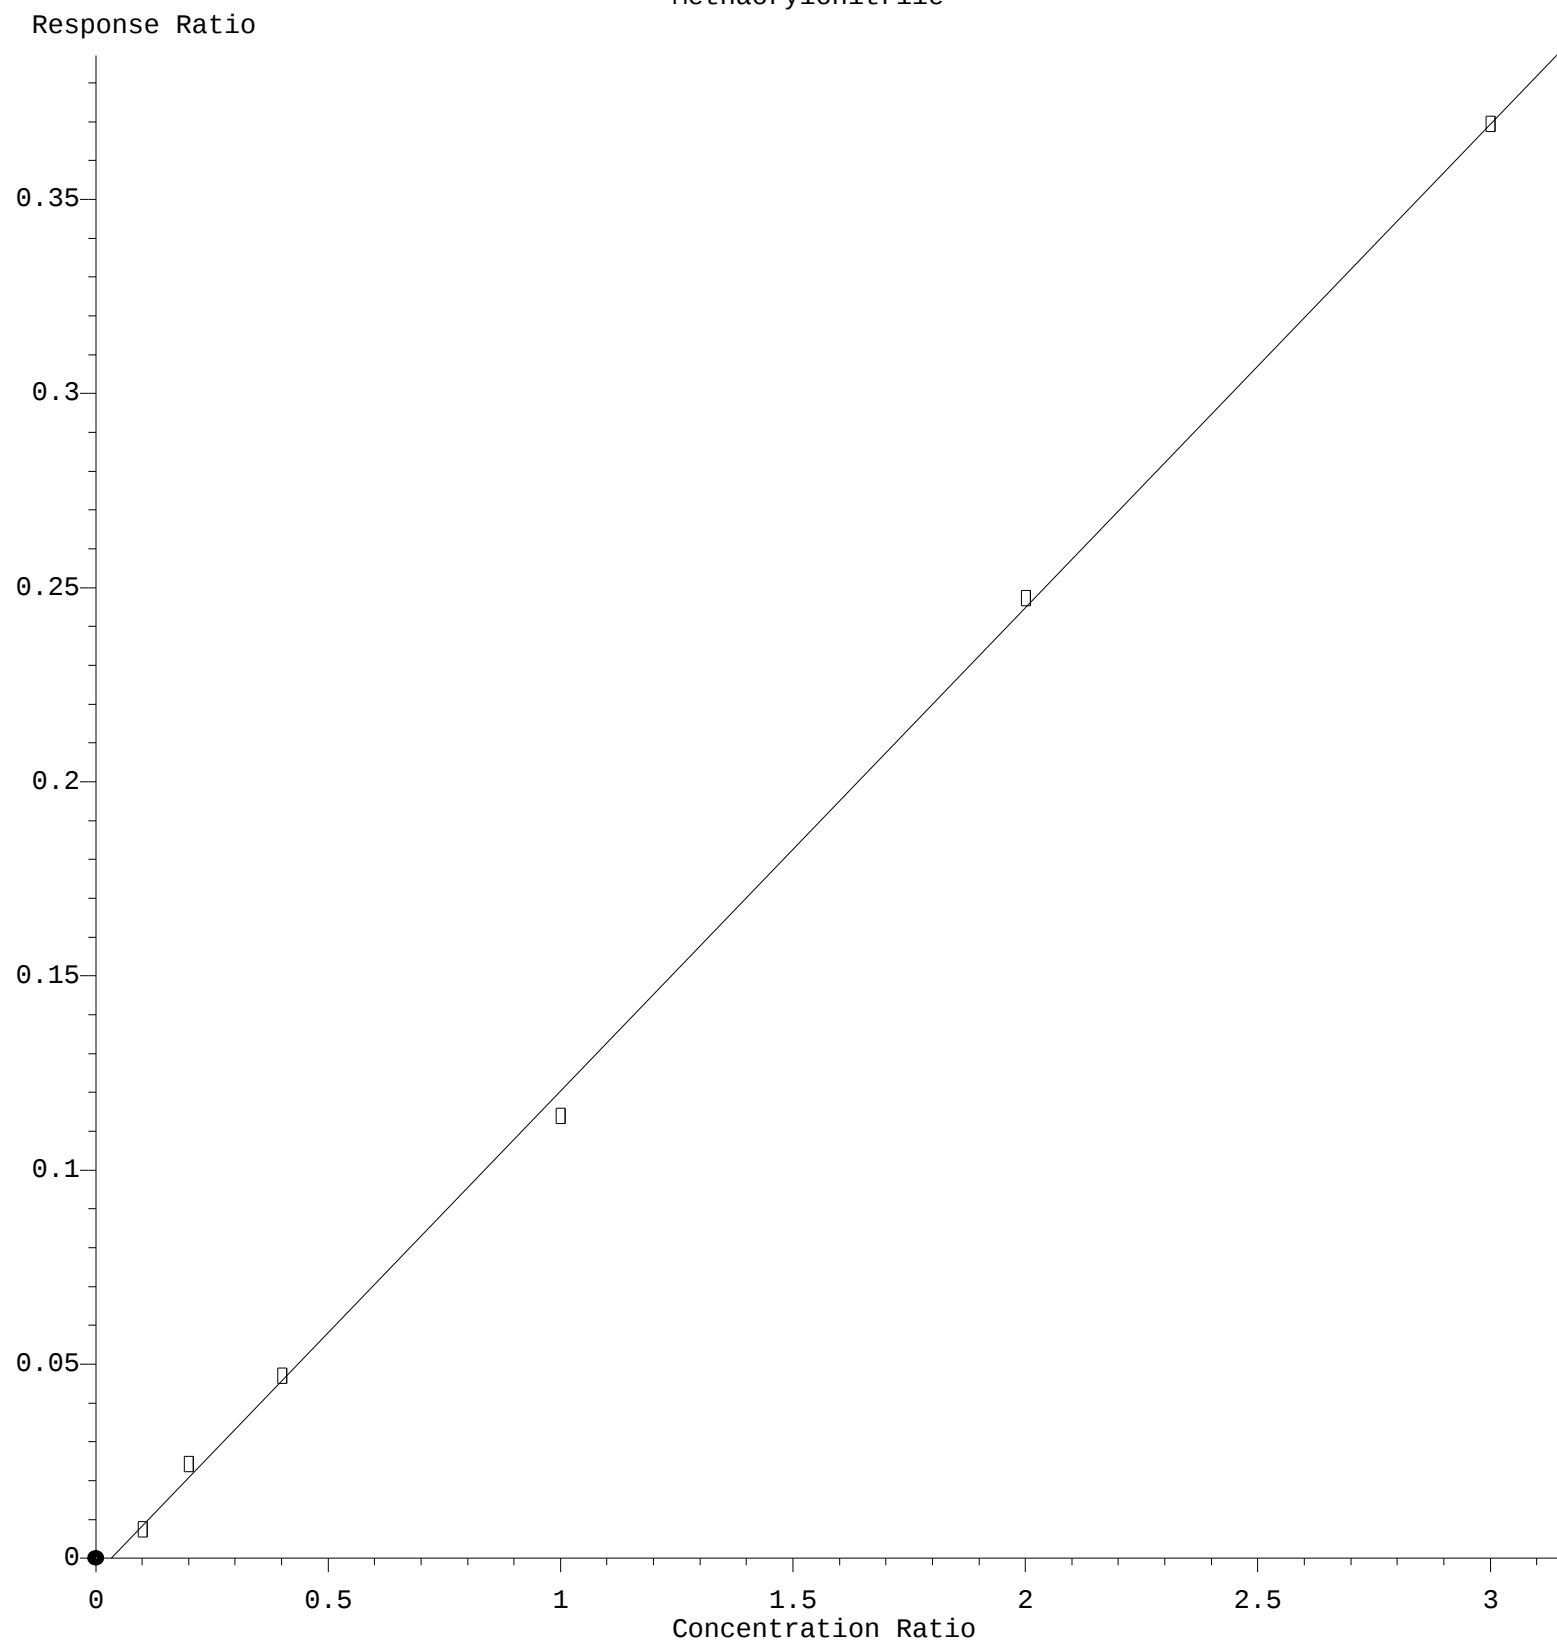

Response = $1.245 \times 10^{-1} \times \text{Amt} - 4.127 \times 10^{-3}$
Coef of Det (r^2) = 0.999399 Curve Fit: Linear
Method Name: Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D032922S.M
Calibration Table Last Updated: Wed Mar 30 02:44:36 2022

Ethyl methacrylate

Response Ratio

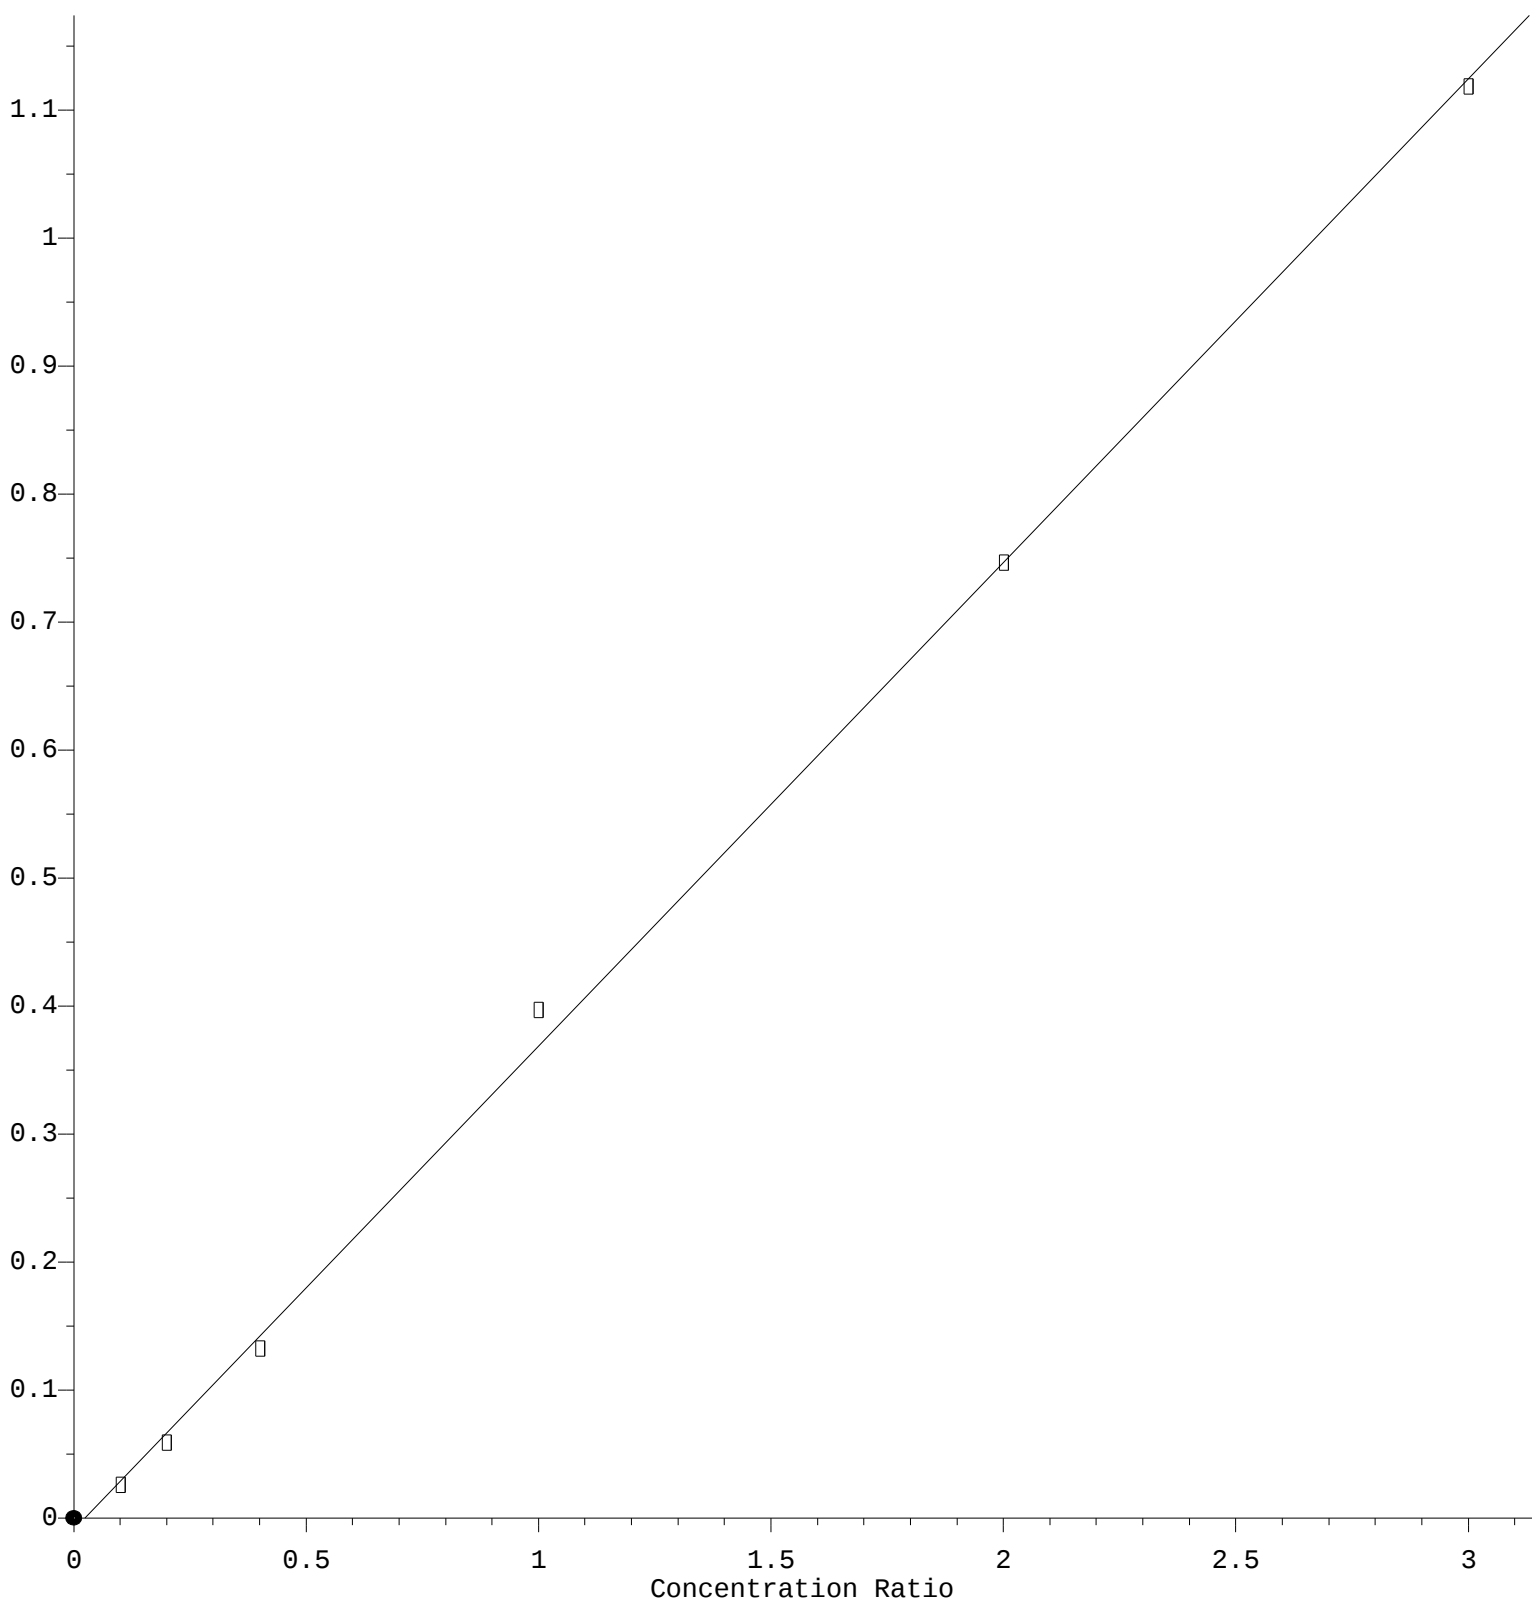

$$\text{Response} = 3.782\text{e-}001 * \text{Amt} - 9.007\text{e-}003$$

Coef of Det (r^2) = 0.998985 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D032922S.M

Calibration Table Last Updated: Wed Mar 30 02:44:36 2022