
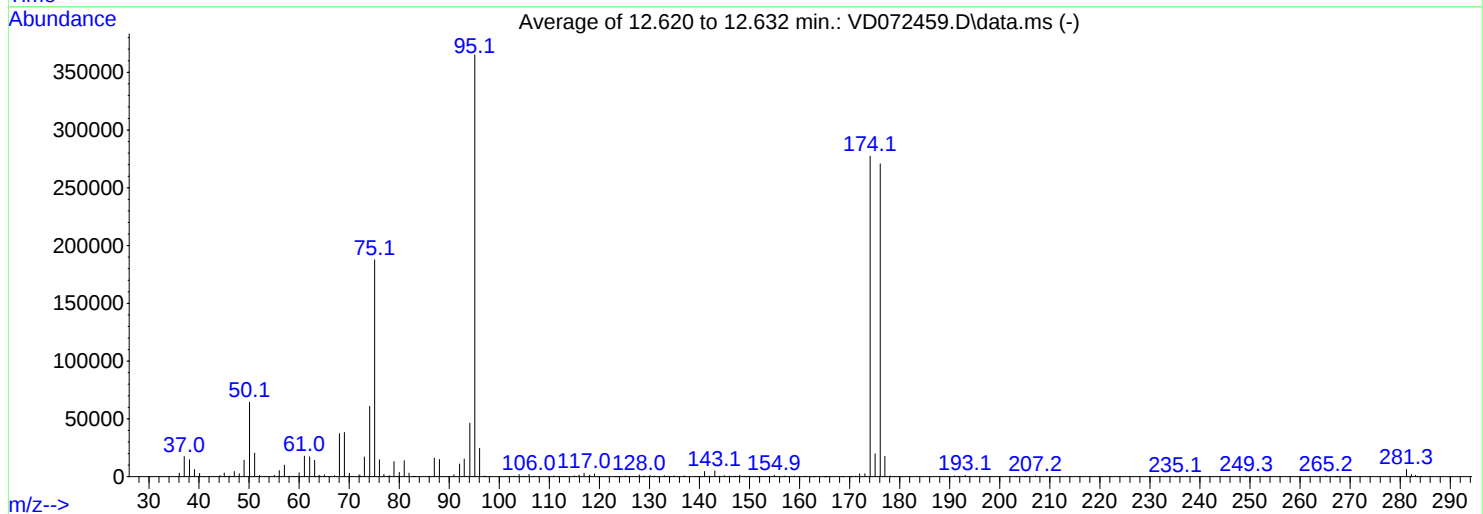


Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD032922\
Data File : VD072459.D
Acq On : 29 Mar 2022 13:00
Operator : VA/SY
Sample : BFB
Misc : 5.00G/5.00ml/MSVOA_D/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D032922S.M
Title : SW846 8260
Last Update : Wed Mar 30 02:44:36 2022

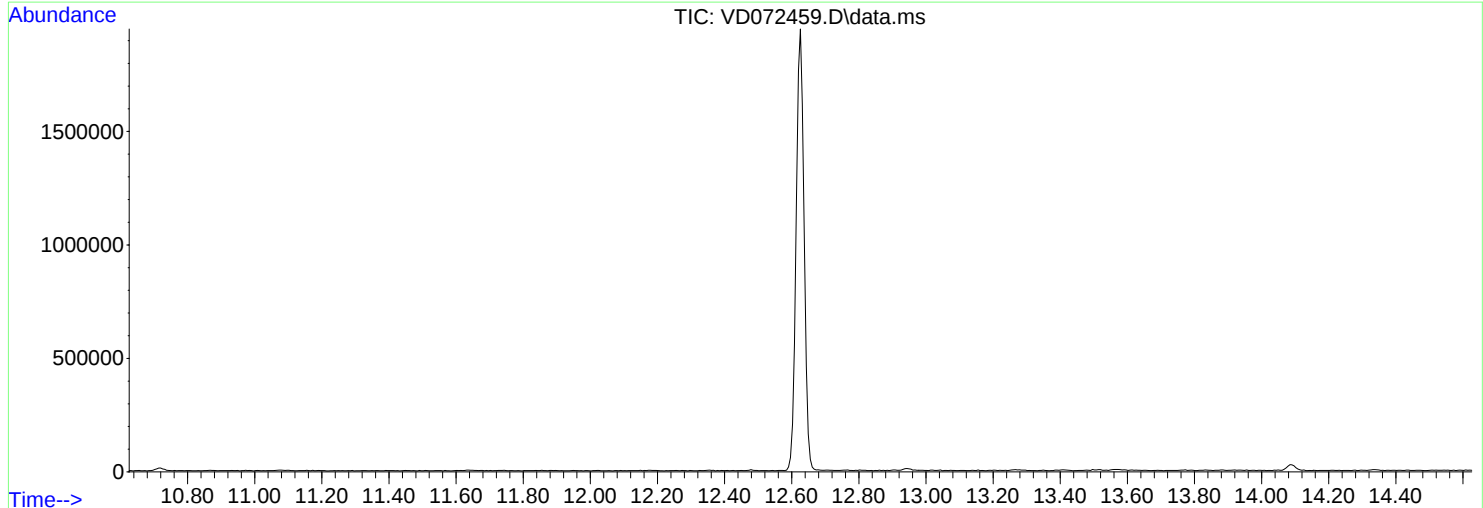

AutoFind: Scans 1819, 1820, 1821; Background Corrected with Scan 1809

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.6	64387	PASS
75	95	30	60	51.4	187627	PASS
95	95	100	100	100.0	365099	PASS
96	95	5	9	6.7	24480	PASS
173	174	0.00	2	0.9	2508	PASS
174	95	50	100	76.0	277376	PASS
175	174	5	9	7.1	19808	PASS
176	174	95	101	97.6	270720	PASS
177	176	5	9	6.5	17587	PASS