


Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD032923\
Data File : VD075538.D
Acq On : 29 Mar 2023 18:00
Operator : KP/SY
Sample : 02121-17
Misc : 6.87G/10.00ml/MSVOA_D/SOIL
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
C11B4

Manual IntegrationsAPPROVED

Quant Time: Mar 31 02:42:30 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\SFAMDLM030123SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Mar 31 01:28:39 2023
Response via : Initial Calibration

Reviewed By :Krupa Patel 04/01/2023
Supervised By :Mahesh Dadoda 04/03/2023

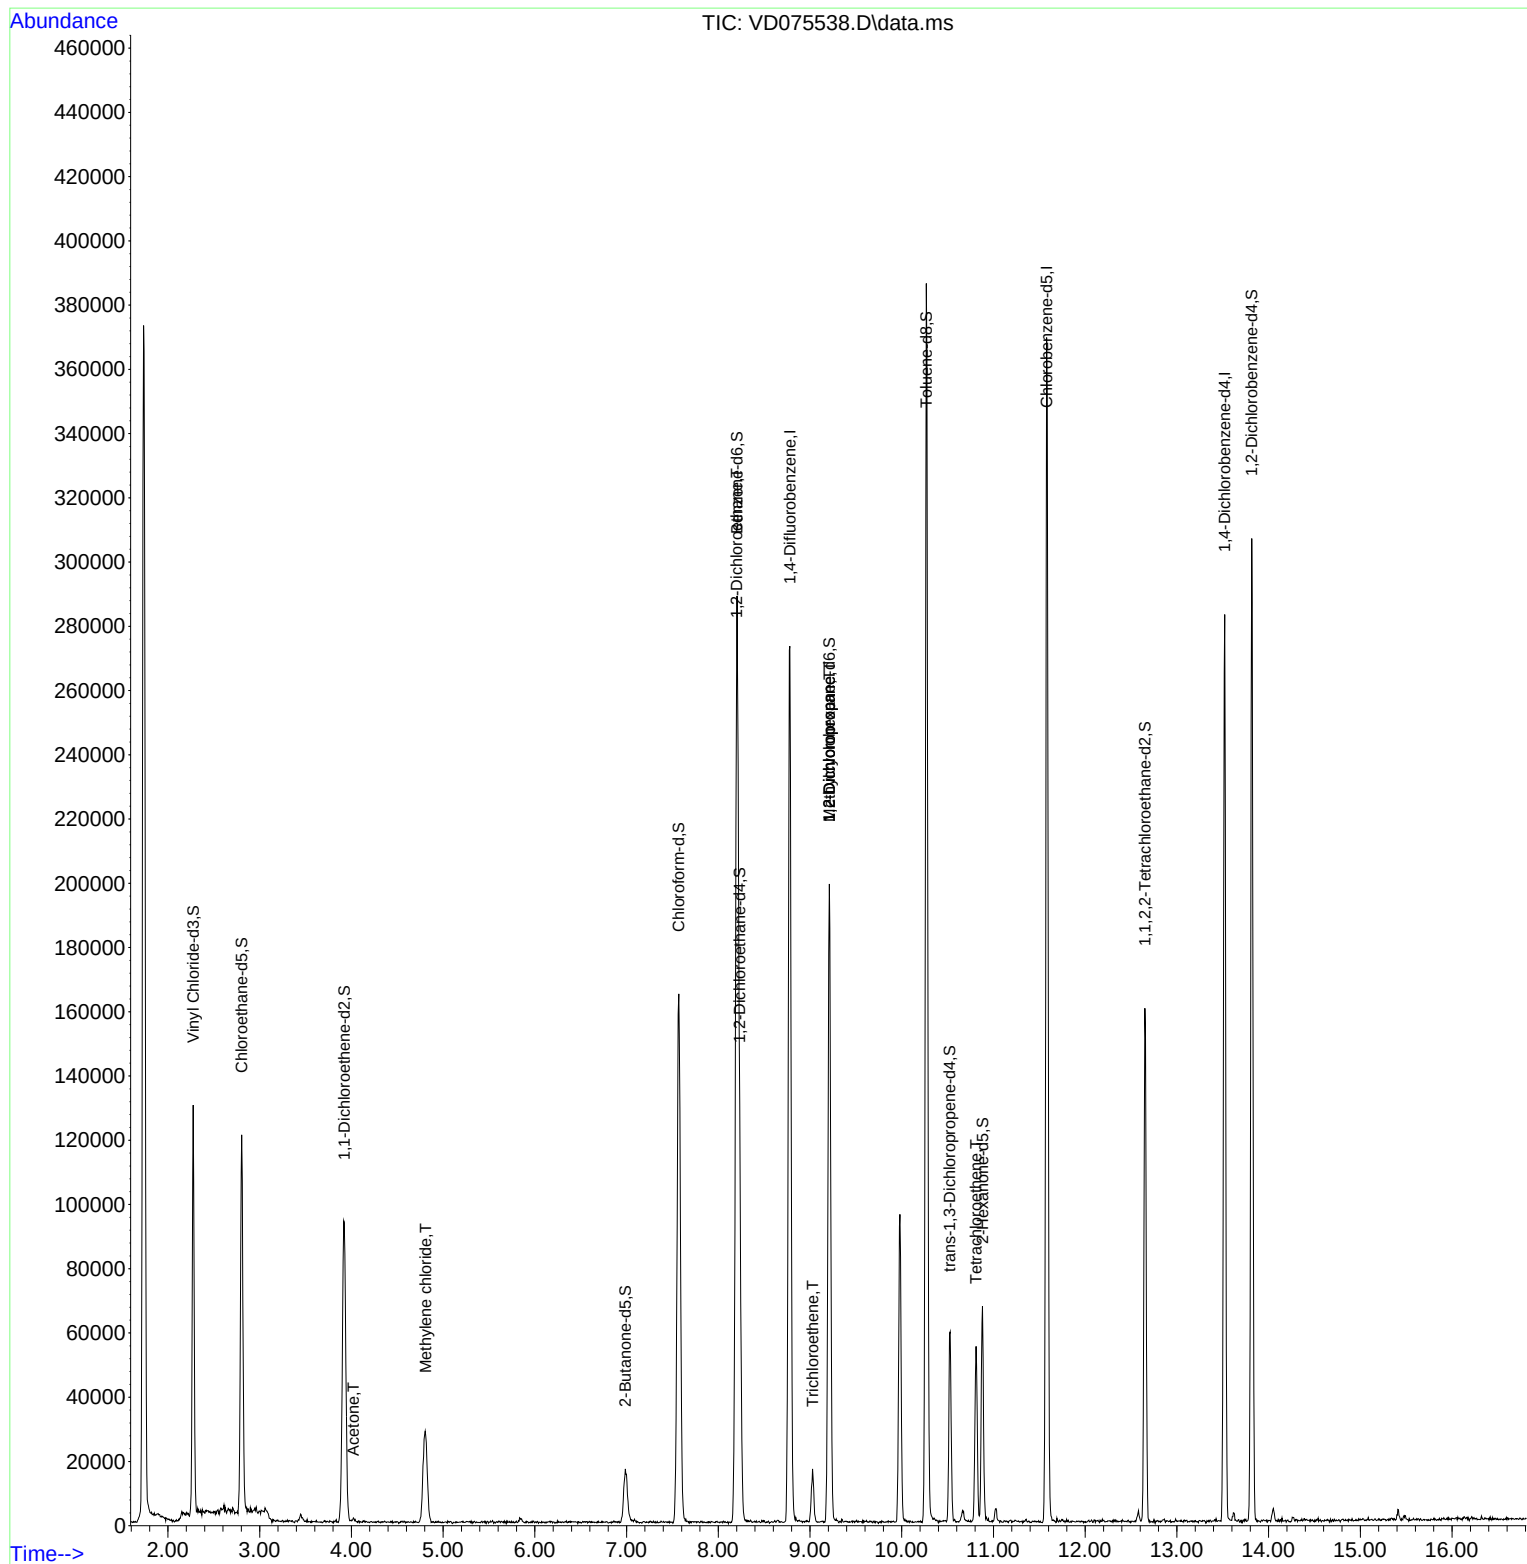




Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD032923\
 Data File : VD075538.D
 Acq On : 29 Mar 2023 18:00
 Operator : KP/SY
 Sample : 02121-17
 Misc : 6.87G/10.00mL/MSVOA_D/SOIL
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 C11B4

Manual IntegrationsAPPROVED

Quant Time: Mar 29 23:38:27 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\SFAMDLM030123SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Mar 29 23:32:17 2023
 Response via : Initial Calibration

Reviewed By :Krupa Patel 04/01/2023
 Supervised By :Mahesh Dadoda 04/03/2023

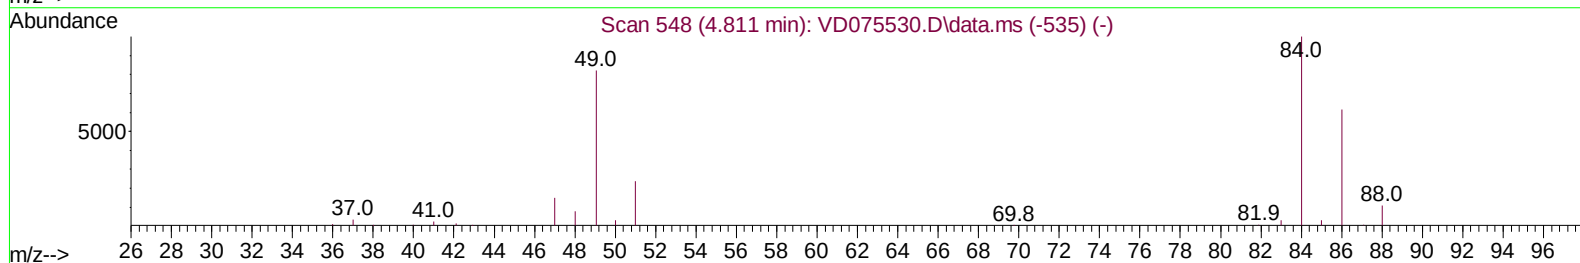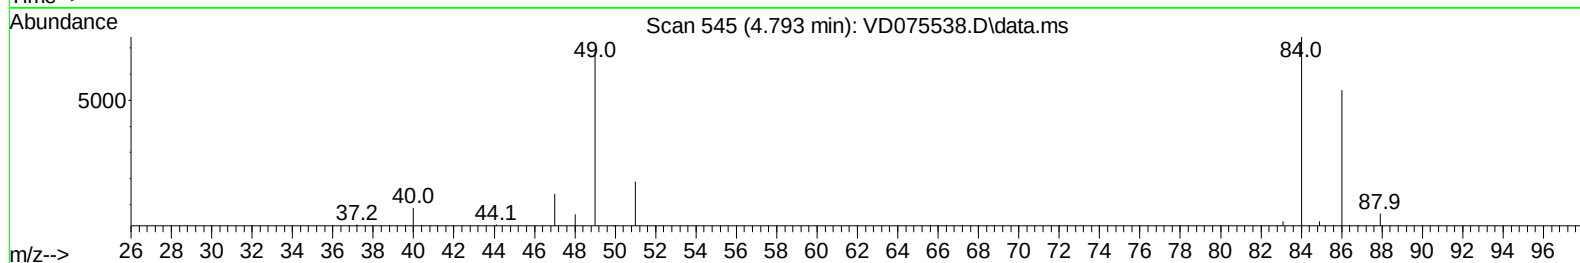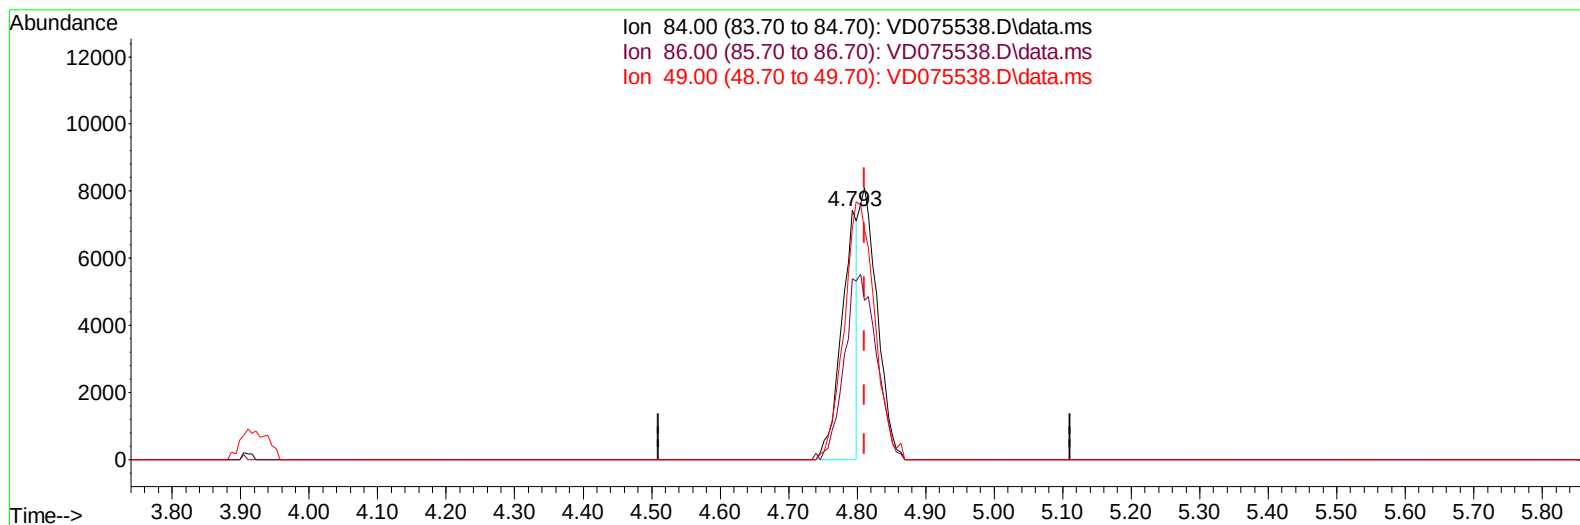

TIC: VD075538.D\data.ms

(16) Methylene chloride (T)

4.793min (-0.018) 2.11 ug/L

response 12061

Ion	Exp%	Act%
84.00	100.00	100.00
86.00	63.20	72.55
49.00	90.90	92.43
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD032923\
 Data File : VD075538.D
 Acq On : 29 Mar 2023 18:00
 Operator : KP/SY
 Sample : 02121-17
 Misc : 6.87G/10.00mL/MSVOA_D/SOIL
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 C11B4

Manual IntegrationsAPPROVED

Quant Time: Mar 29 23:38:27 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\SFAMDLM030123SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Mar 29 23:32:17 2023
 Response via : Initial Calibration

Reviewed By :Krupa Patel 04/01/2023
 Supervised By :Mahesh Dadoda 04/03/2023

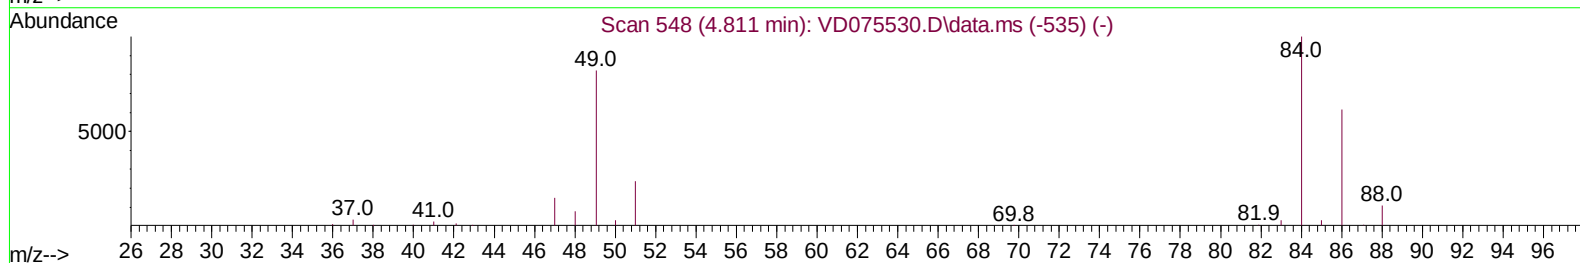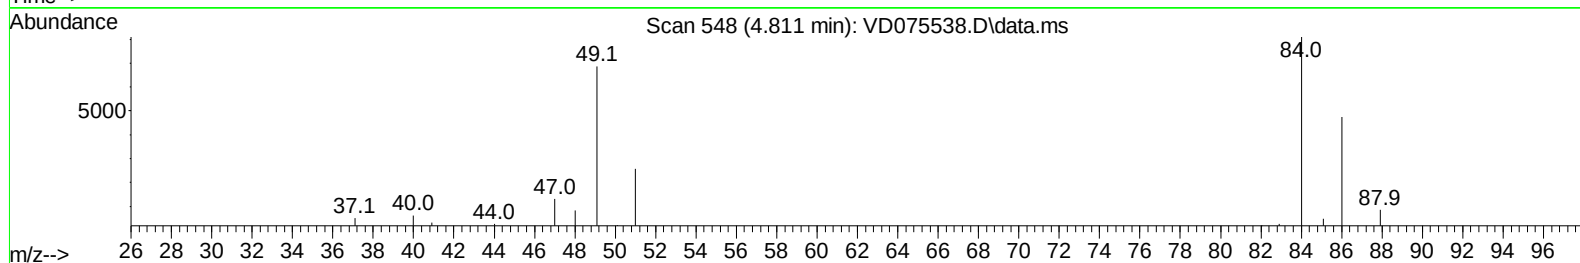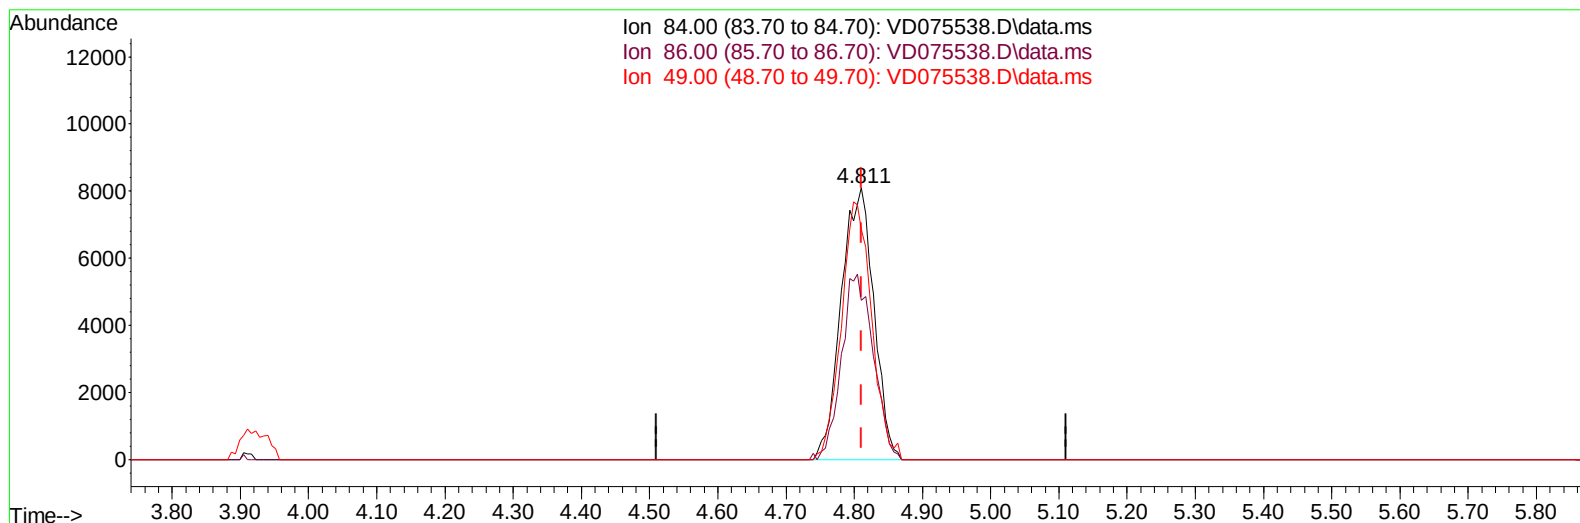

TIC: VD075538.D\data.ms

(16) Methylene chloride (T)

4.811min (-0.000) 4.70 ug/L m

response 26871

Ion	Exp%	Act%
84.00	100.00	100.00
86.00	63.20	58.69
49.00	90.90	84.83
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD032923\
 Data File : VD075538.D
 Acq On : 29 Mar 2023 18:00
 Operator : KP/SY
 Sample : 02121-17
 Misc : 6.87G/10.00ml/MSVOA_D/SOIL
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 C11B4

Manual IntegrationsAPPROVED

Quant Time: Mar 31 02:42:30 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\SFAMDLM030123SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Mar 31 01:28:39 2023
 Response via : Initial Calibration

Reviewed By :Krupa Patel 04/01/2023
 Supervised By :Mahesh Dadoda 04/03/2023

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.781	114	270779	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.581	117	235359	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.522	152	81519	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.275	65	117350	17.454	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	69.800%		
7) Chloroethane-d5	2.805	69	127751	21.957	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	87.840%		
11) 1,1-Dichloroethene-d2	3.922	63	81316	12.948	ug/L	0.00
Spiked Amount 25.000	Range 45 - 110		Recovery =	51.800%		
21) 2-Butanone-d5	6.987	46	27216	43.682	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	87.360%		
24) Chloroform-d	7.569	84	181905	25.634	ug/L	0.00
Spiked Amount 25.000	Range 40 - 150		Recovery =	102.520%		
26) 1,2-Dichloroethane-d4	8.234	65	75465	24.548	ug/L	0.00
Spiked Amount 25.000	Range 70 - 130		Recovery =	98.200%		
32) Benzene-d6	8.204	84	323165	23.120	ug/L	0.00
Spiked Amount 25.000	Range 20 - 135		Recovery =	92.480%		
36) 1,2-Dichloropropane-d6	9.210	67	103433	26.182	ug/L	0.00
Spiked Amount 25.000	Range 70 - 120		Recovery =	104.720%		
41) Toluene-d8	10.269	98	283220	22.211	ug/L	0.00
Spiked Amount 25.000	Range 30 - 130		Recovery =	88.840%		
43) trans-1,3-Dichloroprop...	10.522	79	36238	22.447	ug/L	0.00
Spiked Amount 25.000	Range 30 - 135		Recovery =	89.800%		
47) 2-Hexanone-d5	10.881	63	24436	42.877	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	85.760%		
56) 1,1,2,2-Tetrachloroeth...	12.651	84	84200	25.480	ug/L	0.00
Spiked Amount 25.000	Range 45 - 120		Recovery =	101.920%		
66) 1,2-Dichlorobenzene-d4	13.816	152	88249	30.949	ug/L	0.00
Spiked Amount 25.000	Range 75 - 120		Recovery =	123.800%#		
Target Compounds					Qvalue	
13) Acetone	4.022	43	1363	1.937	ug/L	54
16) Methylene chloride	4.811	84	26871m	4.699	ug/L	
27) 1,2-Dichloroethane	8.199	62	1604	0.375	ug/L #	71
34) Trichloroethene	9.028	95	5446	1.233	ug/L	94
35) Methylcyclohexane	9.210	83	25623	3.716	ug/L #	24
37) 1,2-Dichloropropane	9.210	63	10617	2.554	ug/L #	86
46) Tetrachloroethene	10.810	164	14076	4.159	ug/L	87

(#) = qualifier out of range (m) = manual integration (+) = signals summed