


Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD032923\
Data File : VD075529.D
Acq On : 29 Mar 2023 12:06
Operator : KP/SY
Sample : BFB109
Misc : 5.00G/10.00ml/MSVOA_D/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB109

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\SFAMDLM030123SMA.M
Title : SFAM01.0
Last Update : Fri Mar 31 01:28:39 2023

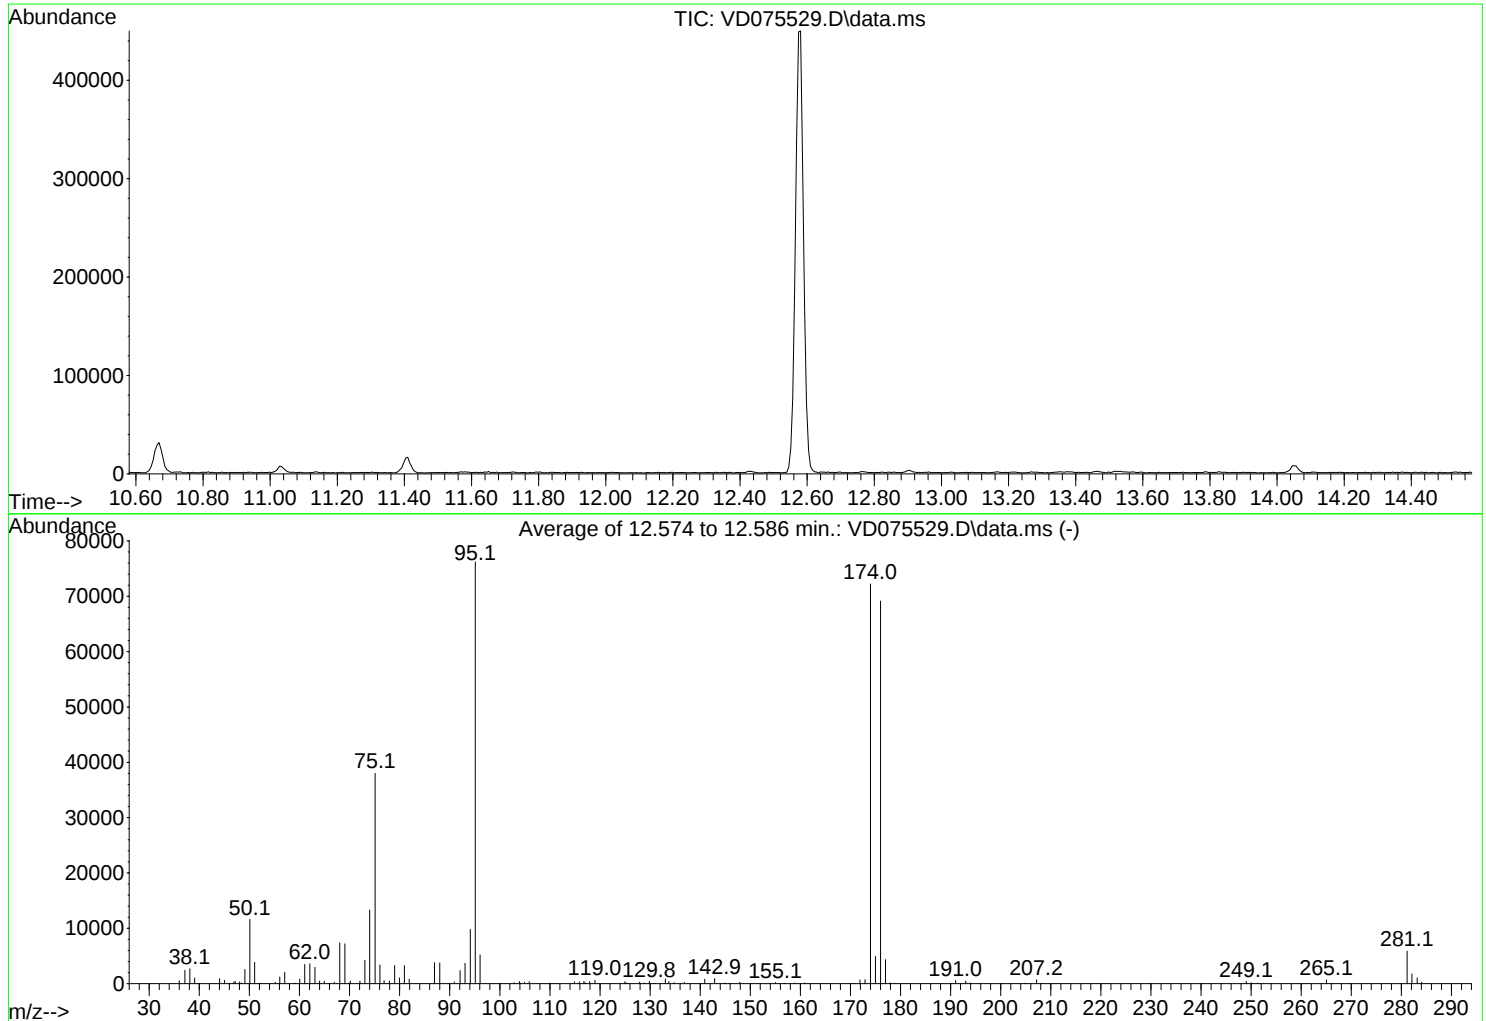

AutoFind: Scans 1868, 1869, 1870; Background Corrected with Scan 1860

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	15.2	11620	PASS
75	95	30	80	49.9	37997	PASS
95	95	100	100	100.0	76219	PASS
96	95	5	9	6.8	5207	PASS
173	174	0.00	2	1.0	714	PASS
174	95	50	120	94.8	72221	PASS
175	174	5	9	6.8	4922	PASS
176	174	95	105	95.7	69120	PASS
177	176	5	10	6.3	4339	PASS

m/z	Abundance
40.00	876.0
43.80	201.0

Instrument :
MSVOA_D
ClientSampleId :
BFB109

m/z	Abundance
36.00	665.0
37.10	2917.0
38.10	2894.0
39.00	1149.0
40.00	984.0
44.10	1040.0
45.10	625.0
47.20	785.0
48.10	546.0
49.10	2836.0
50.10	13436.0
51.00	4338.0
51.90	198.0
55.10	166.0
56.10	1422.0
57.10	2412.0
59.10	193.0
60.00	940.0
61.10	3903.0
62.10	4102.0
63.10	3386.0
64.10	513.0
64.90	671.0
66.90	161.0
68.10	8138.0
69.00	8264.0
70.10	756.0
72.10	492.0
73.00	4670.0
74.00	15164.0
75.10	43000.0
76.10	3548.0
76.90	594.0
78.00	475.0
79.00	3845.0
80.00	1264.0
81.00	3492.0
81.80	687.0
87.00	4015.0
88.00	3808.0
90.90	334.0
92.10	3029.0
93.00	4076.0
94.10	11349.0
95.10	85096.0
96.10	5109.0
103.90	572.0
105.10	244.0
105.80	351.0
109.90	161.0
115.00	423.0
115.90	341.0
116.80	714.0
118.00	421.0
119.00	751.0
125.00	604.0
127.90	408.0
128.80	165.0
129.80	402.0
133.00	640.0
133.80	263.0
134.80	222.0
136.80	241.0
140.90	706.0
142.90	1173.0
144.80	256.0
145.90	165.0
147.90	266.0
155.10	232.0
156.80	258.0
158.90	183.0
161.00	169.0
170.90	171.0
171.90	790.0
172.90	690.0
174.00	78784.0
175.00	4916.0
176.00	76072.0
177.00	5337.0
177.90	206.0
191.10	506.0
192.90	562.0
207.10	692.0
249.00	430.0
265.10	455.0
281.10	5197.0
282.10	1571.0
283.10	992.0
284.10	155.0

Instrument :
MSVOA_D
ClientSampleId :
BFB109

m/z	Abundance
36.10	561.0
37.10	2752.0
38.10	3178.0
39.10	1015.0
40.00	804.0
44.10	863.0
45.00	584.0
46.90	871.0
48.00	434.0
49.10	2941.0
50.10	13119.0
51.10	4271.0
52.10	215.0
55.10	324.0
56.00	1405.0
57.10	2423.0
59.10	158.0
60.10	763.0
61.10	3563.0
62.10	3885.0
63.10	3286.0
63.90	444.0
65.00	393.0
66.90	420.0
68.00	8599.0
69.10	8289.0
70.20	637.0
72.00	452.0
73.00	4523.0
74.00	14327.0
75.10	42008.0
76.10	3647.0
76.90	682.0
77.90	658.0
79.00	3378.0
79.90	832.0
80.90	3680.0
81.90	1018.0
86.90	3961.0
88.00	3911.0
90.90	440.0
92.00	2679.0
93.10	3924.0
94.10	10670.0
95.10	85632.0
96.10	5983.0
97.10	152.0
102.80	249.0
103.90	533.0
104.90	261.0
105.90	402.0
110.10	186.0
111.00	184.0
114.90	322.0
115.80	373.0
117.00	543.0
118.00	496.0
119.00	637.0
124.90	479.0
125.60	186.0
128.10	222.0
129.90	557.0
131.00	154.0
133.10	1042.0
133.80	377.0
134.80	257.0
136.90	181.0
141.00	859.0
142.90	980.0
145.00	304.0
147.80	322.0
154.90	244.0
158.90	167.0
160.80	236.0
171.90	816.0
173.00	942.0
174.00	78912.0
175.00	6246.0
176.00	75288.0
177.00	4476.0
178.00	202.0
178.80	152.0
191.10	508.0
193.10	654.0
193.90	179.0
205.00	254.0
207.10	639.0
249.10	334.0
250.10	236.0
265.00	583.0
281.10	6910.0
282.10	2095.0

Instrument :
MSVOA_D
ClientSampleId :
BFB109

283.10929.0

284.10280.0

Instrument :
MSVOA_D
ClientSampleId :
BFB109

m/z	Abundance
35.90	326.0
37.00	1496.0
38.10	2027.0
39.10	861.0
40.10	955.0
44.00	812.0
45.10	630.0
47.10	552.0
48.40	381.0
49.00	1913.0
50.10	8304.0
51.10	2981.0
55.20	235.0
56.00	824.0
56.90	1317.0
60.00	850.0
61.00	2950.0
62.00	2809.0
63.10	2216.0
64.00	404.0
65.00	251.0
67.00	204.0
68.00	5404.0
69.10	5036.0
69.90	329.0
72.10	482.0
73.10	3436.0
74.00	10398.0
75.10	28984.0
76.00	2926.0
76.90	409.0
77.90	299.0
79.00	2584.0
79.90	1076.0
81.00	2596.0
82.00	730.0
87.00	3416.0
88.00	3483.0
90.90	188.0
92.10	1443.0
93.10	3012.0
94.10	7346.0
95.10	57928.0
96.00	4528.0
102.90	289.0
104.10	284.0
104.80	242.0
105.80	267.0
114.80	216.0
115.80	216.0
116.80	529.0
117.80	233.0
118.90	402.0
125.30	357.0
127.90	362.0
128.80	170.0
129.90	224.0
133.10	852.0
133.70	492.0
136.90	309.0
140.80	867.0
142.90	657.0
148.00	197.0
155.10	170.0
163.10	192.0
171.90	356.0
172.80	509.0
174.00	58968.0
175.00	3604.0
176.00	56000.0
177.00	3205.0
190.90	655.0
193.00	717.0
193.90	184.0
207.20	787.0
208.20	155.0
249.00	445.0
250.10	180.0
251.30	261.0
265.10	927.0
266.00	190.0
281.20	5537.0
282.10	1648.0
283.20	1250.0
284.00	278.0

Instrument :
MSVOA_D
ClientSampleId :
BFB109