




Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD033023\
 Data File : VD075546.D
 Acq On : 30 Mar 2023 14:35
 Operator : KP/SY
 Sample : 02130-02
 Misc : 5.36G/10.00ml/MSVOA_D/SOIL
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 C1191

Manual IntegrationsAPPROVED

Quant Time: Mar 31 01:30:22 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\SFAMDLM030123SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Mar 31 01:28:39 2023
 Response via : Initial Calibration

Reviewed By :Krupa Patel 03/31/2023
 Supervised By :Mahesh Dadoda 04/03/2023

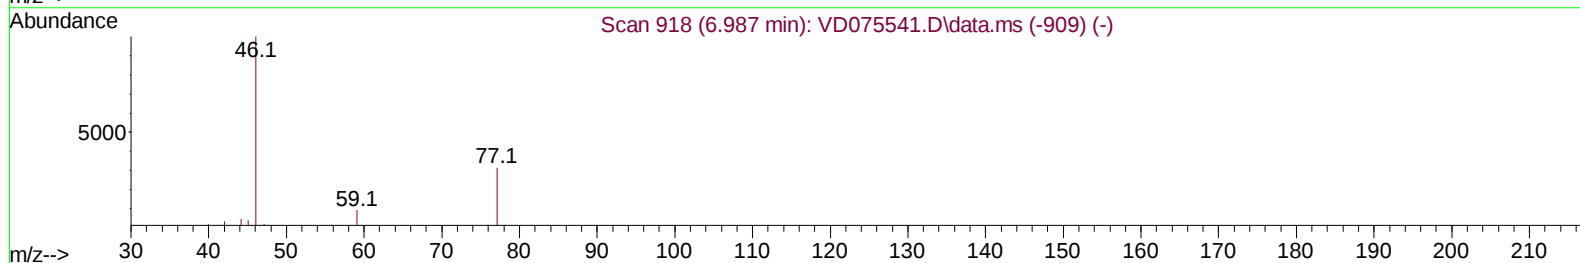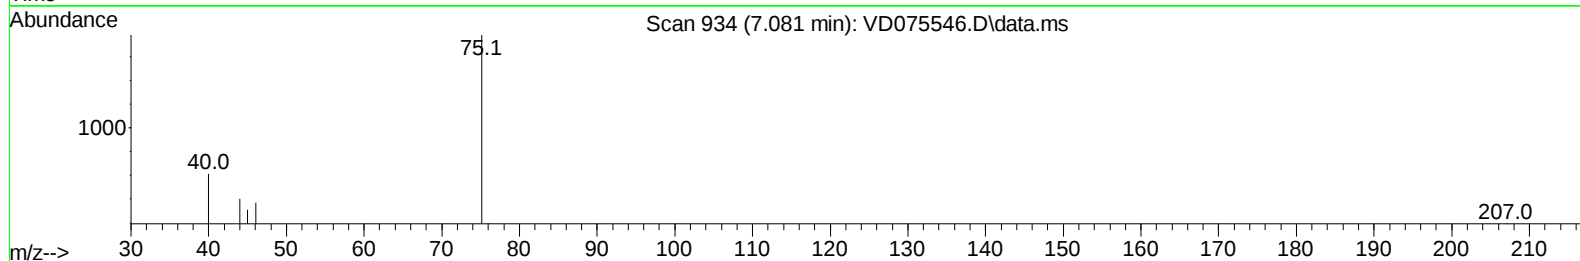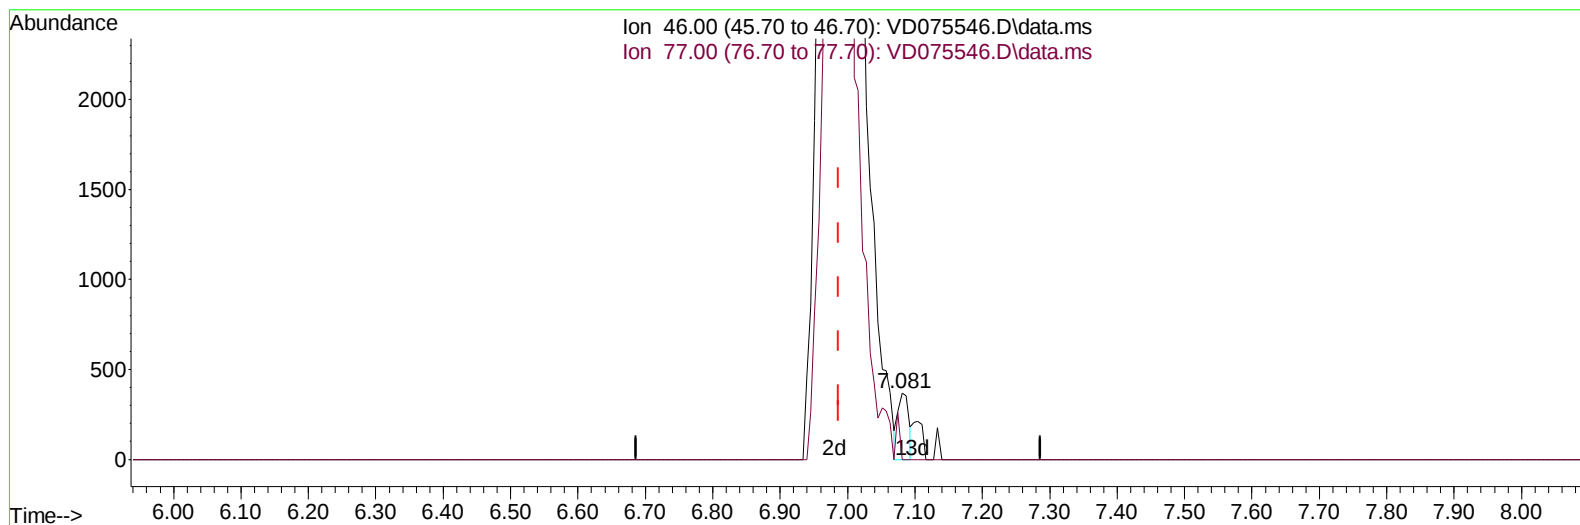

TIC: VD075546.D\data.ms

(21) 2-Butanone-d5 (S)

7.081min (+ 0.094) 0.63 ug/L

response 412

Ion	Exp%	Act%
46.00	100.00	100.00
77.00	30.70	22.33
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD033023\
 Data File : VD075546.D
 Acq On : 30 Mar 2023 14:35
 Operator : KP/SY
 Sample : 02130-02
 Misc : 5.36G/10.00ml/MSVOA_D/SOIL
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 C1191

Manual IntegrationsAPPROVED

Quant Time: Mar 31 01:30:22 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\SFAMDLM030123SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Mar 31 01:28:39 2023
 Response via : Initial Calibration

Reviewed By :Krupa Patel 03/31/2023
 Supervised By :Mahesh Dadoda 04/03/2023

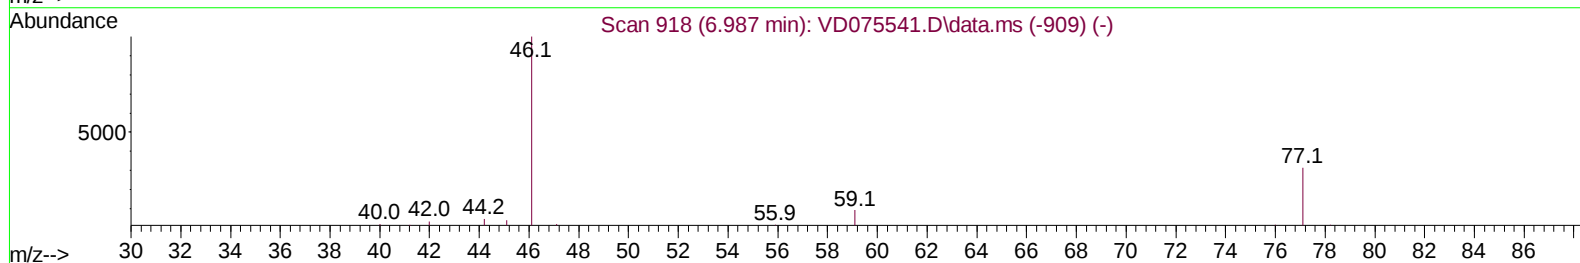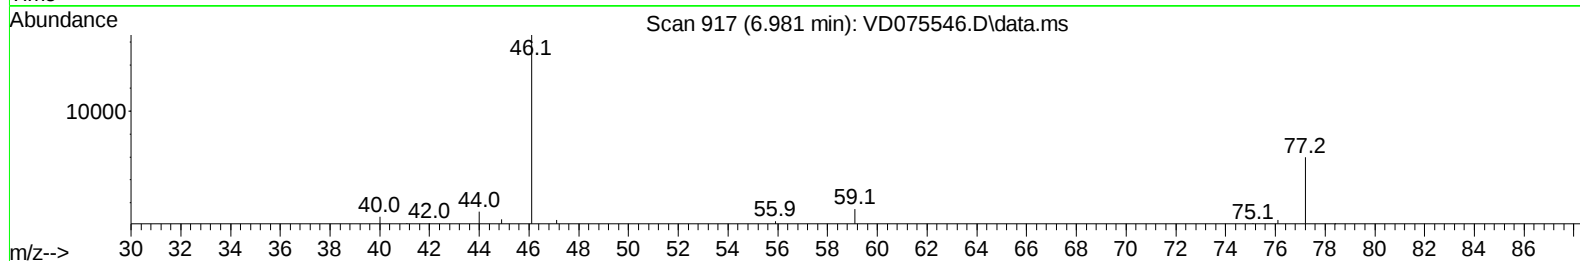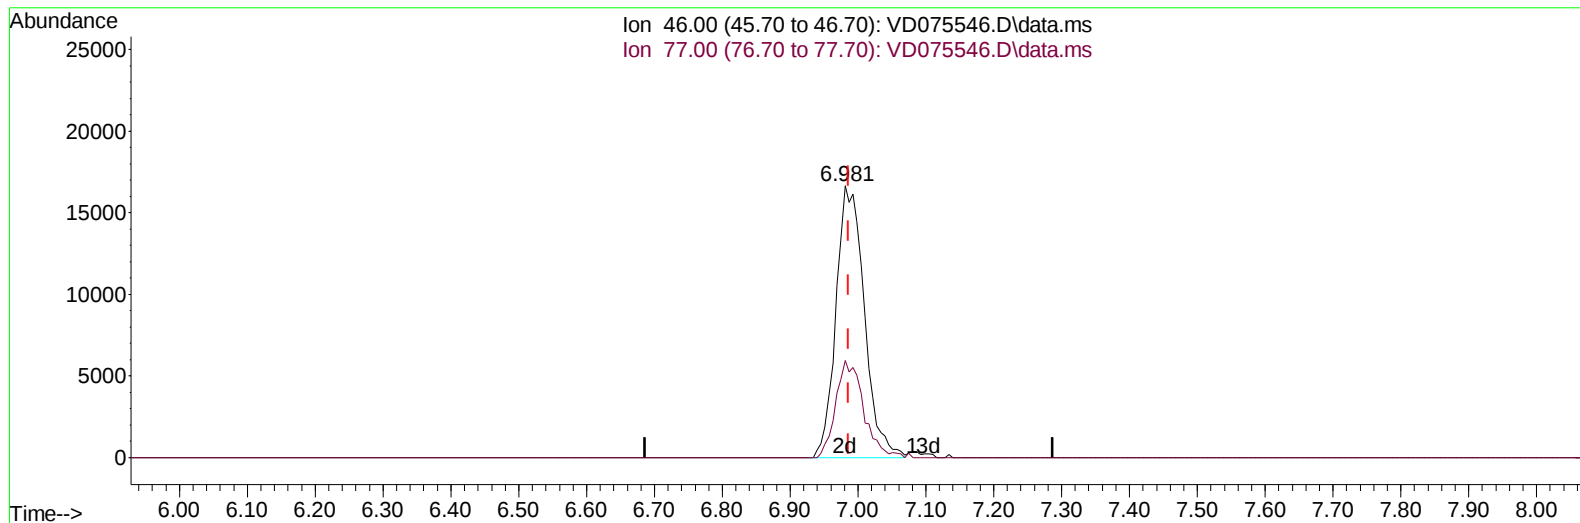

TIC: VD075546.D\data.ms

(21) 2-Butanone-d5 (S)

6.981min (-0.006) 72.92 ug/L m

response 48051

Ion	Exp%	Act%
46.00	100.00	100.00
77.00	30.70	0.19#
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD033023\
 Data File : VD075546.D
 Acq On : 30 Mar 2023 14:35
 Operator : KP/SY
 Sample : 02130-02
 Misc : 5.36G/10.00ml/MSVOA_D/SOIL
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 C1191

Manual IntegrationsAPPROVED

Quant Time: Mar 31 01:30:22 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\SFAMDLM030123SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Mar 31 01:28:39 2023
 Response via : Initial Calibration

Reviewed By :Krupa Patel 03/31/2023
 Supervised By :Mahesh Dadoda 04/03/2023

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.781	114	286372	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.581	117	284055	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.522	152	108921	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.275	65	96002	13.501	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	54.000%	
7) Chloroethane-d5	2.804	69	121393	19.728	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	78.920%	
11) 1,1-Dichloroethene-d2	3.922	63	70855	10.668	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110	Recovery	=	42.680%#	
21) 2-Butanone-d5	6.981	46	48051m	72.923	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	145.840%#	
24) Chloroform-d	7.569	84	206588	27.527	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150	Recovery	=	110.120%	
26) 1,2-Dichloroethane-d4	8.234	65	101752	31.296	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130	Recovery	=	125.200%	
32) Benzene-d6	8.204	84	347492	20.599	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135	Recovery	=	82.400%	
36) 1,2-Dichloropropane-d6	9.210	67	124345	26.080	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120	Recovery	=	104.320%	
41) Toluene-d8	10.269	98	310248	20.160	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130	Recovery	=	80.640%	
43) trans-1,3-Dichloroprop...	10.528	79	52362	26.875	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135	Recovery	=	107.480%	
47) 2-Hexanone-d5	10.881	63	45038	65.478	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	130.960%	
56) 1,1,2,2-Tetrachloroeth...	12.651	84	129985	32.592	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120	Recovery	=	130.360%#	
66) 1,2-Dichlorobenzene-d4	13.816	152	124069	32.565	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120	Recovery	=	130.240%#	
Target Compounds						
16) Methylene chloride	4.804	84	10704	1.770	ug/L	Qvalue 95

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD033023\
Data File : VD075546.D
Acq On : 30 Mar 2023 14:35
Operator : KP/SY
Sample : 02130-02
Misc : 5.36G/10.00ml/MSVOA_D/soil
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
C1191

Manual IntegrationsAPPROVED

Quant Time: Mar 31 01:30:22 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\SFAMDLM030123SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Mar 31 01:28:39 2023
Response via : Initial Calibration

Reviewed By :Krupa Patel 03/31/2023
Supervised By :Mahesh Dadoda 04/03/2023

