
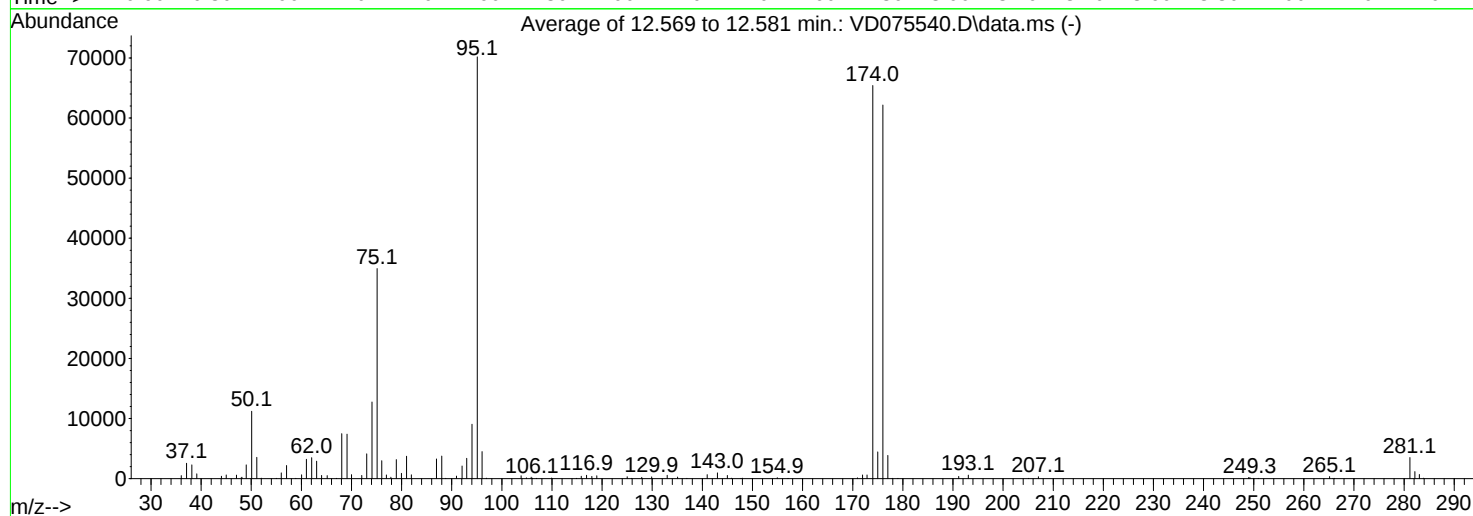


Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD033023\
Data File : VD075540.D
Acq On : 30 Mar 2023 10:01
Operator : KP/SY
Sample : BFB110
Misc : 5.00G/10.00ml/MSVOA_D/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB110

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\SFAMDLM030123SMA.M
Title : SFAM01.0
Last Update : Fri Mar 31 01:28:39 2023

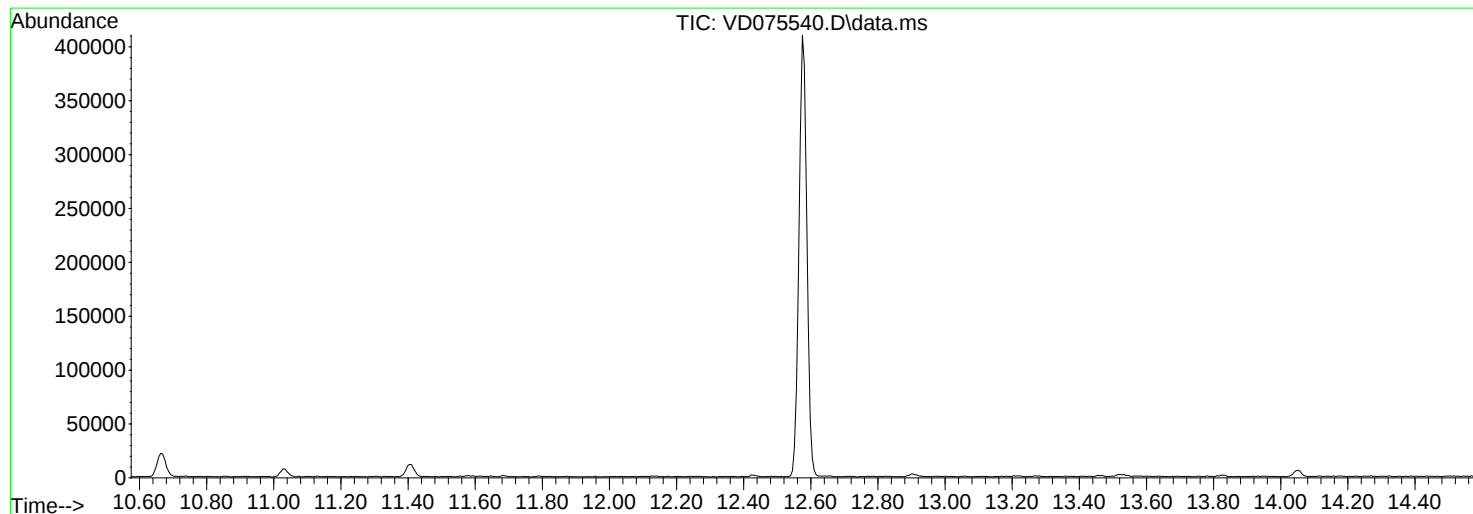

AutoFind: Scans 1867, 1868, 1869; Background Corrected with Scan 1860

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.0	11198	PASS
75	95	30	80	49.8	34952	PASS
95	95	100	100	100.0	70181	PASS
96	95	5	9	6.4	4501	PASS
173	174	0.00	2	0.9	605	PASS
174	95	50	120	93.2	65419	PASS
175	174	5	9	6.8	4450	PASS
176	174	95	105	95.0	62152	PASS
177	176	5	10	6.2	3862	PASS

Scan 1860 (12.528 min): VD075540.D\data.ms
BFB110

m/z	Abundance
40.00	841.0
44.10	326.0

Instrument :
MSVOA_D
ClientSampleId :
BFB110

m/z	Abundance
36.00	464.0
37.10	2464.0
38.10	2350.0
39.10	1073.0
40.00	643.0
44.00	738.0
45.00	404.0
47.00	613.0
48.00	483.0
49.00	2100.0
50.10	9301.0
51.10	3263.0
55.00	172.0
56.00	950.0
57.00	2023.0
60.00	385.0
61.00	2987.0
62.00	3139.0
63.00	2579.0
64.10	486.0
65.20	350.0
68.00	6686.0
69.10	6209.0
70.00	884.0
72.00	534.0
73.00	3750.0
74.10	11892.0
75.10	30912.0
76.00	2732.0
77.00	691.0
77.80	484.0
78.90	2663.0
80.00	685.0
81.00	3375.0
81.90	544.0
87.00	3383.0
88.00	3722.0
90.90	375.0
92.10	2078.0
93.00	2835.0
94.10	8089.0
95.10	60552.0
96.00	4135.0
96.90	237.0
103.90	563.0
104.90	154.0
105.80	308.0
114.90	165.0
115.90	192.0
117.00	462.0
118.00	250.0
119.00	362.0
125.00	195.0
128.00	203.0
129.90	261.0
133.10	406.0
135.00	252.0
141.00	565.0
143.00	770.0
145.10	514.0
172.00	406.0
172.90	693.0
174.00	54848.0
175.00	3587.0
176.00	49264.0
177.00	3645.0
193.00	370.0
207.10	285.0
249.00	306.0
265.20	172.0
265.80	192.0
281.10	2001.0
282.20	1035.0
283.00	429.0

Instrument :
MSVOA_D
ClientSampleId :
BFB110

m/z	Abundance
36.10	533.0
37.10	2852.0
38.20	2123.0
39.20	814.0
40.10	592.0
44.10	1005.0
45.00	441.0
47.00	491.0
48.20	518.0
49.00	2703.0
50.10	12403.0
51.10	3893.0
56.00	1024.0
57.10	2170.0
58.90	200.0
60.10	834.0
61.00	3198.0
62.00	3785.0
63.10	3432.0
64.10	626.0
65.10	584.0
67.00	158.0
68.10	8151.0
69.10	8203.0
70.00	474.0
72.00	556.0
73.10	4109.0
74.10	13141.0
75.10	38792.0
76.10	3426.0
76.90	596.0
79.00	3982.0
79.90	980.0
81.00	4019.0
82.00	808.0
86.90	2907.0
88.00	4073.0
90.90	447.0
92.00	2519.0
93.00	3697.0
94.00	10286.0
95.10	79144.0
96.10	5066.0
103.80	513.0
104.90	242.0
105.90	438.0
106.90	168.0
109.90	159.0
115.80	505.0
116.80	594.0
118.00	421.0
118.90	657.0
125.00	381.0
127.90	285.0
129.90	445.0
132.90	559.0
135.00	271.0
141.00	688.0
143.00	1224.0
145.00	628.0
148.00	211.0
155.00	196.0
157.10	186.0
171.00	235.0
171.90	594.0
172.90	519.0
174.00	73128.0
175.00	4970.0
176.00	69352.0
177.00	4652.0
191.10	682.0
193.00	736.0
207.10	405.0
249.00	235.0
249.30	218.0
250.90	150.0
265.10	427.0
281.20	3901.0
282.10	1100.0
283.10	1059.0

Instrument :
MSVOA_D
ClientSampleId :
BFB110

m/z	Abundance
36.10	519.0
37.10	2332.0
38.10	2423.0
39.10	546.0
40.10	771.0
44.10	466.0
45.00	1022.0
47.10	658.0
48.10	237.0
49.00	2093.0
50.10	11889.0
51.10	3448.0
52.00	266.0
56.00	902.0
57.00	2370.0
60.10	697.0
61.00	3476.0
62.10	3508.0
63.10	2710.0
64.00	478.0
65.10	560.0
68.10	7613.0
69.10	7788.0
70.00	610.0
72.10	497.0
73.10	4497.0
74.10	13251.0
75.10	35152.0
76.00	2792.0
77.00	557.0
77.90	268.0
78.90	2879.0
79.90	1014.0
81.00	3755.0
82.00	606.0
87.00	3540.0
88.00	3479.0
88.80	161.0
91.00	446.0
92.00	1746.0
93.00	3640.0
94.00	8762.0
95.10	70848.0
96.10	4301.0
103.80	389.0
106.10	272.0
110.00	165.0
115.90	481.0
116.90	606.0
117.90	460.0
118.90	391.0
125.00	384.0
125.90	192.0
127.80	179.0
130.00	184.0
133.00	757.0
135.10	312.0
136.90	165.0
140.90	733.0
143.00	882.0
144.90	451.0
145.80	235.0
147.70	151.0
154.90	288.0
170.90	152.0
172.00	802.0
172.80	603.0
174.00	68280.0
175.00	4792.0
176.00	67840.0
177.00	3290.0
177.90	187.0
179.00	161.0
191.20	458.0
193.10	640.0
205.10	150.0
206.90	315.0
249.20	326.0
250.00	179.0
265.10	489.0
266.10	157.0
281.10	4669.0
282.10	1360.0
283.00	558.0
283.90	247.0

Instrument :
MSVOA_D
ClientSampleId :
BFB110