


Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD033119\
Data File : VD061442.D
Acq On : 31 Mar 2019 12:34
Operator : VA/AP
Sample : BFB
Misc : 5.00g/5ml/MSVOA_D/SOIL
ALS Vial : 2 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D032719S.M
Title : SW846 8260
Last Update : Thu Mar 28 09:22:37 2019

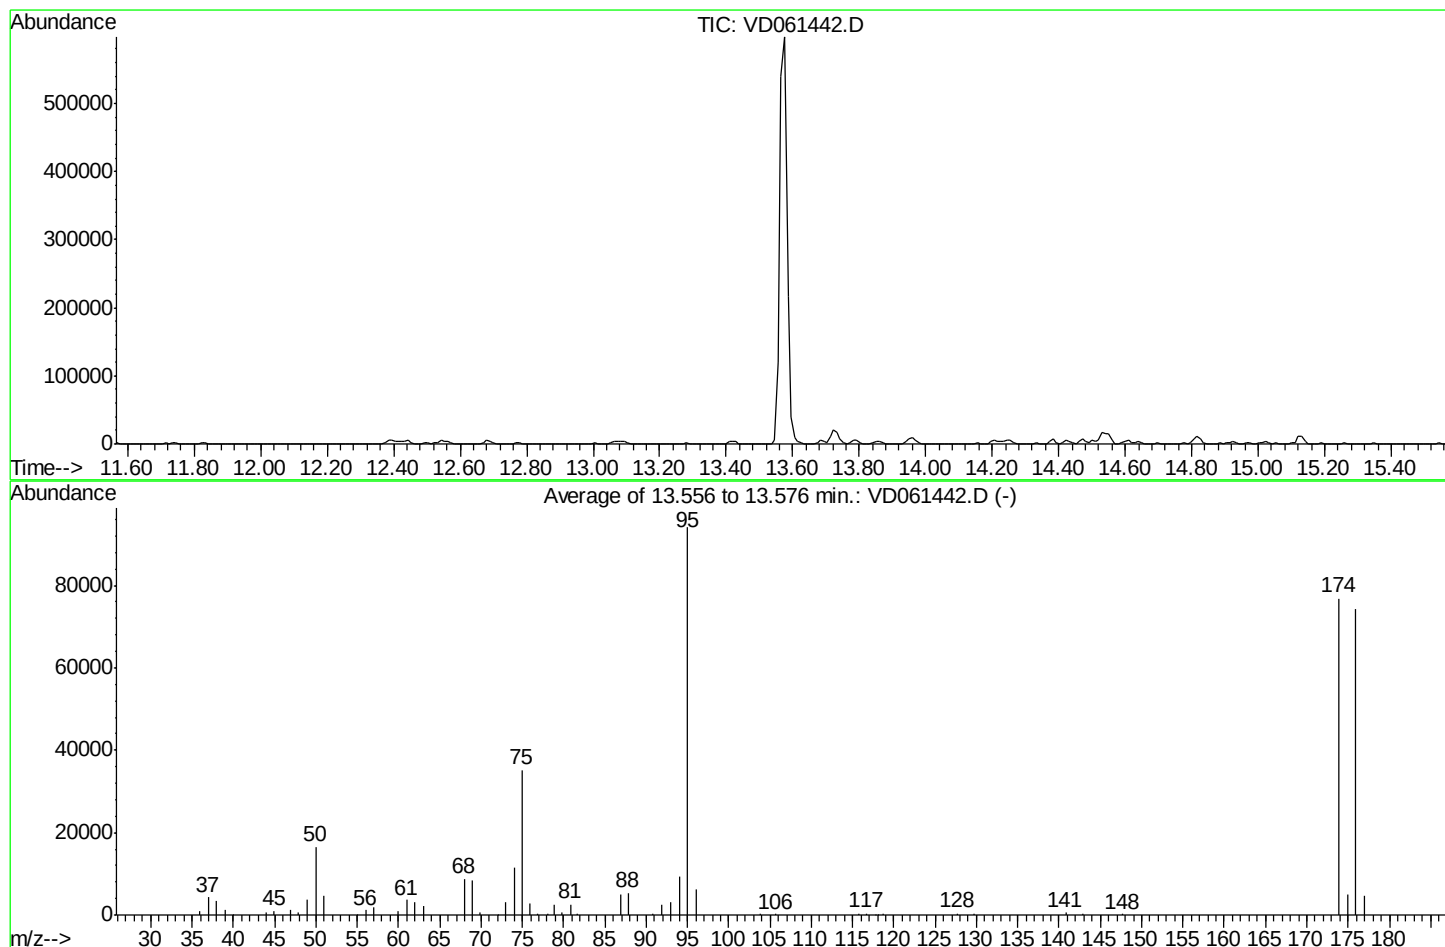

AutoFind: Scans 1232, 1233, 1234; Background Corrected with Scan 1228

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.5	16478	PASS
75	95	30	60	37.5	35281	PASS
95	95	100	100	100.0	94117	PASS
96	95	5	9	6.7	6320	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	81.7	76900	PASS
175	174	5	9	6.6	5111	PASS
176	174	95	101	96.7	74371	PASS
177	176	5	9	6.5	4805	PASS