
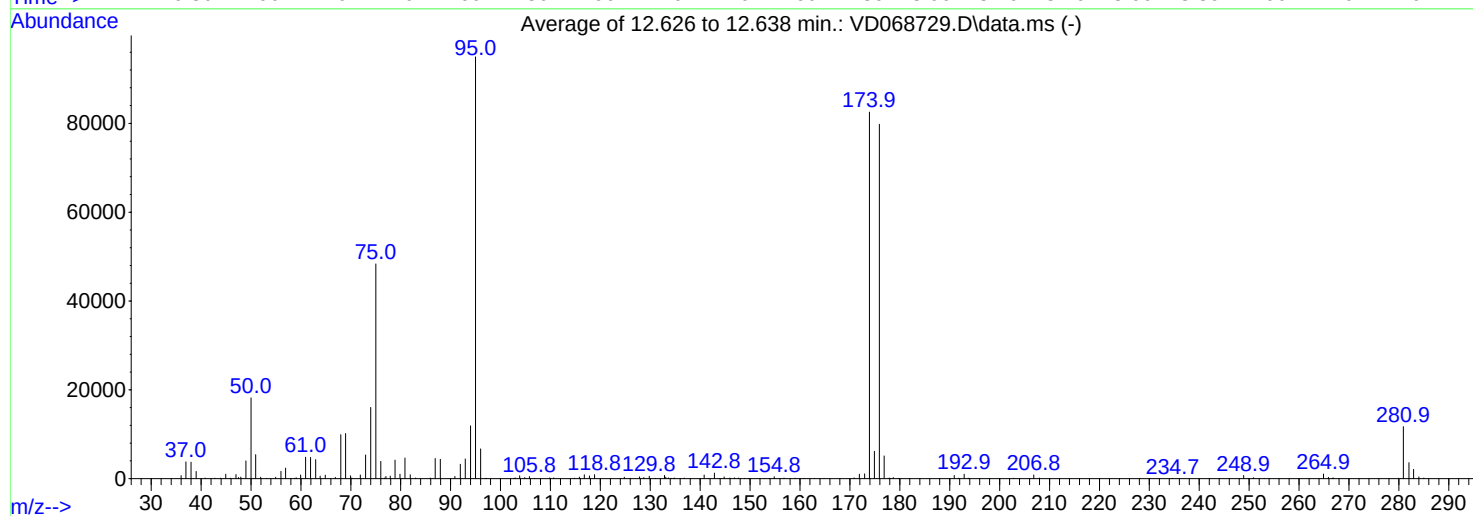


Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD033121\
Data File : VD068729.D
Acq On : 31 Mar 2021 09:19
Operator : VA/SY
Sample : BFB
Misc : 5.00G/5.00ml/MSVOA_D/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D031921S.M
Title : SW846 8260
Last Update : Sat Mar 20 02:00:55 2021

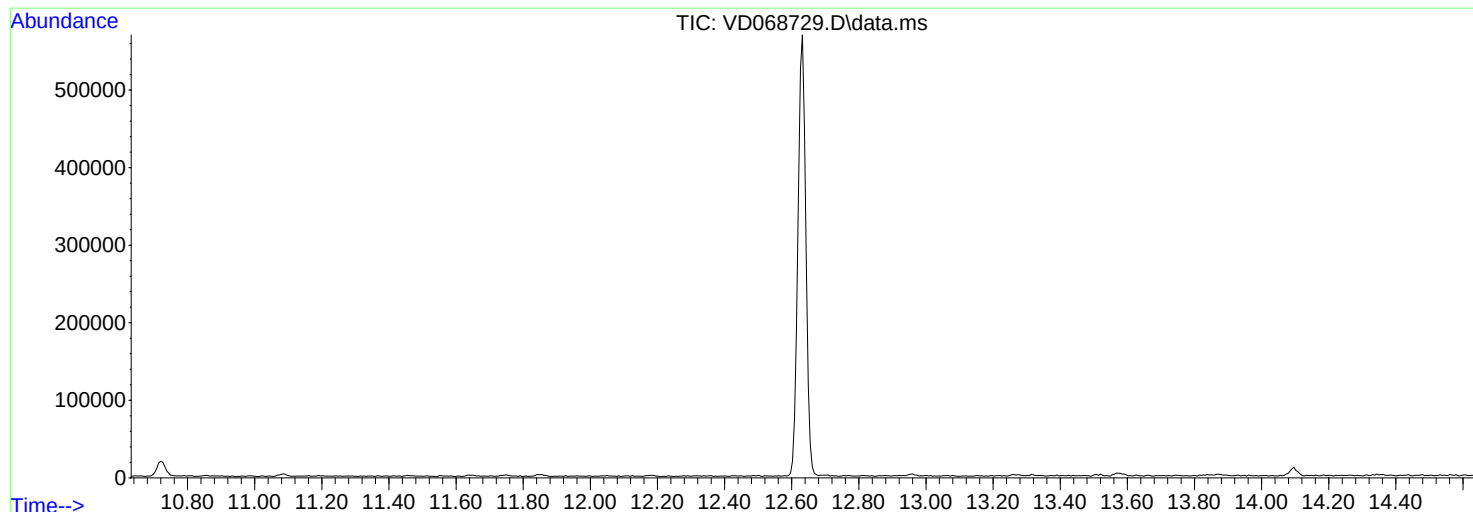

AutoFind: Scans 1820, 1821, 1822; Background Corrected with Scan 1812

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	19.2	18193	PASS
75	95	30	60	50.9	48360	PASS
95	95	100	100	100.0	94976	PASS
96	95	5	9	7.0	6692	PASS
173	174	0.00	2	1.3	1065	PASS
174	95	50	100	86.9	82555	PASS
175	174	5	9	7.5	6178	PASS
176	174	95	101	96.7	79803	PASS
177	176	5	9	6.4	5119	PASS