
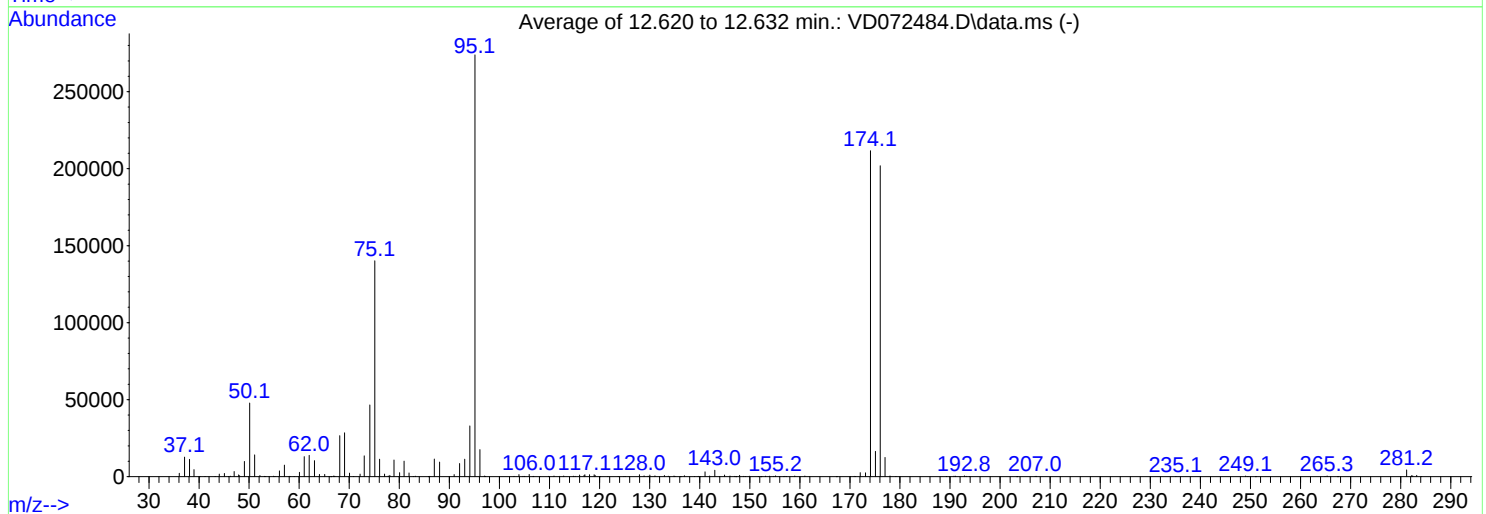


Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD033122\
Data File : VD072484.D
Acq On : 31 Mar 2022 09:49
Operator : VA/SY
Sample : BFB
Misc : 5.00G/5.00ml/MSVOA_D/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D032922S.M
Title : SW846 8260
Last Update : Wed Mar 30 02:44:36 2022

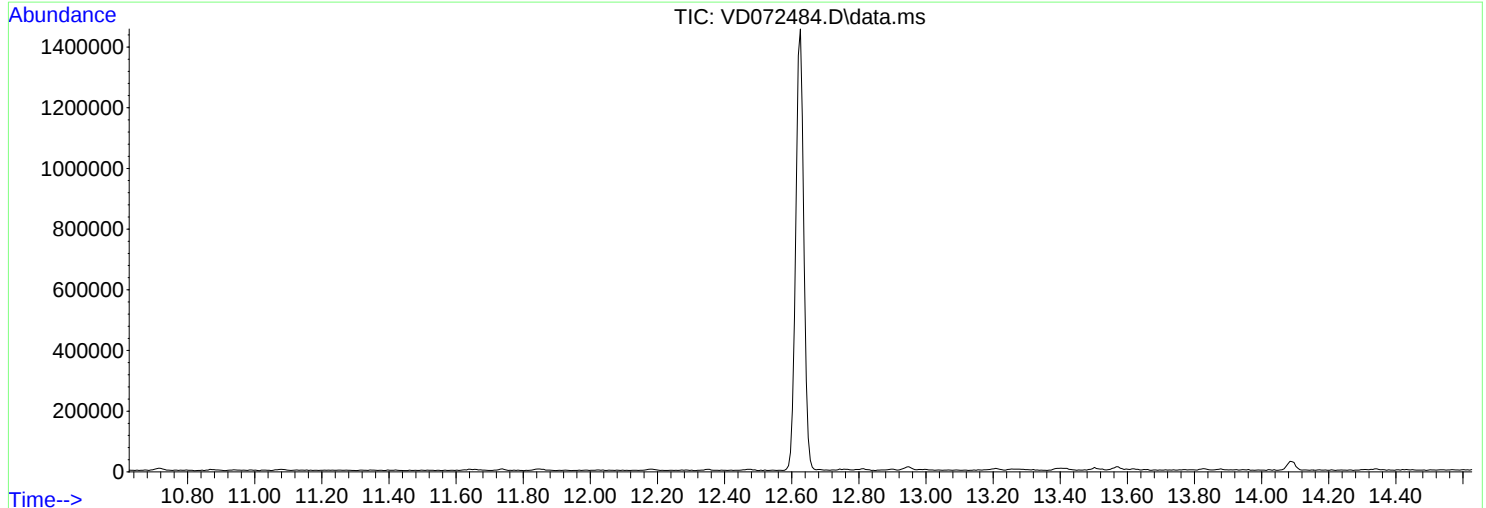

AutoFind: Scans 1819, 1820, 1821; Background Corrected with Scan 1810

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.5	47811	PASS
75	95	30	60	51.2	140176	PASS
95	95	100	100	100.0	273941	PASS
96	95	5	9	6.4	17610	PASS
173	174	0.00	2	1.2	2474	PASS
174	95	50	100	77.3	211712	PASS
175	174	5	9	7.8	16478	PASS
176	174	95	101	95.4	201877	PASS
177	176	5	9	6.2	12464	PASS