


Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD033123\
Data File : VD075551.D
Acq On : 31 Mar 2023 10:08
Operator : KP/SY
Sample : BFB111
Misc : 5.00G/10.00ml/MSVOA_D/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB111

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\SFAMDLM033123SMA.M
Title : SFAM01.0
Last Update : Sat Apr 01 00:08:20 2023

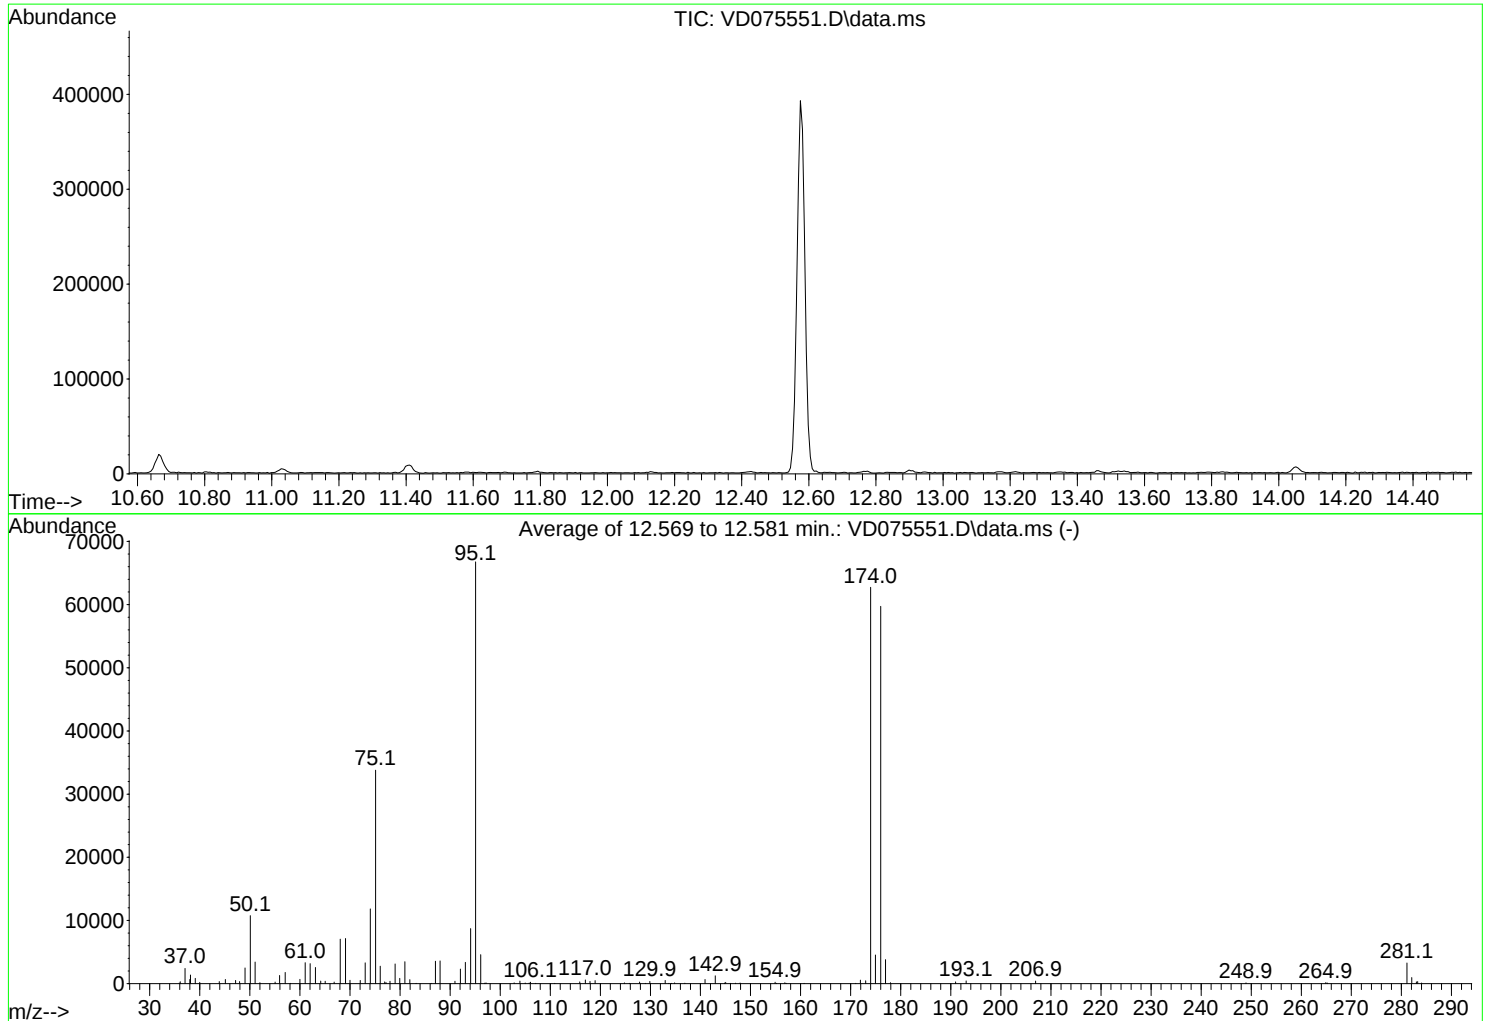

AutoFind: Scans 1867, 1868, 1869; Background Corrected with Scan 1860

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.1	10771	PASS
75	95	30	80	50.6	33803	PASS
95	95	100	100	100.0	66773	PASS
96	95	5	9	6.9	4594	PASS
173	174	0.00	2	0.7	460	PASS
174	95	50	120	93.9	62733	PASS
175	174	5	9	7.2	4525	PASS
176	174	95	105	95.2	59736	PASS
177	176	5	10	6.4	3811	PASS

Scan 1860 (12.528 min): VD075551.D\data.ms
BFB111

m/z	Abundance
40.00	624.0
43.90	405.0

Instrument :
MSVOA_D
ClientSampleId :
BFB111

m/z	Abundance
35.90	320.0
37.00	2106.0
38.00	2000.0
39.10	595.0
40.10	723.0
44.00	770.0
45.10	501.0
47.30	558.0
48.00	282.0
49.00	2209.0
50.10	10402.0
51.10	3220.0
52.00	237.0
55.00	190.0
56.00	1196.0
57.00	1948.0
60.10	638.0
61.10	3224.0
62.10	3177.0
63.10	2418.0
64.20	426.0
65.00	195.0
66.90	165.0
68.10	6282.0
69.10	6773.0
70.00	550.0
72.10	511.0
73.00	2678.0
74.00	9601.0
75.10	28984.0
76.00	2665.0
76.90	316.0
78.00	242.0
79.00	2531.0
80.00	629.0
81.00	3343.0
81.90	726.0
87.00	3193.0
88.00	3429.0
91.00	324.0
92.00	1969.0
93.10	3194.0
94.10	7651.0
95.10	59264.0
96.10	4036.0
96.90	217.0
102.80	170.0
104.00	320.0
106.10	256.0
115.90	299.0
117.00	450.0
118.00	299.0
118.90	324.0
127.90	314.0
129.90	264.0
133.00	291.0
134.80	167.0
140.90	650.0
142.90	1090.0
144.80	304.0
147.90	286.0
154.90	153.0
155.20	151.0
156.80	158.0
171.00	180.0
172.10	607.0
172.90	526.0
174.00	53008.0
174.90	4006.0
176.00	50800.0
177.00	3216.0
193.10	380.0
207.00	360.0
264.90	168.0
281.10	2184.0
282.10	642.0
283.00	360.0
283.40	340.0

Instrument :
MSVOA_D
ClientSampleId :
BFB111

m/z	Abundance
36.10	388.0
37.00	2704.0
38.20	2013.0
39.10	1016.0
39.90	710.0
43.90	779.0
45.10	726.0
47.10	430.0
47.90	438.0
49.10	2861.0
50.10	11553.0
51.10	3515.0
52.00	256.0
55.10	314.0
56.00	1269.0
57.00	1914.0
59.90	884.0
61.00	3458.0
62.00	3280.0
63.10	2767.0
64.10	567.0
65.00	367.0
66.80	254.0
68.00	7420.0
69.10	7119.0
70.00	562.0
72.00	545.0
73.10	3649.0
74.00	13232.0
75.10	38104.0
76.10	3097.0
77.20	531.0
77.90	398.0
79.00	3507.0
80.00	979.0
80.90	3661.0
81.90	603.0
87.10	4378.0
88.00	4109.0
90.90	396.0
92.10	2676.0
93.00	3637.0
94.10	9353.0
95.10	74184.0
96.10	5389.0
97.10	215.0
103.90	373.0
105.80	343.0
107.10	183.0
110.90	188.0
115.90	356.0
117.00	676.0
117.90	342.0
119.00	533.0
124.80	174.0
125.80	178.0
127.80	238.0
129.90	382.0
133.00	551.0
134.20	151.0
134.90	209.0
136.90	218.0
140.80	782.0
143.00	1262.0
145.10	355.0
146.00	165.0
154.90	240.0
156.90	314.0
171.90	581.0
173.00	482.0
174.00	69608.0
175.00	5251.0
176.00	67264.0
176.90	4770.0
177.90	193.0
191.00	423.0
192.90	472.0
207.00	446.0
248.90	206.0
264.90	385.0
281.10	3138.0
282.00	1083.0
283.00	459.0
284.10	175.0

Instrument :
MSVOA_D
ClientSampleId :
BFB111

m/z	Abundance
36.10	565.0
37.10	2443.0
38.10	2137.0
39.10	921.0
40.00	1025.0
44.00	635.0
45.10	767.0
47.00	525.0
48.00	258.0
49.10	2392.0
50.10	10358.0
51.00	3522.0
55.10	271.0
55.90	1391.0
57.10	1432.0
58.10	184.0
60.00	567.0
61.00	3297.0
62.10	3059.0
63.10	2495.0
64.20	194.0
65.10	581.0
66.90	313.0
68.00	7396.0
69.10	7524.0
70.00	523.0
72.00	510.0
73.00	3569.0
74.10	12650.0
75.10	34320.0
76.00	2540.0
77.00	550.0
78.10	527.0
79.00	3307.0
79.90	886.0
81.00	3386.0
82.00	591.0
83.20	152.0
86.20	169.0
87.00	3092.0
88.00	3272.0
91.00	417.0
92.10	2304.0
93.10	3258.0
94.10	9156.0
95.10	66872.0
96.10	4357.0
97.20	213.0
102.80	231.0
103.90	528.0
105.00	278.0
106.00	471.0
115.90	196.0
117.00	671.0
117.90	403.0
119.00	559.0
124.80	243.0
127.80	184.0
129.00	202.0
129.90	427.0
132.90	650.0
133.70	157.0
141.00	562.0
142.90	1369.0
145.00	233.0
147.00	212.0
154.90	280.0
157.10	195.0
160.70	153.0
171.90	488.0
173.10	371.0
174.00	65584.0
174.90	4318.0
176.00	61144.0
177.00	3448.0
178.00	285.0
190.90	436.0
193.10	458.0
206.80	388.0
249.00	219.0
265.20	332.0
281.10	4487.0
282.00	1182.0
283.20	640.0
284.00	171.0

Instrument :
MSVOA_D
ClientSampleId :
BFB111