

Data Path : Z:\VOASRV\HPCHEM1\MSVOA D\DATA\VD040119\
 Data File : VD061475.D
 Acq On : 1 Apr 2019 18:19
 Operator : VA/AP
 Sample : K1689-03
 Misc : 6.32g/5ml/MSVOA D/SOIL
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 NB-08-032919-A

Quant Time: Apr 02 02:07:53 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D032719S.M
 Quant Title : SW846 8260
 QLast Update : Thu Mar 28 09:22:37 2019
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	7.04	168	578789	50.00	ug/l	0.02
34) 1,4-Difluorobenzene	8.21	114	963647	50.00	ug/l	0.02
63) Chlorobenzene-d5	12.37	117	728824	50.00	ug/l	0.01
72) 1,4-Dichlorobenzene-d4	14.51	152	284309	50.00	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	7.46	65	235218	47.57	ug/l	0.02
Spiked Amount	50.000		Recovery	=	95.14%	
35) Dibromofluoromethane	6.92	113	375627	51.01	ug/l	0.02
Spiked Amount	50.000		Recovery	=	102.02%	
50) Toluene-d8	10.41	98	737020	41.73	ug/l	0.02
Spiked Amount	50.000		Recovery	=	83.46%	
62) 4-Bromofluorobenzene	13.55	95	280245	41.38	ug/l	0.00
Spiked Amount	50.000		Recovery	=	82.76%	
Target Compounds						
16) Acetone	3.22	43	41777	32.869	ug/l	95
20) Methylene Chloride	3.82	84	40863	3.972	ug/l	98

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA D\DATA\VD040119\
Data File : VD061475.D
Acq On : 1 Apr 2019 18:19
Operator : VA/AP
Sample : K1689-03
Misc : 6.32g/5ml/MSVOA D/SOIL
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
NB-08-032919-A

Quant Time: Apr 02 02:07:53 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_D\METHOD\82D032719S.M
Quant Title : SW846 8260
QLast Update : Thu Mar 28 09:22:37 2019
Response via : Initial Calibration

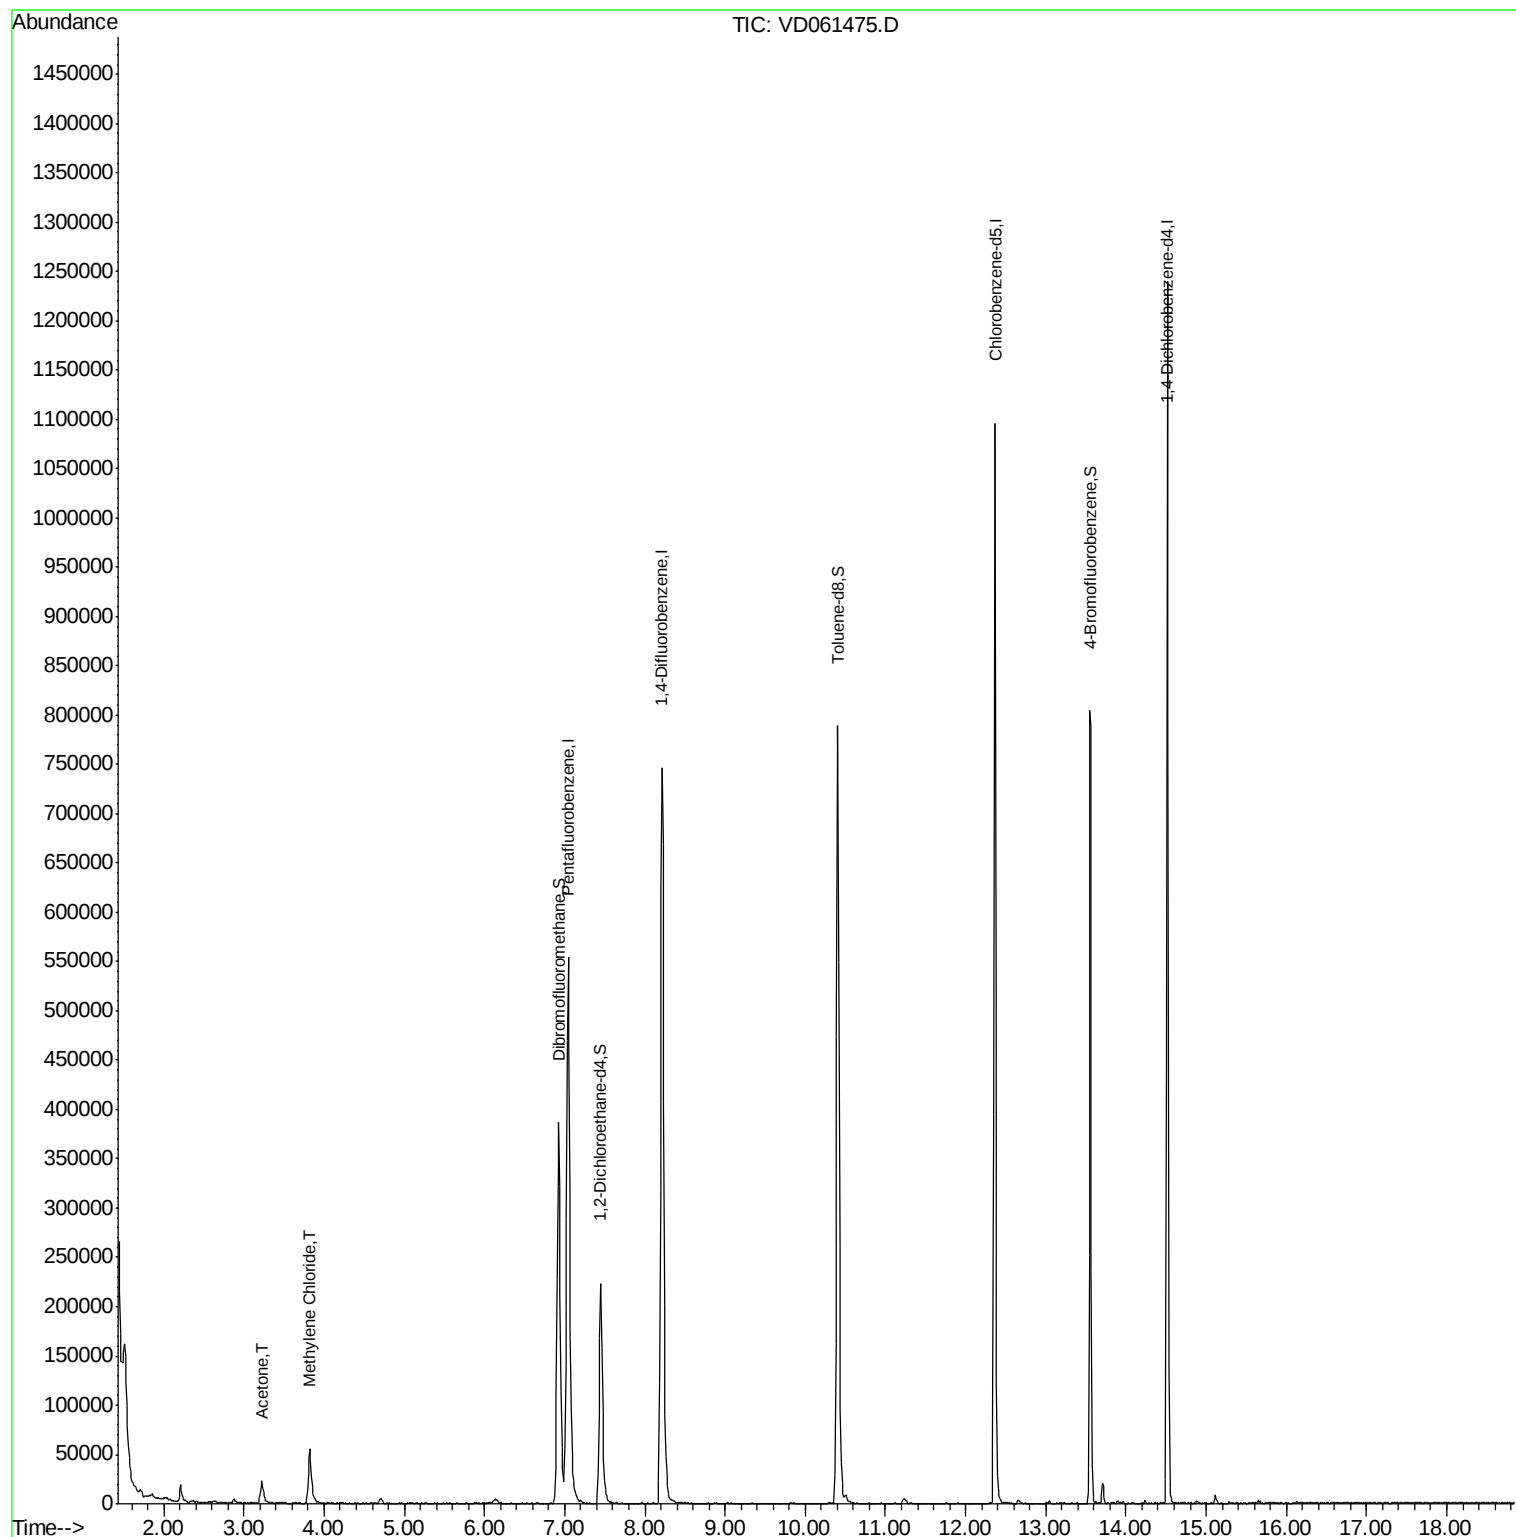



#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 7.04 min Scan# 571

Delta R.T. 0.02 min

Lab File: VD061475.D

Acq: 1 Apr 2019 18:19

Instrument :

MSVOA_D

ClientSampleId :


NB-08-032919-A

Tot Ion:168 Resp: 578789

Ion Ratio Lower Upper

168 100

99 57.3 43.1 64.7

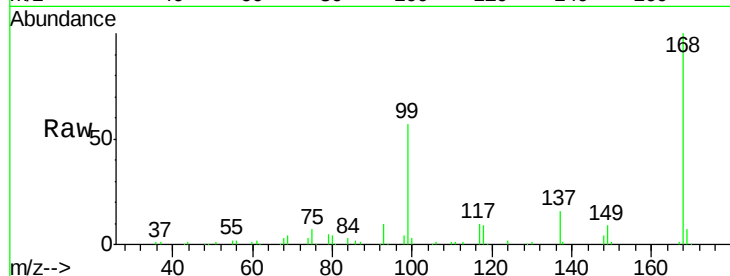

Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.95 (98.65 to 99.65): VDC

7.04

200000

150000



100000

50000

0

6.90 7.00 7.10 7.20

Time-->

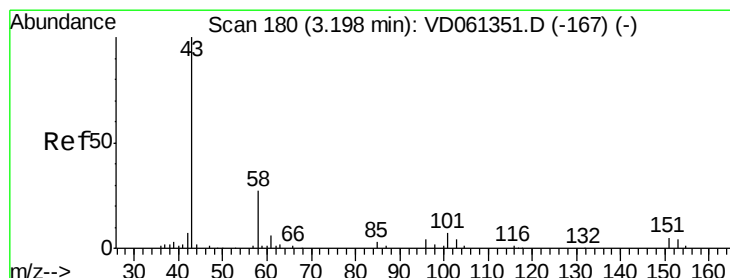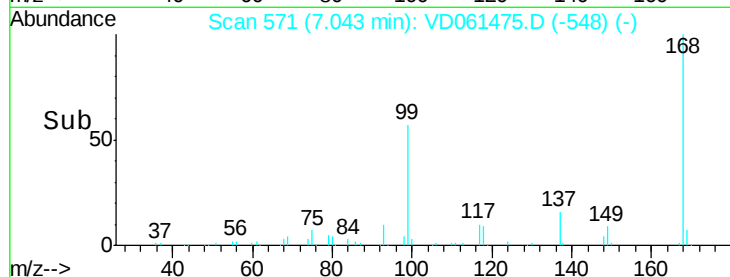

#16

Acetone

Concen: 32.869 ug/l

RT: 3.22 min Scan# 183

Delta R.T. 0.02 min

Lab File: VD061475.D


Acq: 1 Apr 2019 18:19

Tgt Ion: 43 Resp: 41777

Ion Ratio Lower Upper

43 100

58 24.4 21.5 32.3

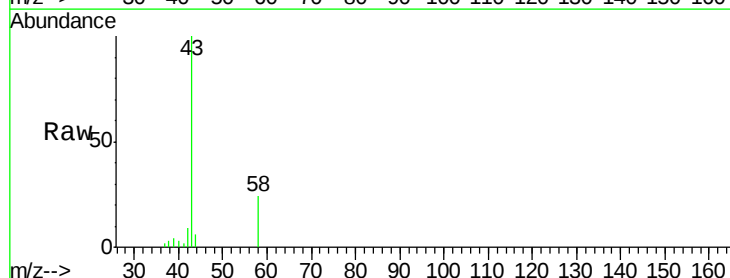

Abundance Ion 42.95 (42.65 to 43.65): VDC

Ion 57.95 (57.65 to 58.65): VDC

3.22

15000


10000

5000

0

3.10 3.20 3.30 3.40

Time-->

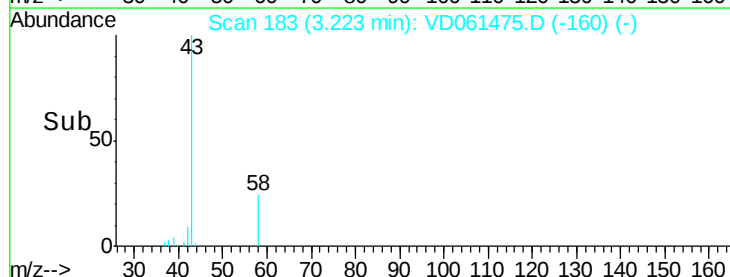



#20

Methylene Chloride

Concen: 3.972 ug/l

RT: 3.82 min Scan# 244

Delta R.T. 0.02 min

Lab File: VD061475.D

Acq: 1 Apr 2019 18:19

Instrument :

MSVOA_D

ClientSampleId :

NB-08-032919-A

Tot Ion: 84 Resp: 40863


Ion Ratio Lower Upper

84 100

49 116.0 91.8 137.8

51 40.3 29.8 44.8

86 64.5 51.8 77.6



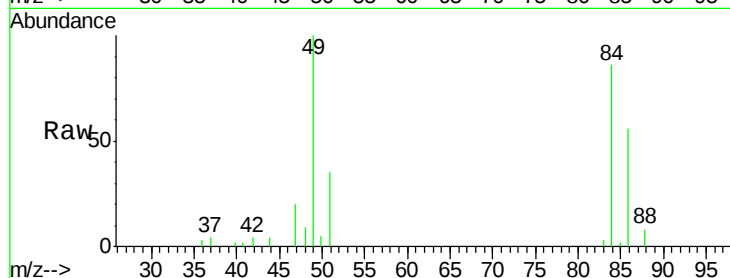


Abundance Ion 83.95 (83.65 to 84.65): VDC

Ion 48.90 (48.60 to 49.60): VDC

Ion 50.90 (50.60 to 51.60): VDC

Ion 85.90 (85.60 to 86.60): VDC

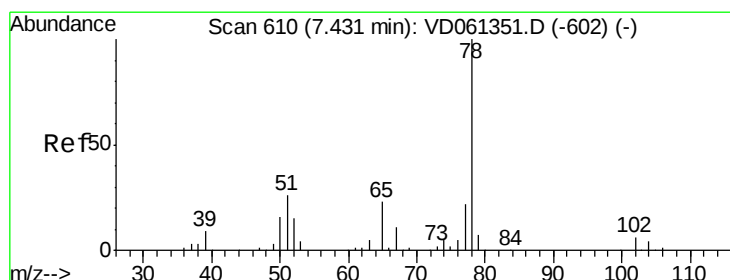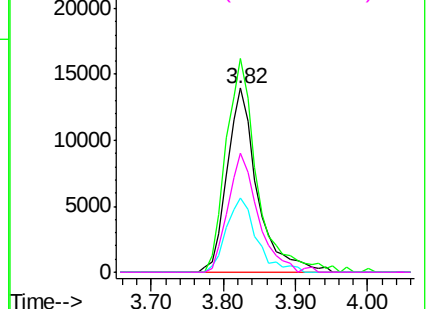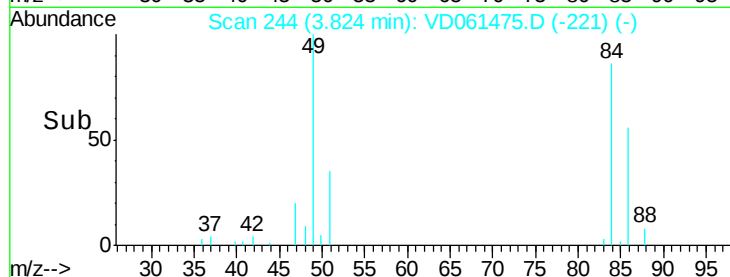

#33

1,2-Dichloroethane-d4

Concen: N.D. ug/l

RT: 7.46 min Scan# 613

Delta R.T. 0.02 min

Lab File: VD061475.D


Acq: 1 Apr 2019 18:19

Tgt Ion: 65 Resp: 235218

Ion Ratio Lower Upper



65 100


67 49.1 0.0 99.8

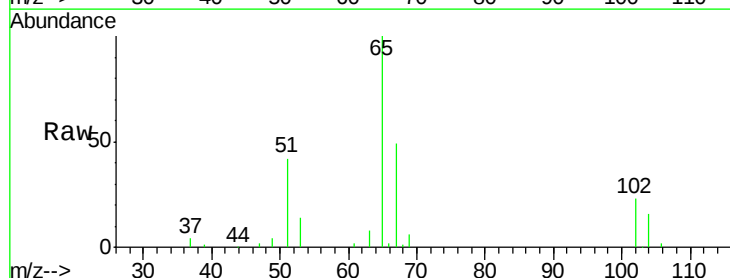

Abundance Ion 64.95 (64.65 to 65.65): VDC

Ion 66.90 (66.60 to 67.60): VDC

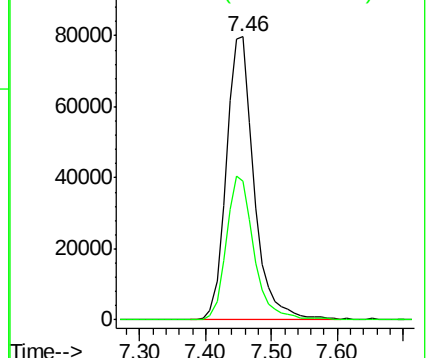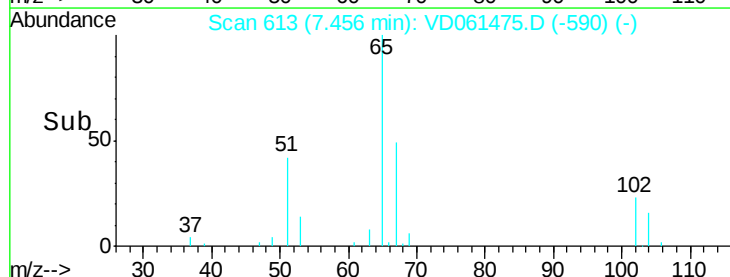

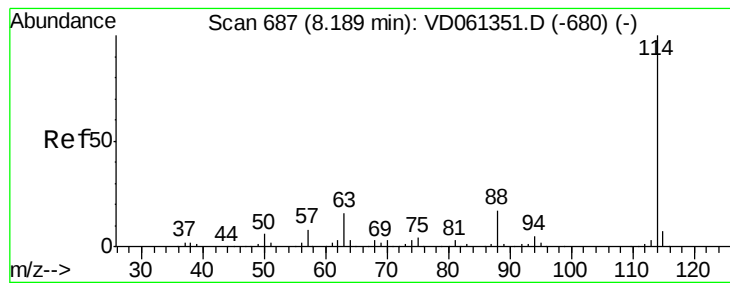

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.21 min Scan# 690

Delta R.T. 0.02 min

Lab File: VD061475.D

Acq: 1 Apr 2019 18:19

Instrument :

MSVOA_D

ClientSampleId :

NB-08-032919-A


Tot Ion:114 Resp: 963647

Ion Ratio Lower Upper

114 100

63 16.2 0.0 31.6




88 15.9 0.0 33.4

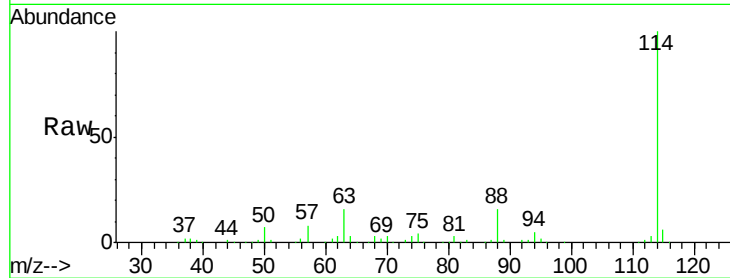

Abundance Ion 114.00 (113.70 to 114.70): V

Ion 62.95 (62.65 to 63.65): V

Ion 87.90 (87.60 to 88.60): V

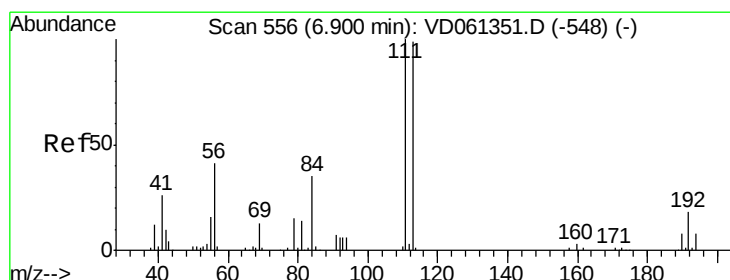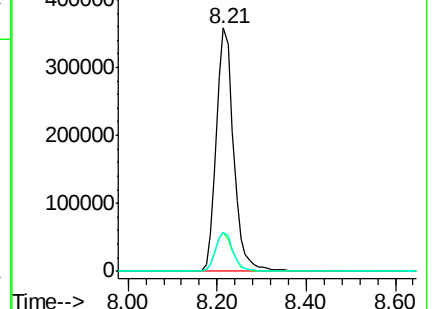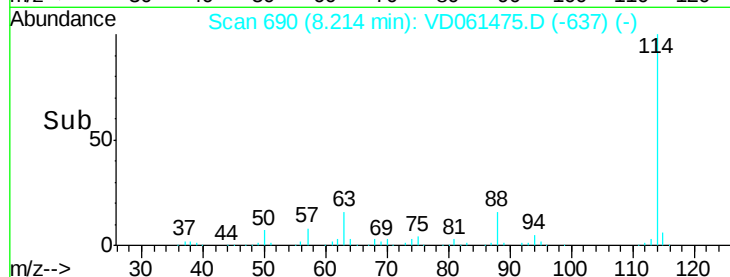

#35

Dibromofluoromethane

Concen: 50.000 ug/l

RT: 6.92 min Scan# 559

Delta R.T. 0.02 min

Lab File: VD061475.D

Acq: 1 Apr 2019 18:19


Tgt Ion:113 Resp: 375627

Ion Ratio Lower Upper

113 100

111 96.5 81.0 121.6



192 16.6 14.4 21.6

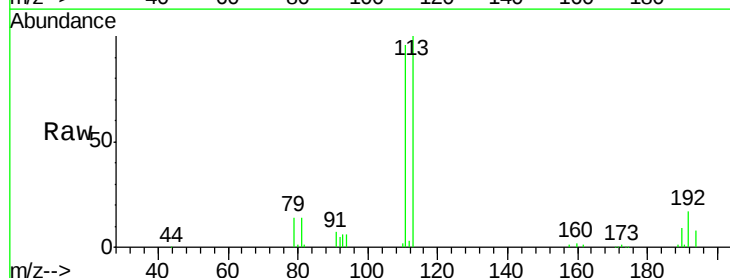


Abundance Ion 112.90 (112.60 to 113.60): V

Ion 110.90 (110.60 to 111.60): V

Ion 191.80 (191.50 to 192.50): V

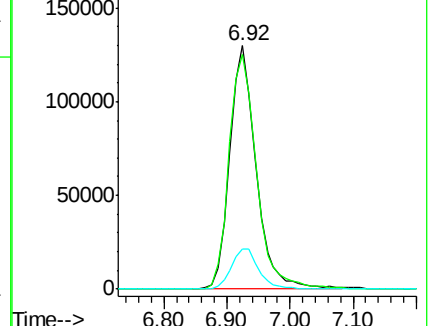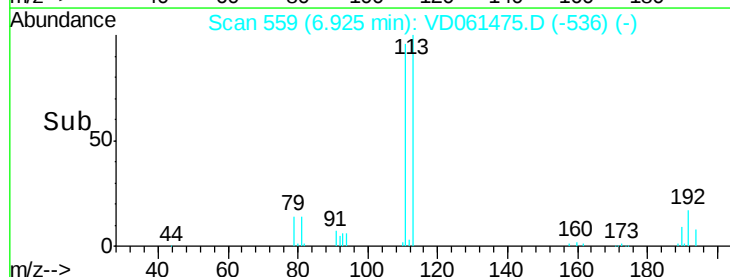

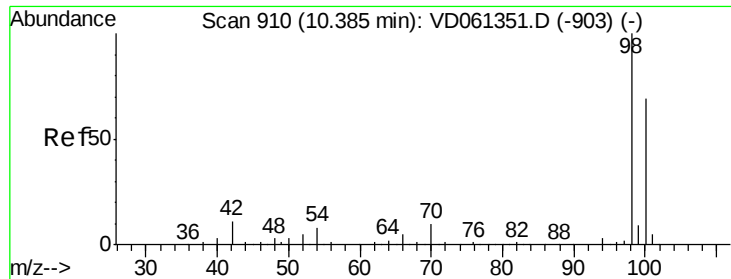

#50

Toluene-d8

Concen: N.D. ug/l

RT: 10.41 min Scan# 913

Delta R.T. 0.02 min

Lab File: VD061475.D

Acq: 1 Apr 2019 18:19

Instrument :

MSVOA_D

ClientSampleId :


NB-08-032919-A

Tot Ion: 98 Resp: 737020

Ion Ratio Lower Upper

98 100

100 69.5 56.2 84.2

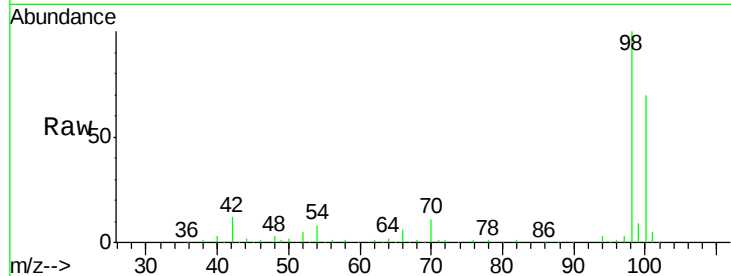

Abundance Ion 98.05 (97.75 to 98.75): VD061351.D (-903) (-)

Ion 100.05 (99.75 to 100.75): VD061351.D (-903) (-)

10.41



300000

200000

100000

0

Time-->

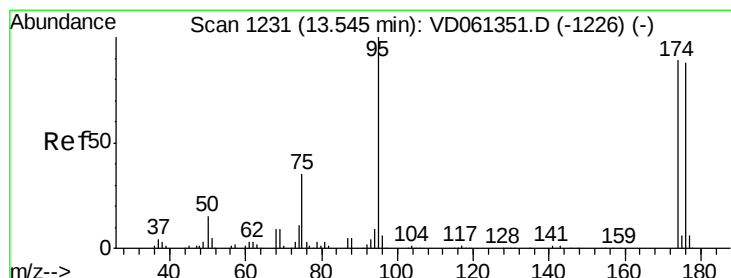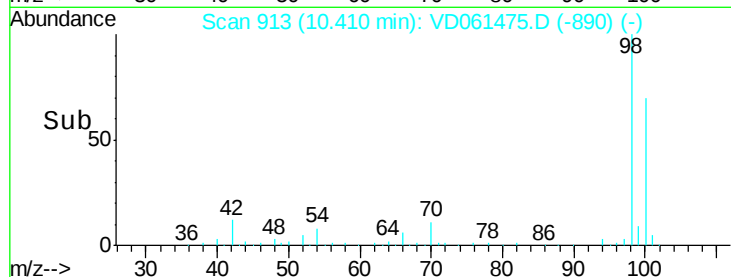

#62

4-Bromofluorobenzene

Concen: N.D. ug/l

RT: 13.55 min Scan# 1232

Delta R.T. 0.01 min

Lab File: VD061475.D

Acq: 1 Apr 2019 18:19


Tgt Ion: 95 Resp: 280245

Ion Ratio Lower Upper

95 100

174 74.8 0.0 178.0

176 71.0 0.0 175.0

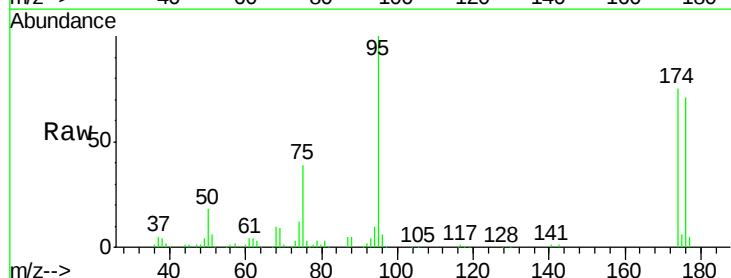

Abundance Ion 95.00 (94.70 to 95.70): VD061351.D (-1226) (-)

Ion 173.90 (173.60 to 174.60): VD061351.D (-1226) (-)

Ion 175.90 (175.60 to 176.60): VD061351.D (-1226) (-)

250000

200000


150000


100000

50000

0

Time-->

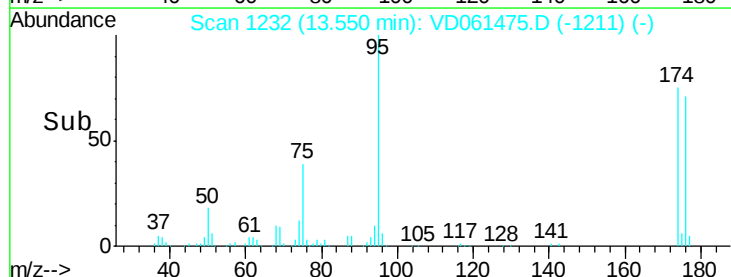


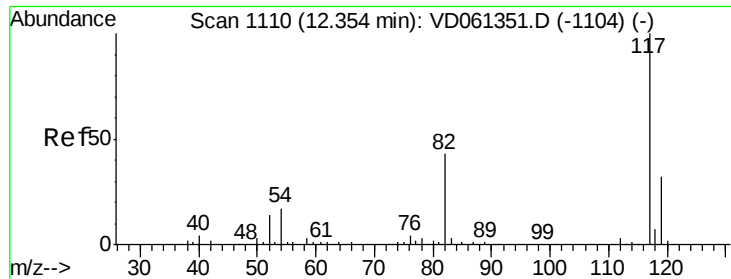




#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 12.37 min Scan# 1112
Delta R.T. 0.01 min
Lab File: VD061475.D
Acq: 1 Apr 2019 18:19

Instrument :
MSVOA_D
ClientSampleId :
NB-08-032919-A

Tot Ion:117 Resp: 728824
Ion Ratio Lower Upper
117 100
82 44.8 34.4 51.6
119 33.2 25.8 38.6

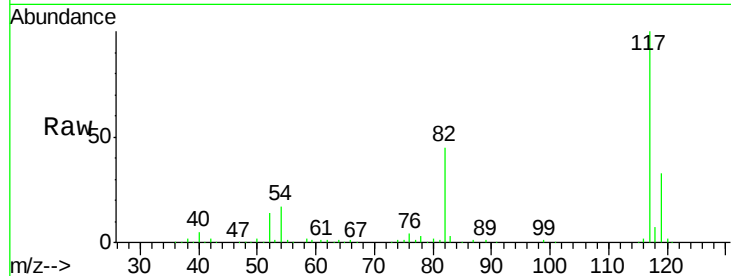


Abundance Ion 116.95 (116.65 to 117.65): V
Ion 82.05 (81.75 to 82.75): V
Ion 118.95 (118.65 to 119.65): V

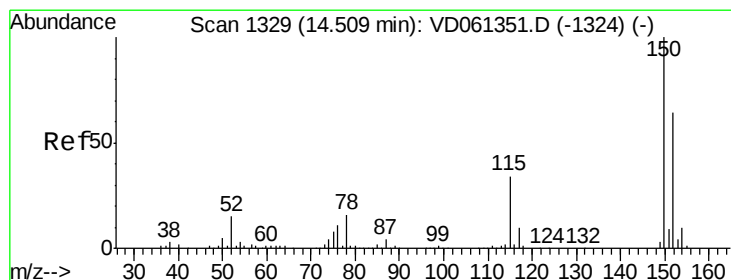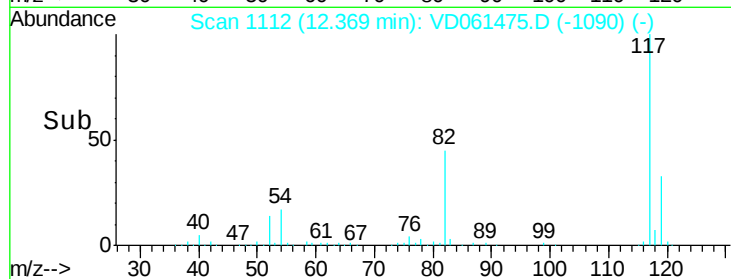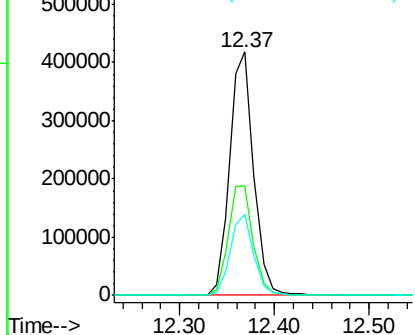

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 14.51 min Scan# 1330
Delta R.T. 0.01 min
Lab File: VD061475.D
Acq: 1 Apr 2019 18:19

Tgt Ion:152 Resp: 284309
Ion Ratio Lower Upper
152 100
115 60.1 26.9 80.6
150 158.0 0.0 318.0

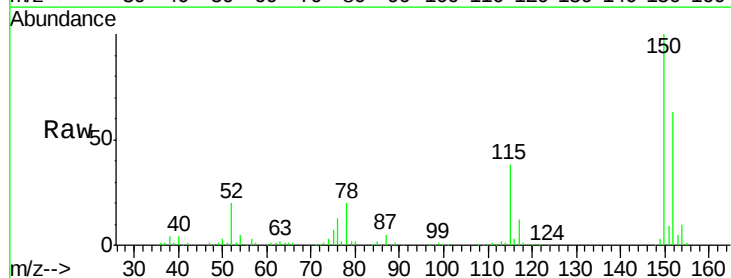

Abundance Ion 151.90 (151.60 to 152.60): V
Ion 115.00 (114.70 to 115.70): V
Ion 149.90 (149.60 to 150.60): V

