


Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD040121\
 Data File : VD068748.D
 Acq On : 01 Apr 2021 10:01
 Operator : VA/SY
 Sample : BFB
 Misc : 5.00G/5.00ml/MSVOA_D/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D031921S.M
 Title : SW846 8260
 Last Update : Sat Mar 20 02:00:55 2021

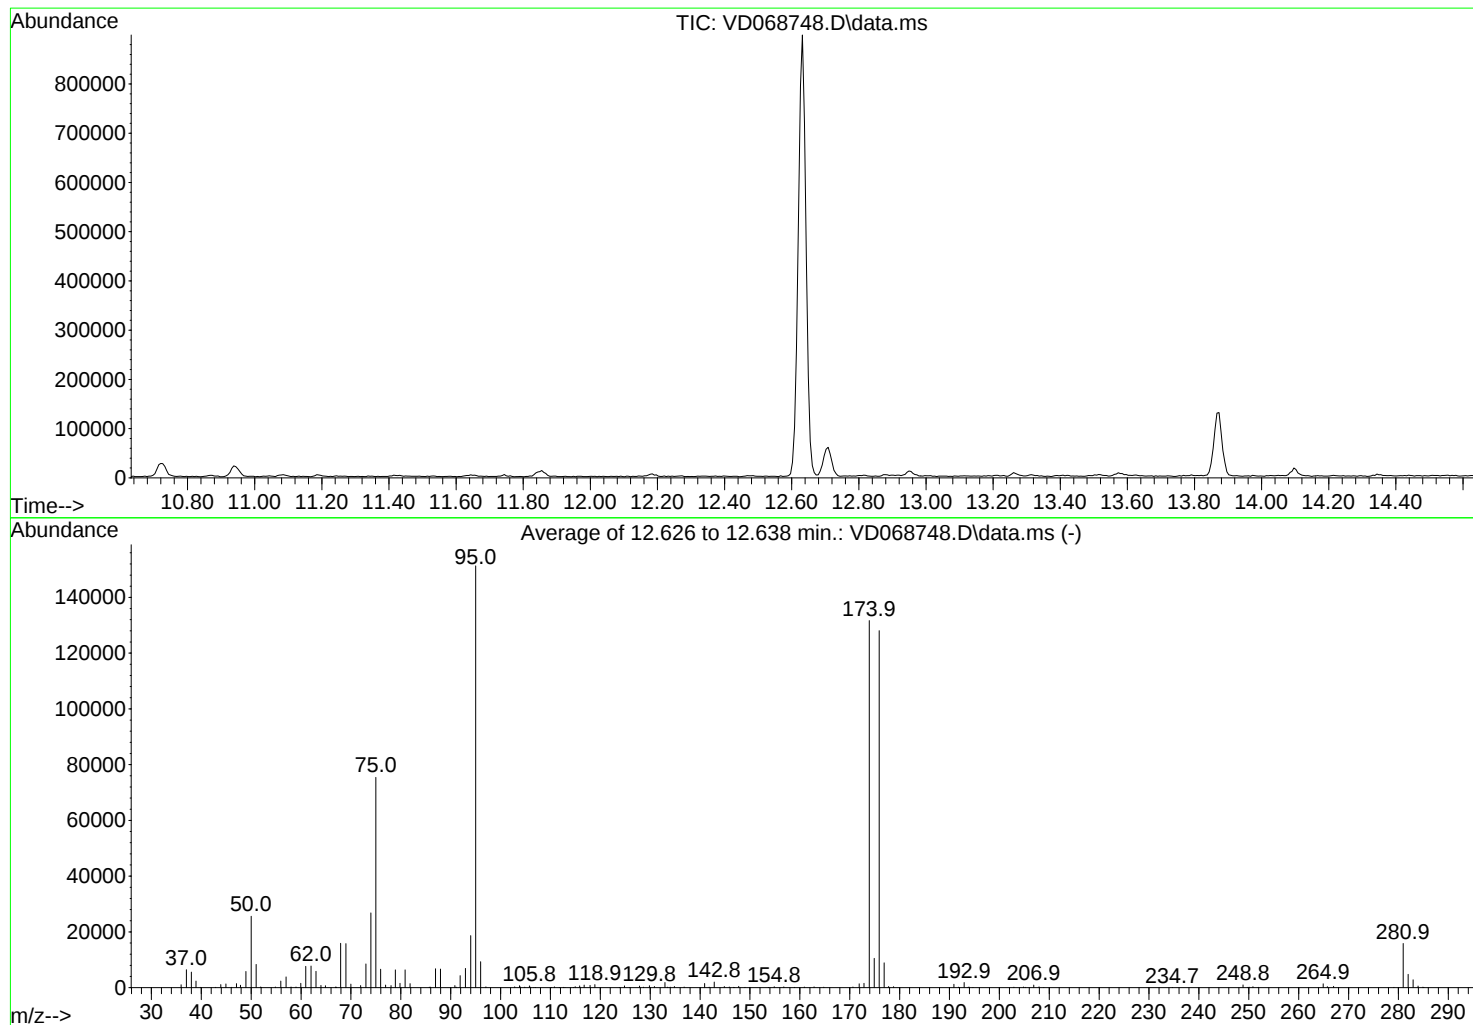

AutoFind: Scans 1820, 1821, 1822; Background Corrected with Scan 1811

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.9	25619	PASS
75	95	30	60	49.8	75427	PASS
95	95	100	100	100.0	151317	PASS
96	95	5	9	6.2	9320	PASS
173	174	0.00	2	1.2	1541	PASS
174	95	50	100	87.0	131685	PASS
175	174	5	9	8.0	10486	PASS
176	174	95	101	97.3	128083	PASS
177	176	5	9	6.9	8892	PASS