

Data Path : Z:\VOASRV\HPCHEM1\MSVOA D\DATA\VD040319\
 Data File : VD061570.D
 Acq On : 3 Apr 2019 22:02
 Operator : VA/AP
 Sample : K2213-15
 Misc : 5.78g/5ml/MSVOA D/SOIL
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :

Quant Time: Apr 04 01:52:18 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D032719S.M
 Quant Title : SW846 8260
 QLast Update : Thu Mar 28 09:22:37 2019
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	7.04	168	507457	50.00	ug/l	0.02
34) 1,4-Difluorobenzene	8.21	114	863869	50.00	ug/l	0.02
63) Chlorobenzene-d5	12.36	117	666180	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	14.52	152	274599	50.00	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	7.45	65	211858	48.87	ug/l	0.02
Spiked Amount 50.000			Recovery	=	97.74%	
35) Dibromofluoromethane	6.92	113	304184	46.08	ug/l	0.02
Spiked Amount 50.000			Recovery	=	92.16%	
50) Toluene-d8	10.40	98	679753	42.93	ug/l	0.02
Spiked Amount 50.000			Recovery	=	85.86%	
62) 4-Bromofluorobenzene	13.55	95	269863	44.45	ug/l	0.00
Spiked Amount 50.000			Recovery	=	88.90%	
Target Compounds						
					Qvalue	
16) Acetone	3.22	43	25009	22.443	ug/l #	84
20) Methylene Chloride	3.82	84	114429	17.066	ug/l	97
31) Cyclohexane	7.04	56	8993	1.204	ug/l #	1
36) 1,1-Dichloropropene	7.04	75	37833	5.018	ug/l #	45
38) Carbon Tetrachloride	7.05	117	48249	5.569	ug/l #	13
81) trans-1,4-Dichloro-2-buten	13.54	75	103703	85.745	ug/l #	18


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA D\DATA\VD040319\
Data File : VD061570.D
Acq On : 3 Apr 2019 22:02
Operator : VA/AP
Sample : K2213-15
Misc : 5.78g/5ml/MSVOA D/SOIL
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :

Quant Time: Apr 04 01:52:18 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_D\METHOD\82D032719S.M
Quant Title : SW846 8260
QLast Update : Thu Mar 28 09:22:37 2019
Response via : Initial Calibration

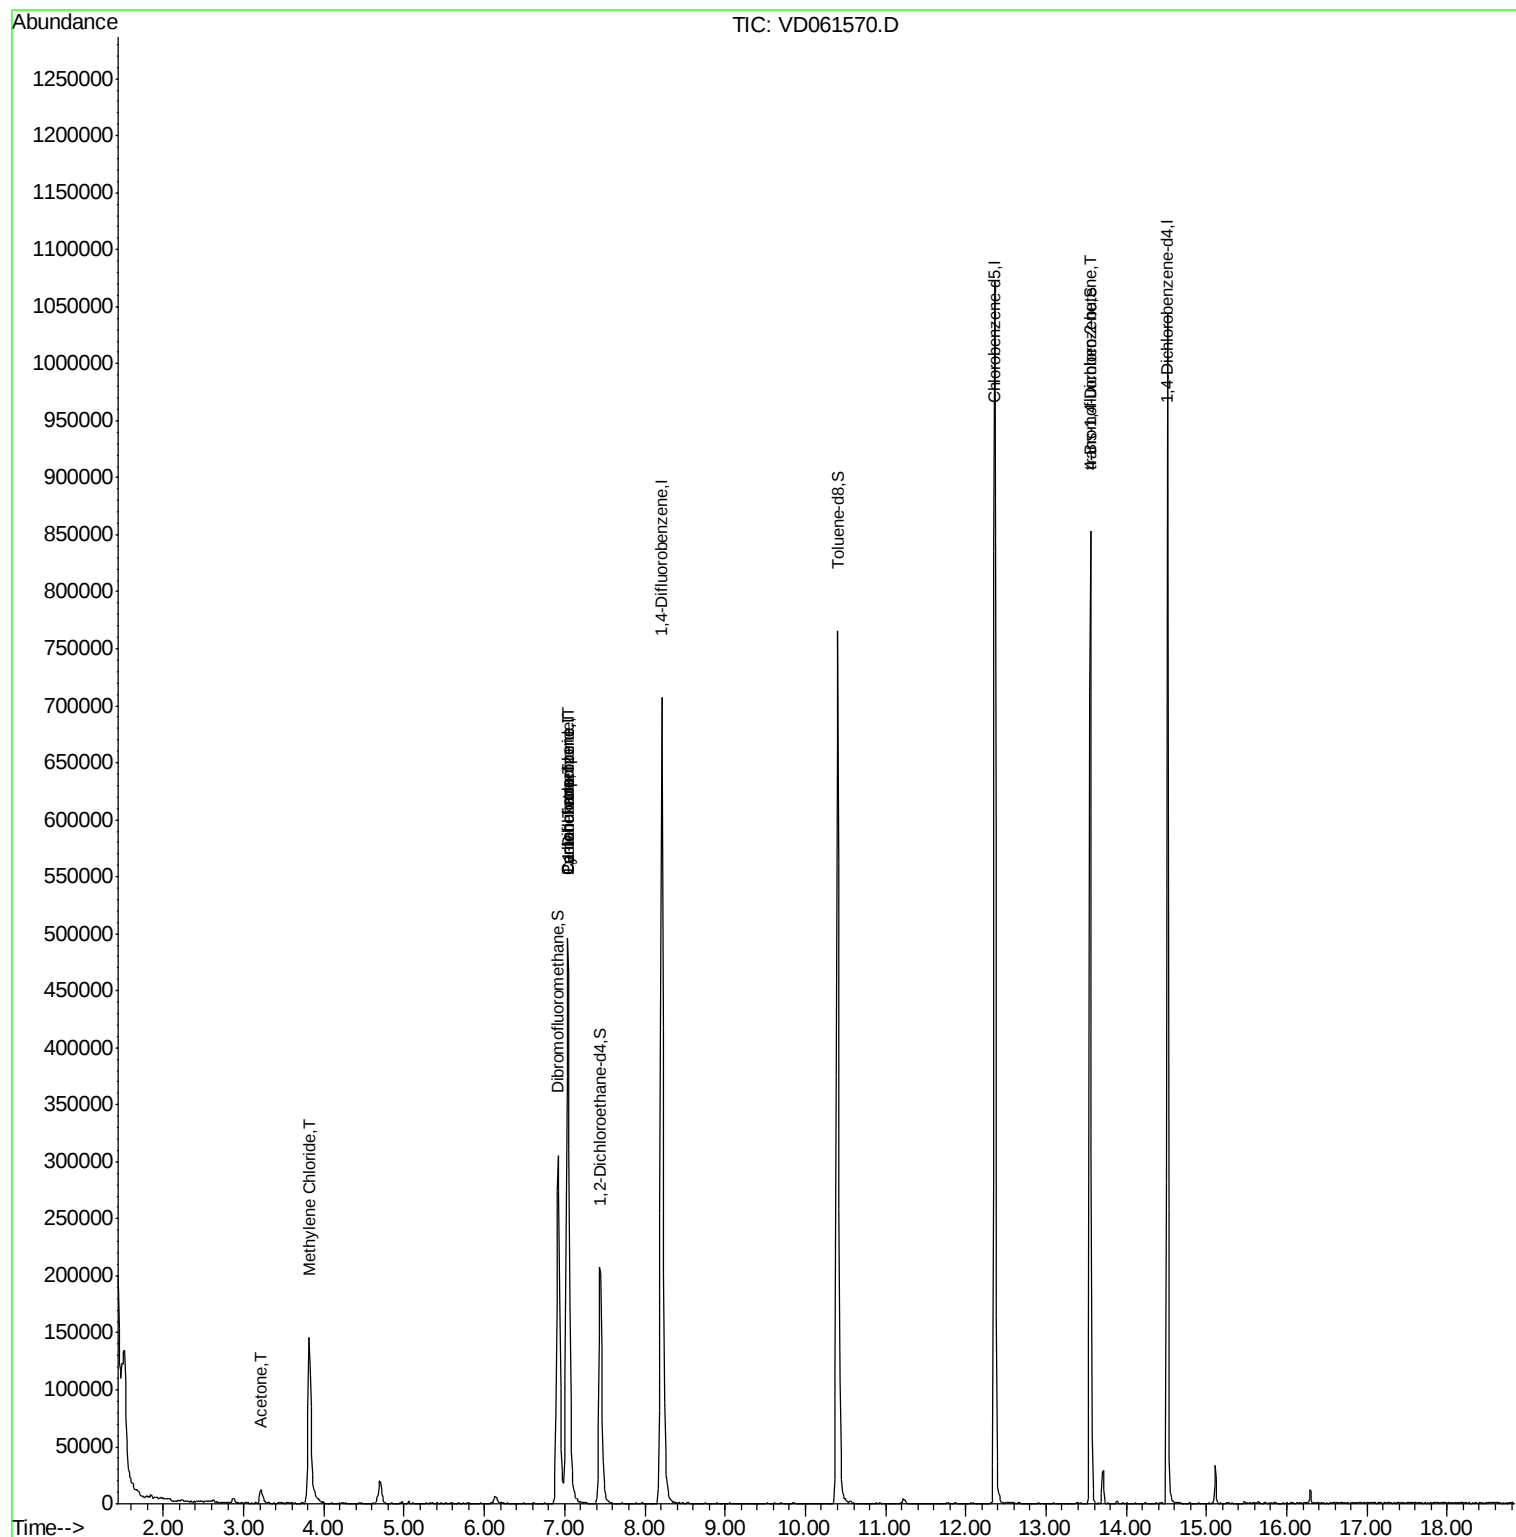

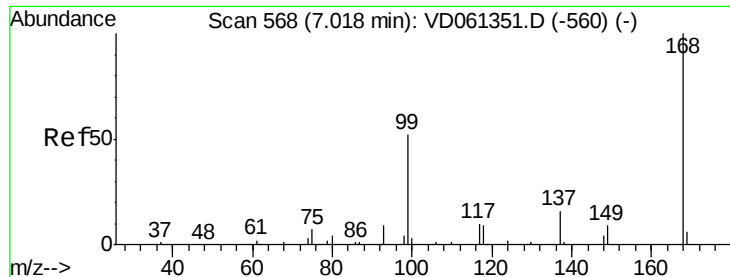

#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 7.04 min Scan# 570

Delta R.T. 0.02 min

Lab File: VD061570.D

Acq: 3 Apr 2019 22:02


Instrument :
MSVOA_D
ClientSampled :

Tot Ion:168 Resp: 507457

Ion Ratio Lower Upper

168 100

99 59.5 43.1 64.7

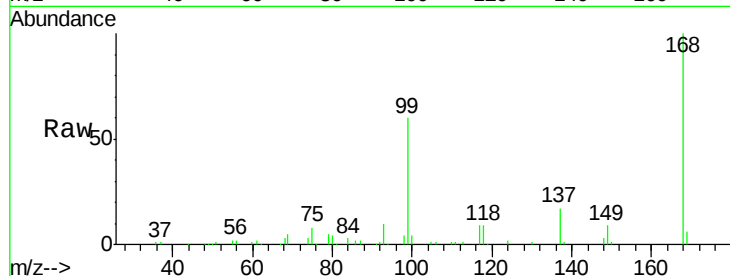

Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.95 (98.65 to 99.65): VDC

7.04



150000

100000

50000

0

Time--> 6.90 7.00 7.10 7.20

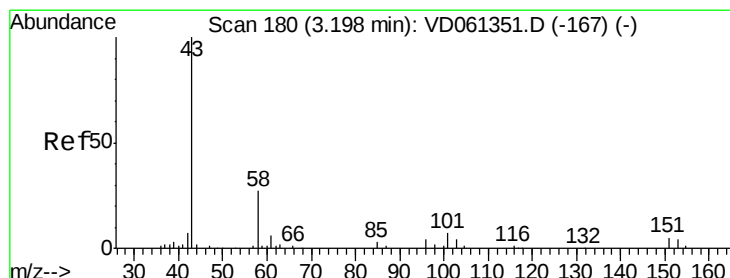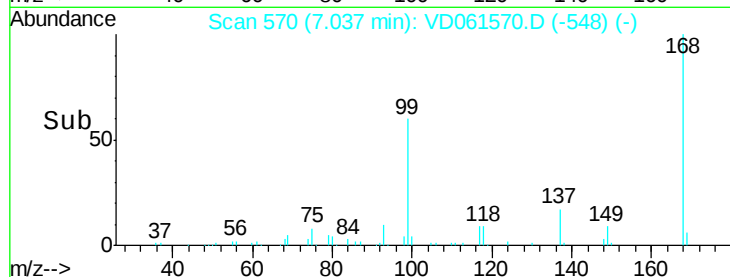

#16

Acetone

Concen: 22.443 ug/l

RT: 3.22 min Scan# 182

Delta R.T. 0.02 min

Lab File: VD061570.D


Acq: 3 Apr 2019 22:02

Tgt Ion: 43 Resp: 25009

Ion Ratio Lower Upper

43 100

58 18.6 21.5 32.3#

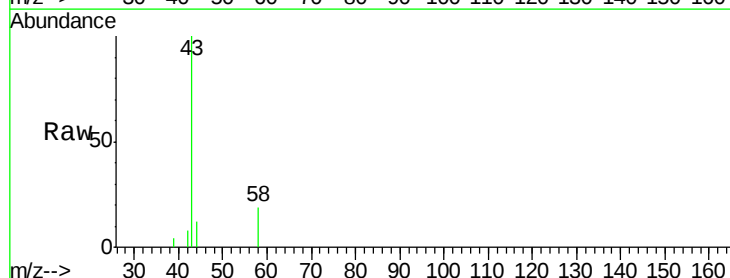

Abundance Ion 42.95 (42.65 to 43.65): VDC

Ion 57.95 (57.65 to 58.65): VDC

3.22

10000

8000


6000


4000

2000

0

Time--> 3.10 3.20 3.30 3.40

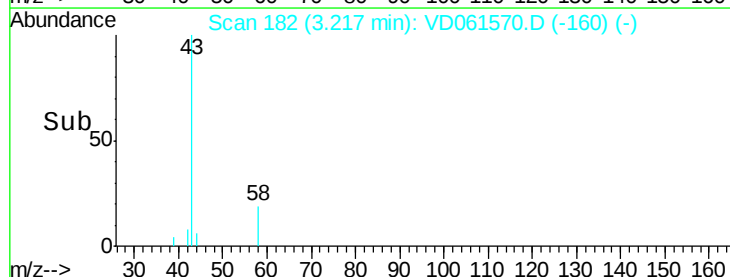


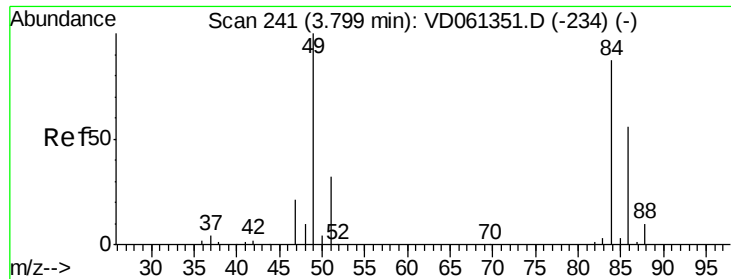




#20
Methylene Chloride
Concen: 17.066 ug/l
RT: 3.82 min Scan# 243
Delta R.T. 0.02 min
Lab File: VD061570.D
Acq: 3 Apr 2019 22:02

Instrument :
MSVOA_D
ClientSampleId :

Tot Ion: 84 Resp: 114429
Ion Ratio Lower Upper
84 100
49 111.3 91.8 137.8
51 35.3 29.8 44.8
86 67.3 51.8 77.6

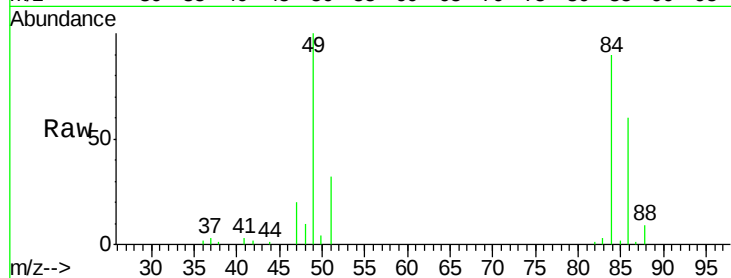


Abundance Ion 83.95 (83.65 to 84.65): VDC
Ion 48.90 (48.60 to 49.60): VDC
Ion 50.90 (50.60 to 51.60): VDC
Ion 85.90 (85.60 to 86.60): VDC

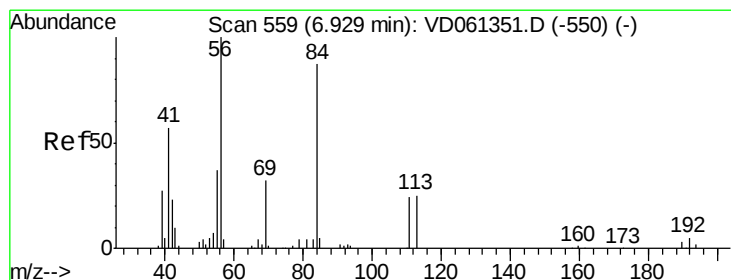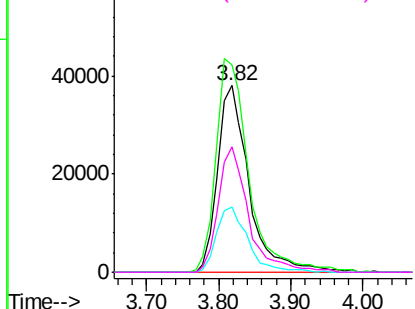
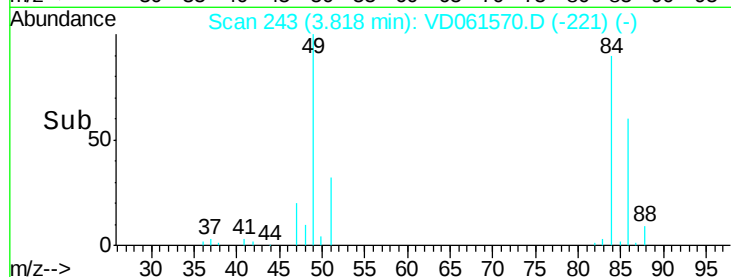



#31
Cyclohexane
Concen: 1.204 ug/l
RT: 7.04 min Scan# 570
Delta R.T. 0.11 min
Lab File: VD061570.D
Acq: 3 Apr 2019 22:02

Tgt Ion: 56 Resp: 8993
Ion Ratio Lower Upper
56 100
69 262.5 25.7 38.5#
84 153.1 70.6 105.8#

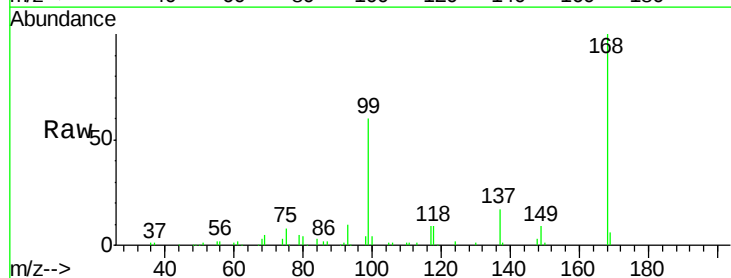

Abundance Ion 55.95 (55.65 to 56.65): VDC
Ion 69.00 (68.70 to 69.70): VDC
Ion 84.05 (83.75 to 84.75): VDC

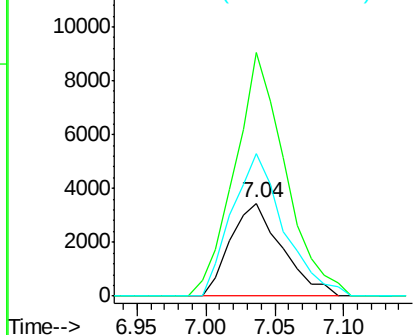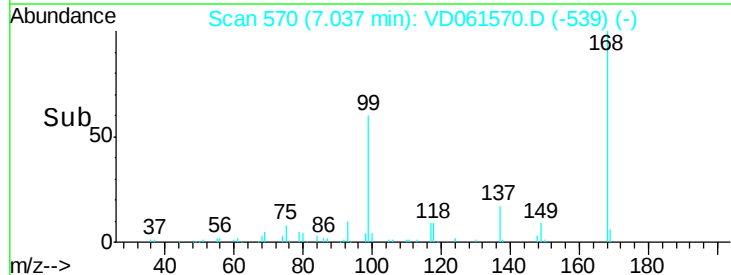

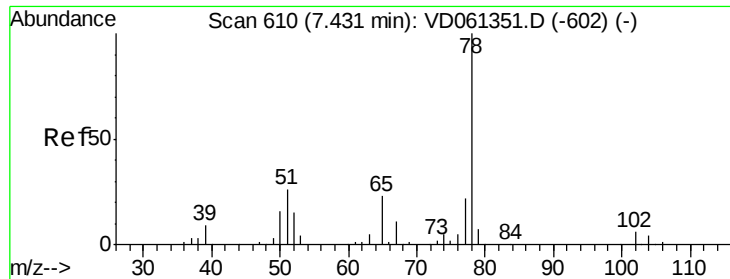

#33

1,2-Dichloroethane-d4

Concen: N.D. ug/l

RT: 7.45 min Scan# 612

Delta R.T. 0.02 min

Lab File: VD061570.D

Acq: 3 Apr 2019 22:02


Instrument :
MSVOA_D
ClientSampleId :

Tot Ion: 65 Resp: 211858

Ion Ratio Lower Upper




65 100

67 48.9 0.0 99.8

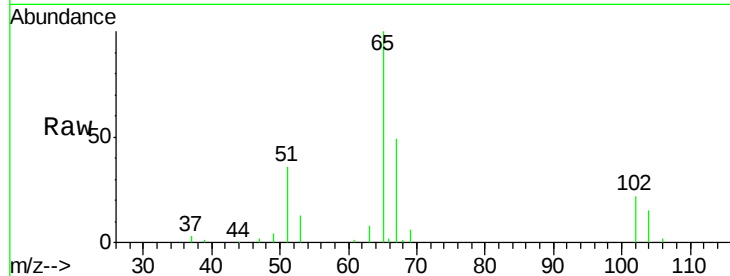

Abundance Ion 64.95 (64.65 to 65.65): VDC

Ion 66.90 (66.60 to 67.60): VDC

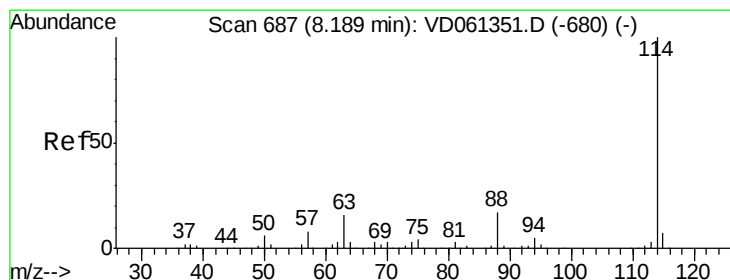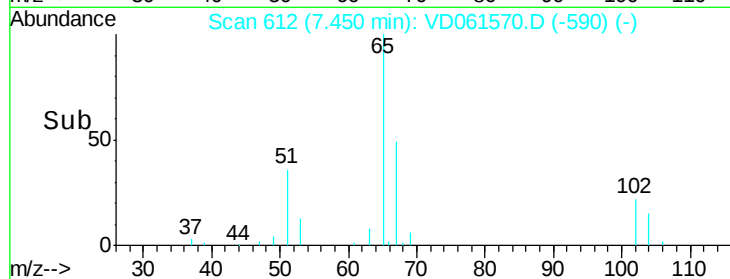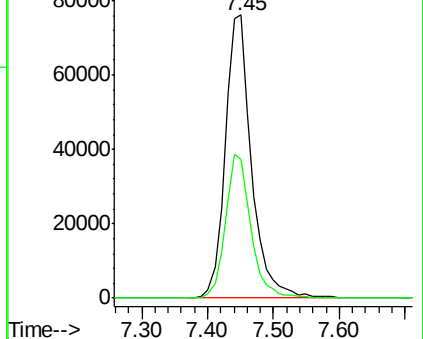

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.21 min Scan# 689

Delta R.T. 0.02 min

Lab File: VD061570.D

Acq: 3 Apr 2019 22:02


Tgt Ion: 114 Resp: 863869

Ion Ratio Lower Upper

114 100

63 17.1 0.0 31.6



88 16.7 0.0 33.4

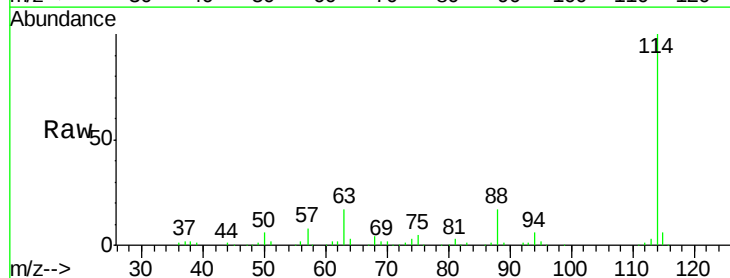


Abundance Ion 114.00 (113.70 to 114.70): V

Ion 62.95 (62.65 to 63.65): VDC

Ion 87.90 (87.60 to 88.60): VDC

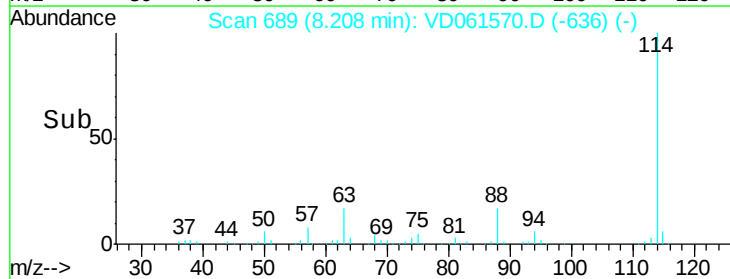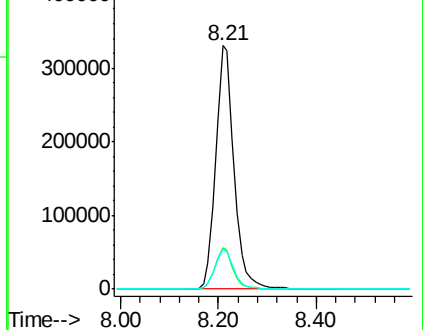

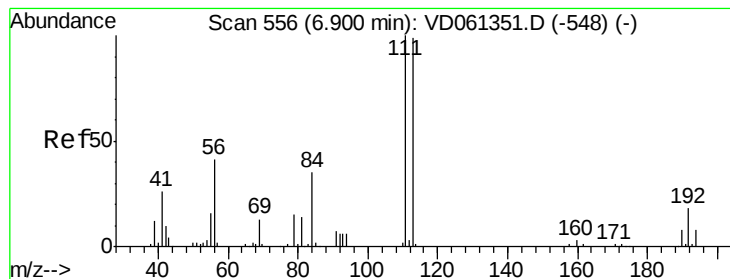

#35

Dibromofluoromethane

Concen: 50.000 ug/l

RT: 6.92 min Scan# 558

Delta R.T. 0.02 min

Lab File: VD061570.D

Acq: 3 Apr 2019 22:02

Instrument :

MSVOA_D

ClientSampled :


Tot Ion:113 Resp: 304184

Ion Ratio Lower Upper

113 100

111 97.4 81.0 121.6




192 15.9 14.4 21.6

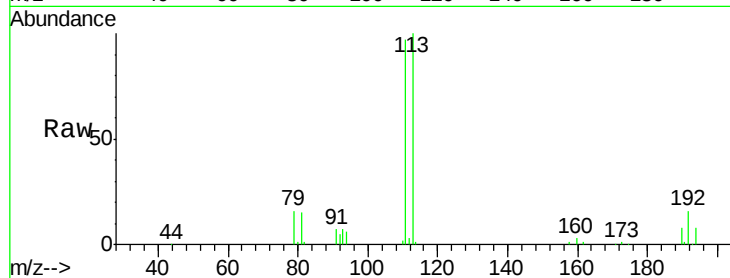

Abundance Ion 112.90 (112.60 to 113.60): V

Ion 110.90 (110.60 to 111.60): V

Ion 191.80 (191.50 to 192.50): V

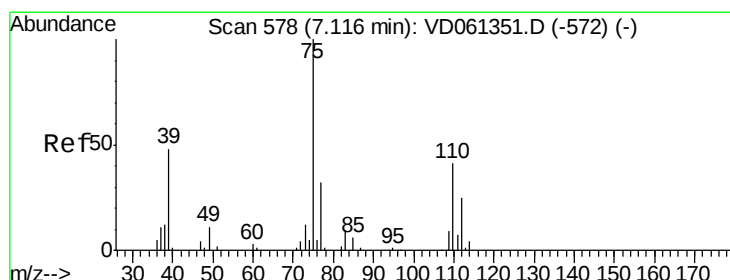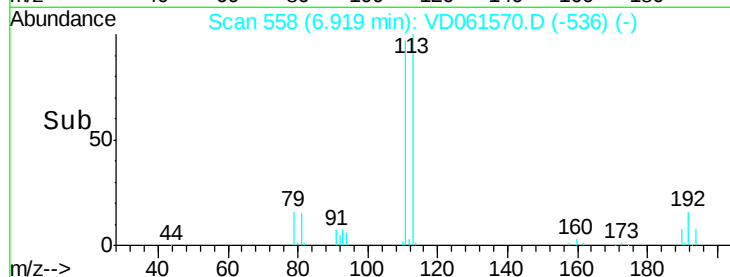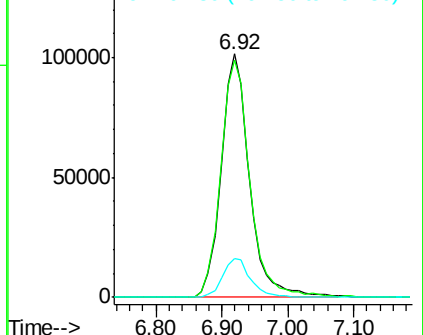

#36

1,1-Dichloropropene

Concen: 5.018 ug/l

RT: 7.04 min Scan# 570

Delta R.T. -0.08 min

Lab File: VD061570.D

Acq: 3 Apr 2019 22:02


Tgt Ion: 75 Resp: 37833

Ion Ratio Lower Upper

75 100

110 7.0 20.4 61.3#



77 0.0 24.9 37.3#

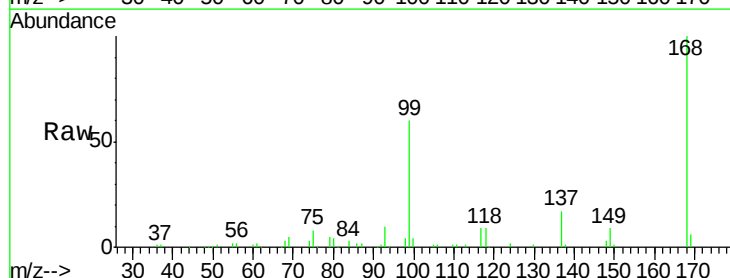


Abundance Ion 75.00 (74.70 to 75.70): V

Ion 109.90 (109.60 to 110.60): V

Ion 76.95 (76.65 to 77.65): V

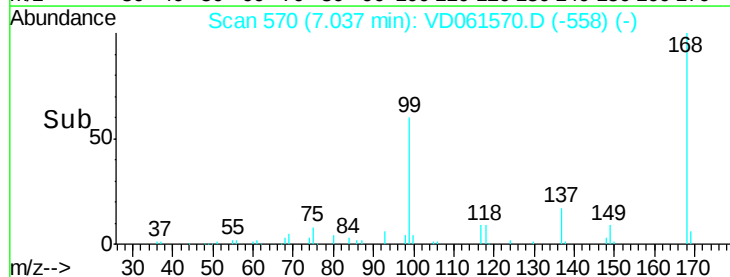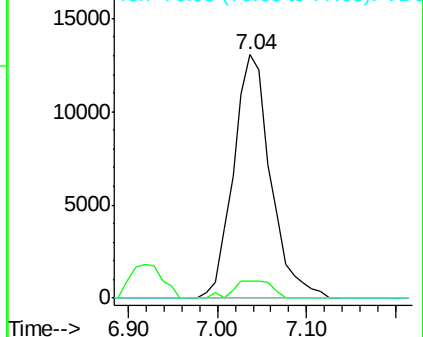


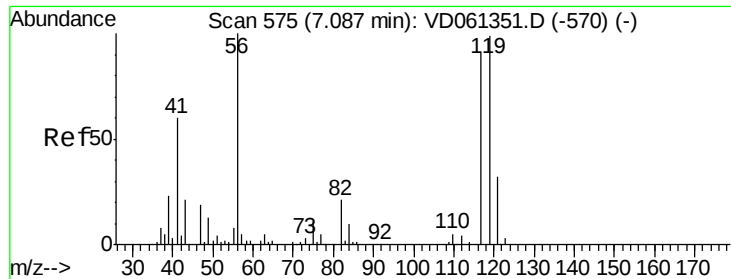




#38
Carbon Tetrachloride
Concen: 5.569 ug/l
RT: 7.05 min Scan# 571
Delta R.T. -0.04 min
Lab File: VD061570.D
Acq: 3 Apr 2019 22:02

Instrument :
MSVOA_D
ClientSampleId :

Tot Ion:117 Resp: 48249
Ion Ratio Lower Upper
117 100
119 3.4 80.1 120.1#
121 0.0 25.6 38.4#

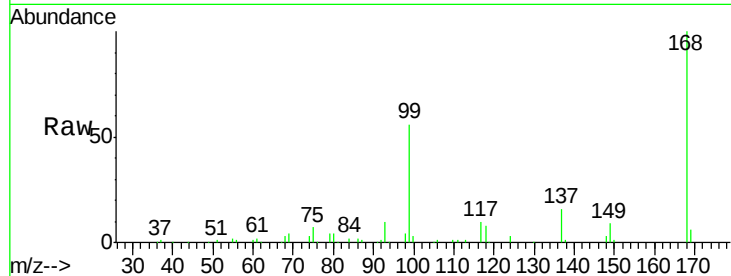


Abundance Ion 116.85 (116.55 to 117.55): V
Ion 118.85 (118.55 to 119.55): V
Ion 120.85 (120.55 to 121.55): V

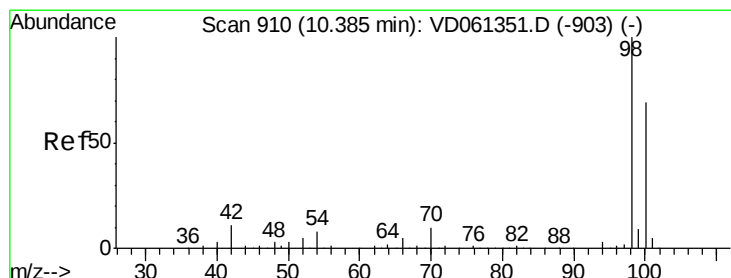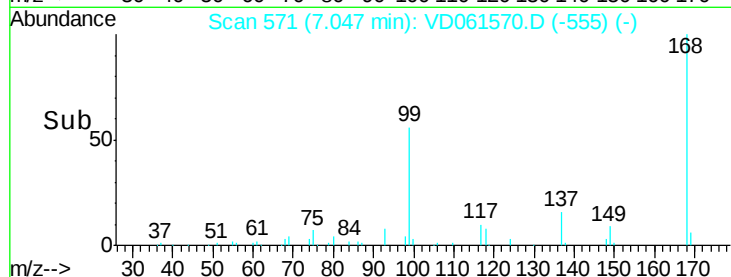
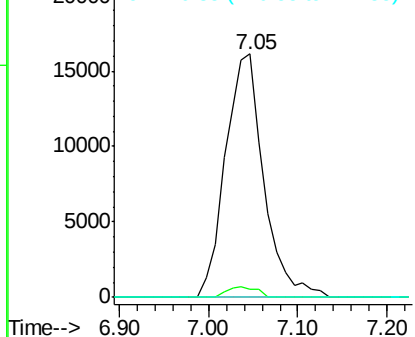



#50
Toluene-d8
Concen: N.D. ug/l
RT: 10.40 min Scan# 912
Delta R.T. 0.02 min
Lab File: VD061570.D
Acq: 3 Apr 2019 22:02

Tgt Ion: 98 Resp: 679753
Ion Ratio Lower Upper
98 100
100 68.6 56.2 84.2

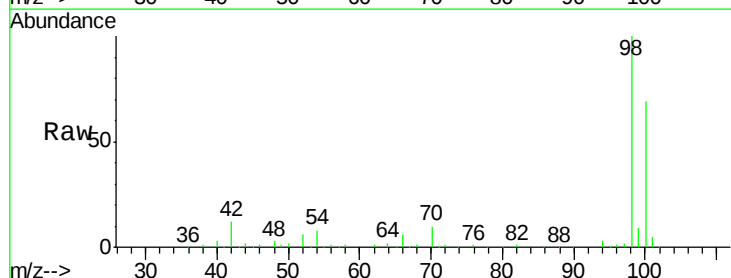

Abundance Ion 98.05 (97.75 to 98.75): VDC
Ion 100.05 (99.75 to 100.75): VDC

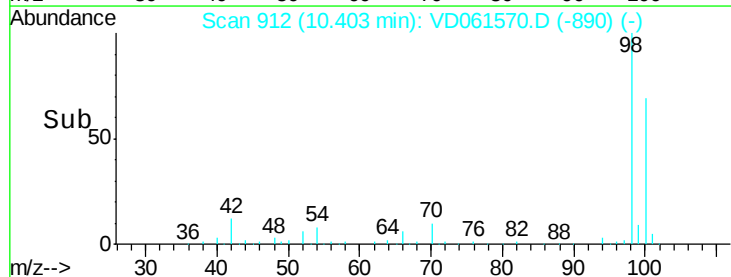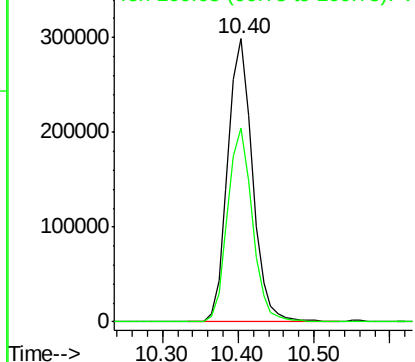


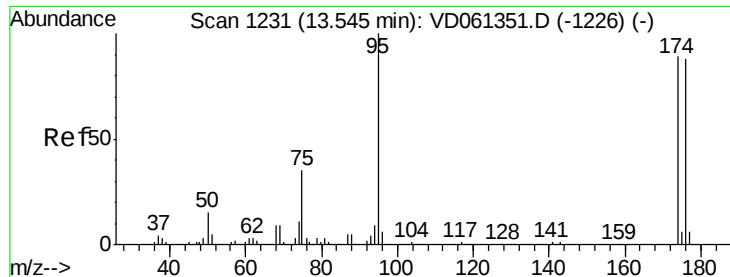




#62
4-Bromofluorobenzene
Concen: N.D. ug/l
RT: 13.55 min Scan# 1232
Delta R.T. 0.01 min
Lab File: VD061570.D
Acq: 3 Apr 2019 22:02

Instrument :
MSVOA_D
ClientSampleId :

Tot Ion: 95 Resp: 269863
Ion Ratio Lower Upper
95 100
174 103.8 0.0 178.0
176 101.7 0.0 175.0

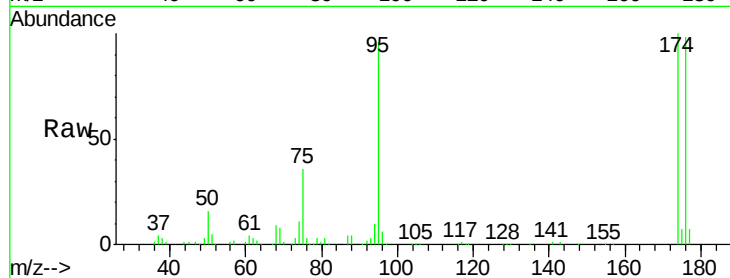


Abundance Ion 95.00 (94.70 to 95.70): V
Ion 173.90 (173.60 to 174.60): V
Ion 175.90 (175.60 to 176.60): V

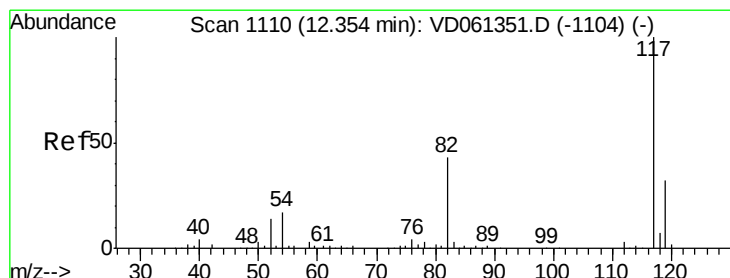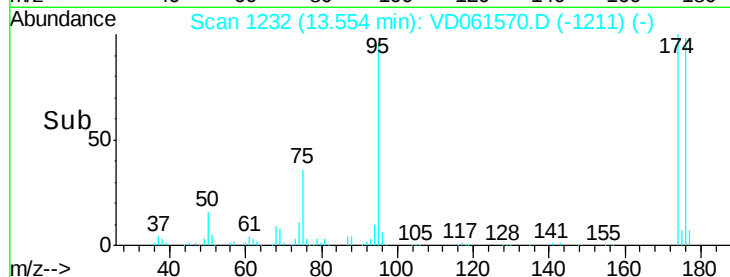
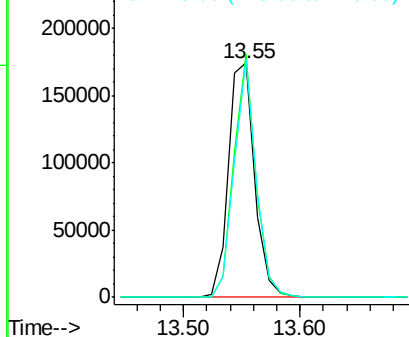



#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 12.36 min Scan# 1111
Delta R.T. 0.01 min
Lab File: VD061570.D
Acq: 3 Apr 2019 22:02

Tgt Ion: 117 Resp: 666180
Ion Ratio Lower Upper
117 100
82 45.7 34.4 51.6
119 33.0 25.8 38.6

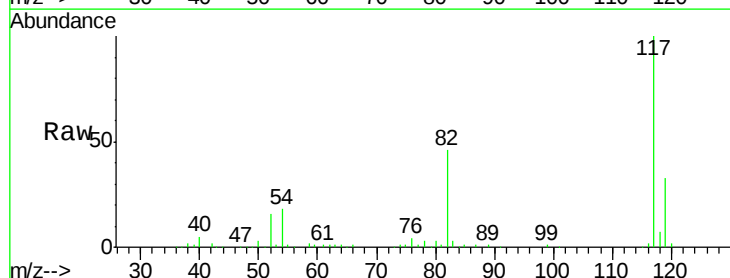

Abundance Ion 116.95 (116.65 to 117.65): V
Ion 82.05 (81.75 to 82.75): V
Ion 118.95 (118.65 to 119.65): V

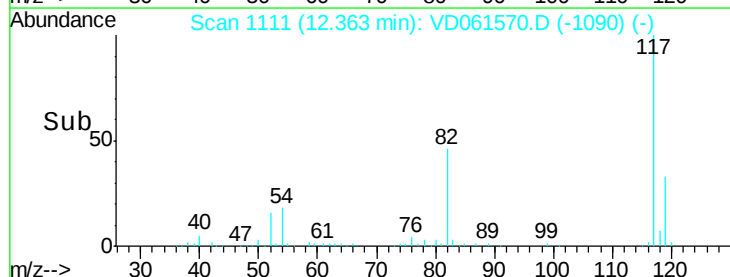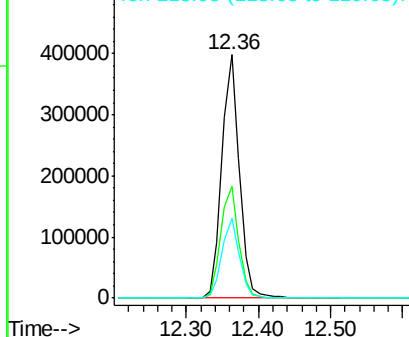

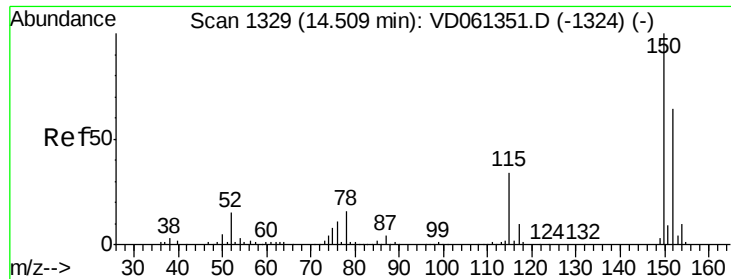


#72




1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 14.52 min Scan# 1330
Delta R.T. 0.01 min
Lab File: VD061570.D
Acq: 3 Apr 2019 22:02

Instrument :
MSVOA_D
ClientSampleId :

Tot Ion:152 Resp: 274599
Ion Ratio Lower Upper
152 100
115 52.5 26.9 80.6
150 156.6 0.0 318.0

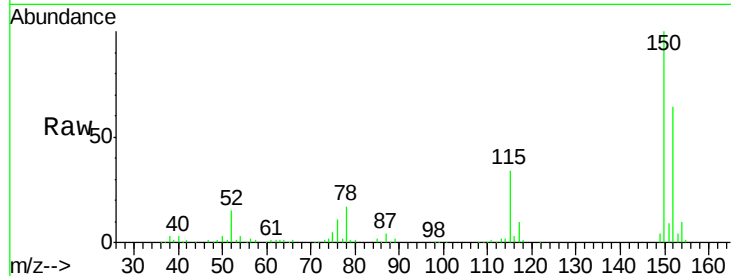


Abundance Ion 151.90 (151.60 to 152.60): V
Ion 115.00 (114.70 to 115.70): V
Ion 149.90 (149.60 to 150.60): V

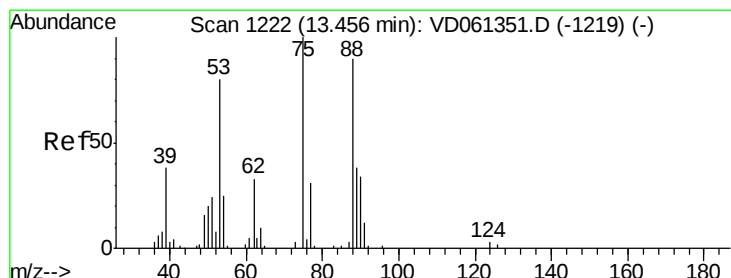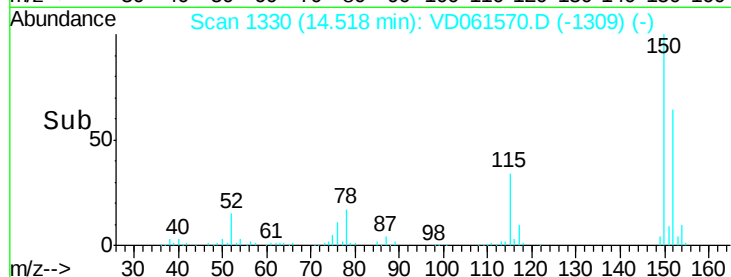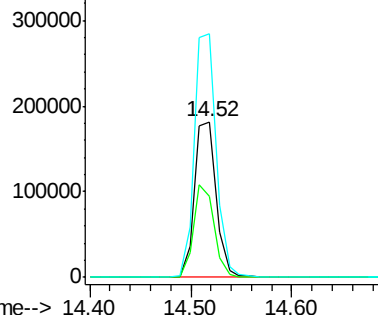

#81

trans-1,4-Dichloro-2-butene
Concen: 85.745 ug/l
RT: 13.54 min Scan# 1231
Delta R.T. 0.09 min
Lab File: VD061570.D
Acq: 3 Apr 2019 22:02

Tgt Ion: 75 Resp: 103703
Ion Ratio Lower Upper
75 100
53 0.0 63.8 95.8#
89 0.0 30.5 45.7#

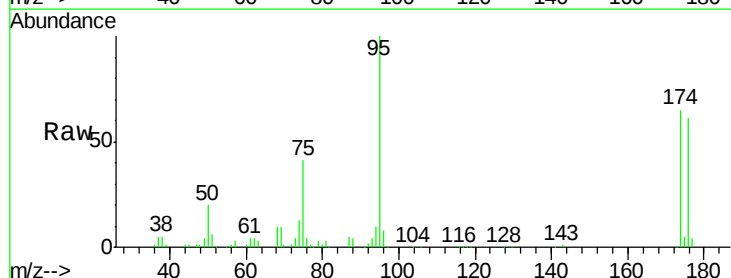

Abundance Ion 75.00 (74.70 to 75.70): VDC
Ion 53.00 (52.70 to 53.70): VDC
Ion 89.00 (88.70 to 89.70): VDC

