




Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD040323\
 Data File : VD075564.D
 Acq On : 03 Apr 2023 10:49
 Operator : KP/SY
 Sample : VD0403SBL01
 Misc : 5.00G/10.00ml/MSVOA_D/SOIL
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 VBLK116

Manual IntegrationsAPPROVED

Quant Time: Apr 04 01:48:47 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\SFAMDLM033123SMA.M
 Quant Title : SFAM01.0
 QLast Update : Sat Apr 01 00:08:20 2023
 Response via : Initial Calibration

Reviewed By :Krupa Patel 04/04/2023
 Supervised By :Mahesh Dadoda 04/04/2023

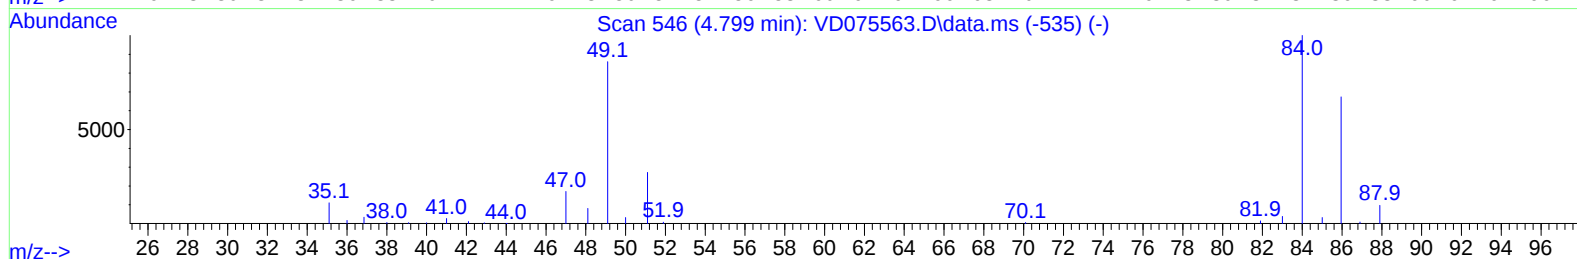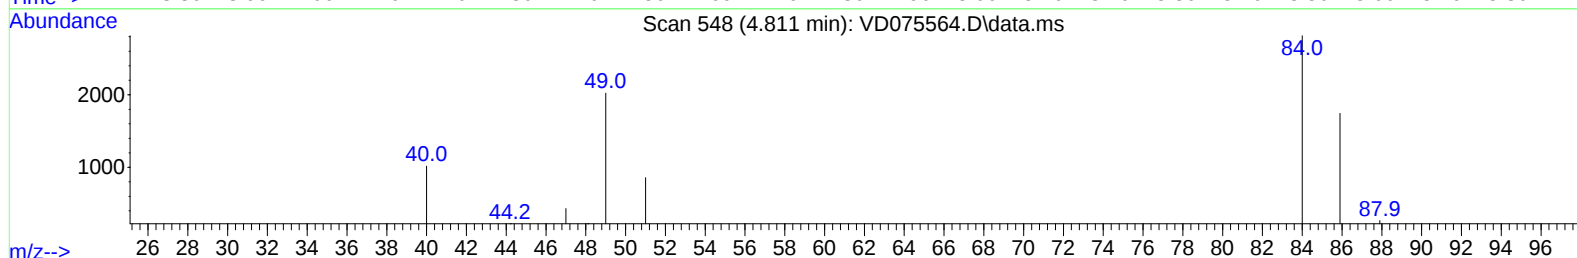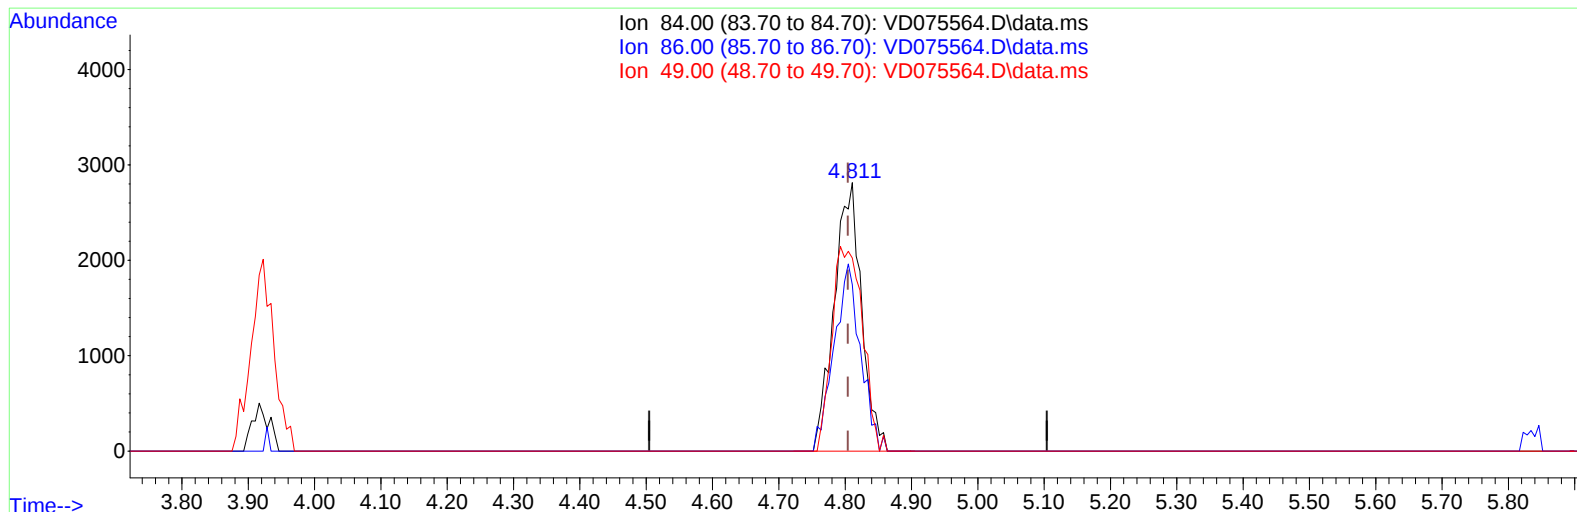

TIC: VD075564.D\data.ms

(16) Methylene chloride (T)

4.811min (+ 0.006) 1.48 ug/L m

response 8066

Ion	Exp%	Act%
84.00	100.00	100.00
86.00	63.40	61.98
49.00	83.60	71.89
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD040323\
 Data File : VD075564.D
 Acq On : 03 Apr 2023 10:49
 Operator : KP/SY
 Sample : VD0403SBL01
 Misc : 5.00G/10.00ml/MSVOA_D/SOIL
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 VBLK116

Manual IntegrationsAPPROVED

Quant Time: Apr 04 01:48:47 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\SFAMDLM033123SMA.M
 Quant Title : SFAM01.0
 QLast Update : Sat Apr 01 00:08:20 2023
 Response via : Initial Calibration

Reviewed By :Krupa Patel 04/04/2023
 Supervised By :Mahesh Dadoda 04/04/2023

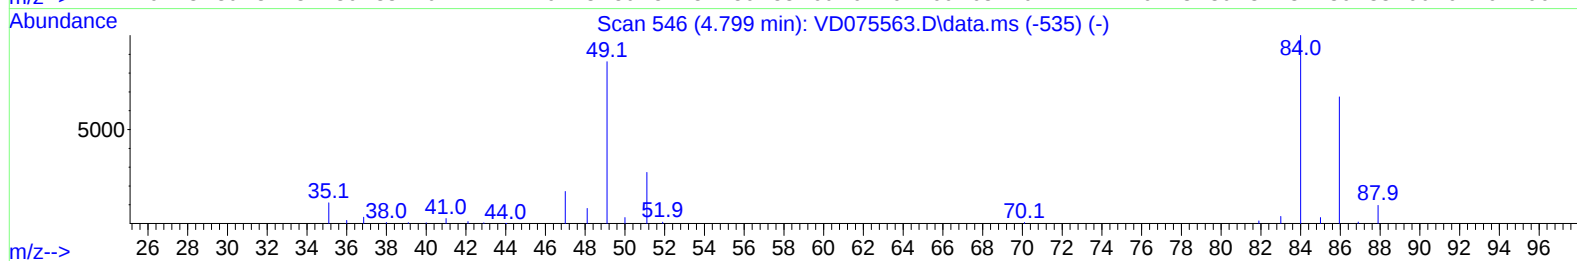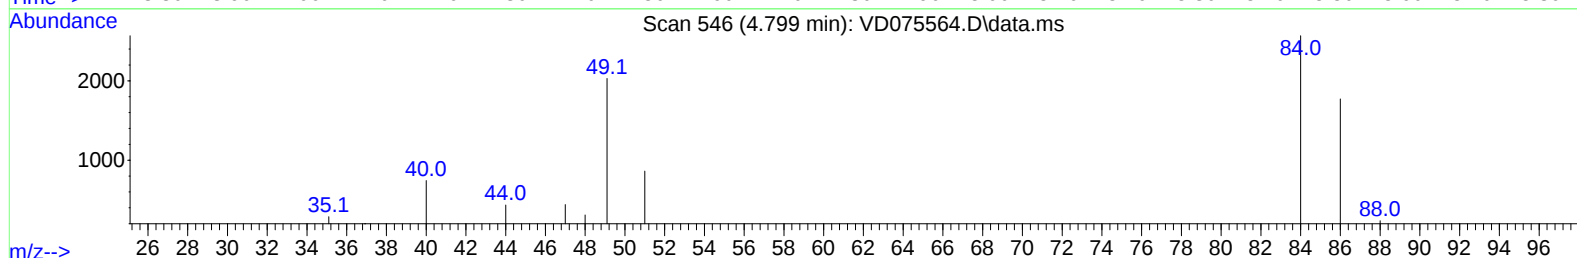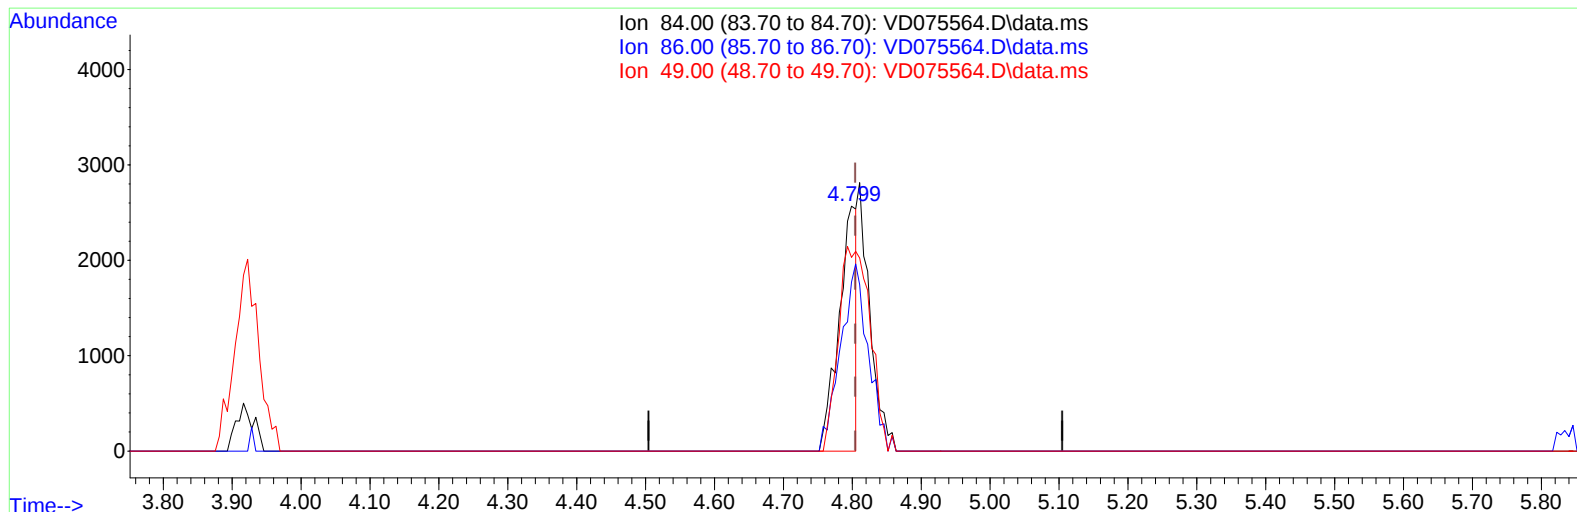

TIC: VD075564.D\data.ms

(16) Methylene chloride (T)

4.799min (-0.006) 0.85 ug/L

response 4603

Ion	Exp%	Act%
84.00	100.00	100.00
86.00	63.40	69.00
49.00	83.60	79.05
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD040323\
 Data File : VD075564.D
 Acq On : 03 Apr 2023 10:49
 Operator : KP/SY
 Sample : VD0403SBL01
 Misc : 5.00G/10.00ml/MSVOA_D/SOIL
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 VBLK116

Manual IntegrationsAPPROVED

Reviewed By :Krupa Patel 04/04/2023
 Supervised By :Mahesh Dadoda 04/04/2023

Quant Time: Apr 04 01:48:47 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\SFAMDLM033123SMA.M
 Quant Title : SFAM01.0
 QLast Update : Sat Apr 01 00:08:20 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.775	114	395688	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.581	117	346419	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.522	152	141365	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.275	65	267703	29.058	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery = 116.240%			
7) Chloroethane-d5	2.805	69	237347	28.952	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery = 115.800%			
11) 1,1-Dichloroethene-d2	3.917	63	171711	23.107	ug/L	-0.01
Spiked Amount 25.000	Range 45 - 110		Recovery = 92.440%			
21) 2-Butanone-d5	6.987	46	33987	56.649	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery = 113.300%			
24) Chloroform-d	7.569	84	241617	25.900	ug/L	0.00
Spiked Amount 25.000	Range 40 - 150		Recovery = 103.600%			
26) 1,2-Dichloroethane-d4	8.228	65	101958	24.662	ug/L	0.00
Spiked Amount 25.000	Range 70 - 130		Recovery = 98.640%			
32) Benzene-d6	8.205	84	528545	26.098	ug/L	0.00
Spiked Amount 25.000	Range 20 - 135		Recovery = 104.400%			
36) 1,2-Dichloropropane-d6	9.210	67	138073	25.582	ug/L	0.00
Spiked Amount 25.000	Range 70 - 120		Recovery = 102.320%			
41) Toluene-d8	10.269	98	494351	26.032	ug/L	0.00
Spiked Amount 25.000	Range 30 - 130		Recovery = 104.120%			
43) trans-1,3-Dichloroprop...	10.528	79	56520	25.120	ug/L	0.00
Spiked Amount 25.000	Range 30 - 135		Recovery = 100.480%			
47) 2-Hexanone-d5	10.881	63	29944	46.883	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery = 93.760%			
56) 1,1,2,2-Tetrachloroeth...	12.651	84	100263	24.797	ug/L	0.00
Spiked Amount 25.000	Range 45 - 120		Recovery = 99.200%			
66) 1,2-Dichlorobenzene-d4	13.816	152	131936	27.207	ug/L	0.00
Spiked Amount 25.000	Range 75 - 120		Recovery = 108.840%			
Target Compounds						Qvalue
16) Methylene chloride	4.811	84	8066m	1.483	ug/L	

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD040323\
Data File : VD075564.D
Acq On : 03 Apr 2023 10:49
Operator : KP/SY
Sample : VD0403SBL01
Misc : 5.00G/10.00ml/MSVOA_D/SOIL
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
VBLK116

Manual IntegrationsAPPROVED

Reviewed By :Krupa Patel 04/04/2023
Supervised By :Mahesh Dadoda 04/04/2023

Quant Time: Apr 04 01:48:47 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\SFAMDLM033123SMA.M
Quant Title : SFAM01.0
QLast Update : Sat Apr 01 00:08:20 2023
Response via : Initial Calibration

