
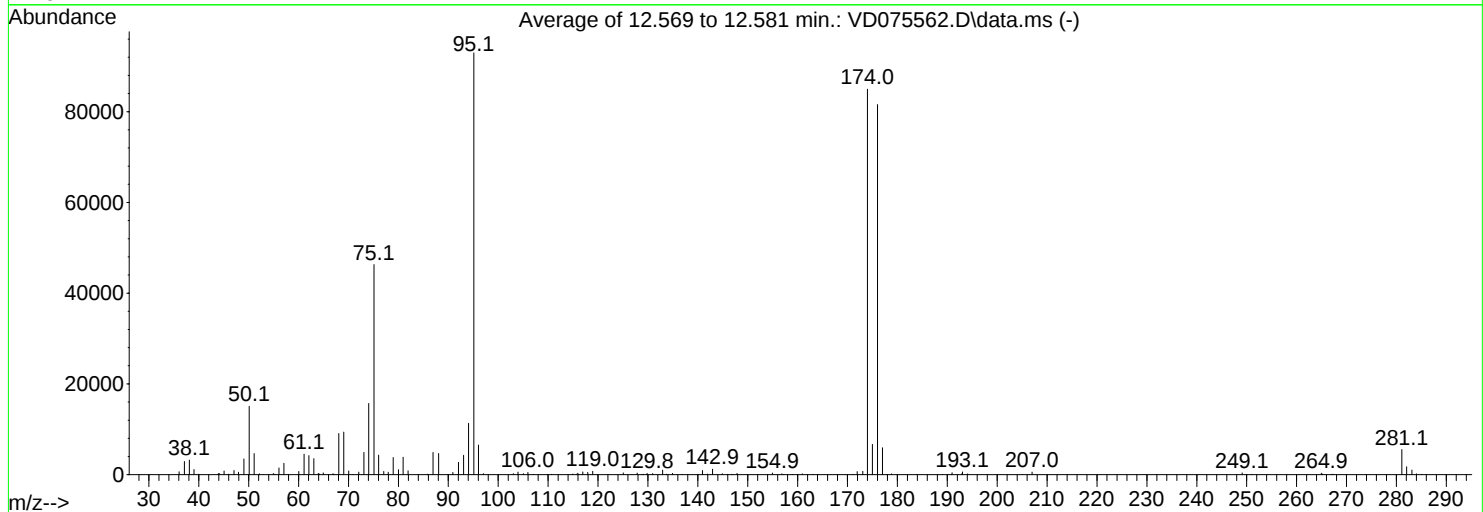


Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD040323\
 Data File : VD075562.D
 Acq On : 03 Apr 2023 09:11
 Operator : KP/SY
 Sample : BFB112
 Misc : 5.00G/10.00ml/MSVOA_D/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 BFB112

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\SFAMDLM033123SMA.M
 Title : SFAM01.0
 Last Update : Sat Apr 01 00:08:20 2023

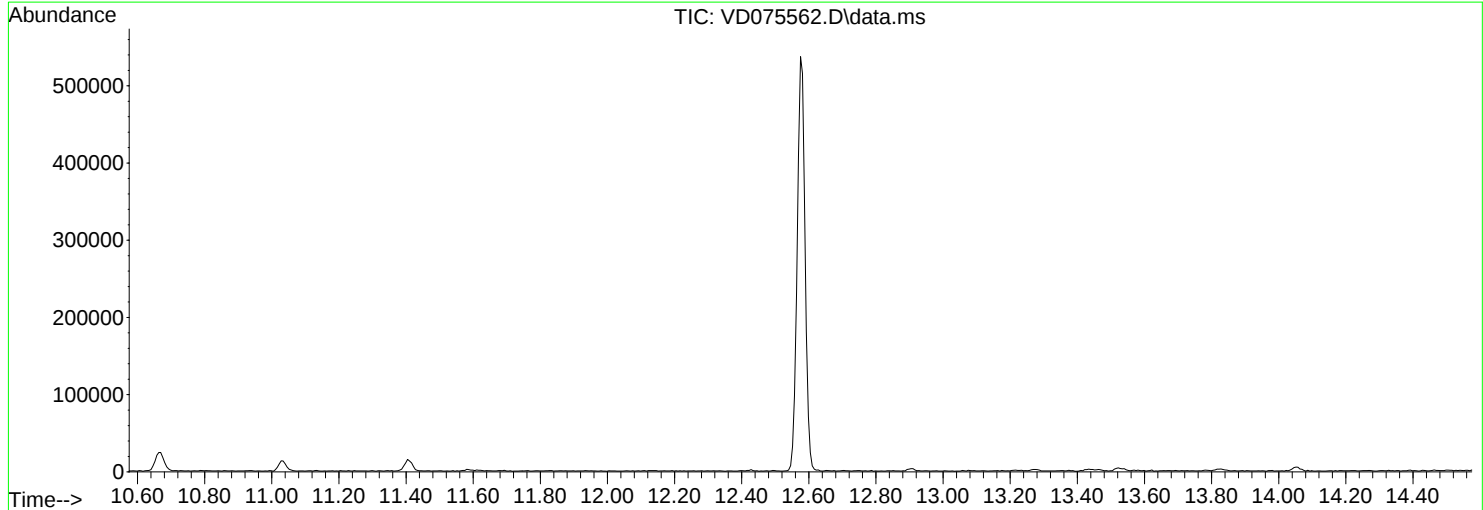

AutoFind: Scans 1867, 1868, 1869; Background Corrected with Scan 1860

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.2	15061	PASS
75	95	30	80	49.8	46320	PASS
95	95	100	100	100.0	92968	PASS
96	95	5	9	7.0	6510	PASS
173	174	0.00	2	0.9	755	PASS
174	95	50	120	91.4	84968	PASS
175	174	5	9	7.9	6672	PASS
176	174	95	105	96.0	81576	PASS
177	176	5	10	7.3	5916	PASS

m/z	Abundance
40.00	878.0
44.10	475.0

Instrument :
MSVOA_D
ClientSampleId :
BFB112

m/z	Abundance
36.10	440.0
37.10	2177.0
38.10	3260.0
39.00	955.0
40.10	1138.0
43.90	741.0
45.00	818.0
47.00	852.0
48.10	543.0
49.10	2794.0
50.10	13231.0
51.10	3775.0
52.20	249.0
55.00	257.0
56.10	1146.0
57.10	2403.0
58.00	174.0
60.10	468.0
61.10	4378.0
62.00	3195.0
63.00	2913.0
64.00	648.0
65.00	364.0
67.00	241.0
68.10	7689.0
69.10	8935.0
70.10	913.0
72.00	665.0
73.10	4355.0
74.10	13476.0
75.10	40800.0
76.00	4048.0
77.00	585.0
78.00	701.0
79.00	3423.0
80.00	1048.0
80.90	3414.0
82.00	897.0
87.00	4054.0
88.10	3303.0
90.90	533.0
92.10	2405.0
93.00	3647.0
94.10	9002.0
95.10	78048.0
96.00	4898.0
103.10	175.0
104.00	372.0
105.00	184.0
106.00	463.0
115.80	397.0
117.00	504.0
118.00	321.0
119.00	647.0
125.10	230.0
127.90	292.0
129.80	280.0
131.00	278.0
133.00	581.0
135.00	271.0
141.00	744.0
141.90	215.0
142.90	1098.0
144.90	165.0
147.80	230.0
154.90	224.0
157.20	160.0
161.00	352.0
171.10	223.0
171.90	520.0
173.00	461.0
174.00	71768.0
175.00	5597.0
176.00	66568.0
177.00	5057.0
190.80	236.0
192.90	493.0
194.10	286.0
207.00	260.0
249.00	265.0
265.20	449.0
281.10	2997.0
282.00	1432.0
283.10	514.0

Instrument :
MSVOA_D
ClientSampleId :
BFB112

m/z	Abundance
36.00	902.0
37.10	3448.0
38.10	3293.0
39.00	1426.0
40.00	983.0
44.10	1142.0
45.10	876.0
47.10	983.0
47.90	418.0
49.00	4058.0
50.10	16089.0
51.10	5433.0
52.10	284.0
54.80	219.0
55.30	184.0
56.00	1643.0
57.10	2812.0
60.00	985.0
61.10	4539.0
62.10	5405.0
63.10	3696.0
64.20	398.0
65.00	441.0
66.80	364.0
68.00	10515.0
69.00	10009.0
70.00	784.0
72.10	526.0
73.10	5117.0
74.00	16960.0
75.10	49880.0
76.10	4967.0
77.10	604.0
77.80	401.0
78.90	3845.0
80.00	1125.0
81.00	4169.0
81.90	963.0
85.80	170.0
87.00	5796.0
88.00	5618.0
90.90	413.0
92.00	3083.0
93.10	4621.0
94.10	13244.0
95.10	103872.0
96.10	8023.0
97.10	273.0
103.10	262.0
103.90	585.0
105.10	255.0
106.00	555.0
115.00	240.0
116.00	435.0
116.90	614.0
117.90	530.0
118.90	899.0
125.00	467.0
127.80	417.0
128.80	255.0
129.90	327.0
130.90	153.0
132.90	1310.0
134.90	340.0
136.90	236.0
140.90	1178.0
142.90	1320.0
145.00	305.0
146.80	262.0
147.90	405.0
155.00	441.0
156.80	255.0
171.90	930.0
173.10	929.0
174.00	92160.0
175.00	7581.0
176.00	89856.0
177.00	6602.0
178.90	337.0
191.00	591.0
193.10	856.0
207.10	756.0
249.10	445.0
250.00	176.0
264.90	511.0
267.30	291.0
281.10	5601.0
282.10	1765.0
283.10	1083.0
284.20	172.0

Instrument :
MSVOA_D
ClientSampleId :
BFB112

m/z	Abundance
36.00	612.0
37.10	3084.0
38.10	3120.0
39.10	1011.0
40.00	865.0
44.10	1070.0
45.10	767.0
46.00	279.0
47.10	946.0
47.90	623.0
49.10	3486.0
50.10	15862.0
51.10	4745.0
52.90	151.0
55.00	262.0
56.10	1681.0
57.00	2318.0
60.00	671.0
61.10	4653.0
62.00	3999.0
63.00	3964.0
63.90	217.0
64.90	342.0
67.10	246.0
68.00	8967.0
69.10	9238.0
70.00	725.0
70.90	155.0
72.10	550.0
73.10	5255.0
74.10	16640.0
75.10	48280.0
76.00	3934.0
77.00	974.0
78.00	487.0
78.90	4114.0
80.00	1075.0
81.00	3982.0
81.90	670.0
85.80	176.0
86.90	4850.0
88.00	5080.0
90.90	530.0
92.10	2707.0
93.00	4544.0
94.00	11690.0
95.10	96984.0
96.10	6610.0
97.00	333.0
102.90	196.0
104.00	712.0
105.10	166.0
105.90	469.0
107.00	222.0
109.90	197.0
110.70	216.0
114.90	196.0
115.90	489.0
116.90	714.0
117.90	588.0
119.00	702.0
125.10	512.0
127.80	403.0
129.10	224.0
129.90	299.0
131.00	303.0
132.90	1082.0
133.70	317.0
134.90	236.0
141.00	870.0
141.90	207.0
143.00	1190.0
144.80	186.0
146.00	172.0
147.00	152.0
147.80	186.0
155.00	383.0
156.90	291.0
159.00	164.0
160.90	164.0
163.10	206.0
172.00	519.0
173.00	874.0
174.00	90976.0
175.00	6838.0
176.00	88304.0
177.00	6089.0
177.90	162.0
178.80	184.0
189.00	166.0
190.90	689.0
193.00	979.0

Instrument :
MSVOA_D
ClientSampleId :
BFB112

194.10	258.0
205.00	153.0
206.90	683.0
249.20	446.0
251.00	194.0
265.00	421.0
267.00	178.0
281.10	8018.0
282.10	1954.0
283.10	1458.0
284.00	379.0
285.10	179.0

Instrument :
MSVOA_D
ClientSampleId :
BFB112