
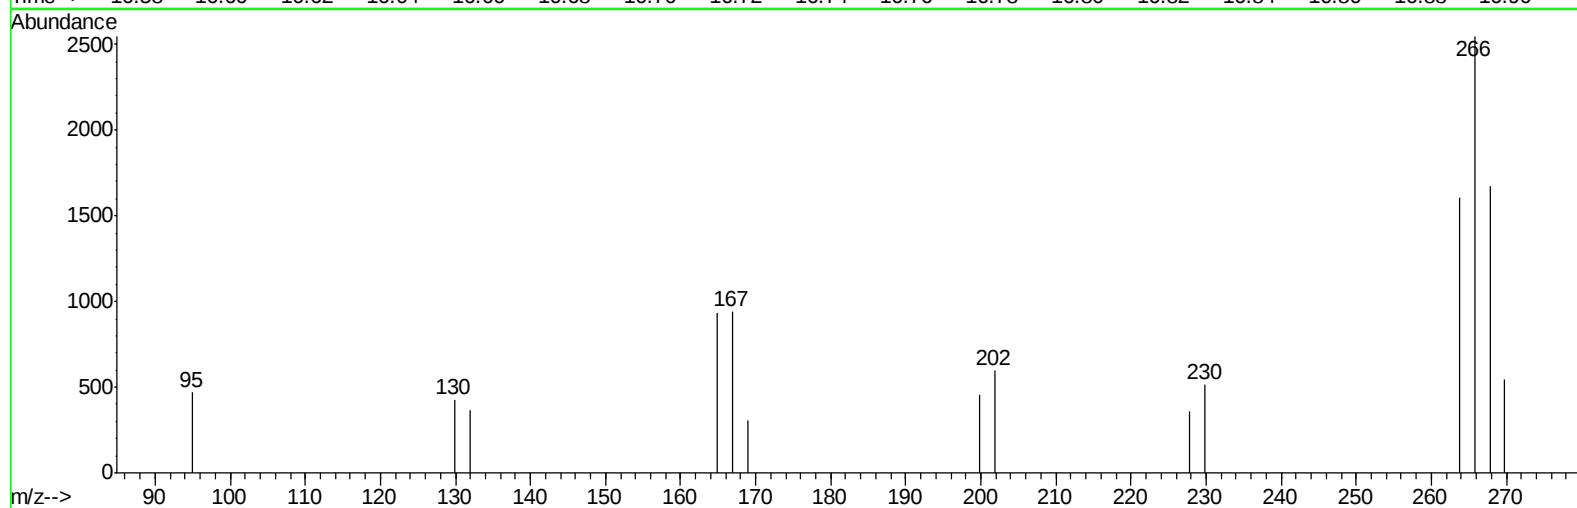


Data Path : Z:\svoasrv\HPCHEM1\BNA N\Data\BN040419\
 Data File : BN005094.D
 Acq On : 04 Apr 2019 15:11
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :

Quant Time: Apr 05 04:34:24 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\8270-BN032619.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Mar 27 05:27:09 2019
 Response via : Initial Calibration

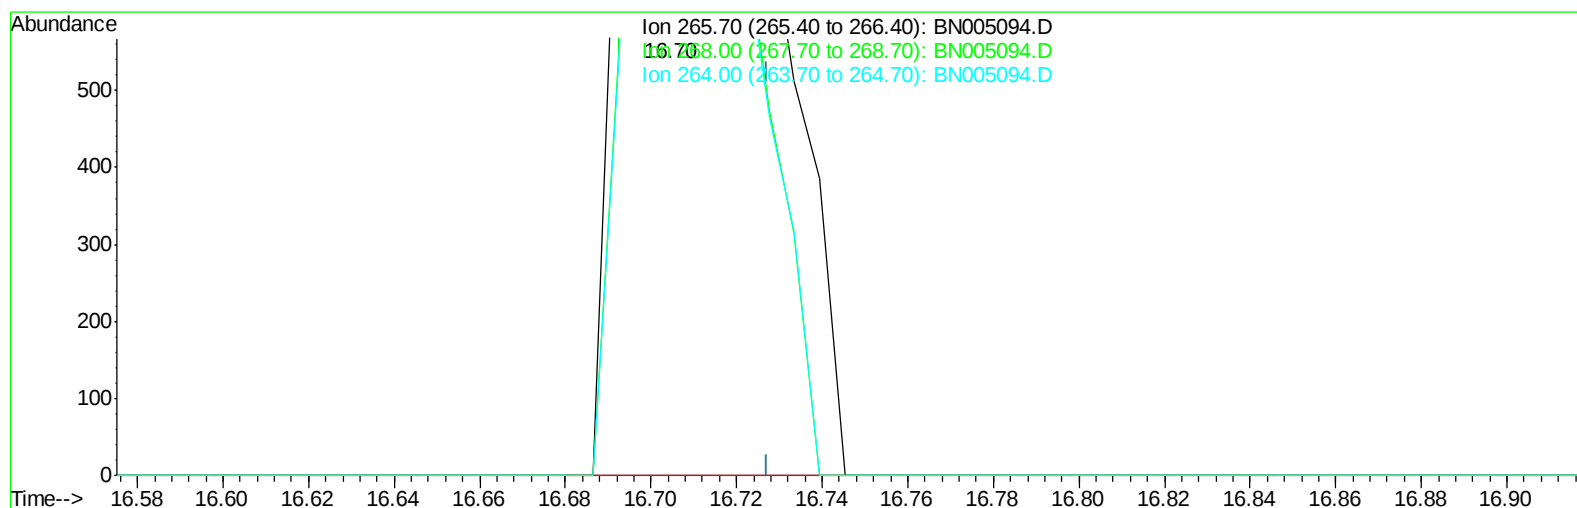

TIC: BN005094.D

(70) Pentachlorophenol (C)

16.704min (-0.023) 0.00ng m



response 4324

Ion	Exp%	Act%
265.70	100	100
268.00	63.50	65.61
264.00	62.50	63.13
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA N\Data\BN040419\
Data File : BN005094.D
Acq On : 04 Apr 2019 15:11
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :

Quant Time: Apr 05 04:34:24 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\8270-BN032619.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 27 05:27:09 2019
Response via : Initial Calibration

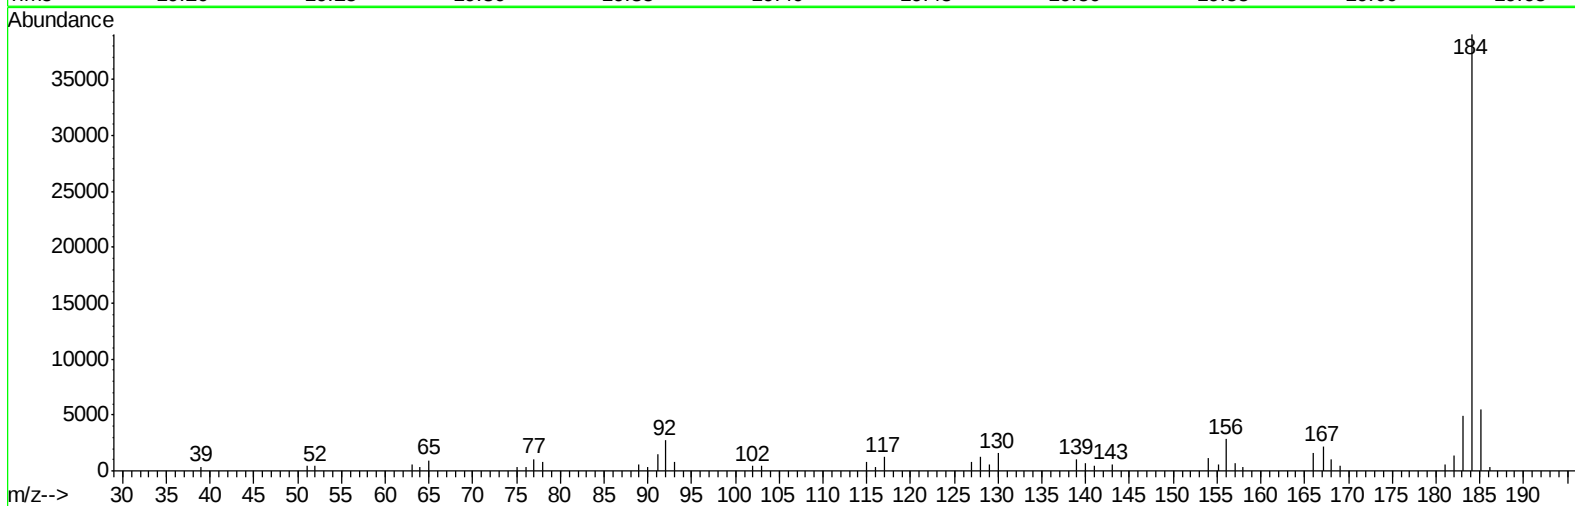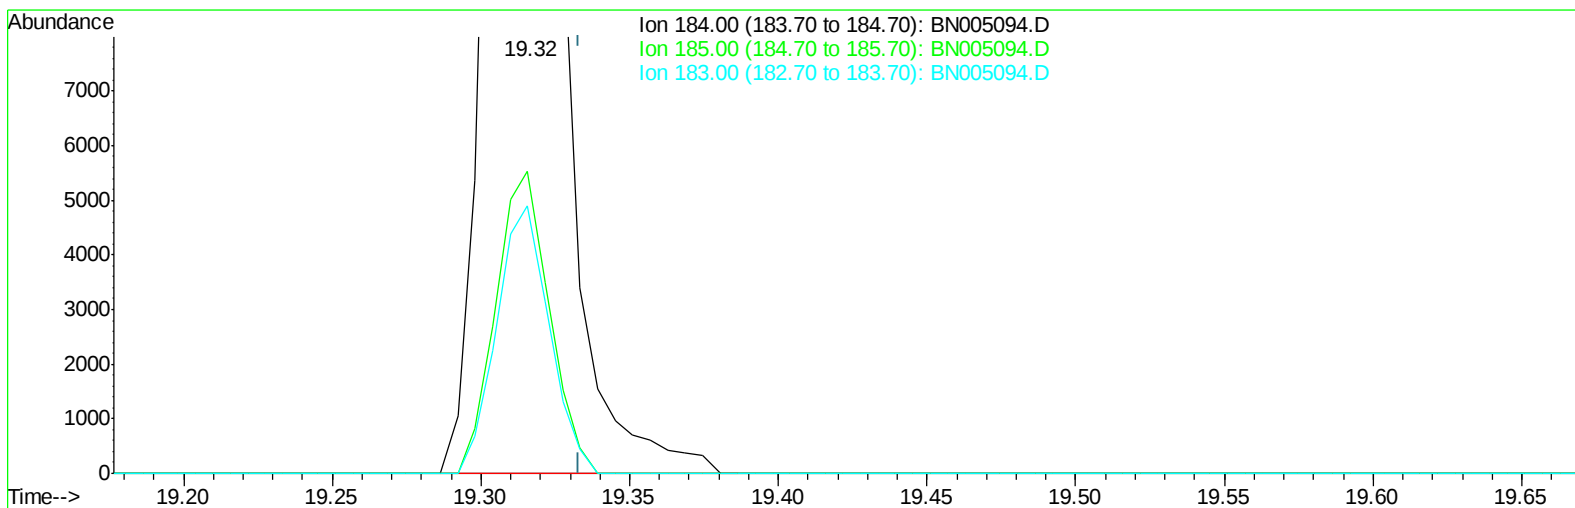

TIC: BN005094.D

(77) Benzidine

19.316min (-0.017) 0.00ng m

response 49567

Ion	Exp%	Act%
184.00	100	100
185.00	14.80	14.15
183.00	12.40	12.55
0.00	0.00	0.00