


Data Path : Z:\voasrv\HPCHEM1\MSVOA D\Data\VD040419\
 Data File : VD061598.D
 Acq On : 5 Apr 2019 1:05
 Operator : VA/AP
 Sample : BFB
 Misc : 5.00µl/5ml/MSVOA D/SOIL
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D032719S.M
 Title : SW846 8260
 Last Update : Thu Mar 28 09:22:37 2019

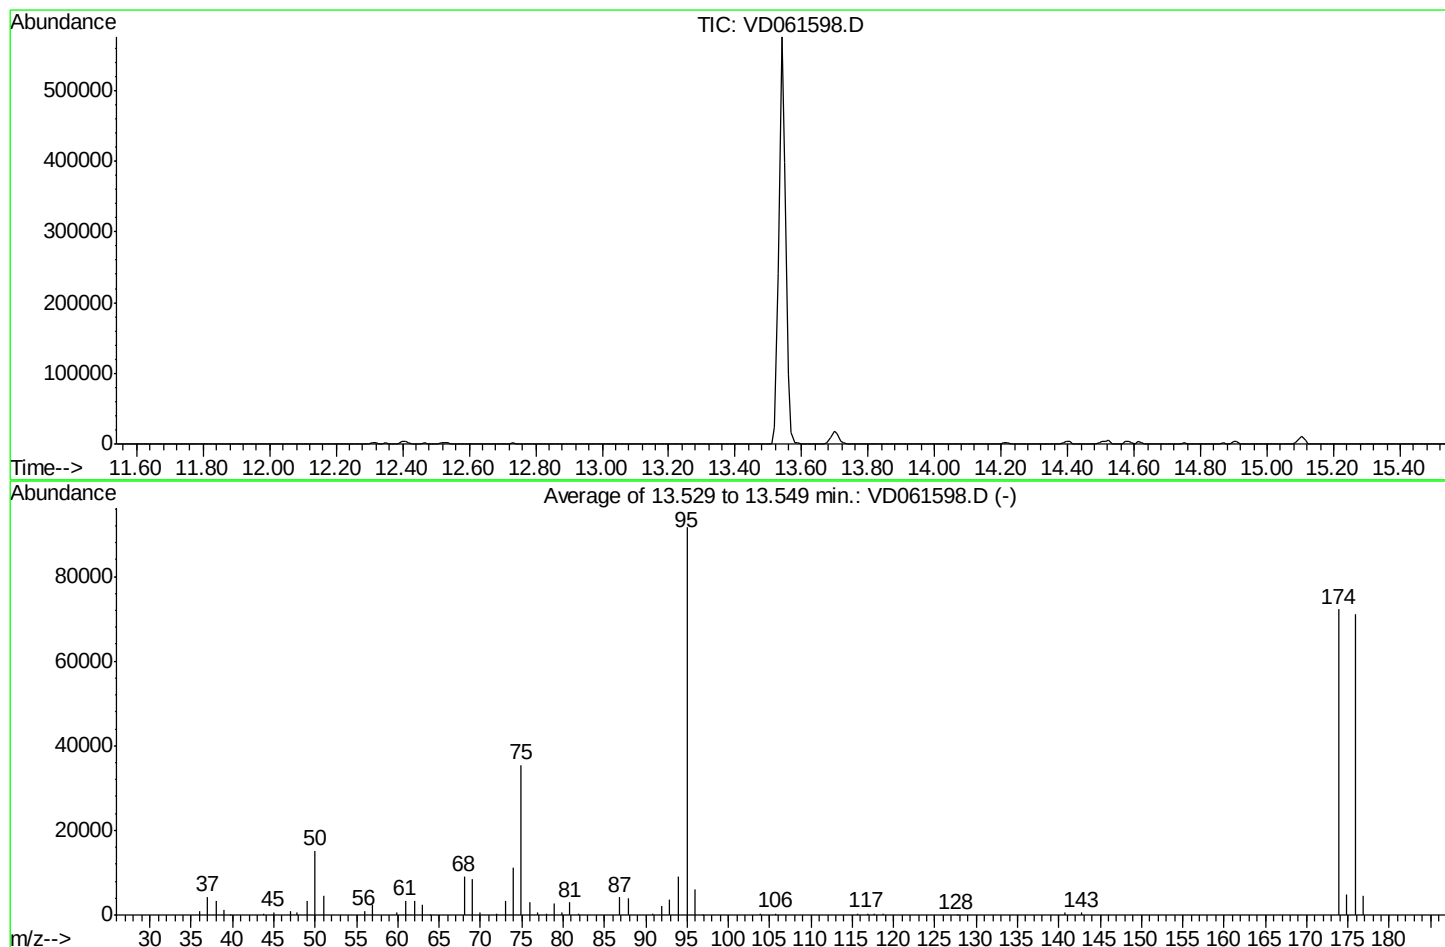

AutoFind: Scans 1230, 1231, 1232; Background Corrected with Scan 1226

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.7	15253	PASS
75	95	30	60	38.6	35405	PASS
95	95	100	100	100.0	91605	PASS
96	95	5	9	6.8	6191	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	78.9	72258	PASS
175	174	5	9	6.9	5001	PASS
176	174	95	101	98.3	71040	PASS
177	176	5	9	6.4	4546	PASS