
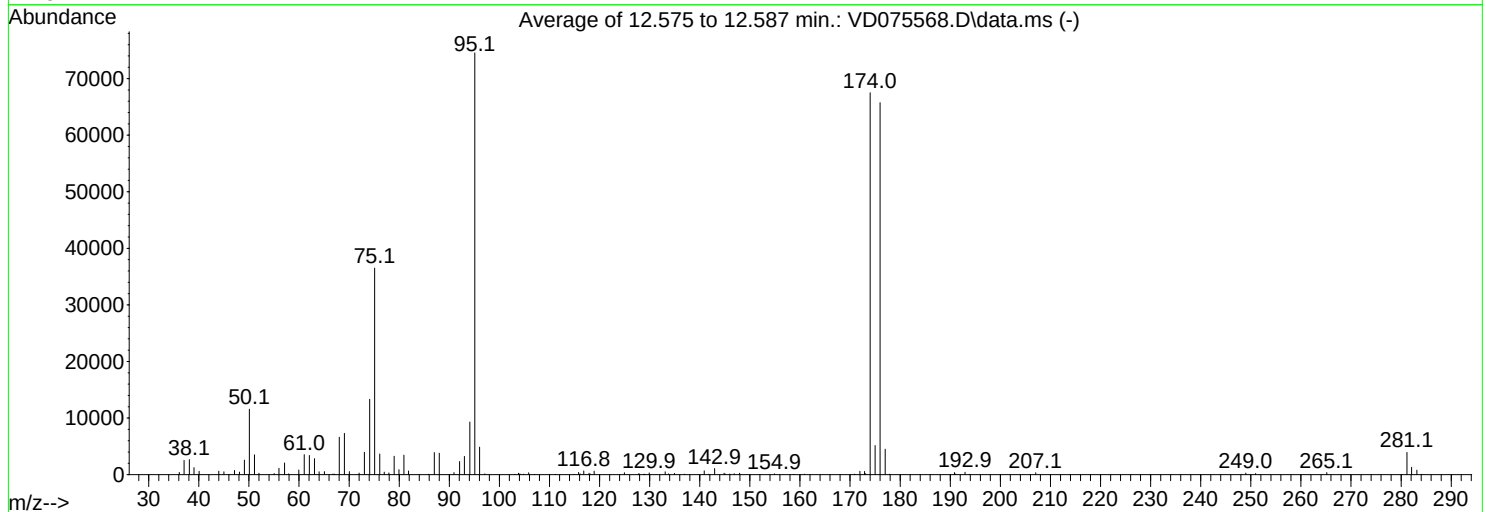


Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD040423\
Data File : VD075568.D
Acq On : 04 Apr 2023 10:05
Operator : KP/SY
Sample : BFB113
Misc : 5.00G/10.00ml/MSVOA_D/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB113

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\SFAMDLM033123SMA.M
Title : SFAM01.0
Last Update : Sat Apr 01 00:08:20 2023

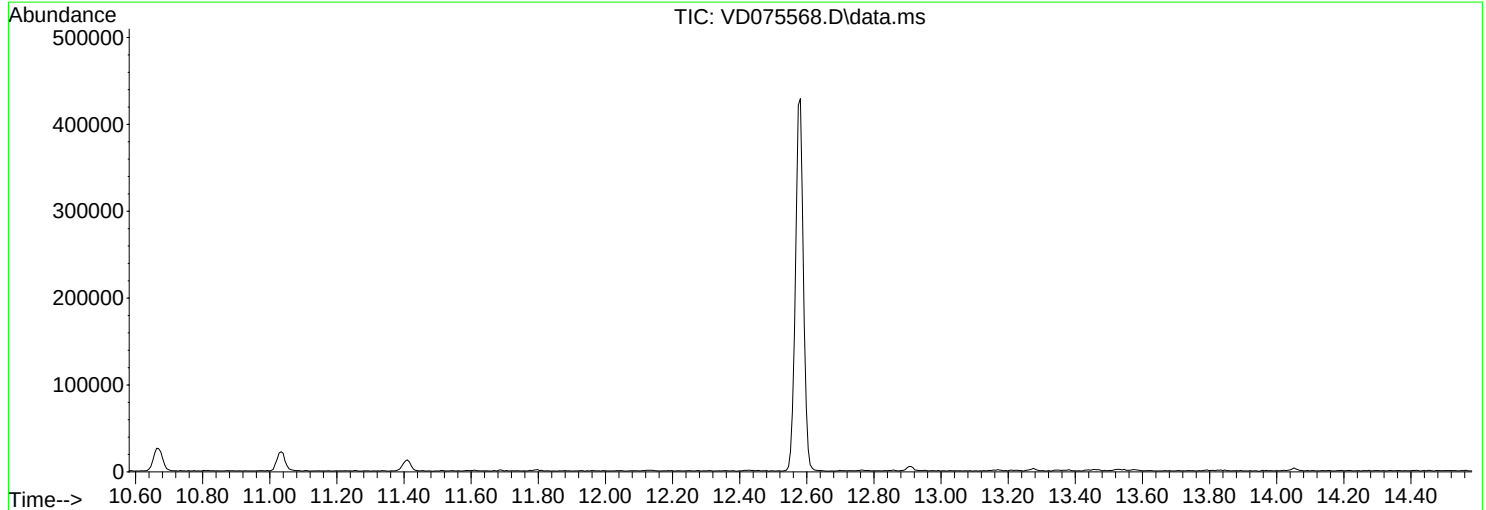

AutoFind: Scans 1868, 1869, 1870; Background Corrected with Scan 1860

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	15.5	11569	PASS
75	95	30	80	49.0	36507	PASS
95	95	100	100	100.0	74555	PASS
96	95	5	9	6.5	4876	PASS
173	174	0.00	2	0.8	559	PASS
174	95	50	120	90.6	67517	PASS
175	174	5	9	7.6	5154	PASS
176	174	95	105	97.4	65744	PASS
177	176	5	10	6.8	4484	PASS

m/z	Abundance
39.90	722.0
43.90	252.0

Instrument :
MSVOA_D
ClientSampleId :
BFB113

m/z	Abundance
36.10	452.0
37.00	2882.0
38.10	2664.0
39.00	1353.0
39.90	981.0
44.10	970.0
45.10	483.0
47.20	802.0
48.10	470.0
49.10	2729.0
50.10	12397.0
51.10	3992.0
52.00	201.0
55.10	260.0
56.00	1287.0
57.10	1976.0
57.90	243.0
59.90	1056.0
61.00	4026.0
62.00	3603.0
63.10	3223.0
63.90	649.0
65.10	409.0
66.80	209.0
67.10	264.0
68.00	7546.0
69.00	7639.0
70.10	800.0
72.00	332.0
73.10	4615.0
74.10	14849.0
75.10	40176.0
76.10	4318.0
77.10	385.0
78.00	353.0
79.00	3673.0
79.90	897.0
81.00	3974.0
81.90	612.0
85.80	160.0
87.00	4528.0
88.00	4324.0
91.00	350.0
92.00	2333.0
93.00	3077.0
94.10	10047.0
95.10	82272.0
96.00	5570.0
97.20	209.0
104.10	402.0
105.90	294.0
107.00	151.0
111.20	152.0
115.80	541.0
116.80	676.0
118.00	379.0
118.90	643.0
124.90	308.0
127.70	209.0
128.80	205.0
129.90	343.0
133.20	289.0
133.80	224.0
135.00	167.0
141.00	937.0
141.80	217.0
143.00	1206.0
144.90	569.0
146.00	226.0
146.80	156.0
148.10	220.0
172.00	602.0
173.00	876.0
174.00	73904.0
175.00	5538.0
176.00	70304.0
177.00	5102.0
190.80	306.0
192.90	341.0
207.10	233.0
249.00	211.0
265.20	297.0
281.10	3602.0
282.10	1208.0
283.10	509.0

Instrument :
MSVOA_D
ClientSampleId :
BFB113

m/z	Abundance
36.10	460.0
37.10	2475.0
38.10	3114.0
39.10	1482.0
40.10	687.0
44.00	980.0
45.00	579.0
46.00	195.0
47.00	958.0
48.10	585.0
49.10	3133.0
50.10	13194.0
51.10	3773.0
51.90	273.0
54.90	164.0
55.20	162.0
56.00	1405.0
57.10	2671.0
58.00	156.0
60.00	887.0
61.10	3789.0
62.00	3923.0
63.10	3307.0
64.00	493.0
65.00	842.0
66.80	162.0
68.10	7300.0
69.00	8091.0
70.00	529.0
71.90	314.0
73.00	4431.0
74.10	14352.0
75.10	40808.0
76.10	4016.0
76.90	468.0
77.90	266.0
79.00	3628.0
80.00	1107.0
81.00	3460.0
81.80	711.0
87.00	4370.0
88.00	4112.0
91.00	457.0
92.10	2633.0
93.00	3944.0
94.10	10113.0
95.10	82872.0
96.10	4965.0
97.00	193.0
103.10	175.0
103.80	483.0
104.80	230.0
105.90	387.0
115.80	644.0
116.90	562.0
117.80	404.0
118.90	783.0
125.00	451.0
127.90	381.0
129.00	219.0
129.90	247.0
133.10	674.0
133.80	178.0
134.80	268.0
137.00	217.0
140.80	644.0
143.00	1076.0
144.70	163.0
145.10	263.0
146.00	155.0
146.80	220.0
147.90	270.0
155.00	177.0
158.80	183.0
160.90	233.0
170.90	270.0
172.00	608.0
172.80	801.0
174.00	72288.0
175.00	5209.0
176.00	73360.0
177.00	4844.0
177.90	283.0
190.90	763.0
192.90	609.0
193.80	180.0
207.00	342.0
249.00	456.0
250.90	295.0
265.10	528.0
281.20	3635.0
282.10	1409.0

Instrument :
MSVOA_D
ClientSampleId :
BFB113

283.20916.0

284.10188.0

Instrument :
MSVOA_D
ClientSampleId :
BFB113

m/z	Abundance
36.10	246.0
37.10	2171.0
38.10	2174.0
39.10	864.0
40.00	1126.0
44.00	641.0
44.90	446.0
47.10	489.0
48.00	292.0
49.00	1861.0
50.10	9116.0
51.10	2776.0
52.10	292.0
55.90	721.0
57.10	1572.0
60.00	522.0
61.10	2775.0
62.10	2690.0
63.10	1965.0
64.10	375.0
65.10	374.0
68.10	4986.0
69.10	6178.0
70.10	265.0
72.10	225.0
73.10	2855.0
74.10	10750.0
75.10	28536.0
76.10	2635.0
77.00	518.0
78.00	288.0
79.00	2447.0
79.90	597.0
80.90	2896.0
81.90	646.0
87.00	2827.0
88.00	2977.0
90.90	306.0
92.00	1979.0
93.00	2674.0
94.10	7726.0
95.10	58520.0
96.10	4092.0
103.80	313.0
105.80	328.0
110.00	169.0
114.90	153.0
116.10	441.0
116.90	711.0
118.10	316.0
119.00	411.0
124.90	305.0
127.80	231.0
129.90	356.0
133.00	609.0
135.00	238.0
140.80	437.0
142.90	940.0
145.00	176.0
146.90	179.0
147.90	260.0
154.80	219.0
171.90	612.0
173.10	512.0
174.00	56360.0
175.00	4714.0
176.00	53568.0
177.00	3506.0
191.10	378.0
193.00	325.0
207.10	429.0
249.00	230.0
251.00	271.0
265.20	276.0
281.10	4570.0
282.10	1302.0
283.10	918.0

Instrument :
MSVOA_D
ClientSampleId :
BFB113