


Data Path : Z:\VOASRV\HPCHEM1\MSVOA D\DATA\VD040519\
Data File : VD061614.D
Acq On : 5 Apr 2019 9:59
Operator : VA/AP
Sample : BFB
Misc : 5.00g/5ml/MSVOA D/SOIL
ALS Vial : 2 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D032719S.M
Title : SW846 8260
Last Update : Thu Mar 28 09:22:37 2019

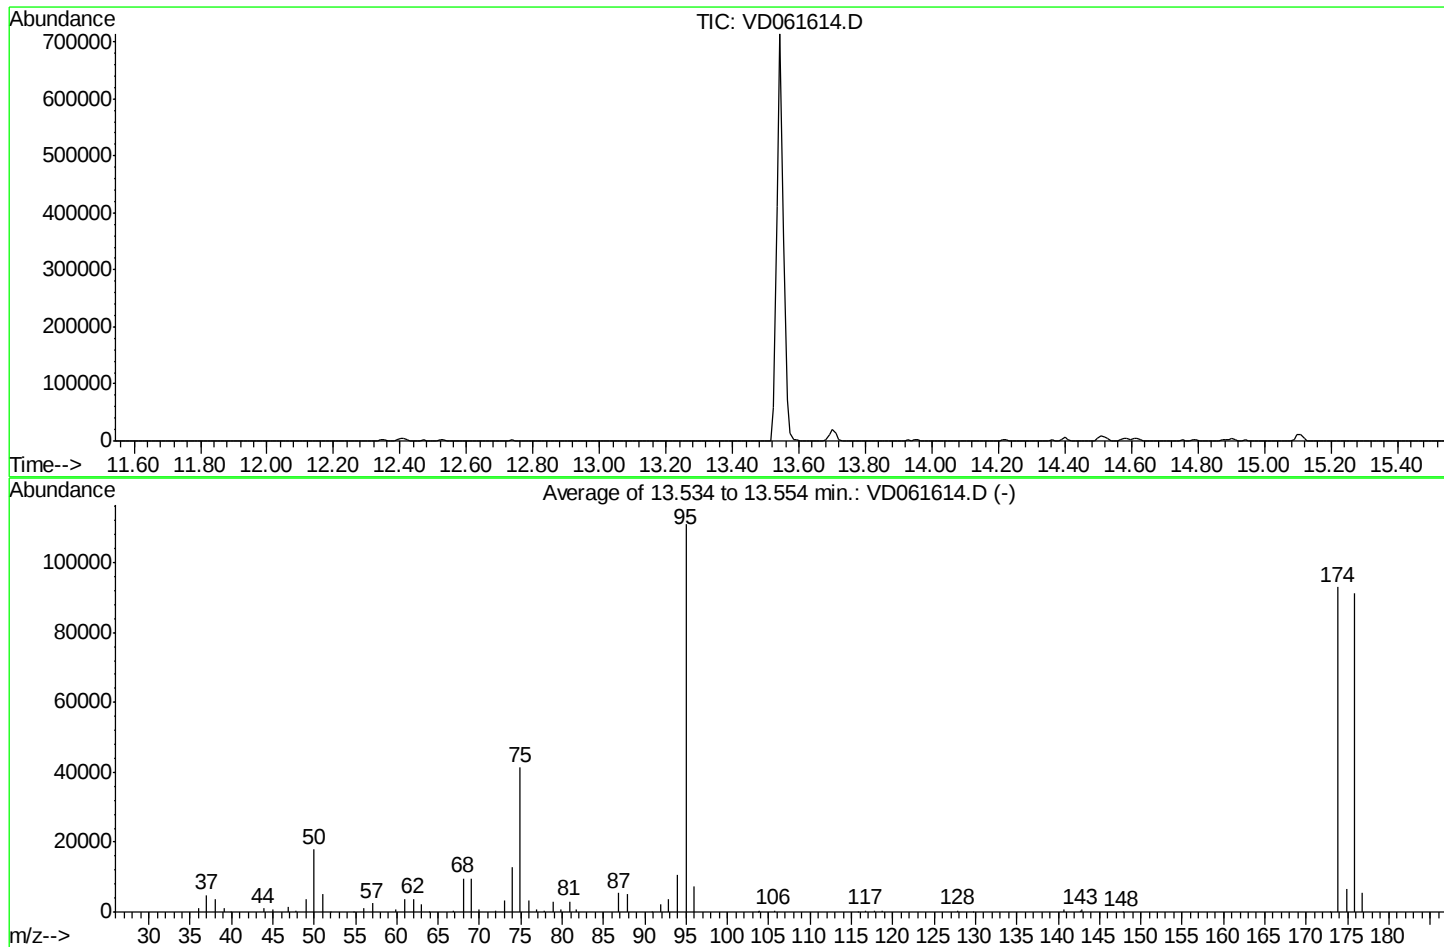

AutoFind: Scans 1230, 1231, 1232; Background Corrected with Scan 1225

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.1	17921	PASS
75	95	30	60	37.2	41250	PASS
95	95	100	100	100.0	110976	PASS
96	95	5	9	6.6	7365	PASS
173	174	0.00	2	0.1	126	PASS
174	95	50	100	83.8	92997	PASS
175	174	5	9	7.0	6545	PASS
176	174	95	101	98.0	91125	PASS
177	176	5	9	5.9	5406	PASS