

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD040522\
 Data File : VD072538.D
 Acq On : 05 Apr 2022 16:42
 Operator : VA/SY
 Sample : N2254-12
 Misc : 5.04G/5.00ml/MSVOA_D/SOIL
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 WC-14A-1A-4-GR-5

Quant Time: Apr 06 01:14:15 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D032922S.M
 Quant Title : SW846 8260
 QLast Update : Wed Mar 30 02:44:36 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	7.973	168	703968	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.861	114	1237092	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.638	117	1117770	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.561	152	478754	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.326	65	351957	41.330	ug/l	0.00
Spiked Amount 50.000	Range 50 - 163		Recovery =	82.660%		
35) Dibromofluoromethane	7.908	113	385596	40.108	ug/l	0.00
Spiked Amount 50.000	Range 54 - 147		Recovery =	80.220%		
50) Toluene-d8	10.332	98	1584673	47.419	ug/l	0.00
Spiked Amount 50.000	Range 49 - 140		Recovery =	94.840%		
62) 4-Bromofluorobenzene	12.620	95	516565	39.579	ug/l	0.00
Spiked Amount 50.000	Range 25 - 144		Recovery =	79.160%		
Target Compounds						Qvalue
10) Methyl Iodide	4.309	142	1394	3.902	ug/l #	60
13) Acrolein	4.132	56	7035	35.251	ug/l #	31
14) Allyl chloride	4.956	41	48762	5.420	ug/l #	58
15) Acrylonitrile	5.485	53	16088	8.927	ug/l #	35
16) Acetone	4.144	43	21035	13.247	ug/l #	71
17) Carbon Disulfide	4.403	76	1852	3.751	ug/l #	52
18) Methyl Acetate	4.950	43	107176	23.958	ug/l #	55
20) Methylene Chloride	4.967	84	37038	3.918	ug/l #	77
23) Vinyl Acetate	6.326	43	331	6.313	ug/l #	75
25) 2-Butanone	7.191	43	17436	7.939	ug/l #	52
31) Cyclohexane	7.979	56	133632	12.001	ug/l #	78
36) 1,1-Dichloropropene	7.973	75	56191	5.595	ug/l #	55
37) Ethyl Acetate	7.191	43	17436	3.423	ug/l #	75
38) Carbon Tetrachloride	7.979	117	74548	5.629	ug/l #	16
39) Methylcyclohexane	9.350	83	1707242	115.332	ug/l	97
41) Methacrylonitrile	7.561	41	1460	2.132	ug/l #	46
43) Isopropyl Acetate	8.444	43	114458	11.713	ug/l #	54
45) 1,2-Dichloropropane	9.350	63	18120	1.940	ug/l #	1
48) Methyl methacrylate	9.402	41	63779	13.444	ug/l #	19
49) 1,4-Dioxane	9.685	88	83	1.424	ug/l #	21
51) 4-Methyl-2-Pentanone	10.255	43	6333	1.208	ug/l	92
55) 1,1,2-Trichloroethane	10.767	97	183366	24.683	ug/l #	21
56) Ethyl methacrylate	10.673	69	81283	9.877	ug/l #	43
59) 2-Hexanone	10.944	43	187538	52.598	ug/l #	33
74) N-amyl acetate	12.261	43	95692	11.795	ug/l #	62
75) 1,1,2,2-Tetrachloroethane	12.696	83	15472	2.113	ug/l #	27
76) 1,2,3-Trichloropropane	12.620	75	256650	49.152	ug/l #	100
81) trans-1,4-Dichloro-2-b...	12.620	75	256650	120.609	ug/l #	8


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD040522\
Data File : VD072538.D
Acq On : 05 Apr 2022 16:42
Operator : VA/SY
Sample : N2254-12
Misc : 5.04G/5.00ml/MSVOA_D/SOIL
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
WC-14A-1A-4-GR-5

Quant Time: Apr 06 01:14:15 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D032922S.M
Quant Title : SW846 8260
QLast Update : Wed Mar 30 02:44:36 2022
Response via : Initial Calibration




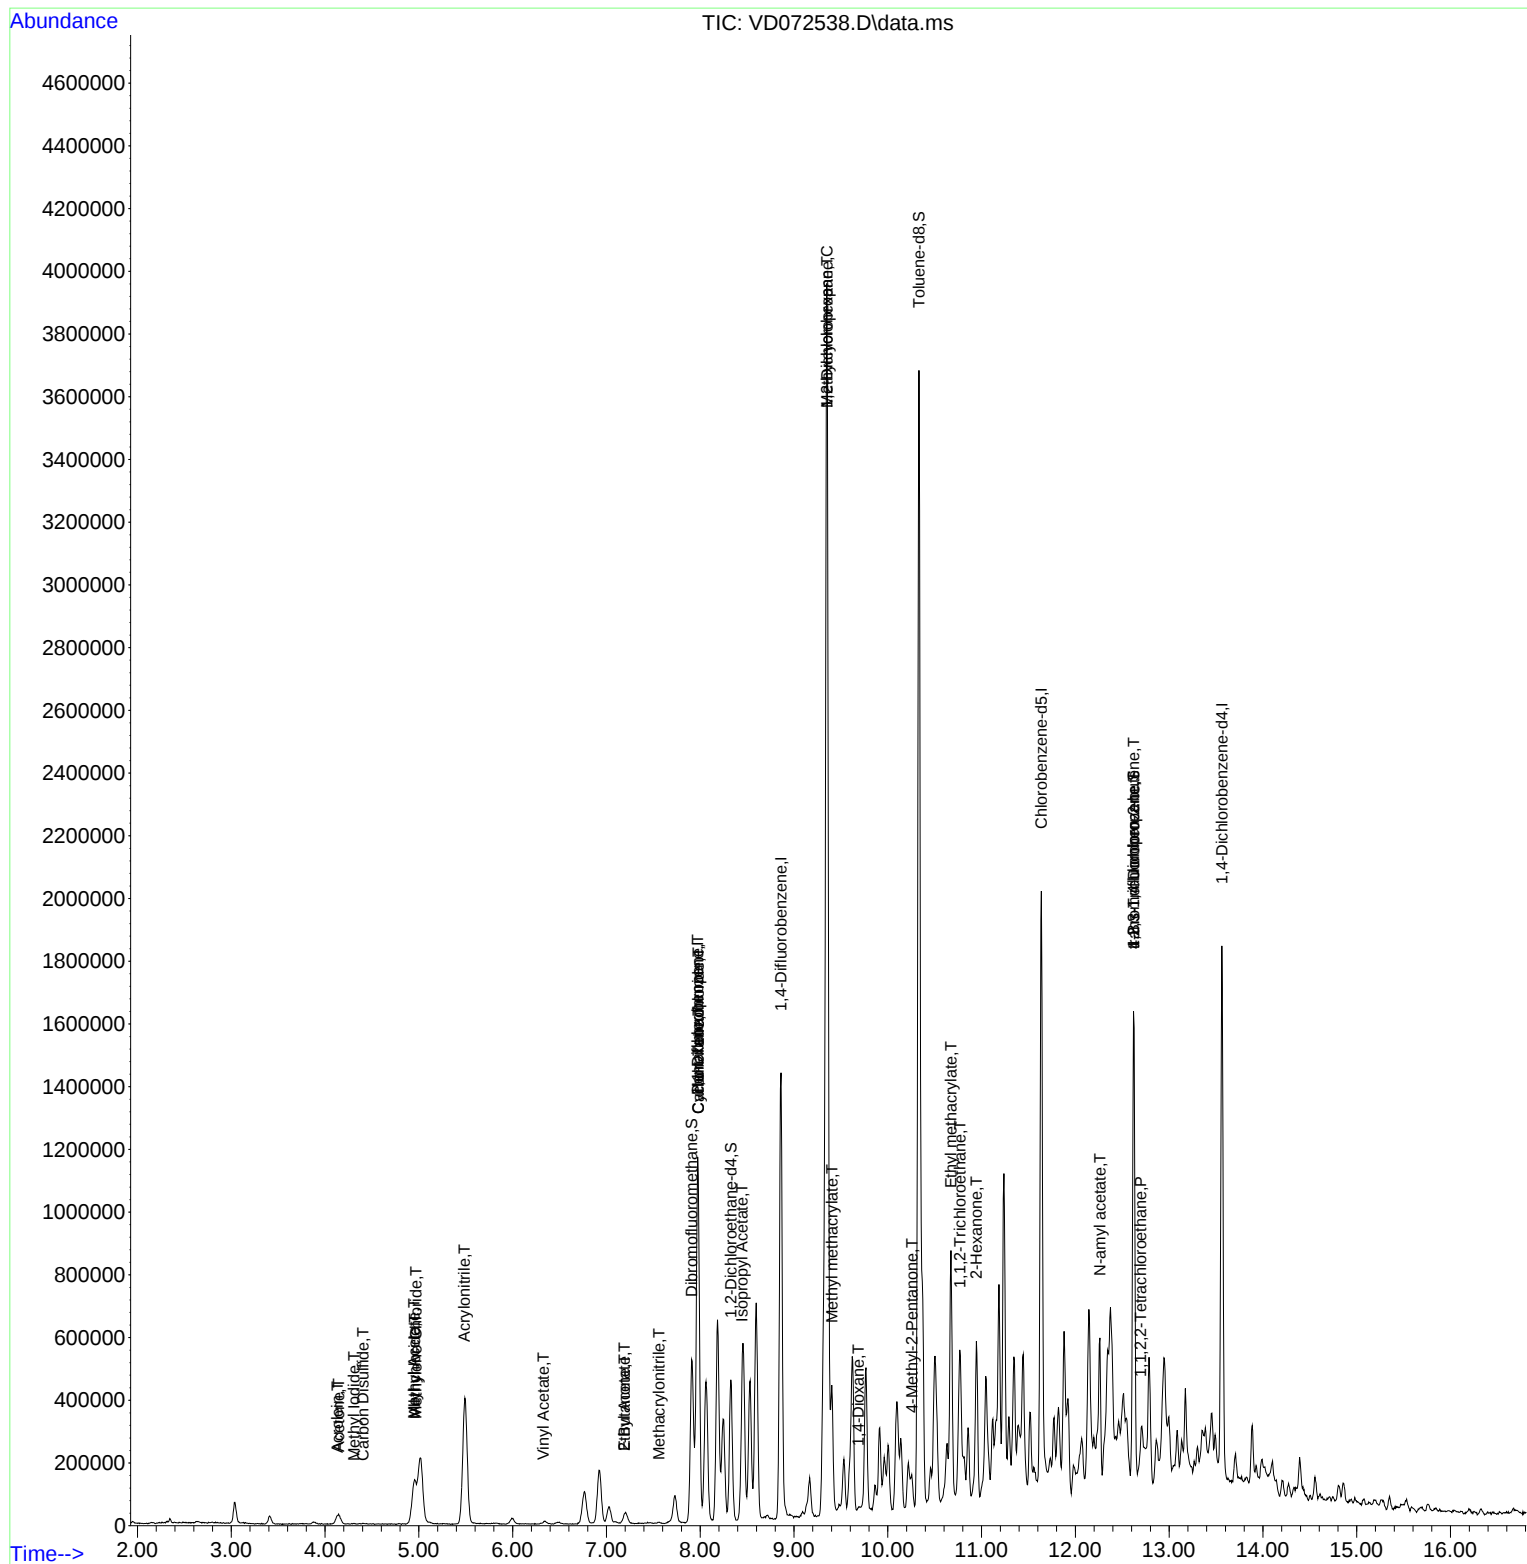




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.973 min Scan# 1029
Delta R.T. -0.006 min
Lab File: VD072538.D
Acq: 05 Apr 2022 16:42




Instrument :
MSVOA_D
ClientSampleId :
WC-14A-1A-4-GR-5


Tgt Ion:168 Resp: 703968
Ion Ratio Lower Upper
168 100
99 60.9 49.8 74.6

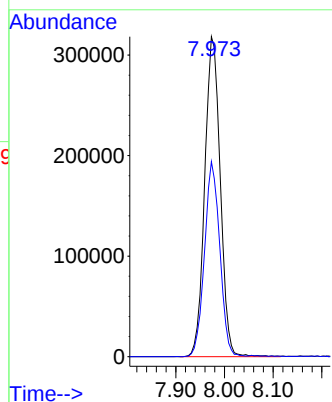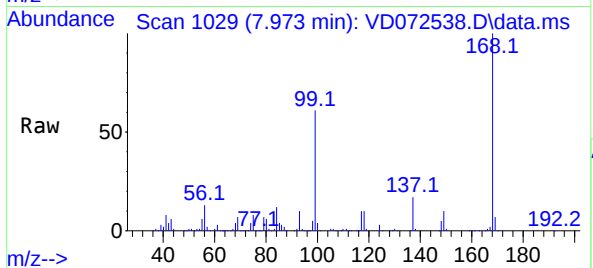

#10
Methyl Iodide
Concen: 3.902 ug/l
RT: 4.309 min Scan# 406
Delta R.T. 0.006 min
Lab File: VD072538.D
Acq: 05 Apr 2022 16:42

Tgt Ion:142 Resp: 1394
Ion Ratio Lower Upper
142 100
127 18.9 37.3 55.9#
141 0.0 11.7 17.5#


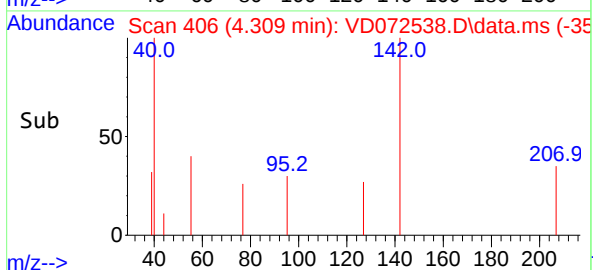






#13
Acrolein
Concen: 35.251 ug/l
RT: 4.132 min Scan# 31
Delta R.T. 0.212 min
Lab File: VD072538.D
Acq: 05 Apr 2022 16:42




Instrument :
MSVOA_D
ClientSampleId :
WC-14A-1A-4-GR-5


Tgt Ion: 56 Resp: 7035
Ion Ratio Lower Upper
56 100
55 14.2 57.1 85.7#



#14
Allyl chloride
Concen: 5.420 ug/l
RT: 4.956 min Scan# 516
Delta R.T. 0.236 min
Lab File: VD072538.D
Acq: 05 Apr 2022 16:42

Tgt Ion: 41 Resp: 48762
Ion Ratio Lower Upper
41 100
39 44.7 59.3 88.9#
76 0.0 25.7 38.5#


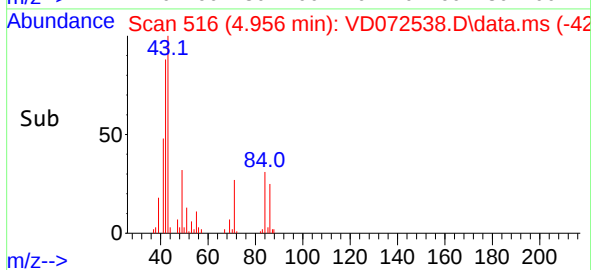






#15
Acrylonitrile
Concen: 8.927 ug/l
RT: 5.485 min Scan# 606
Delta R.T. 0.059 min
Lab File: VD072538.D
Acq: 05 Apr 2022 16:42




Instrument :
MSVOA_D
ClientSampleId :
WC-14A-1A-4-GR-5


Tgt Ion: 53 Resp: 16088
Ion Ratio Lower Upper
53 100
52 10.3 67.2 100.8#
51 55.6 30.3 45.5#

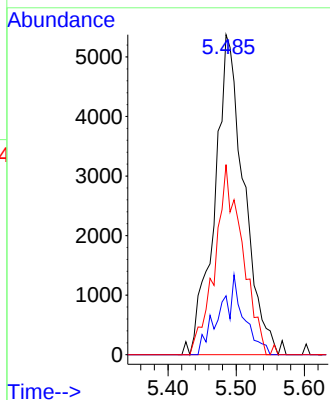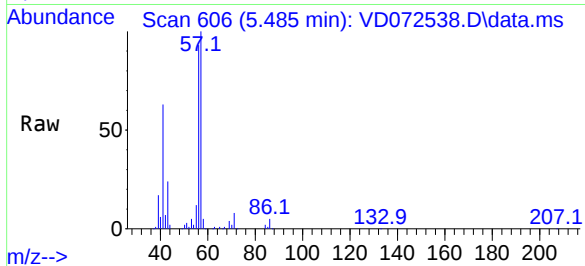

#16
Acetone
Concen: 13.247 ug/l
RT: 4.144 min Scan# 378
Delta R.T. -0.012 min
Lab File: VD072538.D
Acq: 05 Apr 2022 16:42

Tgt Ion: 43 Resp: 21035
Ion Ratio Lower Upper
43 100
58 12.5 22.1 33.1#


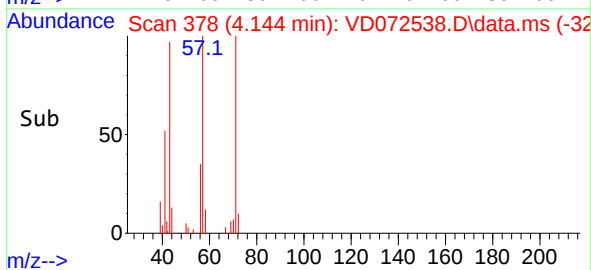
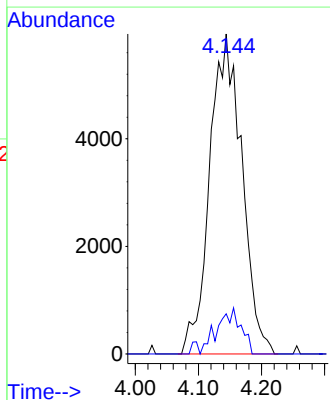
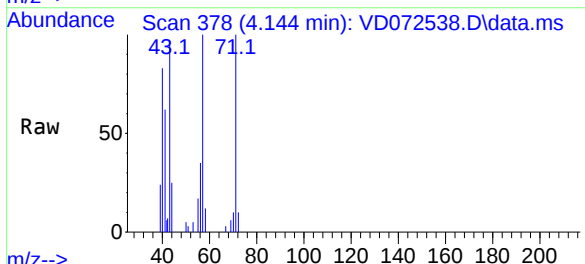




#17
Carbon Disulfide
Concen: 3.751 ug/l
RT: 4.403 min Scan# 41
Delta R.T. -0.011 min
Lab File: VD072538.D
Acq: 05 Apr 2022 16:42




Instrument :
MSVOA_D
ClientSampleId :
WC-14A-1A-4-GR-5


Tgt Ion: 76 Resp: 1852
Ion Ratio Lower Upper
76 100
78 26.7 7.5 11.3#

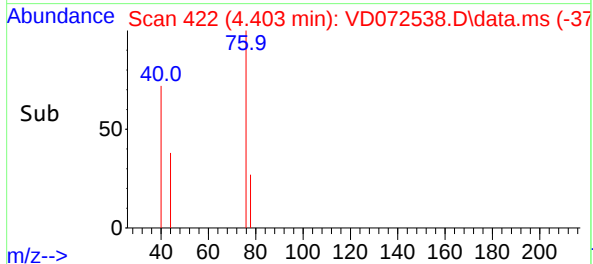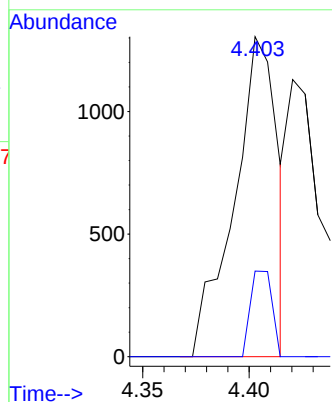

#18
Methyl Acetate
Concen: 23.958 ug/l
RT: 4.950 min Scan# 515
Delta R.T. 0.235 min
Lab File: VD072538.D
Acq: 05 Apr 2022 16:42

Tgt Ion: 43 Resp: 107176
Ion Ratio Lower Upper
43 100
74 0.0 16.7 25.1#


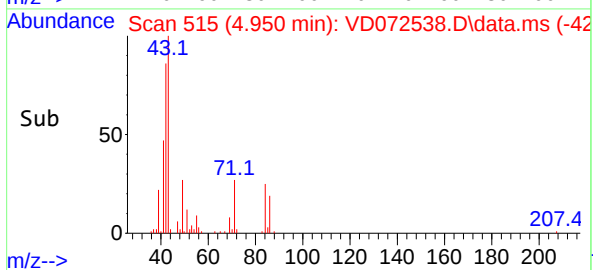
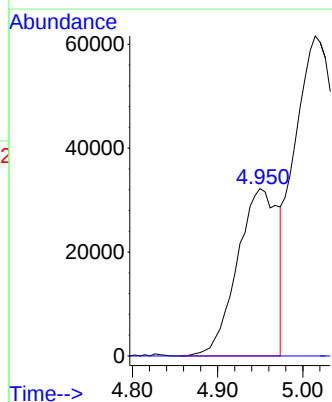
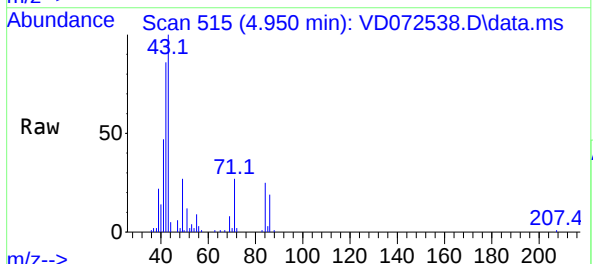




#20
Methylene Chloride
Concen: 3.918 ug/l
RT: 4.967 min Scan# 517
Delta R.T. 0.006 min
Lab File: VD072538.D
Acq: 05 Apr 2022 16:42




Instrument :
MSVOA_D
ClientSampleId :
WC-14A-1A-4-GR-5


Tgt Ion: 84 Resp: 37038
Ion Ratio Lower Upper
84 100
49 103.8 112.8 169.2#
51 40.1 32.6 48.8
86 76.3 47.9 71.9#

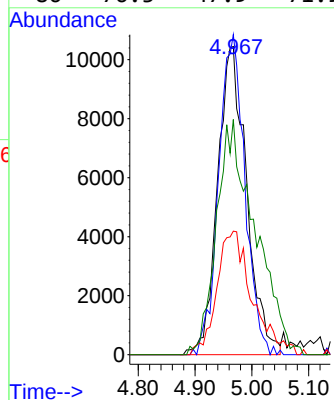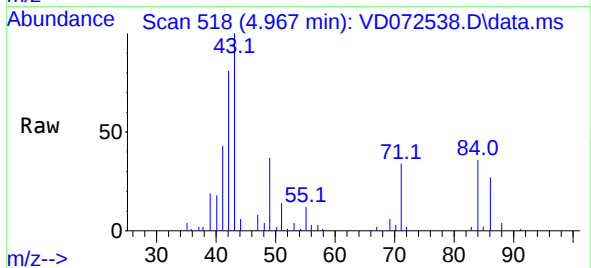

#23
Vinyl Acetate
Concen: 6.313 ug/l
RT: 6.326 min Scan# 749
Delta R.T. 0.023 min
Lab File: VD072538.D
Acq: 05 Apr 2022 16:42

Tgt Ion: 43 Resp: 331
Ion Ratio Lower Upper
43 100
86 0.0 7.1 10.7#


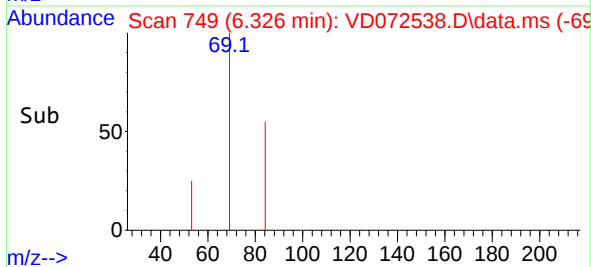
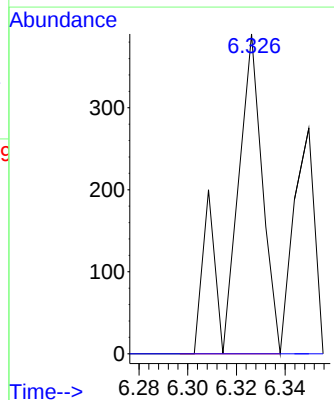
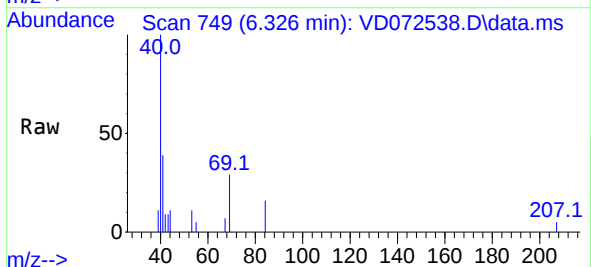




#25
2-Butanone
Concen: 7.939 ug/l
RT: 7.191 min Scan# 896
Delta R.T. -0.018 min
Lab File: VD072538.D
Acq: 05 Apr 2022 16:42




Instrument :
MSVOA_D
ClientSampleId :
WC-14A-1A-4-GR-5


Tgt Ion: 43 Resp: 17436
Ion Ratio Lower Upper
43 100
72 0.0 18.6 27.8#

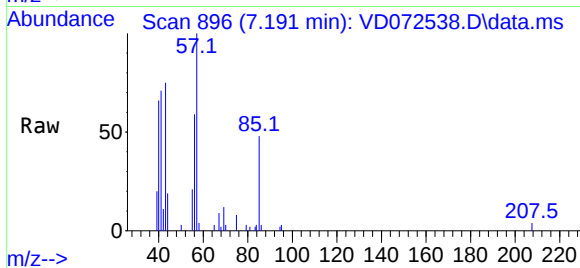

#31
Cyclohexane
Concen: 12.001 ug/l
RT: 7.979 min Scan# 1030
Delta R.T. -0.006 min
Lab File: VD072538.D
Acq: 05 Apr 2022 16:42

Tgt Ion: 56 Resp: 133632
Ion Ratio Lower Upper
56 100
69 49.6 25.4 38.2#
84 94.0 63.0 94.4

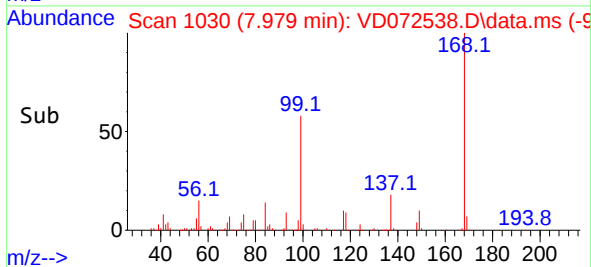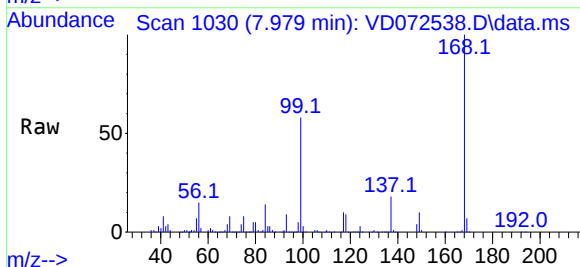



#33

1,2-Dichloroethane-d4

Concen: 41.330 ug/l

RT: 8.326 min Scan# 1089

Delta R.T. 0.000 min

Lab File: VD072538.D

Acq: 05 Apr 2022 16:42

Instrument :

MSVOA_D

ClientSampleId :





WC-14A-1A-4-GR-5

Tgt Ion: 65 Resp: 351957

Ion Ratio Lower Upper

65 100

67 53.8 0.0 101.4

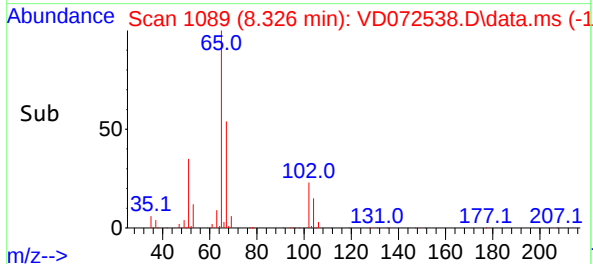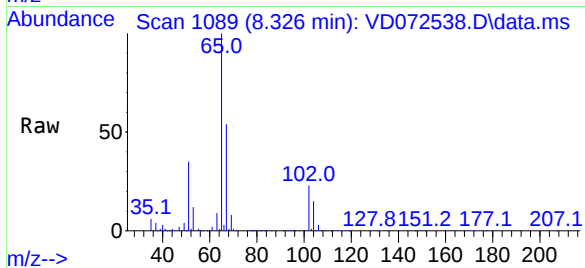

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.861 min Scan# 1180

Delta R.T. 0.000 min

Lab File: VD072538.D

Acq: 05 Apr 2022 16:42




Tgt Ion: 114 Resp: 1237092


Ion Ratio Lower Upper

114 100

63 19.1 0.0 46.6

88 16.1 0.0 33.2

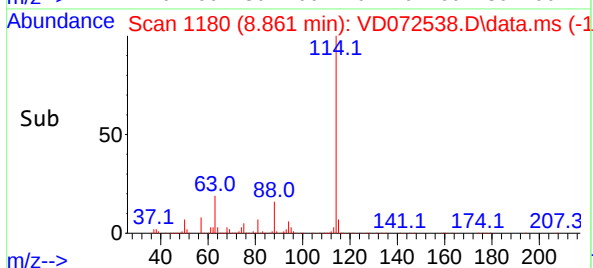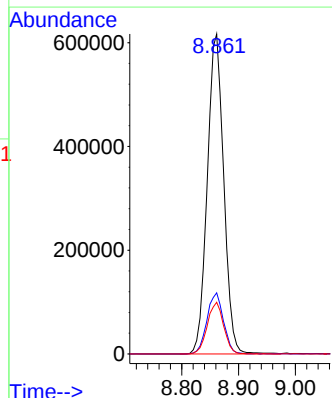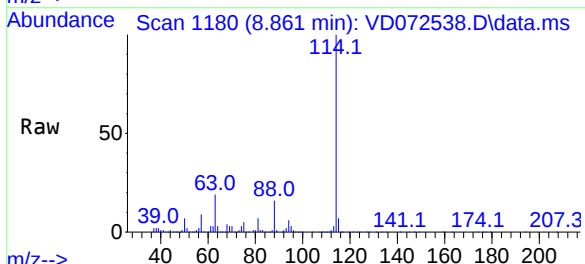



#35

Dibromofluoromethane

Concen: 40.108 ug/l

RT: 7.908 min Scan# 1018

Delta R.T. -0.006 min

Lab File: VD072538.D

Acq: 05 Apr 2022 16:42

Instrument :

MSVOA_D

ClientSampleId :

WC-14A-1A-4-GR-5





Tgt Ion:113 Resp: 385596

Ion Ratio Lower Upper

113 100

111 102.2 83.8 125.6

192 18.5 14.6 21.8

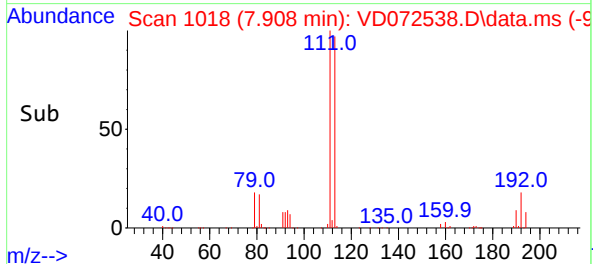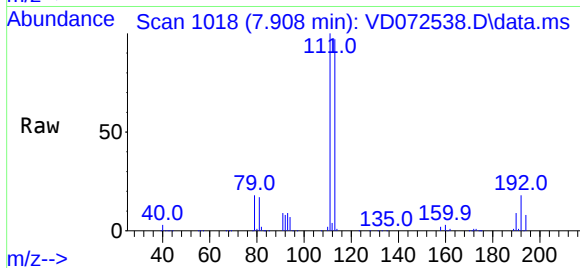

#36

1,1-Dichloropropene

Concen: 5.595 ug/l

RT: 7.973 min Scan# 1029

Delta R.T. -0.135 min

Lab File: VD072538.D

Acq: 05 Apr 2022 16:42




Tgt Ion: 75 Resp: 56191


Ion Ratio Lower Upper

75 100

110 10.1 16.4 49.1#

77 3.2 24.2 36.2#


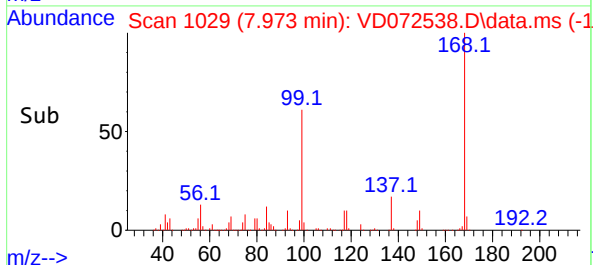
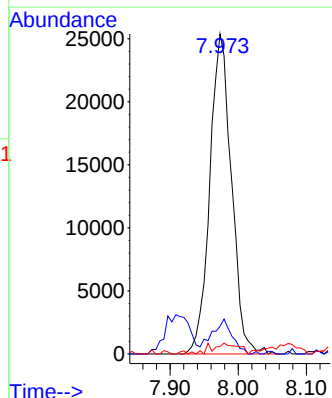
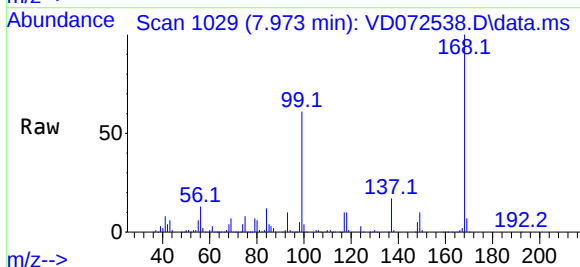




#37
Ethyl Acetate
Concen: 3.423 ug/l
RT: 7.191 min Scan# 896
Delta R.T. -0.100 min
Lab File: VD072538.D
Acq: 05 Apr 2022 16:42




Instrument :
MSVOA_D
ClientSampleId :
WC-14A-1A-4-GR-5


Tgt Ion: 43 Resp: 17436
Ion Ratio Lower Upper
43 100
61 0.0 9.8 14.8#
70 2.7 6.9 10.3#

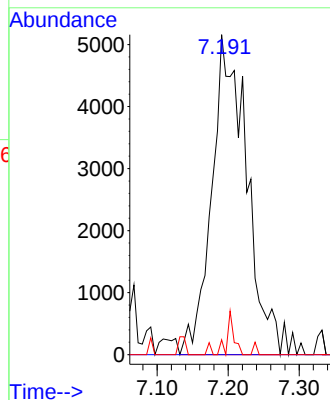

#38
Carbon Tetrachloride
Concen: 5.629 ug/l
RT: 7.979 min Scan# 1030
Delta R.T. -0.112 min
Lab File: VD072538.D
Acq: 05 Apr 2022 16:42

Tgt Ion: 117 Resp: 74548
Ion Ratio Lower Upper
117 100
119 4.3 75.8 113.6#
121 0.6 24.5 36.7#

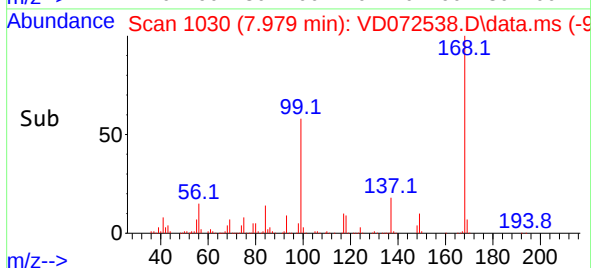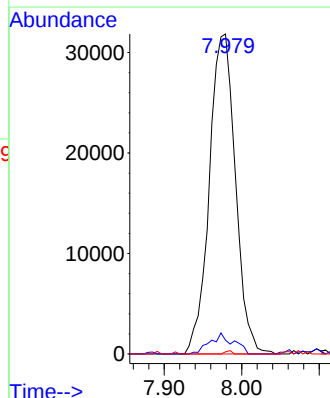



#39

Methylcyclohexane

Concen: 115.332 ug/l

RT: 9.350 min Scan# 11

Delta R.T. -0.005 min

Lab File: VD072538.D

Acq: 05 Apr 2022 16:42

Instrument :

MSVOA_D

ClientSampleId :

WC-14A-1A-4-GR-5





Tgt Ion: 83 Resp: 1707242

Ion Ratio Lower Upper

83 100

55 76.8 63.2 94.8

98 50.5 38.2 57.4

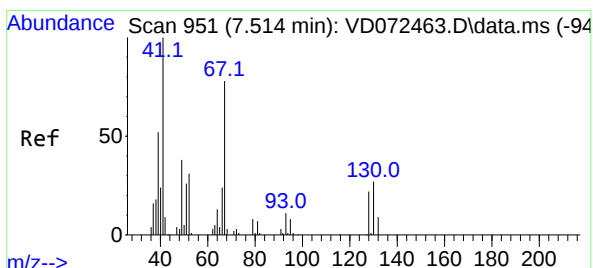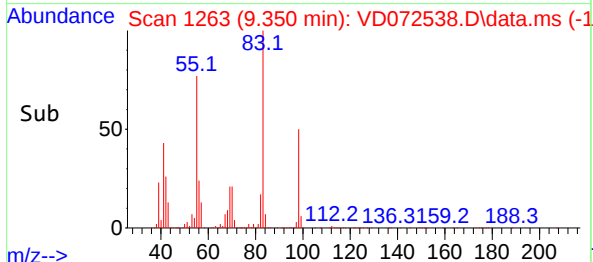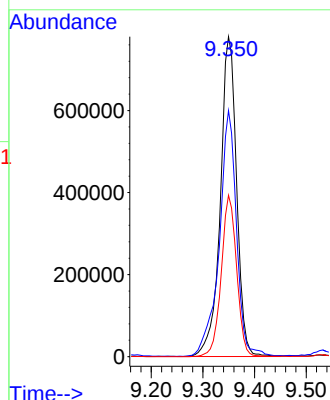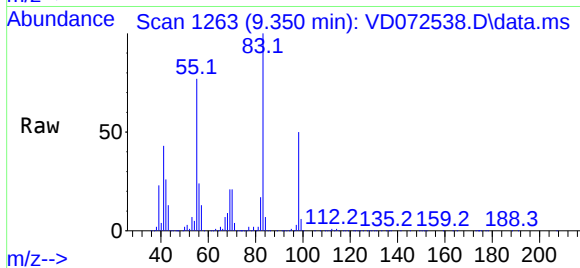

#41

Methacrylonitrile

Concen: 2.132 ug/l

RT: 7.561 min Scan# 959

Delta R.T. 0.047 min

Lab File: VD072538.D

Acq: 05 Apr 2022 16:42

Tgt Ion: 41 Resp: 1460




Ion Ratio Lower Upper


41 100

39 37.1 44.6 67.0#

67 0.0 48.2 72.4#

52 0.0 22.8 34.2#


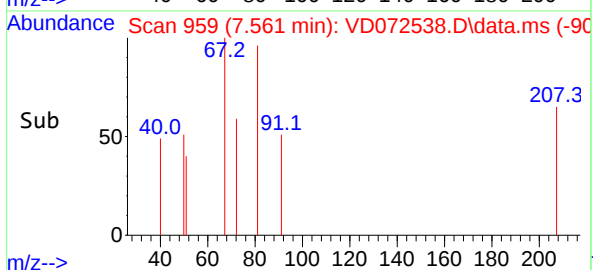
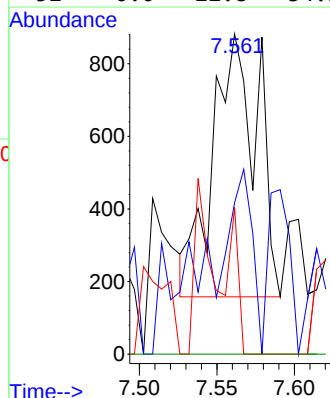
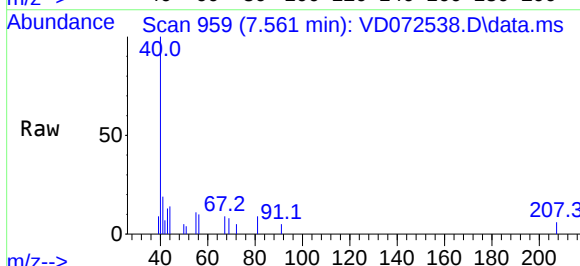




#43
Isopropyl Acetate
Concen: 11.713 ug/l
RT: 8.444 min Scan# 1110
Delta R.T. -0.006 min
Lab File: VD072538.D
Acq: 05 Apr 2022 16:42




Instrument :
MSVOA_D
ClientSampleId :
WC-14A-1A-4-GR-5


Tgt Ion: 43 Resp: 114458
Ion Ratio Lower Upper
43 100
61 0.0 22.4 33.6#
87 0.0 8.7 13.1#

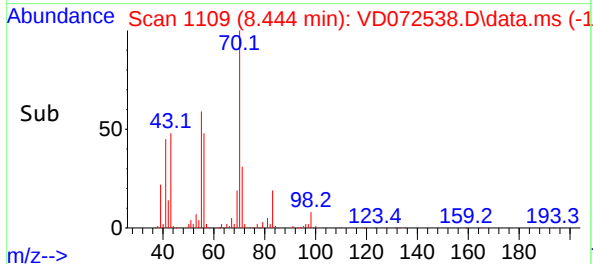

#45
1,2-Dichloropropane
Concen: 1.940 ug/l
RT: 9.350 min Scan# 1263
Delta R.T. -0.035 min
Lab File: VD072538.D
Acq: 05 Apr 2022 16:42

Tgt Ion: 63 Resp: 18120
Ion Ratio Lower Upper
63 100
65 214.7 26.2 39.4#

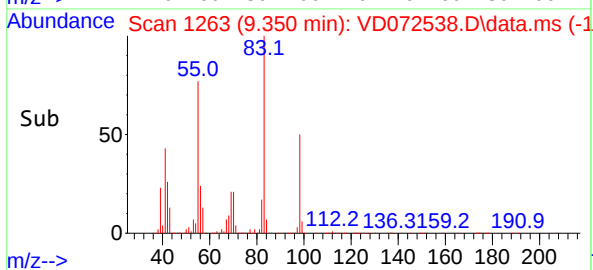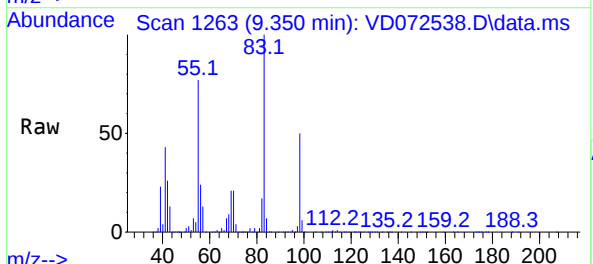



#48

Methyl methacrylate

Concen: 13.444 ug/l

RT: 9.402 min Scan# 11

Delta R.T. -0.047 min

Lab File: VD072538.D

Acq: 05 Apr 2022 16:42

Instrument :

MSVOA_D

ClientSampleId :

WC-14A-1A-4-GR-5





Tgt Ion: 41 Resp: 63779

Ion Ratio Lower Upper

41 100

69 0.0 56.7 85.1#

39 0.0 42.7 64.1#

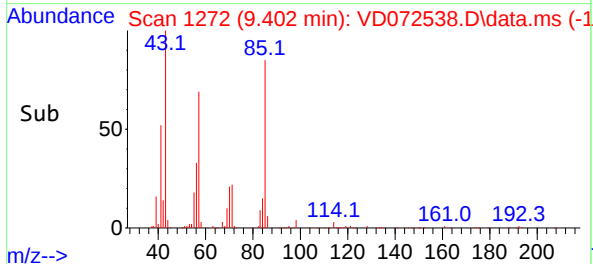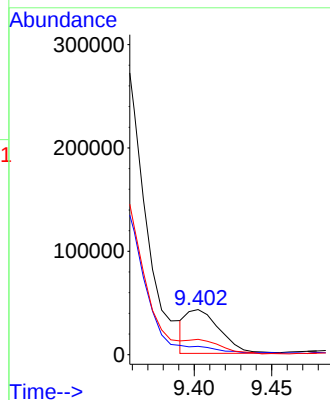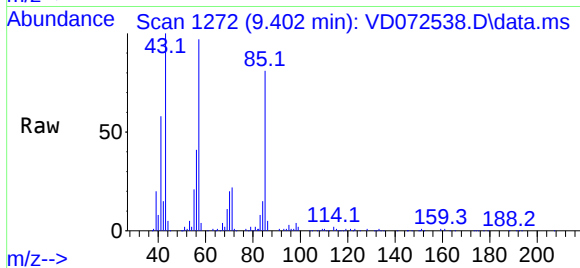

#49

1,4-Dioxane

Concen: 1.424 ug/l

RT: 9.685 min Scan# 1320

Delta R.T. 0.229 min

Lab File: VD072538.D

Acq: 05 Apr 2022 16:42




Tgt Ion: 88 Resp: 83


Ion Ratio Lower Upper

88 100

43 0.0 31.0 46.4#

58 0.0 58.1 87.1#


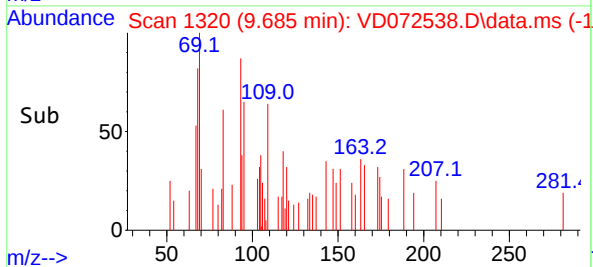
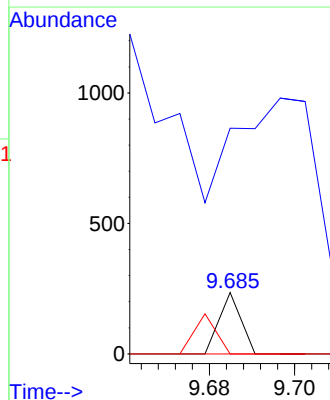
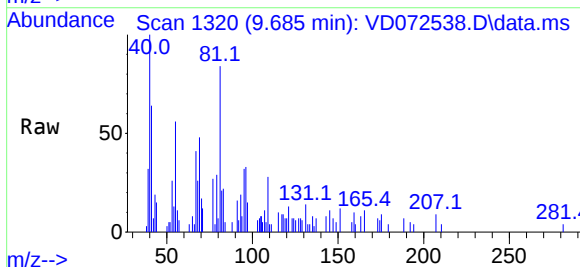




#50
Toluene-d8
Concen: 47.419 ug/l
RT: 10.332 min Scan# 1417
Delta R.T. -0.006 min
Lab File: VD072538.D
Acq: 05 Apr 2022 16:42




Instrument :
MSVOA_D
ClientSampleId :
WC-14A-1A-4-GR-5


Tgt Ion: 98 Resp: 1584673
Ion Ratio Lower Upper
98 100
100 63.1 52.4 78.6

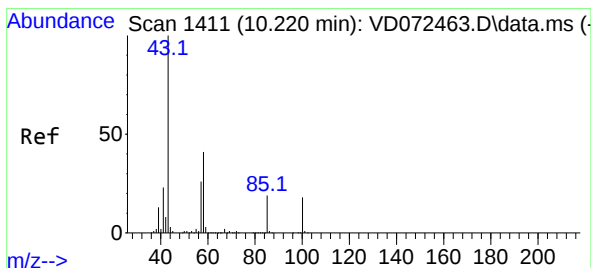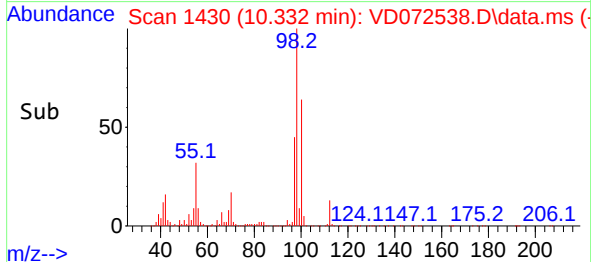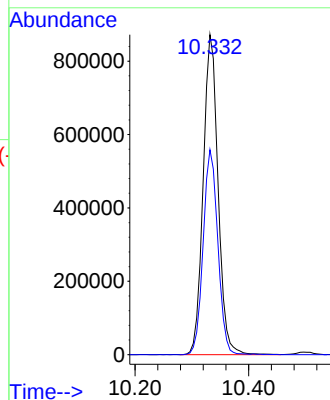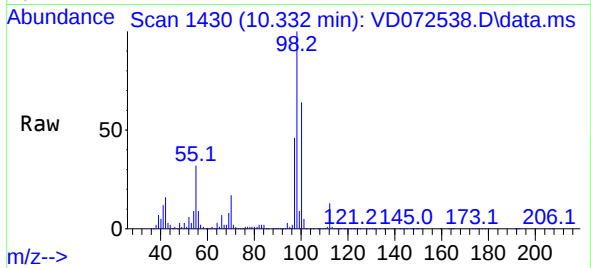

#51
4-Methyl-2-Pentanone
Concen: 1.208 ug/l
RT: 10.255 min Scan# 1417
Delta R.T. 0.035 min
Lab File: VD072538.D
Acq: 05 Apr 2022 16:42

Tgt Ion: 43 Resp: 6333
Ion Ratio Lower Upper
43 100
58 31.2 28.6 43.0

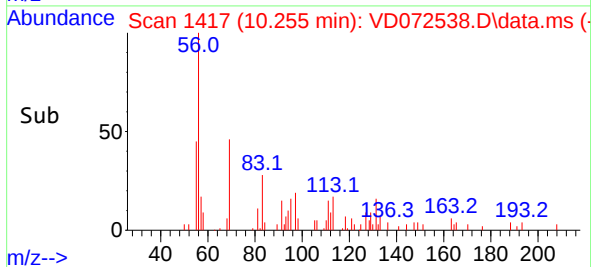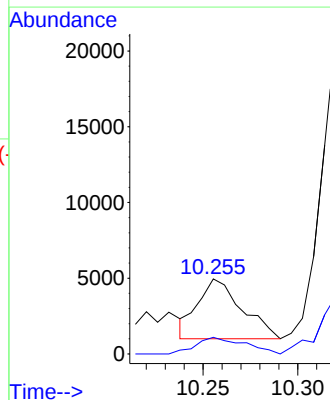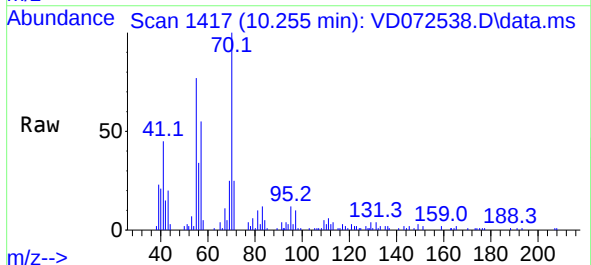







#55
1,1,2-Trichloroethane
Concen: 24.683 ug/l
RT: 10.767 min Scan# 11
Delta R.T. -0.029 min
Lab File: VD072538.D
Acq: 05 Apr 2022 16:42

Instrument :
MSVOA_D
ClientSampleId :
WC-14A-1A-4-GR-5

Tgt Ion: 97 Resp: 183366




Ion	Ratio	Lower	Upper
97	100		
83	9.5	69.0	103.4#
85	3.5	42.6	63.8#
99	0.4	51.7	77.5#

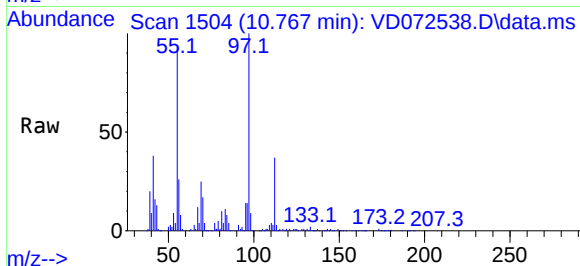


#56
Ethyl methacrylate
Concen: 9.877 ug/l
RT: 10.673 min Scan# 1488
Delta R.T. 0.018 min
Lab File: VD072538.D
Acq: 05 Apr 2022 16:42

Tgt Ion: 69 Resp: 81283

Ion	Ratio	Lower	Upper
69	100		
41	135.4	63.0	94.6#
39	68.8	33.8	50.8#

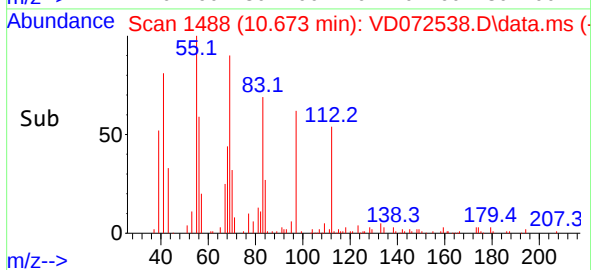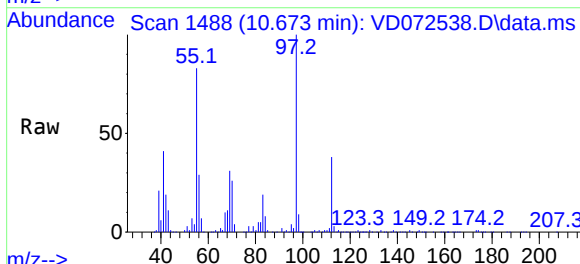



#59

2-Hexanone

Concen: 52.598 ug/l

RT: 10.944 min Scan# 11

Delta R.T. -0.035 min

Lab File: VD072538.D

Acq: 05 Apr 2022 16:42

Instrument :

MSVOA_D

ClientSampleId :





WC-14A-1A-4-GR-5

Tgt Ion: 43 Resp: 187538

Ion Ratio Lower Upper

43 100

58 4.0 25.3 75.9#

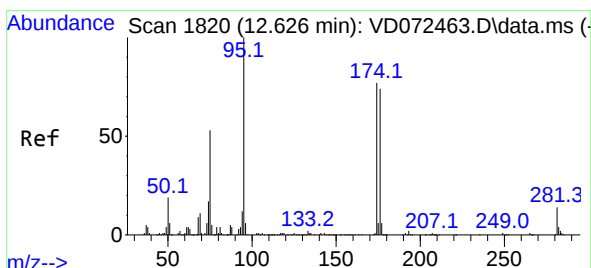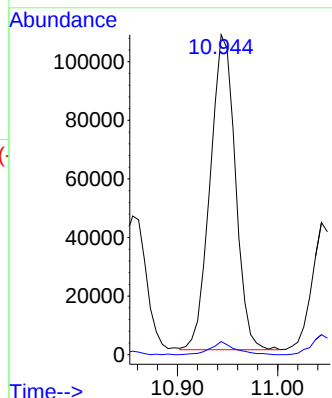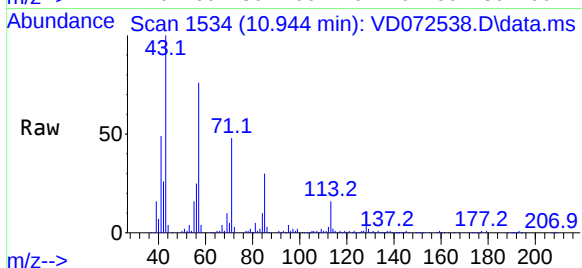

#62

4-Bromofluorobenzene

Concen: 39.579 ug/l

RT: 12.620 min Scan# 1819

Delta R.T. -0.006 min

Lab File: VD072538.D

Acq: 05 Apr 2022 16:42




Tgt Ion: 95 Resp: 516565


Ion Ratio Lower Upper

95 100

174 76.1 0.0 152.8


176 72.5 0.0 145.4

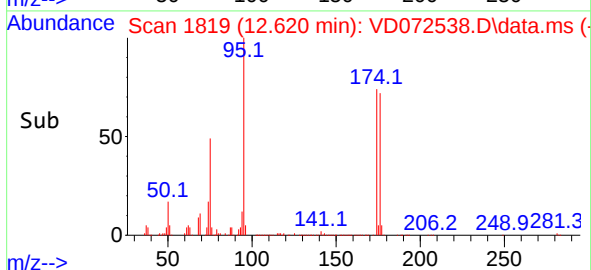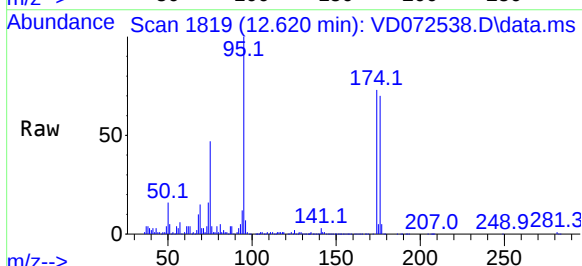



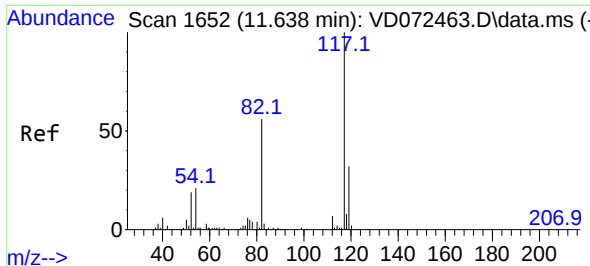


#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.638 min Scan# 117770
Delta R.T. 0.000 min
Lab File: VD072538.D
Acq: 05 Apr 2022 16:42

Instrument :
MSVOA_D
ClientSampleId :
WC-14A-1A-4-GR-5



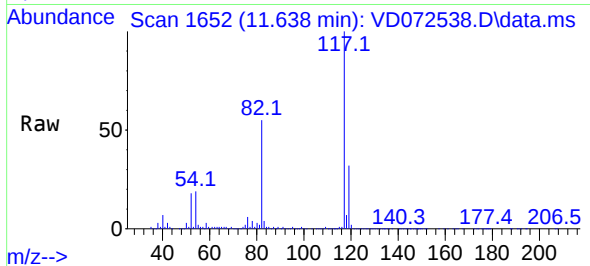



Tgt Ion:117 Resp: 1117770
Ion Ratio Lower Upper
117 100
82 54.3 45.3 67.9
119 32.3 26.6 40.0

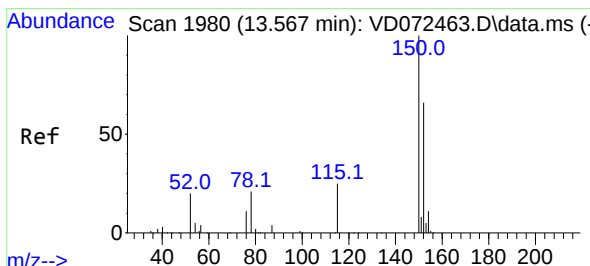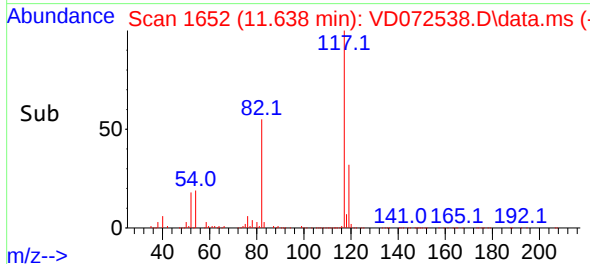

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.561 min Scan# 1979
Delta R.T. -0.006 min
Lab File: VD072538.D
Acq: 05 Apr 2022 16:42

Tgt Ion:152 Resp: 478754
Ion Ratio Lower Upper
152 100
115 61.6 31.3 93.8
150 157.4 0.0 348.6

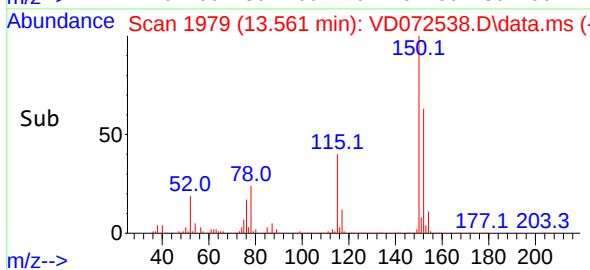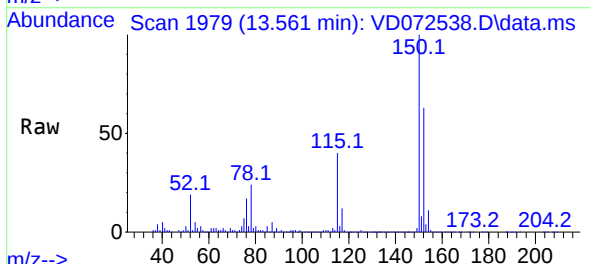







#74
N-amy1 acetate
Concen: 11.795 ug/l
RT: 12.261 min Scan# 11
Delta R.T. -0.018 min
Lab File: VD072538.D
Acq: 05 Apr 2022 16:42

Instrument :
MSVOA_D
ClientSampleId :
WC-14A-1A-4-GR-5

Tgt Ion: 43 Resp: 95692




Ion	Ratio	Lower	Upper
43	100		
70	24.1	31.3	46.9#
55	0.0	20.0	30.0#
61	0.0	17.8	26.8#

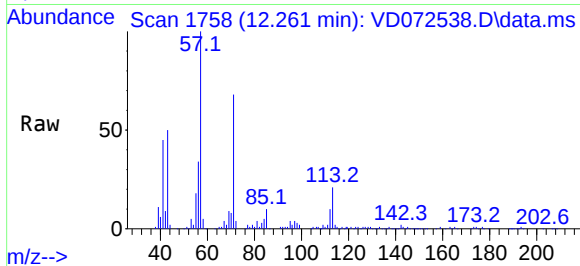


#75
1,1,2,2-Tetrachloroethane
Concen: 2.113 ug/l
RT: 12.696 min Scan# 1832
Delta R.T. -0.023 min
Lab File: VD072538.D
Acq: 05 Apr 2022 16:42

Tgt Ion: 83 Resp: 15472

Ion	Ratio	Lower	Upper
83	100		
131	5.1	5.0	14.9
85	0.0	32.6	98.0#


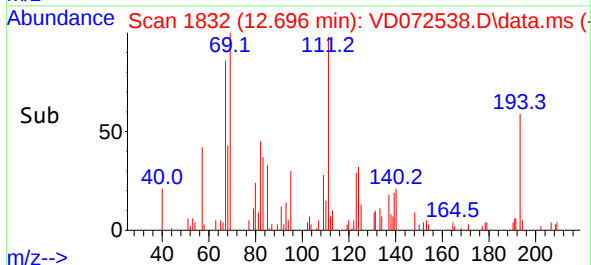
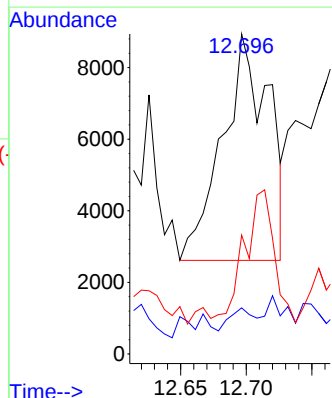
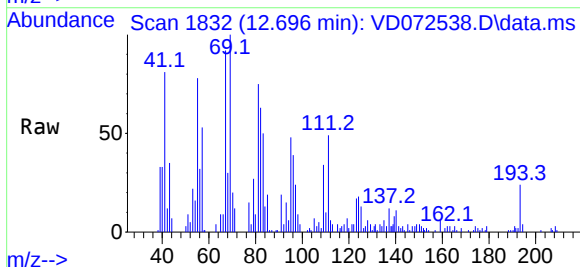




#76
1,2,3-Trichloropropane
Concen: 49.152 ug/l
RT: 12.620 min Scan# 1819
Delta R.T. -0.153 min
Lab File: VD072538.D
Acq: 05 Apr 2022 16:42

Instrument :
MSVOA_D
ClientSampleId :
WC-14A-1A-4-GR-5

Tgt Ion: 75 Resp: 256650
Ion Ratio Lower Upper
75 100
77 1.7 0.0 0.0#

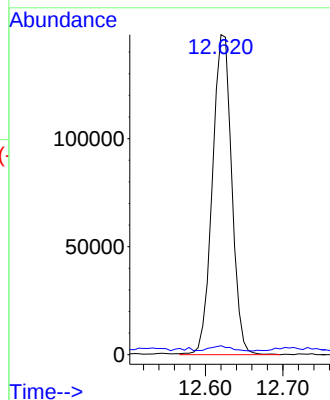

#81
trans-1,4-Dichloro-2-butene
Concen: 120.609 ug/l
RT: 12.620 min Scan# 1819
Delta R.T. 0.100 min
Lab File: VD072538.D
Acq: 05 Apr 2022 16:42

Tgt Ion: 75 Resp: 256650
Ion Ratio Lower Upper
75 100
53 1.3 86.5 129.7#
89 0.0 33.9 50.9#

