
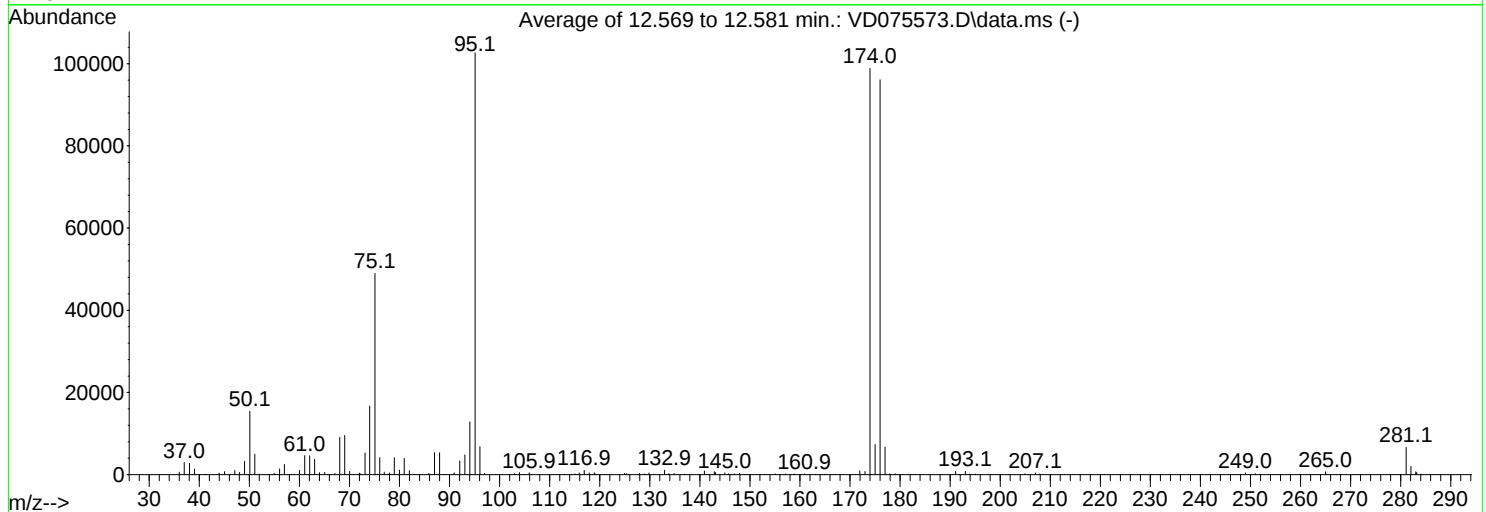


Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD040523\
Data File : VD075573.D
Acq On : 05 Apr 2023 11:20
Operator : KP/SY
Sample : BFB114
Misc : 5.00G/10.00ml/MSVOA_D/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB114

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\SFAMDLM033123SMA.M
Title : SFAM01.0
Last Update : Sat Apr 01 00:08:20 2023

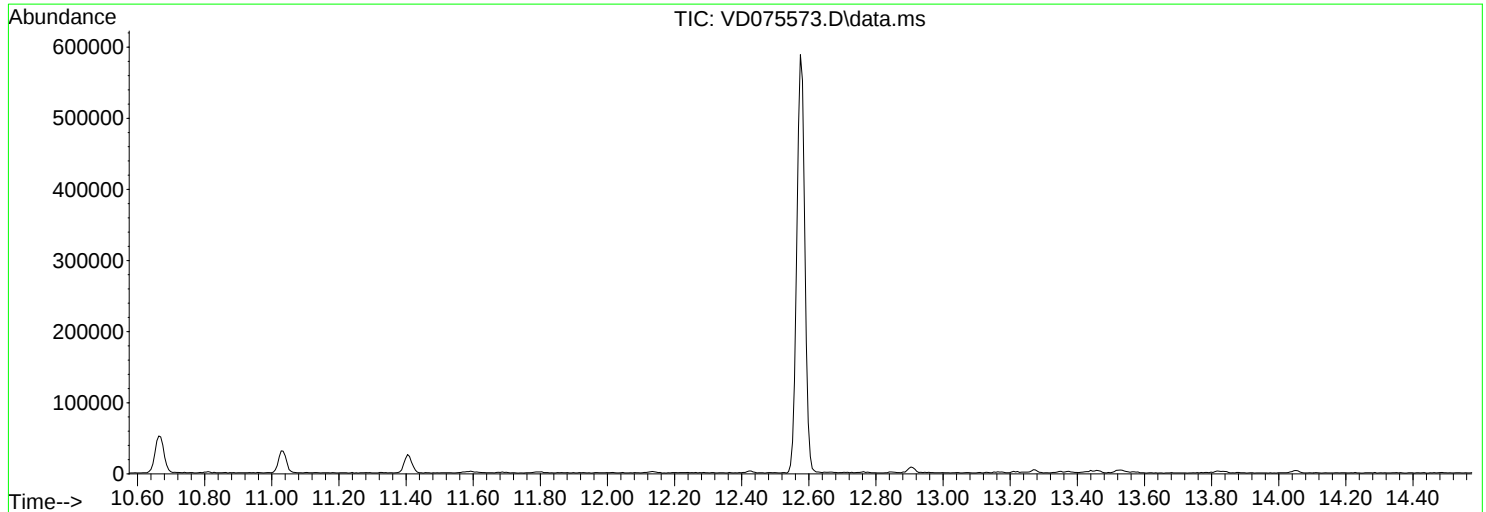

AutoFind: Scans 1867, 1868, 1869; Background Corrected with Scan 1860

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	15.0	15420	PASS
75	95	30	80	47.7	48989	PASS
95	95	100	100	100.0	102640	PASS
96	95	5	9	6.6	6799	PASS
173	174	0.00	2	0.8	786	PASS
174	95	50	120	96.3	98864	PASS
175	174	5	9	7.4	7324	PASS
176	174	95	105	97.2	96096	PASS
177	176	5	10	7.0	6693	PASS

Scan 1860 (12.528 min): VD075573.D\data.ms
BFB114

m/z	Abundance
40.00	1142.0
43.90	572.0
207.20	173.0

Instrument :
MSVOA_D
ClientSampleId :
BFB114

m/z	Abundance
35.90	537.0
37.00	2696.0
38.00	2490.0
39.00	1335.0
40.00	952.0
41.20	202.0
43.90	873.0
45.10	573.0
47.20	809.0
48.00	411.0
49.00	2944.0
50.10	14894.0
51.10	4559.0
53.00	169.0
54.90	359.0
56.00	1476.0
57.00	2324.0
60.00	1083.0
61.10	4050.0
62.10	3654.0
63.00	3732.0
64.10	454.0
65.20	366.0
67.10	333.0
68.10	8104.0
69.10	8582.0
70.00	706.0
72.00	399.0
73.10	4713.0
74.10	16209.0
75.10	46872.0
76.10	3616.0
77.00	630.0
78.00	531.0
79.00	4026.0
80.00	985.0
80.90	3913.0
82.00	1226.0
86.00	212.0
87.00	4339.0
88.00	4443.0
88.90	289.0
90.90	369.0
92.10	3611.0
93.10	4145.0
94.10	11385.0
95.10	93528.0
96.10	6107.0
97.00	247.0
103.30	204.0
104.00	442.0
105.90	345.0
111.90	154.0
115.10	187.0
115.80	331.0
116.90	1026.0
117.90	369.0
119.00	755.0
124.90	358.0
125.90	194.0
127.80	235.0
129.00	237.0
129.80	430.0
130.80	150.0
132.90	855.0
133.80	214.0
134.90	341.0
136.80	161.0
140.90	1028.0
142.00	248.0
142.90	1154.0
145.00	516.0
145.70	232.0
146.70	167.0
148.10	237.0
155.10	233.0
157.10	215.0
161.00	168.0
171.90	991.0
173.00	492.0
174.00	85368.0
175.00	6048.0
176.00	85256.0
177.00	6259.0
177.80	205.0
178.80	164.0
191.20	344.0
193.10	498.0
207.10	486.0
207.80	157.0
248.90	181.0
251.10	195.0

Instrument :
MSVOA_D
ClientSampleId :
BFB114

265.00	475.0
281.10	4390.0
282.00	1362.0
283.00	965.0

Instrument :
MSVOA_D
ClientSampleId :
BFB114

m/z	Abundance
36.00	708.0
37.00	3455.0
38.10	3022.0
39.10	1599.0
40.00	1023.0
44.00	983.0
45.00	784.0
46.20	178.0
47.00	970.0
48.10	660.0
49.10	3809.0
50.10	16212.0
51.10	5075.0
52.00	331.0
55.00	400.0
56.10	1234.0
57.00	2836.0
60.00	998.0
61.00	4983.0
62.00	5100.0
63.00	4115.0
64.00	556.0
65.00	797.0
67.20	210.0
68.00	10049.0
69.00	10520.0
70.10	659.0
72.00	742.0
73.10	5711.0
74.10	18304.0
75.10	53360.0
76.10	5139.0
76.90	643.0
78.10	519.0
78.90	4512.0
80.00	1353.0
81.00	4433.0
81.90	992.0
85.80	417.0
87.00	5840.0
88.00	6047.0
91.00	693.0
92.00	3587.0
93.00	5647.0
94.10	13759.0
95.10	112120.0
96.00	7968.0
96.90	392.0
103.00	296.0
103.90	697.0
105.00	221.0
106.00	524.0
107.00	250.0
115.00	244.0
115.90	536.0
116.90	1017.0
117.90	439.0
118.80	609.0
125.00	520.0
125.80	201.0
128.00	400.0
128.90	236.0
129.90	615.0
130.90	187.0
133.00	1091.0
133.80	454.0
134.80	250.0
136.90	208.0
140.90	1022.0
143.10	1568.0
145.00	461.0
146.00	280.0
146.90	337.0
147.90	293.0
148.90	174.0
149.80	167.0
155.00	314.0
156.80	214.0
158.90	160.0
160.80	219.0
165.00	167.0
172.00	754.0
173.00	997.0
174.00	107032.0
175.00	8608.0
176.00	101392.0
177.00	6648.0
177.90	216.0
179.10	417.0
191.00	683.0
191.90	172.0
193.10	786.0

Instrument :
MSVOA_D
ClientSampleId :
BFB114

193.90	287.0
195.10	211.0
203.10	170.0
204.90	340.0
207.00	479.0
207.80	192.0
249.00	374.0
250.90	253.0
265.00	722.0
266.00	163.0
281.10	7035.0
282.10	2115.0
283.00	1192.0
284.00	179.0
284.20	180.0

Instrument :
MSVOA_D
ClientSampleId :
BFB114

m/z	Abundance
36.10	672.0
37.00	2690.0
38.10	2729.0
39.00	1208.0
40.00	1172.0
44.10	1003.0
45.10	901.0
46.10	163.0
47.10	1251.0
48.00	582.0
49.10	2939.0
50.10	15155.0
51.10	5199.0
52.00	182.0
54.90	268.0
56.10	1446.0
57.00	2339.0
59.00	157.0
60.00	1030.0
61.00	4826.0
62.10	5035.0
63.10	3359.0
63.90	498.0
65.10	423.0
67.00	365.0
68.00	9036.0
69.10	9573.0
70.00	949.0
72.20	570.0
73.10	5420.0
74.00	15606.0
75.10	46736.0
76.00	3780.0
76.90	618.0
77.70	427.0
78.10	302.0
79.00	3875.0
80.00	927.0
80.90	3477.0
81.90	768.0
83.00	192.0
85.80	182.0
87.00	5982.0
88.00	5493.0
90.80	333.0
92.00	2833.0
93.00	4637.0
94.00	13402.0
95.10	102272.0
96.10	6322.0
97.00	204.0
102.90	391.0
104.00	435.0
105.80	565.0
110.00	209.0
112.90	219.0
115.10	157.0
116.00	460.0
116.90	1140.0
117.90	544.0
119.10	514.0
125.40	655.0
127.90	401.0
129.90	280.0
133.00	1240.0
134.80	281.0
140.90	591.0
141.80	154.0
142.90	1041.0
144.90	303.0
145.80	340.0
147.00	232.0
147.80	289.0
157.10	236.0
158.80	274.0
160.90	212.0
163.10	181.0
165.00	214.0
171.00	195.0
171.90	1046.0
173.00	869.0
174.00	104192.0
175.00	7316.0
176.00	101640.0
177.00	7173.0
178.00	182.0
179.00	172.0
191.10	1154.0
193.00	1234.0
193.90	172.0
195.00	227.0
205.00	356.0

Instrument :
MSVOA_D
ClientSampleId :
BFB114

207.00	881.0
208.00	301.0
249.00	750.0
250.80	221.0
265.00	736.0
267.10	209.0
281.10	8587.0
282.10	2573.0
283.20	1615.0
283.90	211.0

Instrument :
MSVOA_D
ClientSampleId :
BFB114