


Instrument :
MSVOA_D
ClientSampleId :


4-Bromofluorobenzene

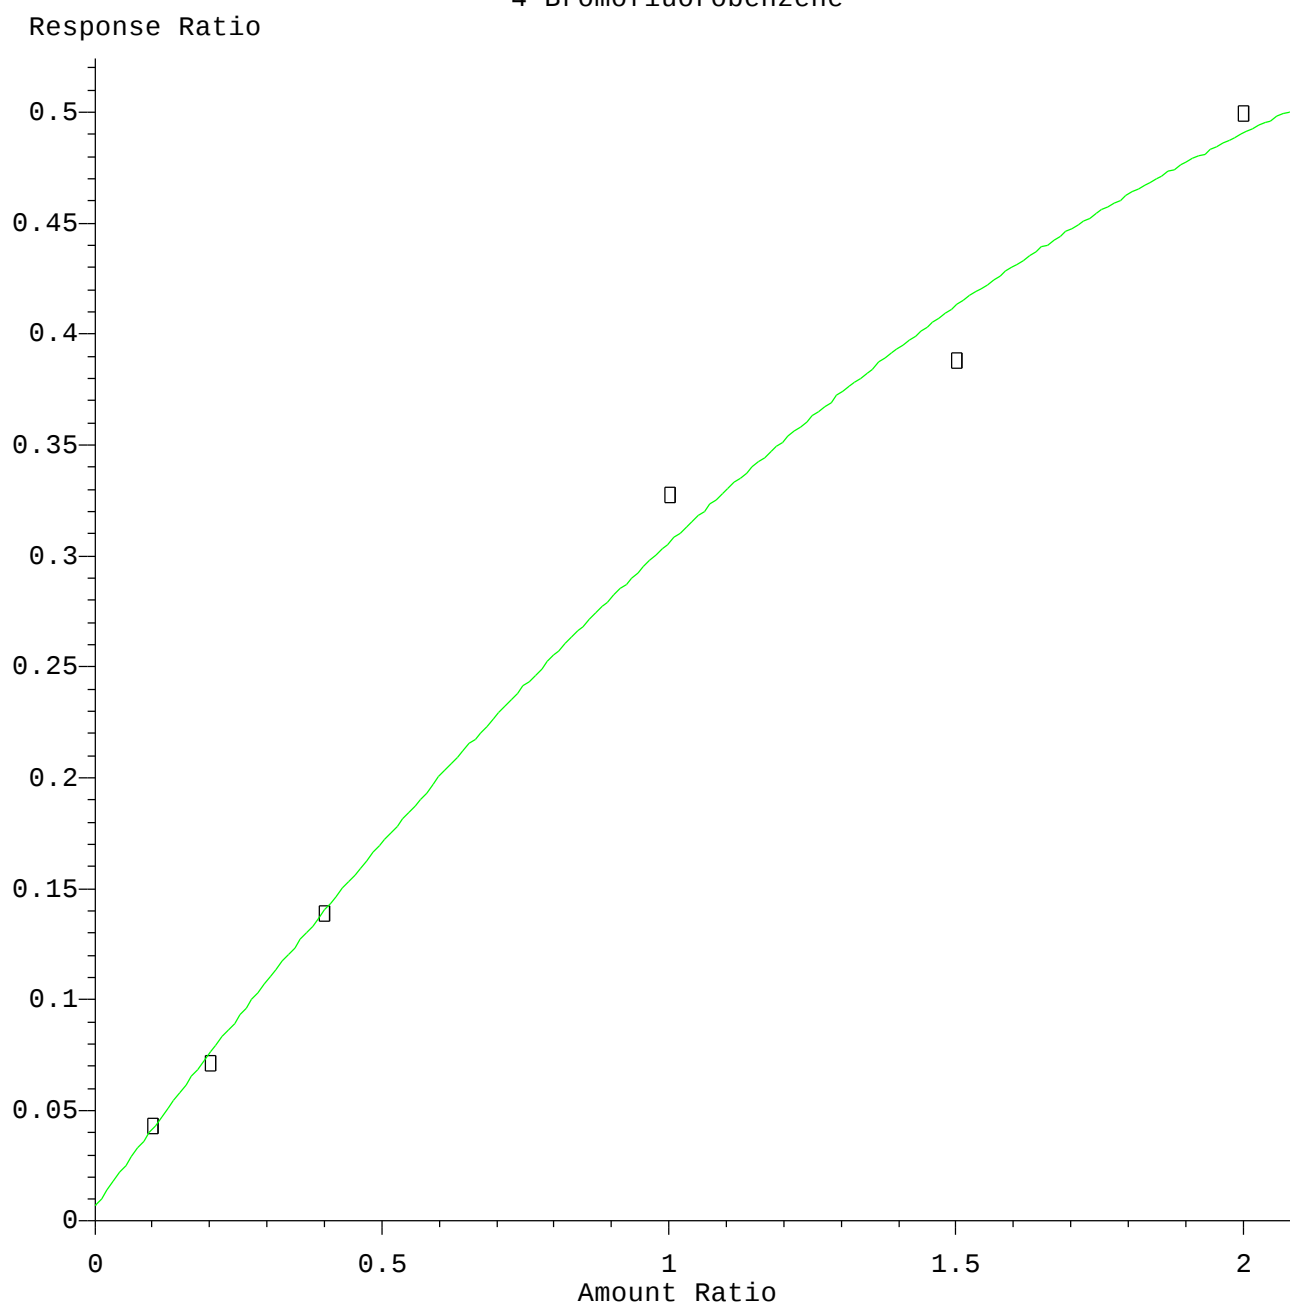

$R = -5.74e-002 A^2 + 3.57e-001 A + 6.66e-003$
Coef of Det (r^2) = 0.993 Curve Fit: Quadratic

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D040619S.M
Calibration Table Last Updated: Mon Apr 08 10:04:03 2019

Instrument :
MSVOA_D
ClientSampleId :

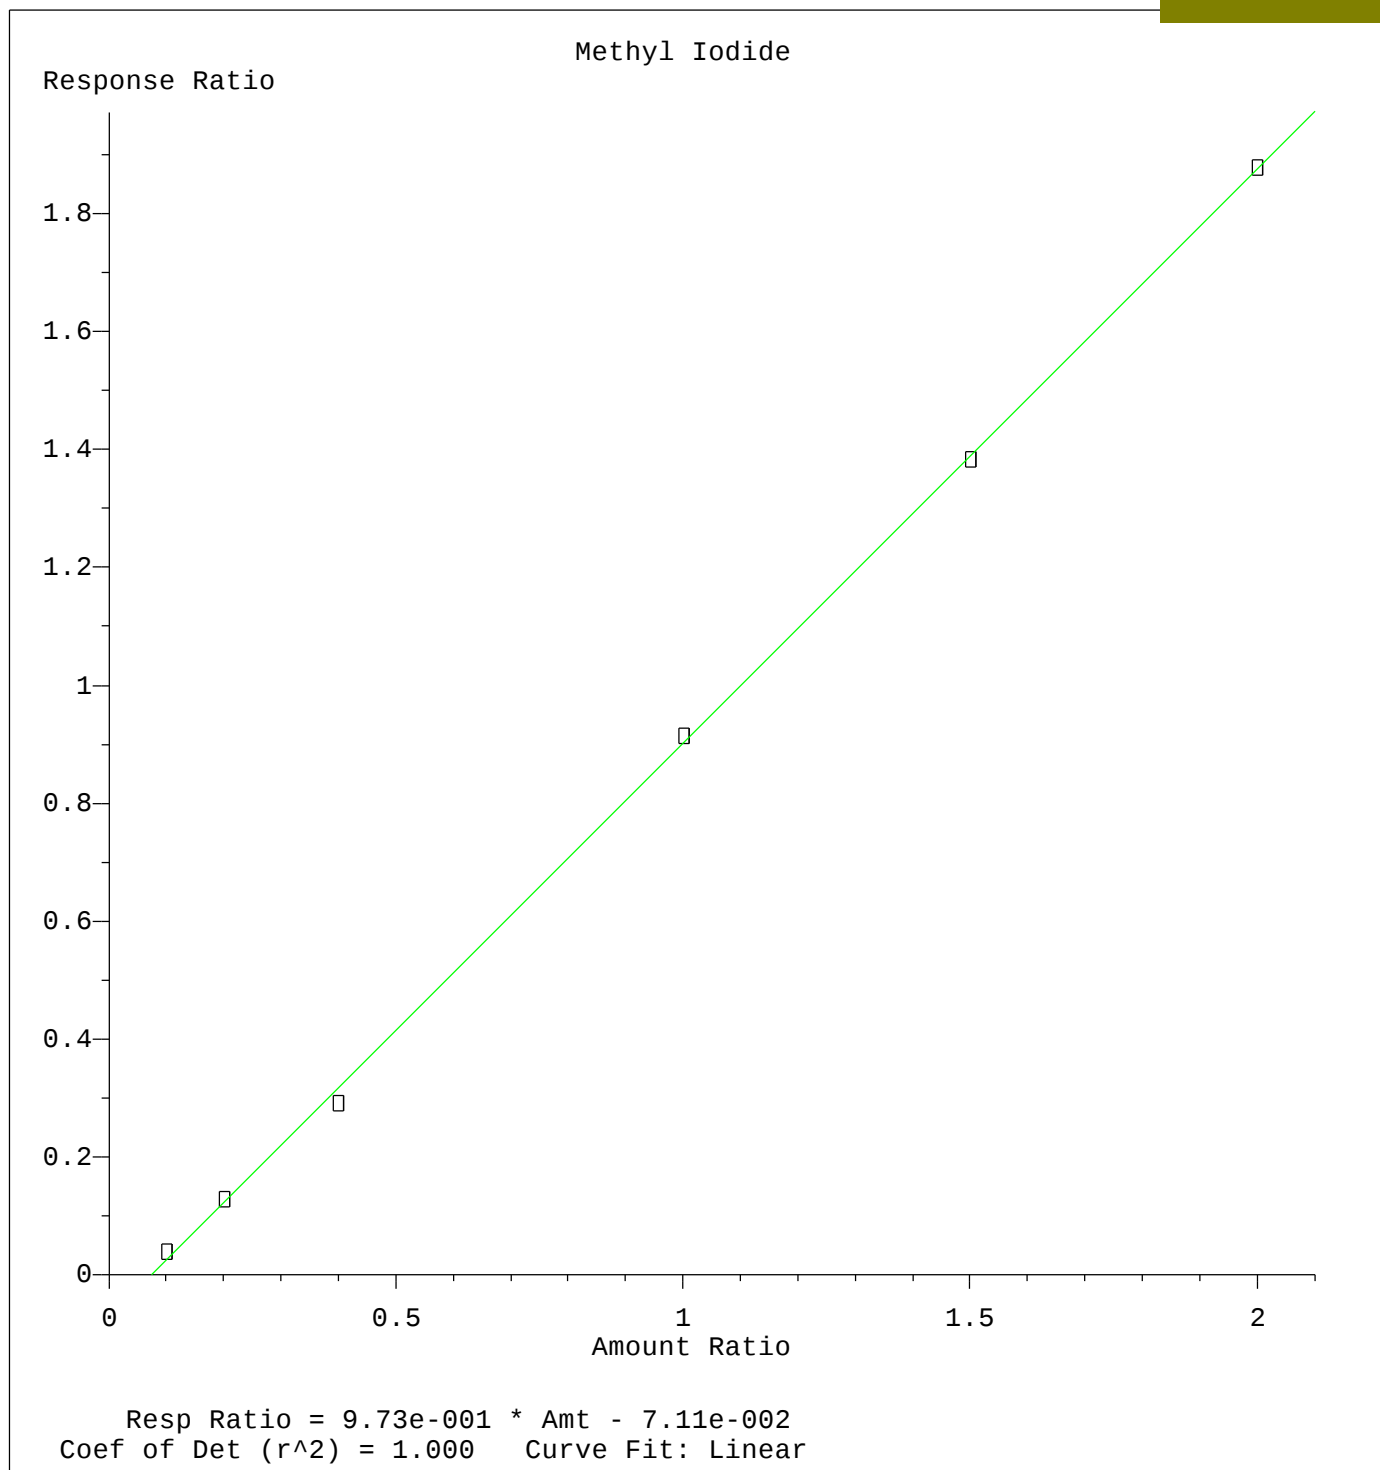

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D040619S.M
Calibration Table Last Updated: Mon Apr 08 10:04:03 2019