

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD040623\
 Data File : VD075588.D
 Acq On : 06 Apr 2023 11:22
 Operator : KP/SY
 Sample : VD0406SBL01
 Misc : 5.00G/10.00ml/MSVOA_D/SOIL
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 VBLK120

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\SFAMDLM033123SMA.M
 Title : SFAM01.0

Signal : TIC: VD075588.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.622	4	6	8	rBV	576	532	0.04%	0.005%
2	1.740	19	26	37	rBV	645345	1265920	90.62%	11.820%
3	2.275	112	117	125	rBV	229402	336123	24.06%	3.139%
4	2.805	200	207	217	rBV	184376	346549	24.81%	3.236%
5	3.287	288	289	293	rVB2	689	728	0.05%	0.007%
6	3.522	327	329	330	rVB	1057	501	0.04%	0.005%
7	3.852	382	385	386	rBV2	600	638	0.05%	0.006%
8	3.922	386	397	408	rVV	186221	497175	35.59%	4.642%
9	4.087	423	425	428	rBV2	686	639	0.05%	0.006%
10	4.152	431	436	438	rVB2	1104	1432	0.10%	0.013%
11	4.269	453	456	459	rBV3	1552	2336	0.17%	0.022%
12	4.581	507	509	513	rVB2	641	584	0.04%	0.005%
13	4.616	513	515	518	rBV	704	582	0.04%	0.005%
14	4.805	538	547	556	rBV2	11218	34481	2.47%	0.322%
15	5.052	586	589	592	rVB2	572	539	0.04%	0.005%
16	5.087	592	595	598	rBV2	487	676	0.05%	0.006%
17	5.187	610	612	617	rVB2	466	545	0.04%	0.005%
18	5.346	634	639	645	rVB2	874	1798	0.13%	0.017%
19	5.399	645	648	651	rBV	619	1001	0.07%	0.009%
20	5.640	687	689	691	rBV	786	763	0.05%	0.007%
21	5.822	716	720	721	rBV2	861	958	0.07%	0.009%
22	5.834	721	722	724	rBV	1115	761	0.05%	0.007%
23	6.158	774	777	781	rVB2	637	805	0.06%	0.008%
24	6.569	845	847	850	rVB2	714	693	0.05%	0.006%
25	6.616	850	855	858	rBV2	784	1441	0.10%	0.013%
26	6.863	896	897	901	rBV2	426	514	0.04%	0.005%
27	6.981	909	917	925	rBV	21838	62673	4.49%	0.585%
28	7.287	966	969	970	rBV	1017	885	0.06%	0.008%
29	7.457	996	998	1002	rVB2	621	802	0.06%	0.007%
30	7.569	1006	1017	1030	rBV	217649	566138	40.52%	5.286%
31	7.705	1038	1040	1041	rVB2	1090	559	0.04%	0.005%
32	7.769	1050	1051	1056	rVB2	858	694	0.05%	0.006%
33	7.993	1086	1089	1092	rBV2	787	1011	0.07%	0.009%
34	8.116	1106	1110	1113	rBV2	472	628	0.04%	0.006%
35	8.204	1113	1125	1141	rBV2	489862	1397018	100.00%	13.045%
36	8.404	1158	1159	1161	rBV	658	495	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD040623\
 Data File : VD075588.D
 Acq On : 06 Apr 2023 11:22
 Operator : KP/SY
 Sample : VD0406SBL01
 Misc : 5.00G/10.00ml/MSVOA_D/SOIL
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 VBLK120

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\SFAMDLM033123SMA.M
 Title : SFAM01.0

37	8.487	1171	1173	1175	rVB	1015	660	0.05%	0.006%
38	8.510	1175	1177	1179	rBV	868	653	0.05%	0.006%
39	8.546	1181	1183	1185	rBV3	618	532	0.04%	0.005%
40	8.669	1202	1204	1206	rVB2	574	519	0.04%	0.005%
41	8.693	1206	1208	1211	rVB	555	559	0.04%	0.005%
42	8.781	1211	1223	1238	rBV	426362	873088	62.50%	8.152%
43	9.022	1258	1264	1268	rVB3	2419	5023	0.36%	0.047%
44	9.210	1287	1296	1306	rBV	275439	560606	40.13%	5.235%
45	9.363	1321	1322	1326	rVB2	606	541	0.04%	0.005%
46	9.540	1348	1352	1355	rVB2	533	792	0.06%	0.007%
47	9.593	1358	1361	1363	rVV	884	1048	0.08%	0.010%
48	9.751	1386	1388	1389	rBV	746	627	0.04%	0.006%
49	9.834	1398	1402	1403	rBV3	1382	1132	0.08%	0.011%
50	9.928	1416	1418	1419	rBV	608	519	0.04%	0.005%
51	9.981	1419	1427	1437	rVV	143482	271852	19.46%	2.538%
52	10.063	1437	1441	1443	rVB2	1212	1355	0.10%	0.013%
53	10.175	1458	1460	1463	rVB	786	750	0.05%	0.007%
54	10.269	1468	1476	1488	rBV	665110	1194733	85.52%	11.156%
55	10.528	1514	1520	1529	rVB	97433	165507	11.85%	1.545%
56	10.604	1531	1533	1535	rBV	516	493	0.04%	0.005%
57	10.663	1537	1543	1550	rVB	41357	73834	5.29%	0.689%
58	10.810	1565	1568	1571	rVB3	2491	2935	0.21%	0.027%
59	10.881	1571	1580	1587	rBV	82733	145604	10.42%	1.360%
60	11.034	1600	1606	1614	rVV	34461	57567	4.12%	0.538%
61	11.181	1627	1631	1633	rBV	683	1088	0.08%	0.010%
62	11.310	1652	1653	1657	rBV2	626	558	0.04%	0.005%
63	11.404	1664	1669	1679	rVB2	17735	27845	1.99%	0.260%
64	11.581	1691	1699	1711	rBV	575021	1001369	71.68%	9.350%
65	11.687	1715	1717	1722	rVB4	2677	2796	0.20%	0.026%
66	11.745	1725	1727	1730	rBV	1203	969	0.07%	0.009%
67	11.804	1731	1737	1741	rVB4	2322	4256	0.30%	0.040%
68	11.940	1759	1760	1763	rBV2	579	540	0.04%	0.005%
69	12.004	1769	1771	1772	rBV	719	538	0.04%	0.005%
70	12.134	1788	1793	1799	rVB3	2455	4199	0.30%	0.039%
71	12.428	1838	1843	1847	rBV4	2631	4873	0.35%	0.046%
72	12.581	1862	1869	1874	rBV3	16350	26230	1.88%	0.245%
73	12.651	1874	1881	1889	rVB	204752	343547	24.59%	3.208%
74	12.845	1911	1914	1919	rBV3	893	1546	0.11%	0.014%
75	12.904	1919	1924	1929	rVV2	8970	13452	0.96%	0.126%
76	13.145	1963	1965	1966	rBV2	604	598	0.04%	0.006%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD040623\
 Data File : VD075588.D
 Acq On : 06 Apr 2023 11:22
 Operator : KP/SY
 Sample : VD0406SBL01
 Misc : 5.00G/10.00ml/MSVOA_D/SOIL
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 VBLK120

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\SFAMDLM033123SMA.M
 Title : SFAM01.0

77	13.163	1966	1968	1972	rVV2	2511	3256	0.23%	0.030%
78	13.216	1974	1977	1979	rVV2	2077	2076	0.15%	0.019%
79	13.269	1982	1986	1992	rVB3	2841	5155	0.37%	0.048%
80	13.457	2010	2018	2022	rBV3	4369	8188	0.59%	0.076%
81	13.522	2022	2029	2037	rVV	406490	679051	48.61%	6.341%
82	13.816	2071	2079	2087	rBV	391943	645512	46.21%	6.027%
83	14.051	2113	2119	2123	rBV2	6358	9814	0.70%	0.092%
84	14.139	2130	2134	2136	rBV3	718	1025	0.07%	0.010%
85	14.163	2136	2138	2139	rVV	731	494	0.04%	0.005%
86	14.475	2188	2191	2192	rBV	860	821	0.06%	0.008%
87	14.604	2208	2213	2216	rBV3	1783	2838	0.20%	0.026%
88	15.022	2282	2284	2288	rBV2	732	1058	0.08%	0.010%
89	15.104	2293	2298	2302	rBV3	3440	5839	0.42%	0.055%
90	15.334	2332	2337	2340	rVV3	3349	4053	0.29%	0.038%
91	15.410	2347	2350	2355	rVB2	2999	4536	0.32%	0.042%
92	15.451	2355	2357	2359	rBV2	658	504	0.04%	0.005%
93	15.522	2365	2369	2373	rVB2	3008	3939	0.28%	0.037%
94	15.628	2385	2387	2390	rBV3	796	817	0.06%	0.008%
95	15.857	2424	2426	2429	rVB	1177	767	0.05%	0.007%
96	15.892	2429	2432	2434	rVV	1270	1320	0.09%	0.012%
97	15.957	2438	2443	2445	rBV2	931	1767	0.13%	0.016%
98	16.492	2533	2534	2537	rBV2	908	694	0.05%	0.006%
99	16.522	2537	2539	2541	rVV	709	566	0.04%	0.005%
100	16.651	2559	2561	2562	rBV	1047	548	0.04%	0.005%




Sum of corrected areas: 10709588

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD040623\
Data File : VD075588.D
Acq On : 06 Apr 2023 11:22
Operator : KP/SY
Sample : VD0406SBL01
Misc : 5.00G/10.00ml/MSVOA_D/SOIL
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
VBLK120

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\SFAMDLM033123SMA.M
Quant Title : SFAM01.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

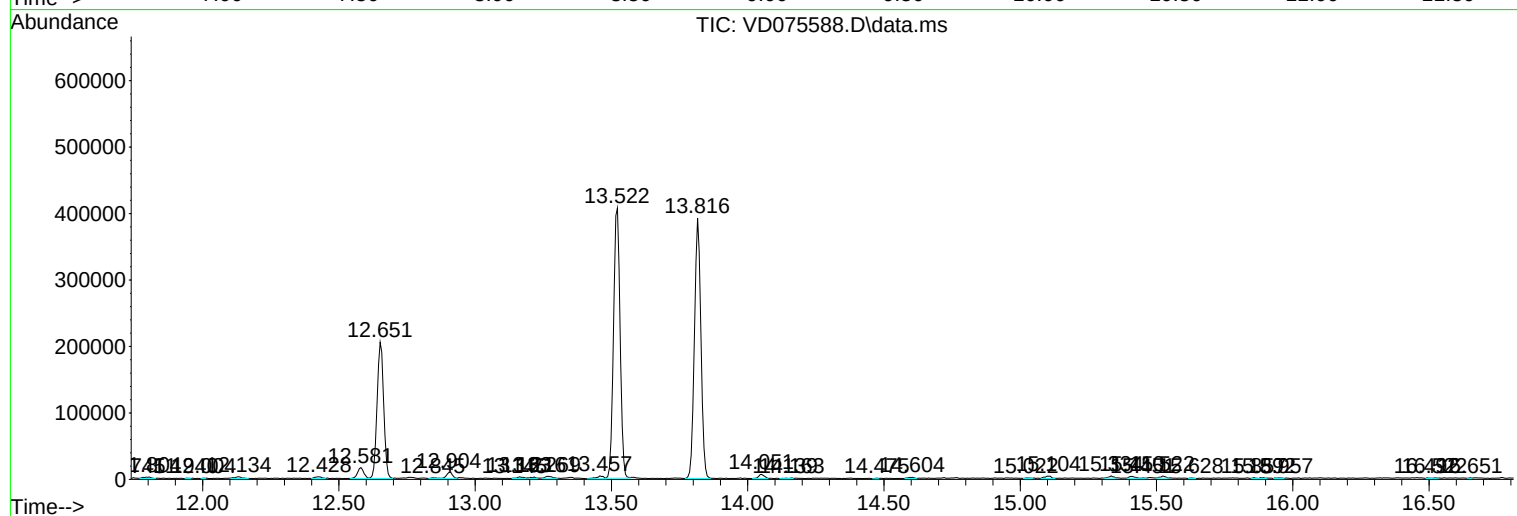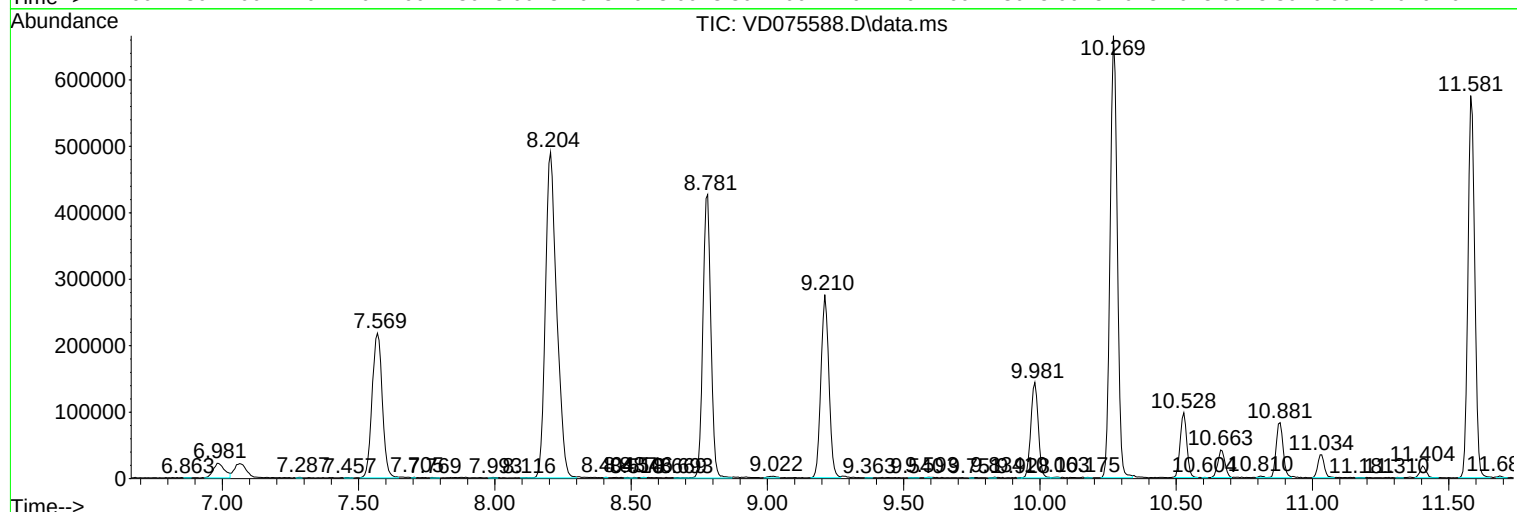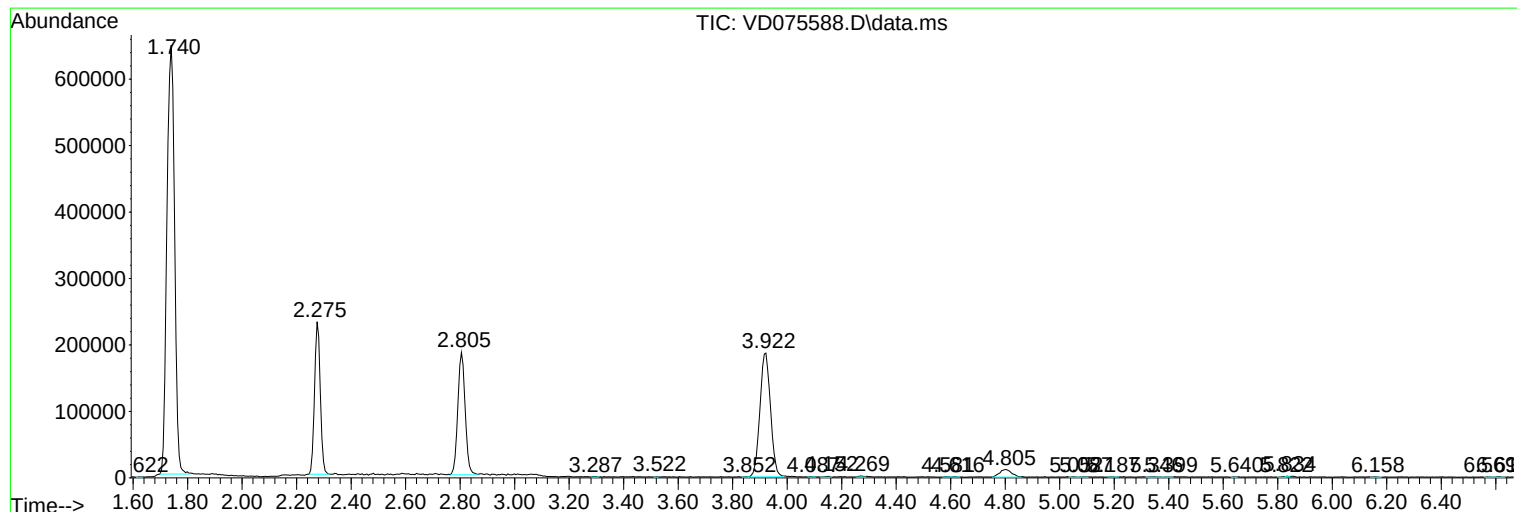

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD040623\
Data File : VD075588.D
Acq On : 06 Apr 2023 11:22
Operator : KP/SY
Sample : VD0406SBL01
Misc : 5.00G/10.00ml/MSVOA_D/SOIL
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
VBLK120

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\SFAMDLM033123SMA.M
Quant Title : SFAM01.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD040623\
Data File : VD075588.D
Acq On : 06 Apr 2023 11:22
Operator : KP/SY
Sample : VD0406SBL01
Misc : 5.00G/10.00ml/MSVOA_D/SOIL
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
VBLK120

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\SFAMDLM033123SMA.M
Quant Title : SFAM01.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------