


Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD040623\
Data File : VD075586.D
Acq On : 06 Apr 2023 10:04
Operator : KP/SY
Sample : BFB115
Misc : 5.00G/10.00ml/MSVOA_D/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB115

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\SFAMDLM033123SMA.M
Title : SFAM01.0
Last Update : Sat Apr 01 00:08:20 2023

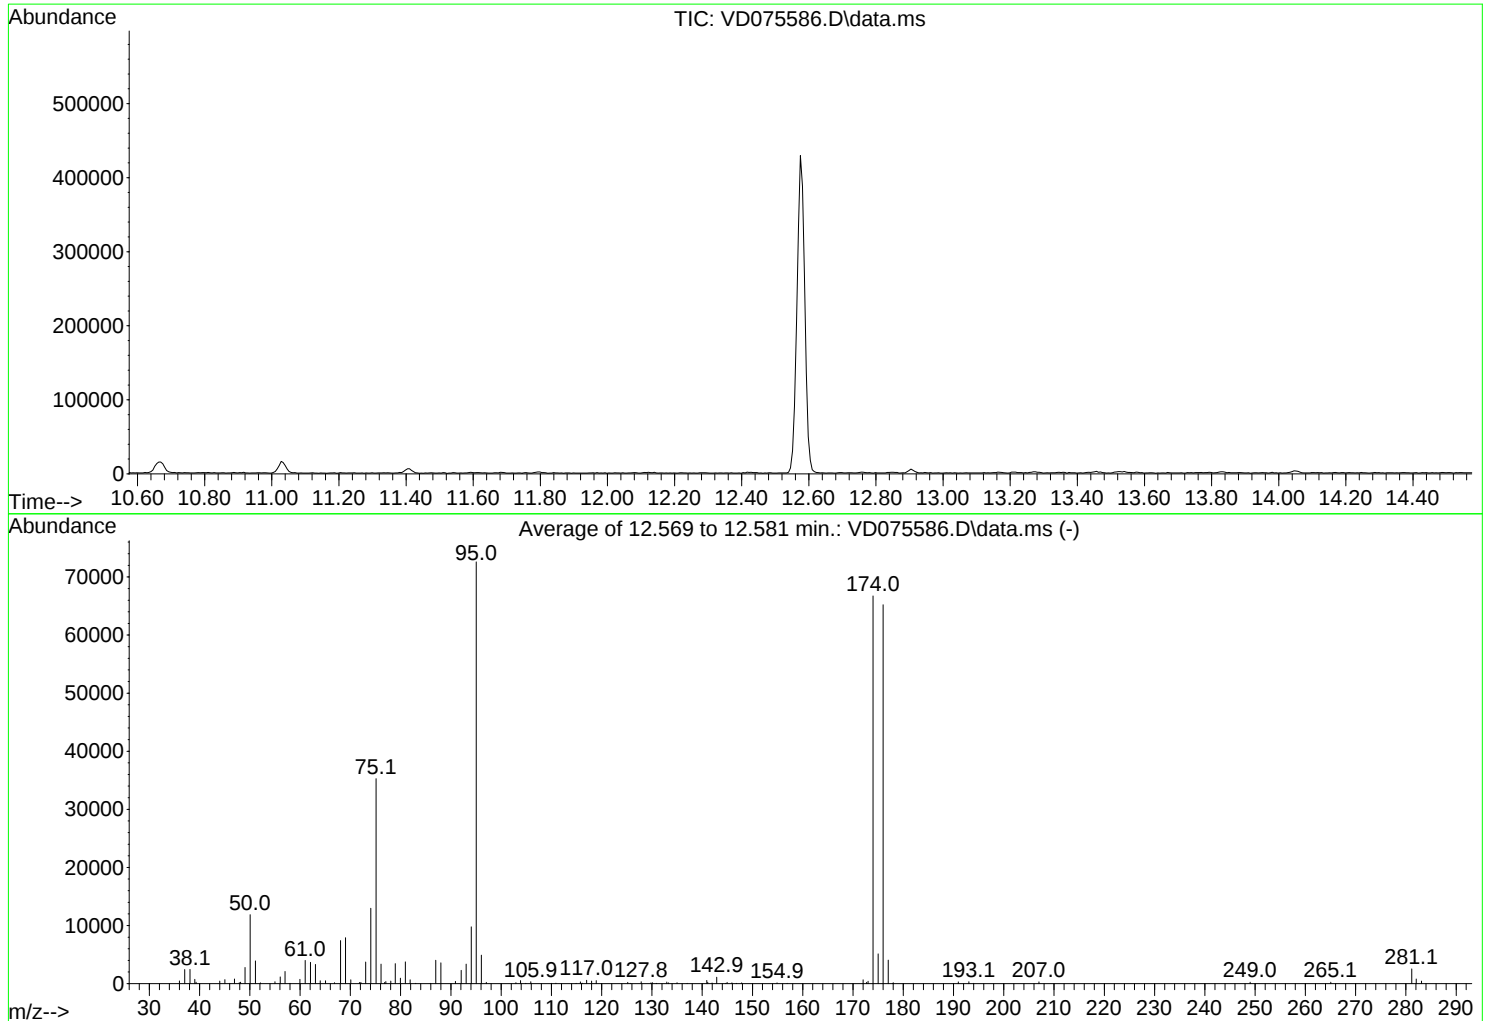

AutoFind: Scans 1867, 1868, 1869; Background Corrected with Scan 1860

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.3	11860	PASS
75	95	30	80	48.6	35269	PASS
95	95	100	100	100.0	72605	PASS
96	95	5	9	6.8	4904	PASS
173	174	0.00	2	0.6	406	PASS
174	95	50	120	91.9	66736	PASS
175	174	5	9	7.7	5118	PASS
176	174	95	105	97.7	65216	PASS
177	176	5	10	6.2	4042	PASS

Scan 1860 (12.528 min): VD075586.D\data.ms
BFB115

m/z	Abundance
40.00	822.0
44.00	497.0

Instrument :
MSVOA_D
ClientSampleId :
BFB115

m/z	Abundance
36.00	344.0
37.00	2304.0
38.10	2426.0
39.30	782.0
40.00	680.0
43.90	982.0
45.00	684.0
46.90	780.0
47.90	477.0
49.10	3014.0
50.10	10869.0
51.10	3587.0
55.00	210.0
56.00	1000.0
57.00	1819.0
58.00	174.0
59.90	616.0
61.00	3318.0
62.00	3529.0
63.10	2837.0
64.00	586.0
65.00	437.0
66.80	230.0
68.10	6233.0
69.10	7541.0
70.10	614.0
71.80	306.0
73.00	3384.0
74.10	12625.0
75.10	30424.0
76.10	2772.0
77.20	351.0
78.10	507.0
78.90	2901.0
80.00	749.0
81.00	3382.0
81.90	630.0
87.00	3236.0
88.00	2889.0
90.90	228.0
92.10	2108.0
93.00	2955.0
94.00	8587.0
95.10	63920.0
96.00	3883.0
97.00	235.0
103.90	570.0
105.90	337.0
115.80	183.0
117.00	376.0
118.10	321.0
118.90	516.0
125.20	277.0
127.90	371.0
130.10	213.0
132.90	373.0
140.90	955.0
142.90	1108.0
145.00	332.0
145.90	178.0
172.00	866.0
173.00	561.0
174.00	56320.0
175.00	4385.0
176.00	55344.0
177.00	3648.0
177.90	238.0
191.00	225.0
193.00	186.0
207.10	297.0
265.10	191.0
281.10	1505.0
282.10	387.0
283.10	270.0

Instrument :
MSVOA_D
ClientSampleId :
BFB115

m/z	Abundance
36.00	615.0
37.10	2976.0
38.10	2739.0
39.00	1427.0
40.00	884.0
44.00	1058.0
45.10	762.0
47.00	783.0
48.10	405.0
49.10	2735.0
50.00	12840.0
51.10	4532.0
52.10	227.0
55.10	512.0
56.00	1311.0
57.00	2710.0
60.00	777.0
61.00	4976.0
62.10	4010.0
63.00	3923.0
64.00	535.0
65.00	573.0
66.90	248.0
68.10	8345.0
69.00	8604.0
70.10	722.0
71.80	298.0
72.20	428.0
73.00	4334.0
74.00	14402.0
75.10	39344.0
76.10	3822.0
77.00	769.0
78.00	494.0
78.90	3868.0
79.90	1192.0
81.00	4721.0
81.90	711.0
87.00	4865.0
88.00	3981.0
90.90	375.0
92.00	2694.0
93.10	3527.0
94.10	11048.0
95.00	80760.0
96.10	5783.0
97.10	160.0
102.90	288.0
103.90	544.0
104.90	172.0
105.90	304.0
110.90	256.0
114.90	162.0
115.80	492.0
117.00	680.0
118.00	447.0
118.90	478.0
125.30	223.0
127.90	241.0
130.10	277.0
133.30	435.0
135.00	251.0
137.00	164.0
141.10	670.0
142.00	153.0
142.90	1041.0
144.90	372.0
145.90	244.0
146.80	160.0
147.80	186.0
154.90	311.0
171.80	480.0
173.00	656.0
174.00	73656.0
175.00	6078.0
176.00	72568.0
177.00	4706.0
178.10	265.0
191.00	367.0
193.10	370.0
207.10	268.0
249.00	354.0
265.10	301.0
281.20	2919.0
282.00	944.0
283.00	533.0

Instrument :
MSVOA_D
ClientSampleId :
BFB115

m/z	Abundance
36.00	478.0
37.10	2021.0
38.10	2171.0
39.10	807.0
40.00	696.0
44.10	758.0
45.10	595.0
46.00	157.0
47.00	832.0
48.20	327.0
49.00	2616.0
50.10	11870.0
51.10	3592.0
52.10	221.0
54.90	254.0
56.10	1127.0
57.00	1760.0
60.00	863.0
61.00	3661.0
62.10	3484.0
63.10	3149.0
64.00	382.0
65.10	463.0
68.00	7627.0
69.10	7582.0
70.10	636.0
72.00	274.0
73.10	3467.0
74.00	11862.0
75.10	36040.0
76.10	3513.0
76.80	574.0
78.00	323.0
79.00	3580.0
80.00	912.0
80.90	3175.0
81.90	661.0
83.00	160.0
85.90	174.0
87.00	3998.0
88.00	3852.0
90.90	564.0
92.10	2073.0
93.00	3610.0
94.10	9725.0
95.00	73136.0
96.00	5046.0
97.10	248.0
103.00	248.0
103.80	439.0
105.90	380.0
110.00	155.0
115.70	241.0
116.10	225.0
117.00	719.0
117.90	540.0
118.90	612.0
125.10	204.0
125.70	153.0
127.80	418.0
129.80	447.0
130.90	163.0
133.00	501.0
135.00	257.0
140.90	708.0
141.90	177.0
142.90	1158.0
144.70	186.0
147.90	251.0
154.90	154.0
156.90	164.0
172.10	665.0
172.70	625.0
174.00	70232.0
175.00	4891.0
176.00	67736.0
177.00	3773.0
178.00	172.0
190.90	358.0
193.00	464.0
194.00	182.0
206.90	357.0
249.00	420.0
264.90	248.0
281.10	3193.0
282.00	1089.0
283.20	522.0

Instrument :
MSVOA_D
ClientSampleId :
BFB115