

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD040821\
 Data File : VD068792.D
 Acq On : 08 Apr 2021 16:36
 Operator : VA/SY
 Sample : M1908-07
 Misc : 5.06G/5.00ml/MSVOA_D/SOIL
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 FILL(0.5-1.0)

Quant Time: Apr 09 01:48:23 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D040721S.M
 Quant Title : SW846 8260
 QLast Update : Thu Apr 08 03:50:31 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	7.985	168	428654	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	8.867	114	766916	50.00	ug/l	0.00
63) Chlorobenzene-d5	11.643	117	806978	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.573	152	375619	50.00	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.332	65	199495	44.04	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	=	88.08%
35) Dibromofluoromethane	7.920	113	240116	48.14	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	=	96.28%
50) Toluene-d8	10.343	98	979280	52.04	ug/l	0.00
Spiked Amount	50.000	Range	49 - 140	Recovery	=	104.08%
62) 4-Bromofluorobenzene	12.631	95	358892	57.42	ug/l	0.00
Spiked Amount	50.000	Range	25 - 144	Recovery	=	114.84%
Target Compounds						
20) Methylene Chloride	4.973	84	54490	6.54	ug/l	Qvalue 91


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD040821\
Data File : VD068792.D
Acq On : 08 Apr 2021 16:36
Operator : VA/SY
Sample : M1908-07
Misc : 5.06G/5.00ml/MSVOA_D/SOIL
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
FILL(0.5-1.0)

Quant Time: Apr 09 01:48:23 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D040721S.M
Quant Title : SW846 8260
QLast Update : Thu Apr 08 03:50:31 2021
Response via : Initial Calibration




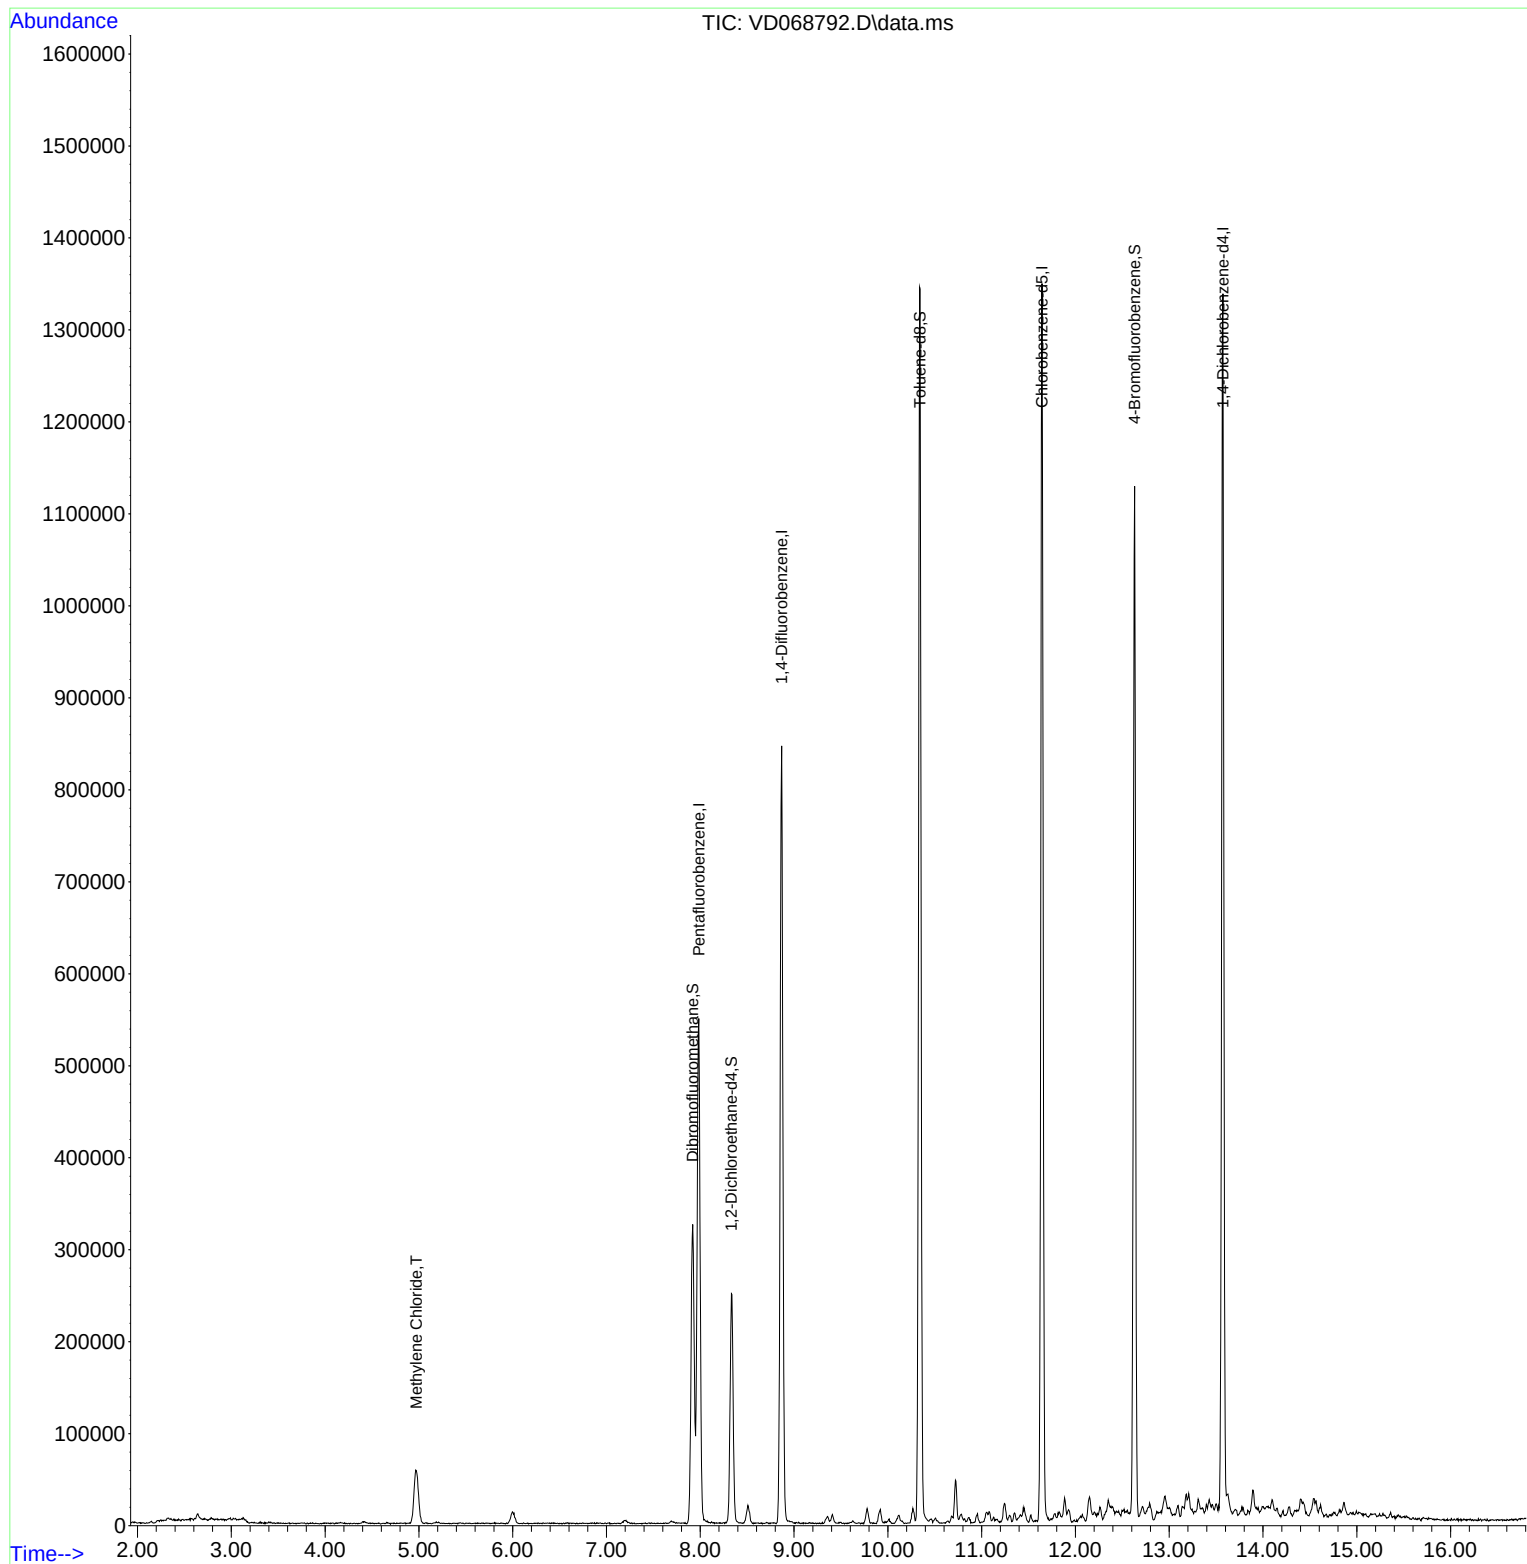


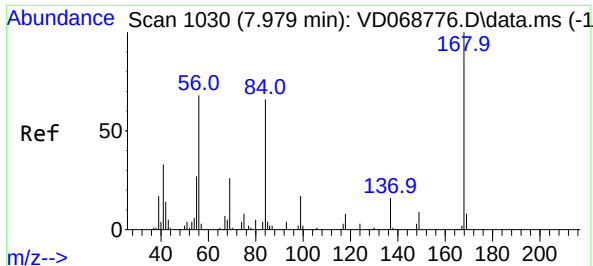

#1
Pentafluorobenzene
Concen: 50.00 ug/l
RT: 7.985 min Scan# 1031
Delta R.T. 0.006 min
Lab File: VD068792.D
Acq: 08 Apr 2021 16:36




Instrument :
MSVOA_D
ClientSampleId :
FILL(0.5-1.0)


Tgt Ion:168 Resp: 428654
Ion Ratio Lower Upper
168 100
99 53.2 46.2 69.2

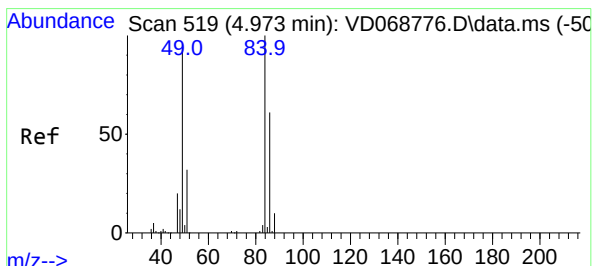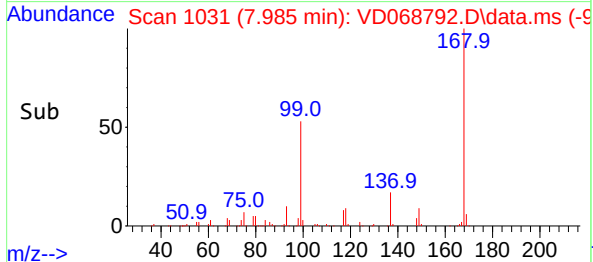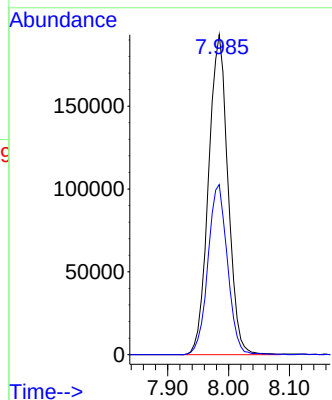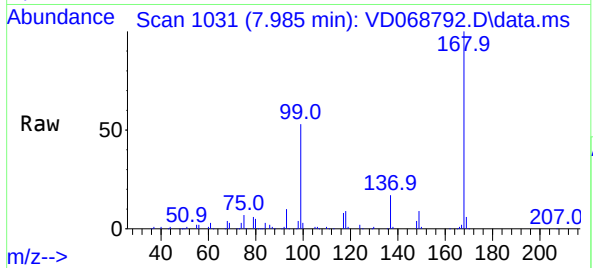

#20
Methylene Chloride
Concen: 6.54 ug/l
RT: 4.973 min Scan# 519
Delta R.T. 0.000 min
Lab File: VD068792.D
Acq: 08 Apr 2021 16:36

Tgt Ion: 84 Resp: 54490
Ion Ratio Lower Upper
84 100
49 92.6 83.4 125.0
51 28.0 23.4 35.2
86 56.2 51.0 76.4


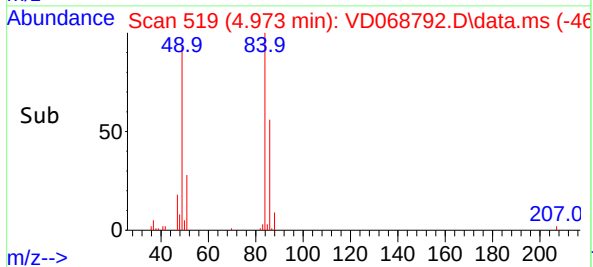
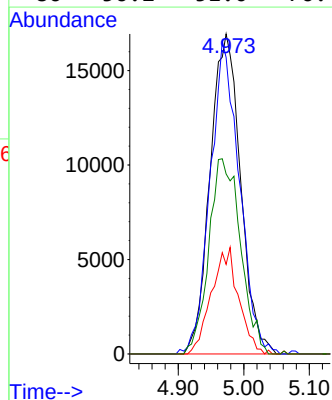
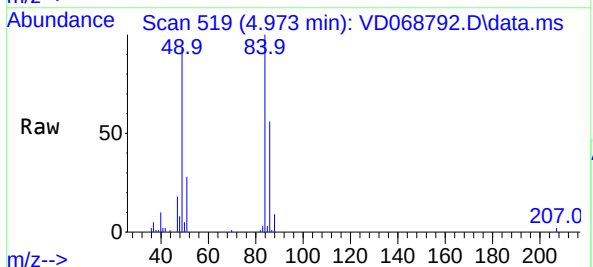


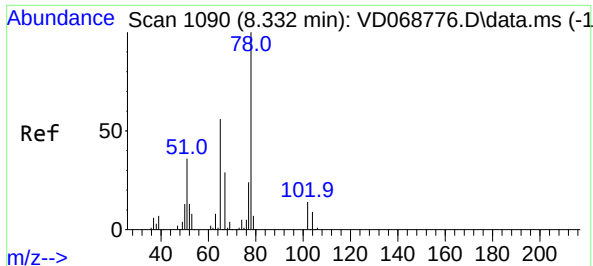

#33
1,2-Dichloroethane-d4
Concen: 44.04 ug/l
RT: 8.332 min Scan# 1090
Delta R.T. -0.000 min
Lab File: VD068792.D
Acq: 08 Apr 2021 16:36




Instrument :
MSVOA_D
ClientSampleId :
FILL(0.5-1.0)


Tgt Ion: 65 Resp: 199495
Ion Ratio Lower Upper
65 100
67 53.1 0.0 106.0

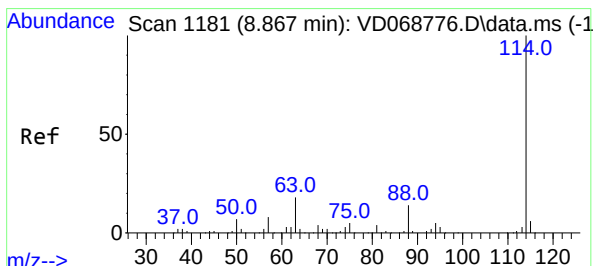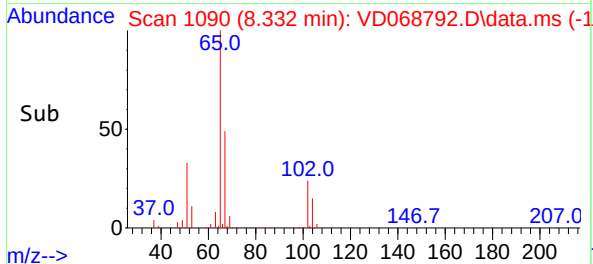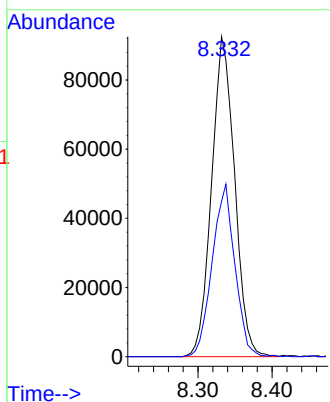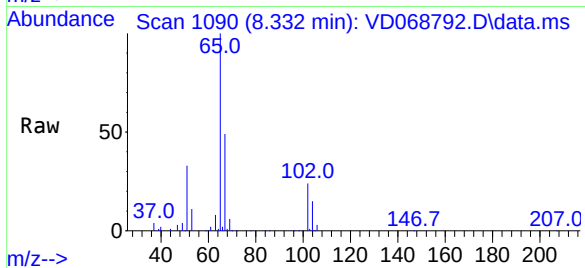

#34
1,4-Difluorobenzene
Concen: 50.00 ug/l
RT: 8.867 min Scan# 1181
Delta R.T. -0.000 min
Lab File: VD068792.D
Acq: 08 Apr 2021 16:36

Tgt Ion: 114 Resp: 766916
Ion Ratio Lower Upper
114 100
63 17.3 0.0 38.2
88 15.1 0.0 29.4


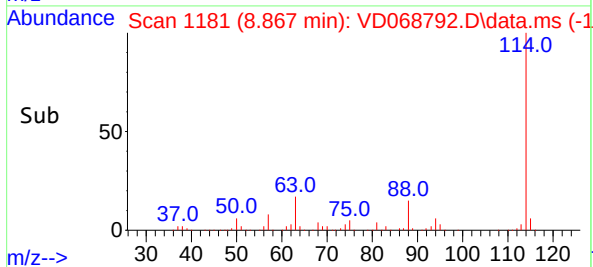
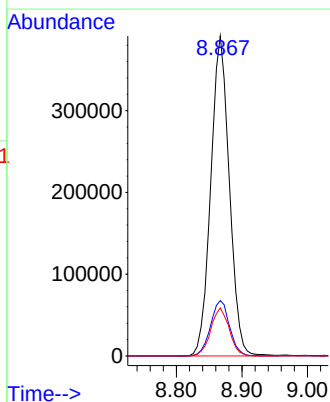
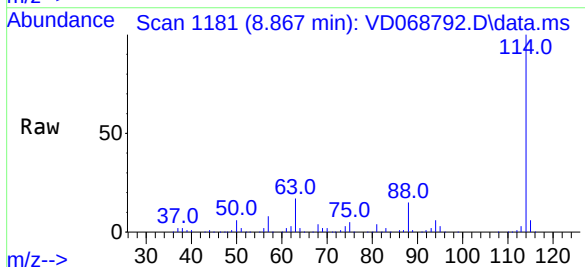


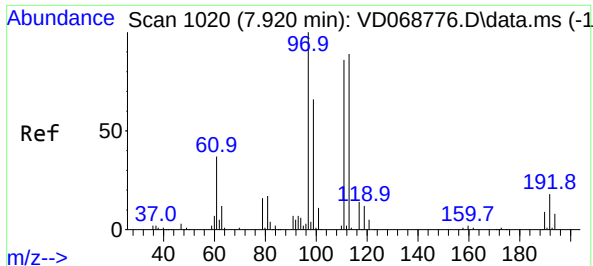

#35
Dibromofluoromethane
Concen: 48.14 ug/l
RT: 7.920 min Scan# 1020
Delta R.T. -0.000 min
Lab File: VD068792.D
Acq: 08 Apr 2021 16:36




Instrument :
MSVOA_D
ClientSampleId :
FILL(0.5-1.0)


Tgt Ion:113 Resp: 240116
Ion Ratio Lower Upper
113 100
111 100.9 82.5 123.7
192 19.4 15.1 22.7

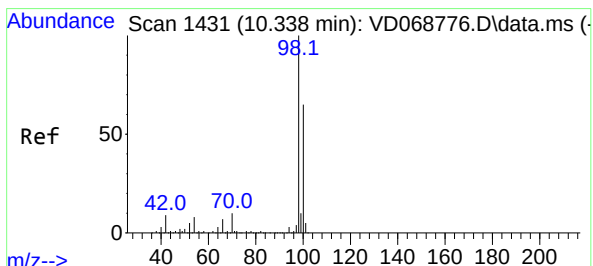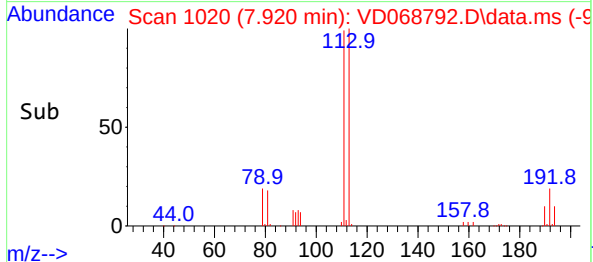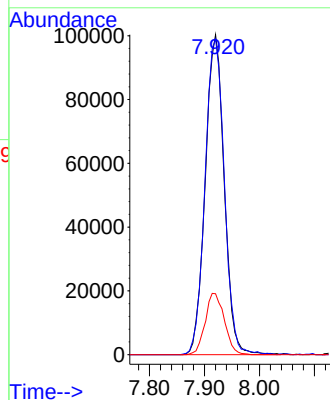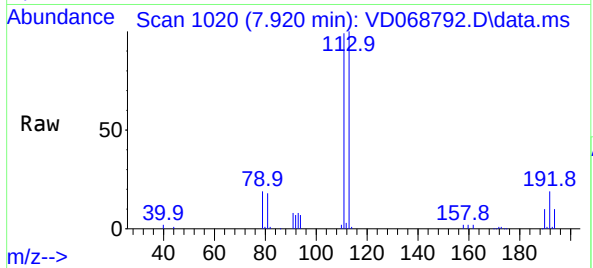

#50
Toluene-d8
Concen: 52.04 ug/l
RT: 10.343 min Scan# 1432
Delta R.T. 0.005 min
Lab File: VD068792.D
Acq: 08 Apr 2021 16:36

Tgt Ion: 98 Resp: 979280
Ion Ratio Lower Upper
98 100
100 63.9 51.8 77.6


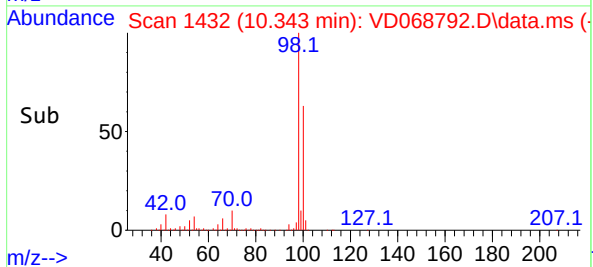
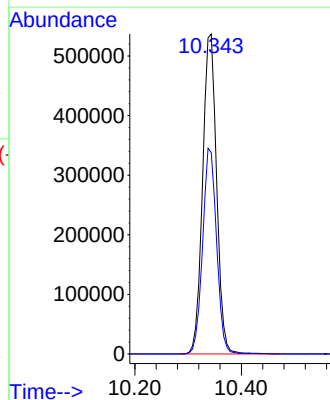
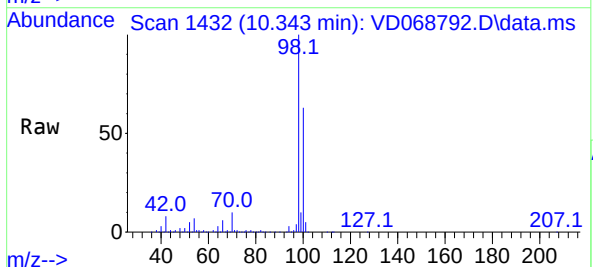


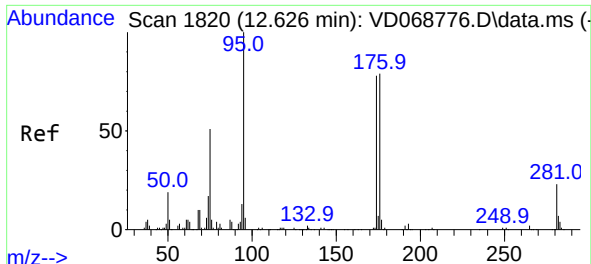

#62
4-Bromofluorobenzene
Concen: 57.42 ug/l
RT: 12.631 min Scan# 1821
Delta R.T. 0.005 min
Lab File: VD068792.D
Acq: 08 Apr 2021 16:36




Instrument :
MSVOA_D
ClientSampleId :
FILL(0.5-1.0)


Tgt Ion: 95 Resp: 358892
Ion Ratio Lower Upper
95 100
174 84.4 0.0 168.0
176 81.0 0.0 160.2

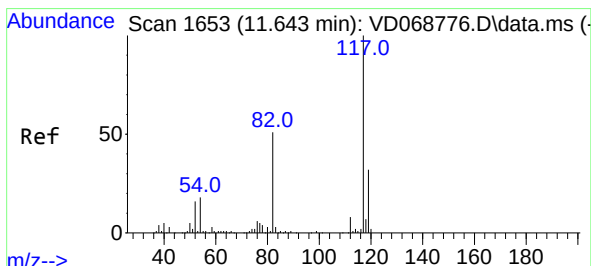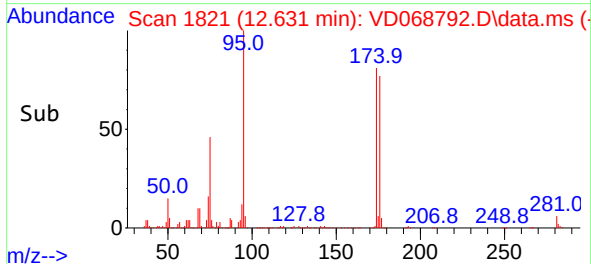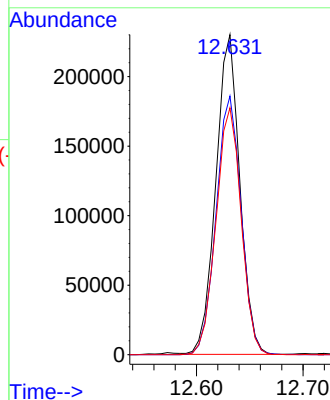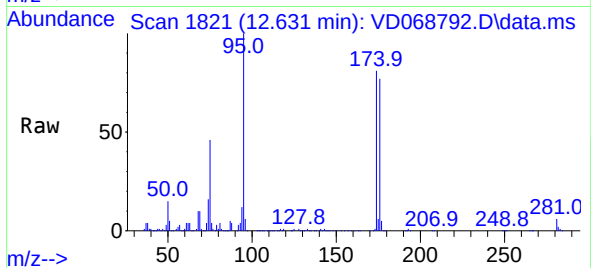

#63
Chlorobenzene-d5
Concen: 50.00 ug/l
RT: 11.643 min Scan# 1653
Delta R.T. 0.000 min
Lab File: VD068792.D
Acq: 08 Apr 2021 16:36

Tgt Ion: 117 Resp: 806978
Ion Ratio Lower Upper
117 100
82 51.3 43.5 65.3
119 30.5 26.7 40.1

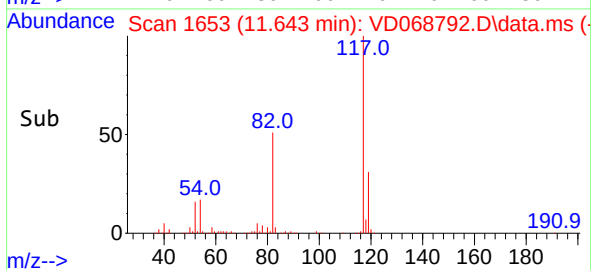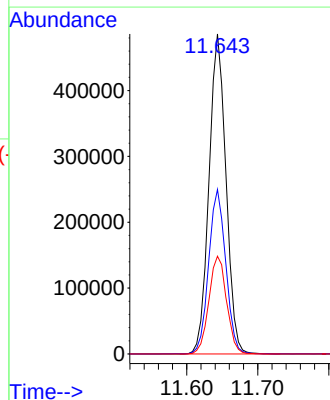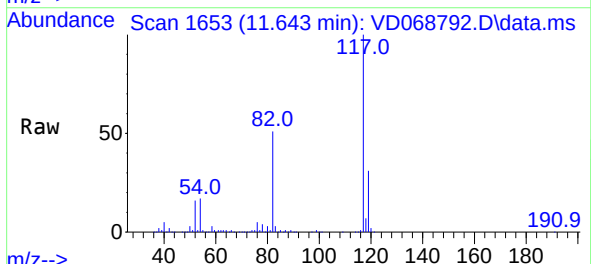

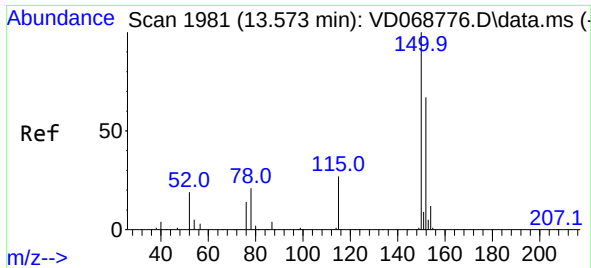

#72
1,4-Dichlorobenzene-d4
Concen: 50.00 ug/l
RT: 13.573 min Scan# 1981
Delta R.T. -0.000 min
Lab File: VD068792.D
Acq: 08 Apr 2021 16:36

Instrument :
MSVOA_D
ClientSampleId :
FILL(0.5-1.0)

Tgt Ion:152 Resp: 375619
Ion Ratio Lower Upper
152 100
115 57.4 29.3 87.8
150 154.8 0.0 347.6

