

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD040821\
 Data File : VD068793.D
 Acq On : 08 Apr 2021 17:04
 Operator : VA/SY
 Sample : M1979-20
 Misc : 4.94G/5.00ml/MSVOA_D/SOIL
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 S-20

Quant Time: Apr 09 01:03:42 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D040721S.M
 Quant Title : SW846 8260
 QLast Update : Thu Apr 08 03:50:31 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	7.985	168	400675	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	8.867	114	741008	50.00	ug/l	0.00
63) Chlorobenzene-d5	11.644	117	775657	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.573	152	372929	50.00	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.332	65	181139	42.78	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	=	85.56%
35) Dibromofluoromethane	7.920	113	217470	45.12	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	=	90.24%
50) Toluene-d8	10.338	98	932342	51.28	ug/l	0.00
Spiked Amount	50.000	Range	49 - 140	Recovery	=	102.56%
62) 4-Bromofluorobenzene	12.632	95	340969	56.46	ug/l	0.00
Spiked Amount	50.000	Range	25 - 144	Recovery	=	112.92%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD040821\
Data File : VD068793.D
Acq On : 08 Apr 2021 17:04
Operator : VA/SY
Sample : M1979-20
Misc : 4.94G/5.00ml/MSVOA_D/SOIL
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
S-20

Quant Time: Apr 09 01:03:42 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D040721S.M
Quant Title : SW846 8260
QLast Update : Thu Apr 08 03:50:31 2021
Response via : Initial Calibration




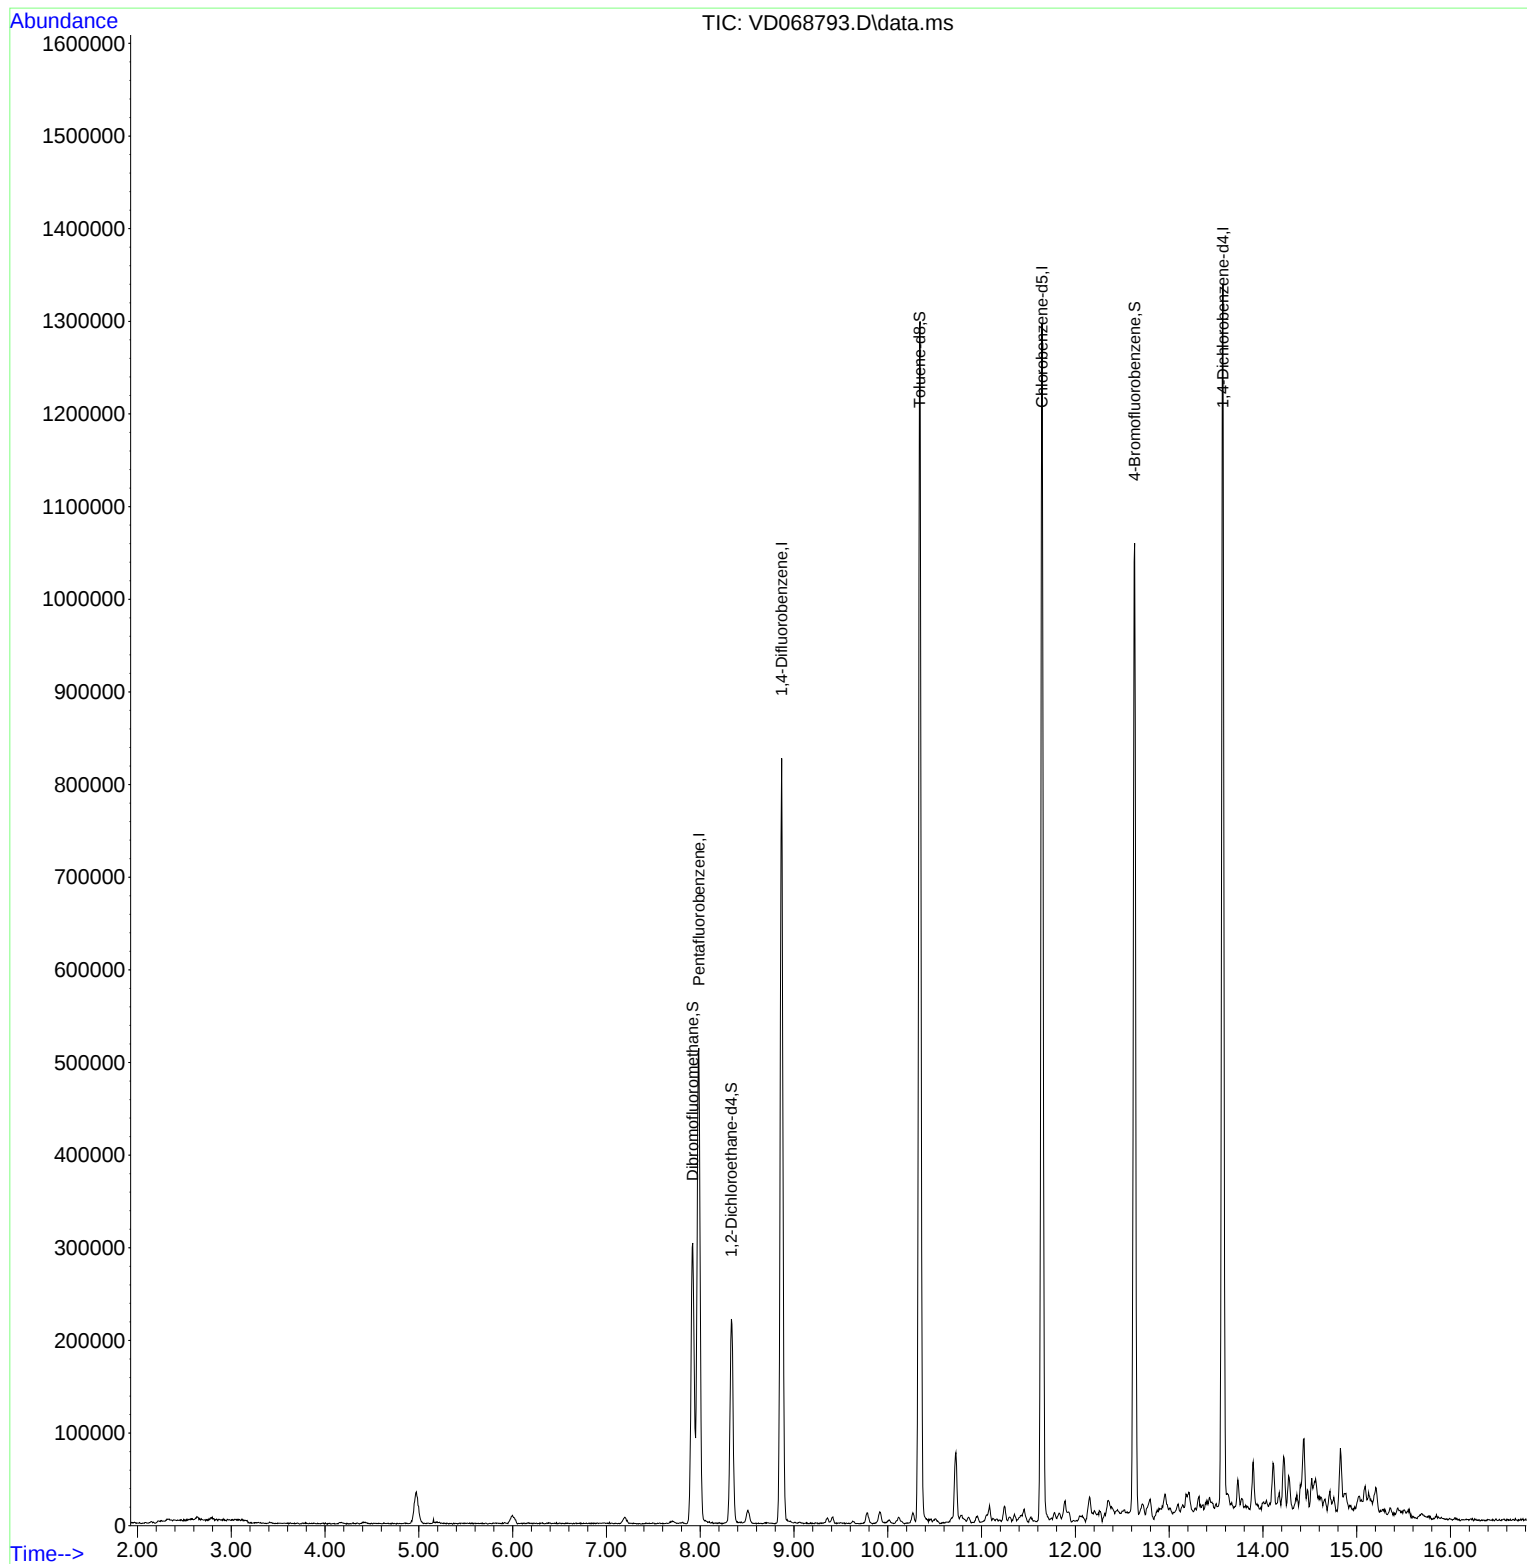


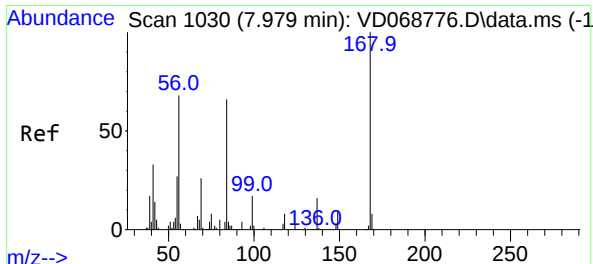

#1
Pentafluorobenzene
Concen: 50.00 ug/l
RT: 7.985 min Scan# 1031
Delta R.T. 0.006 min
Lab File: VD068793.D
Acq: 08 Apr 2021 17:04




Instrument :
MSVOA_D
ClientSampled :
S-20


Tgt Ion:168 Resp: 400675
Ion Ratio Lower Upper
168 100
99 53.7 46.2 69.2

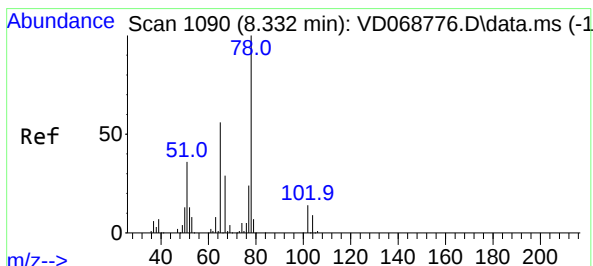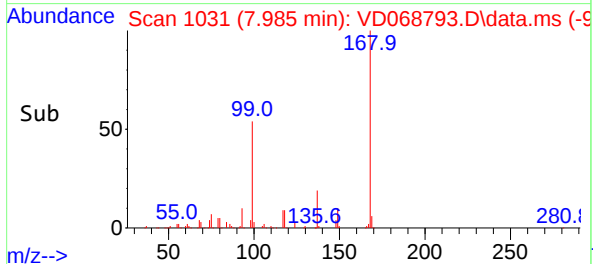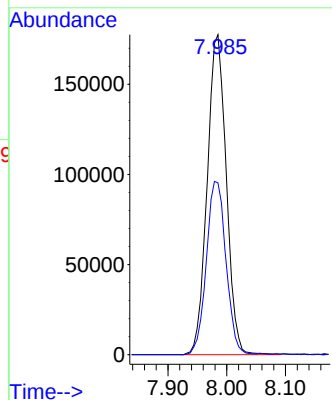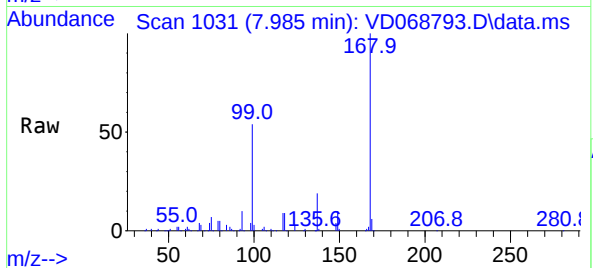

#33
1,2-Dichloroethane-d4
Concen: 42.78 ug/l
RT: 8.332 min Scan# 1090
Delta R.T. 0.000 min
Lab File: VD068793.D
Acq: 08 Apr 2021 17:04

Tgt Ion: 65 Resp: 181139
Ion Ratio Lower Upper
65 100
67 51.6 0.0 106.0

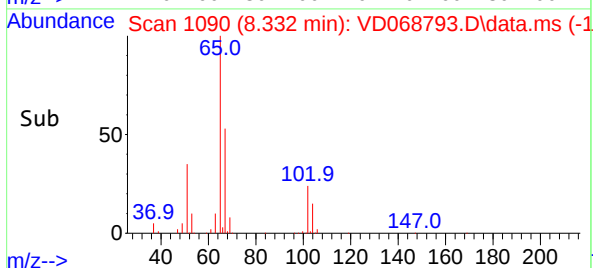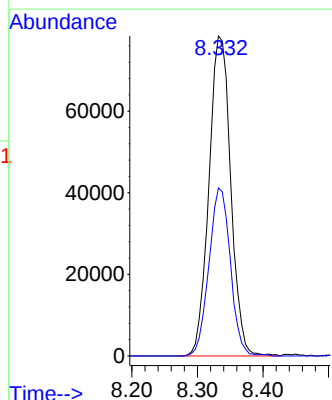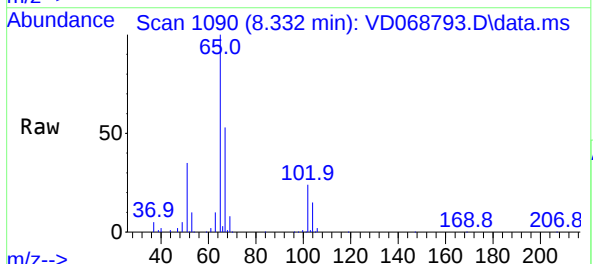




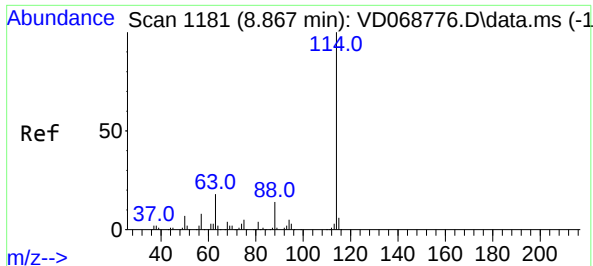


#34

1,4-Difluorobenzene
Concen: 50.00 ug/l
RT: 8.867 min Scan# 1181
Delta R.T. 0.000 min
Lab File: VD068793.D
Acq: 08 Apr 2021 17:04

Instrument :
MSVOA_D
ClientSampled :
S-20




Tgt Ion:114 Resp: 741008
Ion Ratio Lower Upper
114 100
63 16.9 0.0 38.2
88 14.3 0.0 29.4

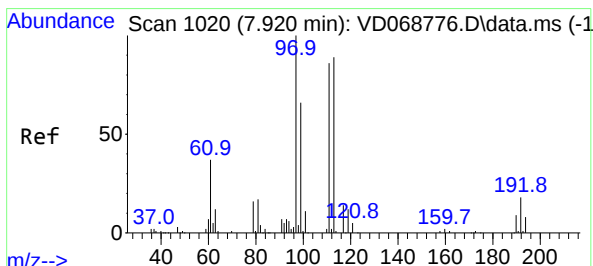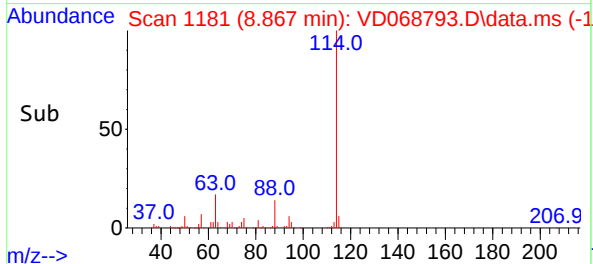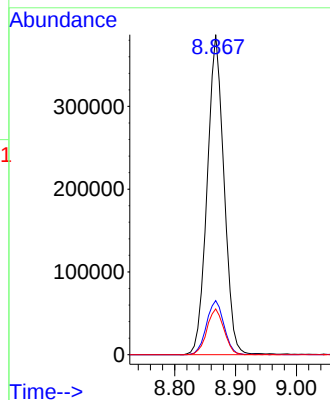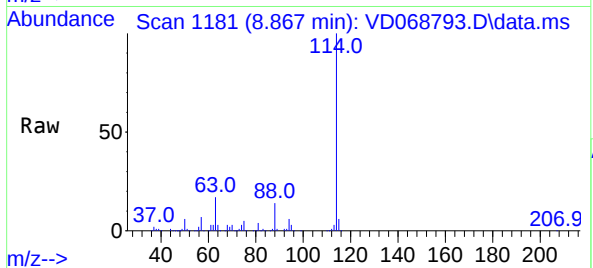


#35

Dibromofluoromethane
Concen: 45.12 ug/l
RT: 7.920 min Scan# 1020
Delta R.T. 0.000 min
Lab File: VD068793.D
Acq: 08 Apr 2021 17:04

Tgt Ion:113 Resp: 217470
Ion Ratio Lower Upper
113 100
111 105.3 82.5 123.7
192 20.6 15.1 22.7


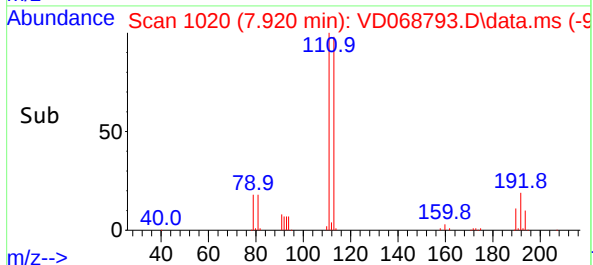
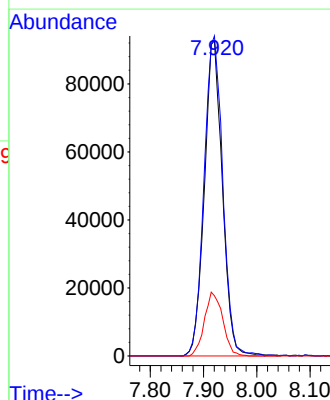
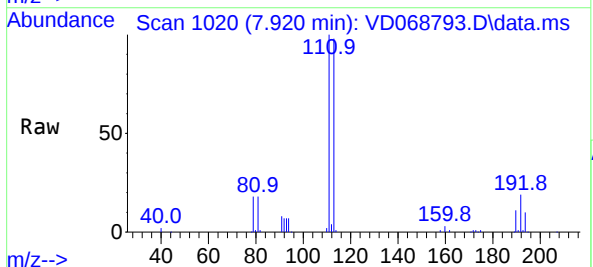


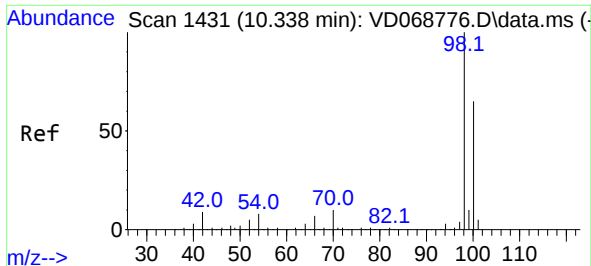

#50
Toluene-d8
Concen: 51.28 ug/l
RT: 10.338 min Scan# 1431
Delta R.T. -0.000 min
Lab File: VD068793.D
Acq: 08 Apr 2021 17:04




Instrument :
MSVOA_D
ClientSampled :
S-20


Tgt Ion: 98 Resp: 932342
Ion Ratio Lower Upper
98 100
100 64.9 51.8 77.6

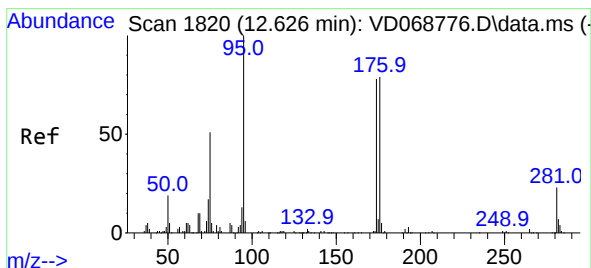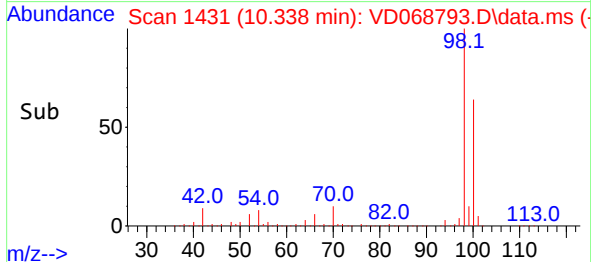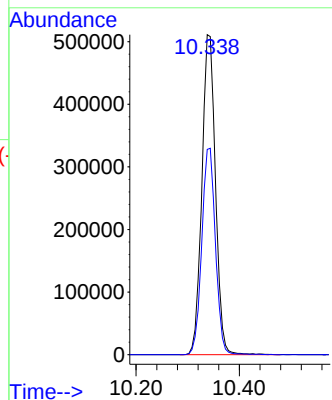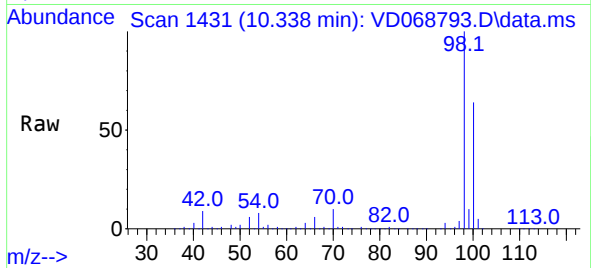

#62
4-Bromofluorobenzene
Concen: 56.46 ug/l
RT: 12.632 min Scan# 1821
Delta R.T. 0.006 min
Lab File: VD068793.D
Acq: 08 Apr 2021 17:04

Tgt Ion: 95 Resp: 340969
Ion Ratio Lower Upper
95 100
174 88.0 0.0 168.0
176 84.9 0.0 160.2


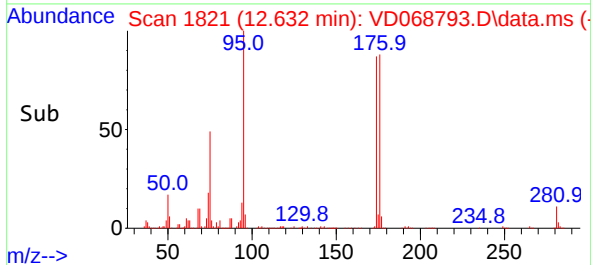
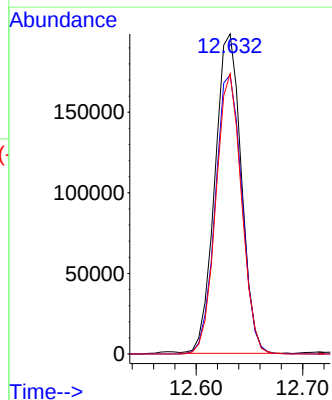
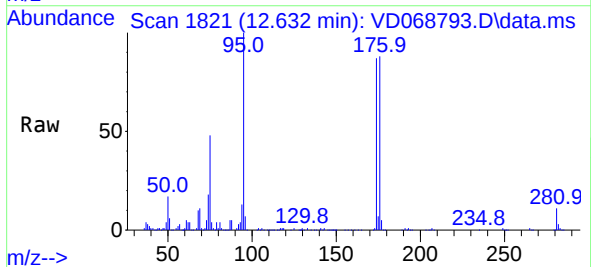


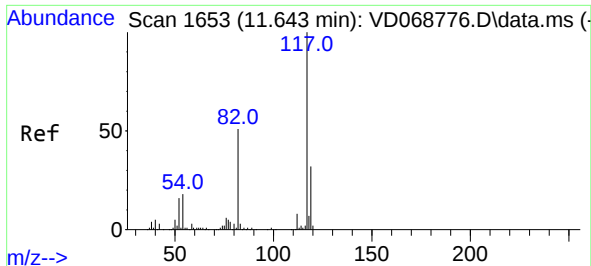

#63
Chlorobenzene-d5
Concen: 50.00 ug/l
RT: 11.644 min Scan# 1653
Delta R.T. 0.001 min
Lab File: VD068793.D
Acq: 08 Apr 2021 17:04

Instrument :
MSVOA_D
ClientSampleId :
S-20

Tgt Ion:	117	Resp:	775657
Ion	Ratio	Lower	Upper
117	100		
82	53.0	43.5	65.3
119	32.8	26.7	40.1

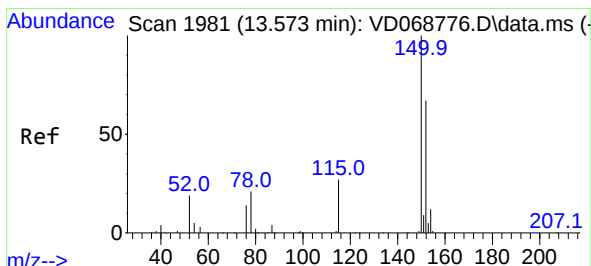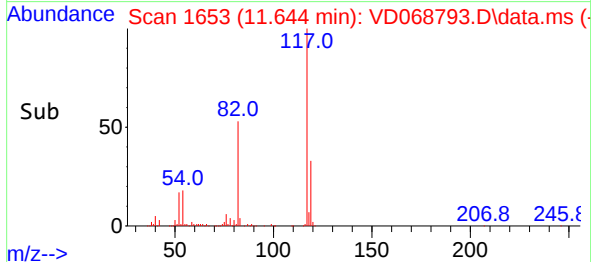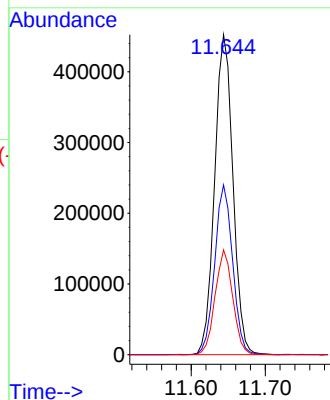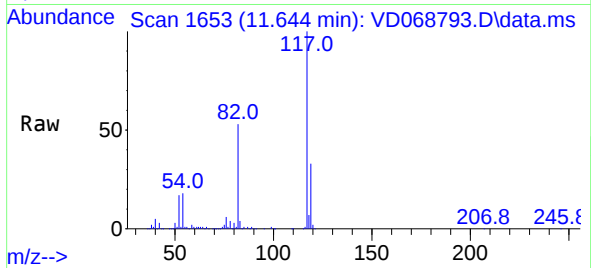

#72
1,4-Dichlorobenzene-d4
Concen: 50.00 ug/l
RT: 13.573 min Scan# 1981
Delta R.T. -0.000 min
Lab File: VD068793.D
Acq: 08 Apr 2021 17:04

Tgt Ion:	152	Resp:	372929
Ion	Ratio	Lower	Upper
152	100		
115	57.3	29.3	87.8
150	157.5	0.0	347.6

