
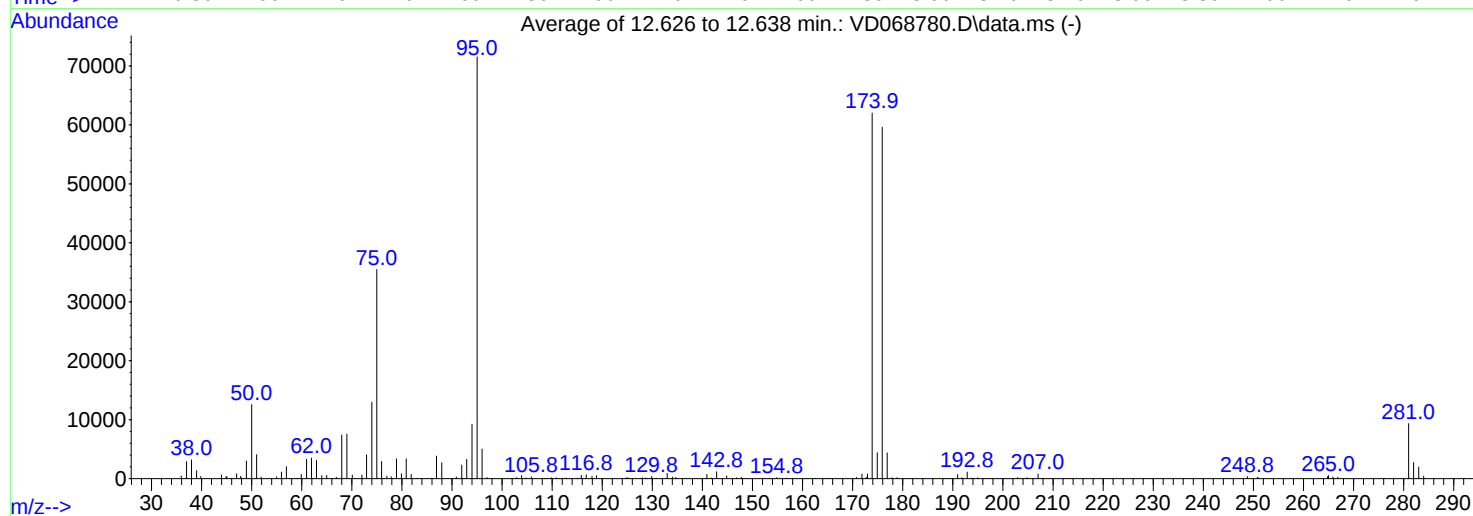


Data Path : Z:\voasrv\HPCHEM1\MSVOA\_D\Data\VD040821\  
Data File : VD068780.D  
Acq On : 08 Apr 2021 10:37  
Operator : VA/SY  
Sample : BFB  
Misc : 5.00G/5.00ml/MSVOA\_D/SOIL  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
MSVOA\_D  
ClientSampleId :  
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA\_D\Method\82D040721S.M  
Title : SW846 8260  
Last Update : Thu Apr 08 03:50:31 2021

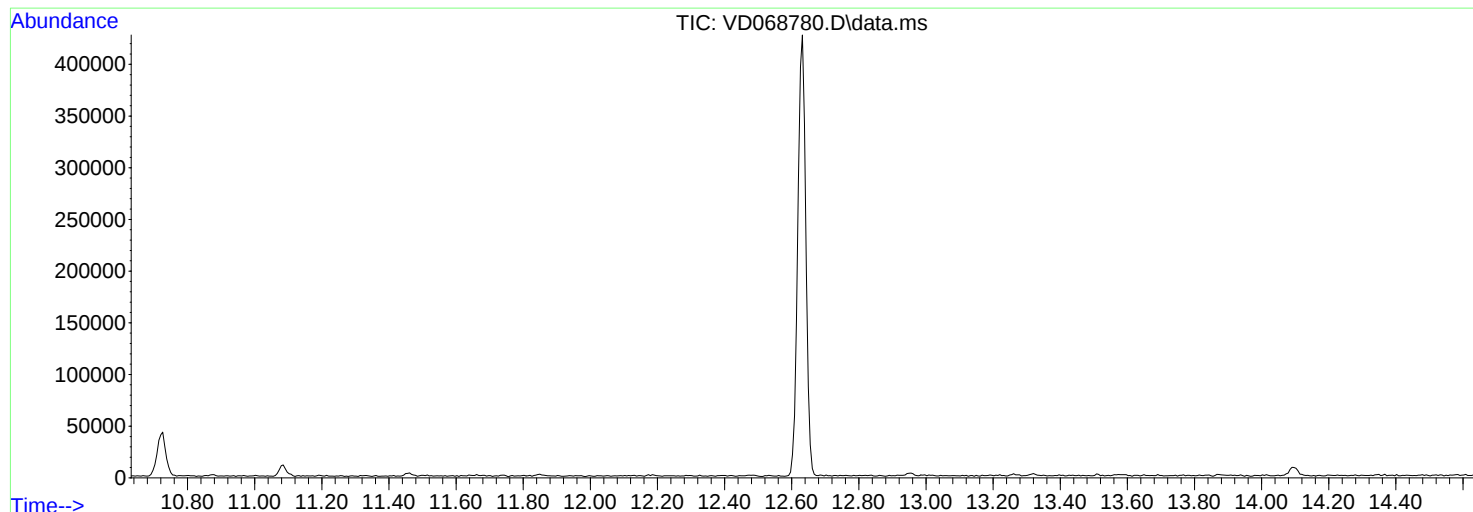

AutoFind: Scans 1820, 1821, 1822; Background Corrected with Scan 1812

| Target | Rel. to | Lower  | Upper  | Rel.  | Raw   | Result    |
|--------|---------|--------|--------|-------|-------|-----------|
| Mass   | Mass    | Limit% | Limit% | Abn%  | Abn   | Pass/Fail |
| 50     | 95      | 15     | 40     | 17.5  | 12551 | PASS      |
| 75     | 95      | 30     | 60     | 49.6  | 35461 | PASS      |
| 95     | 95      | 100    | 100    | 100.0 | 71541 | PASS      |
| 96     | 95      | 5      | 9      | 7.0   | 5031  | PASS      |
| 173    | 174     | 0.00   | 2      | 1.3   | 785   | PASS      |
| 174    | 95      | 50     | 100    | 86.7  | 62005 | PASS      |
| 175    | 174     | 5      | 9      | 7.1   | 4405  | PASS      |
| 176    | 174     | 95     | 101    | 96.1  | 59584 | PASS      |
| 177    | 176     | 5      | 9      | 7.3   | 4361  | PASS      |