

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD040822\
 Data File : VD072554.D
 Acq On : 08 Apr 2022 12:06
 Operator : VA/SY
 Sample : VD0408SBL01
 Misc : 5.00G/5.00ml/MSVOA_D/SOIL
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 VD0408SBL01

Quant Time: Apr 09 00:34:04 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D032922S.M
 Quant Title : SW846 8260
 QLast Update : Wed Mar 30 02:44:36 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	7.973	168	538683	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.861	114	990202	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.638	117	904508	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.561	152	405970	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.326	65	290291	44.548	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	=	89.100%
35) Dibromofluoromethane	7.908	113	319267	41.489	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	=	82.980%
50) Toluene-d8	10.332	98	1178757	44.067	ug/l	0.00
Spiked Amount	50.000	Range	49 - 140	Recovery	=	88.140%
62) 4-Bromofluorobenzene	12.620	95	403546	38.629	ug/l	0.00
Spiked Amount	50.000	Range	25 - 144	Recovery	=	77.260%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD040822\
Data File : VD072554.D
Acq On : 08 Apr 2022 12:06
Operator : VA/SY
Sample : VD0408SBL01
Misc : 5.00G/5.00ml/MSVOA_D/SOIL
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
VD0408SBL01

Quant Time: Apr 09 00:34:04 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D032922S.M
Quant Title : SW846 8260
QLast Update : Wed Mar 30 02:44:36 2022
Response via : Initial Calibration

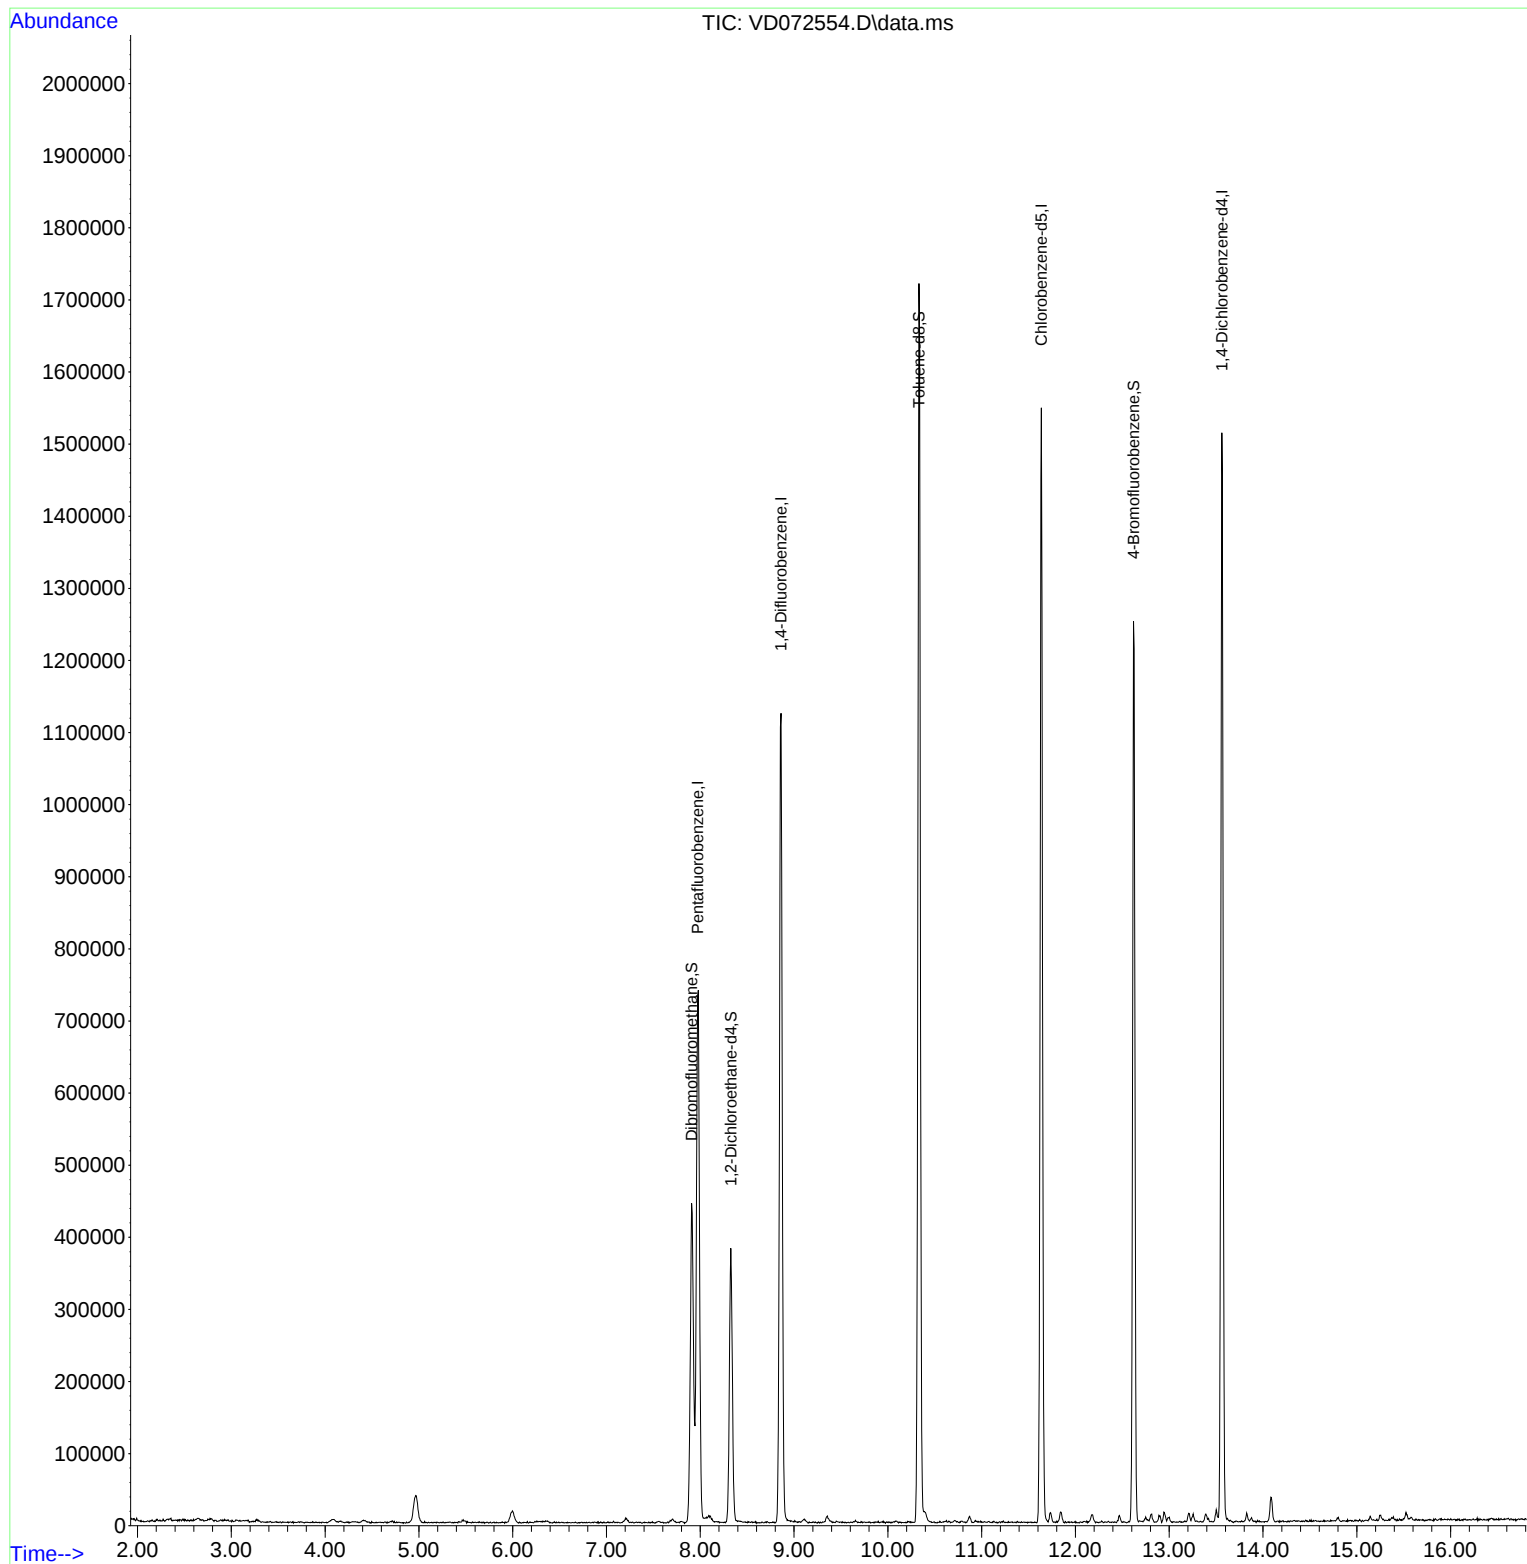

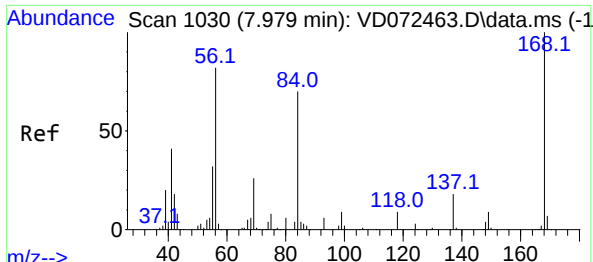

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 7.973 min Scan# 1029

Delta R.T. -0.006 min

Lab File: VD072554.D

Acq: 08 Apr 2022 12:06

Instrument :

MSVOA_D

ClientSampleId :





VD0408SBL01

Tgt Ion:168 Resp: 538683

Ion Ratio Lower Upper

168 100

99 60.7 49.8 74.6

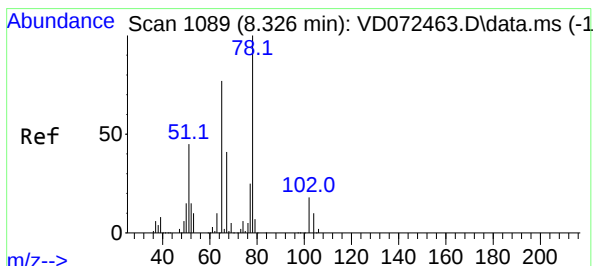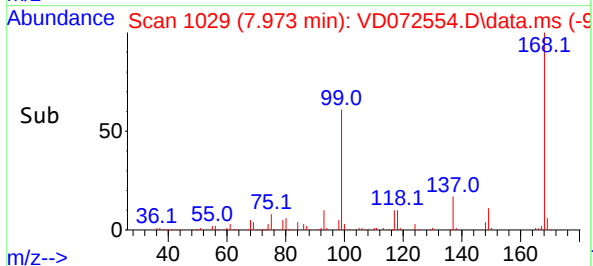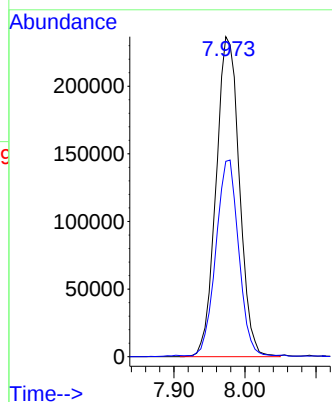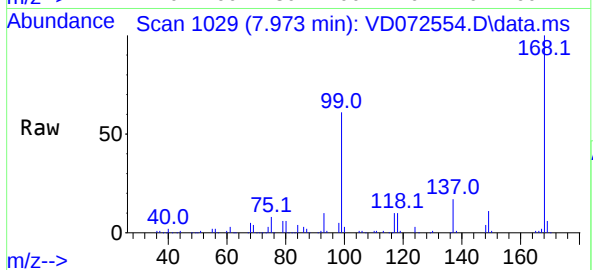

1,2-Dichloroethane-d4

Concen: 44.548 ug/l

RT: 8.326 min Scan# 1089

Delta R.T. -0.000 min

Lab File: VD072554.D




Acq: 08 Apr 2022 12:06


Tgt Ion: 65 Resp: 290291

Ion Ratio Lower Upper

65 100

67 53.5 0.0 101.4


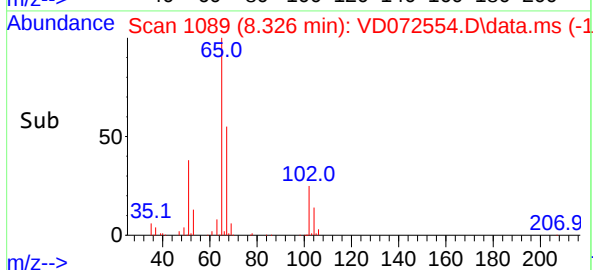
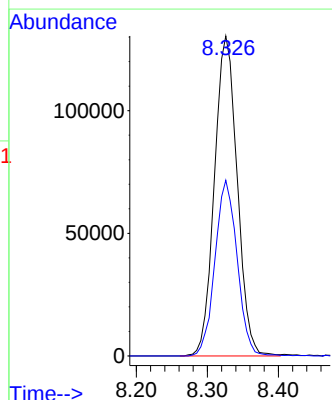
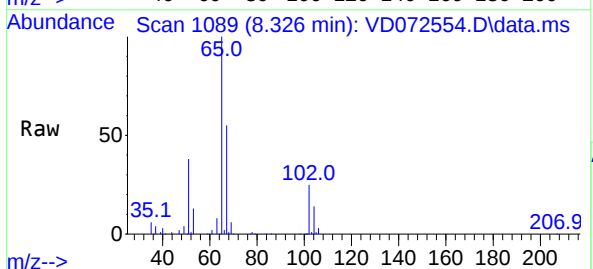


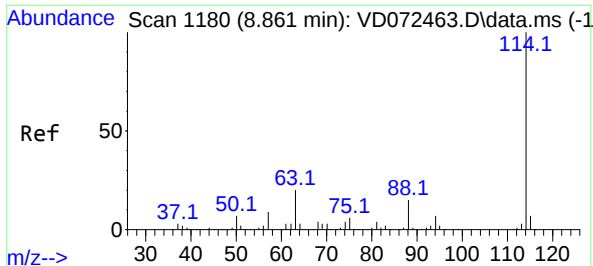

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 8.861 min Scan# 1180
Delta R.T. -0.000 min
Lab File: VD072554.D
Acq: 08 Apr 2022 12:06




Instrument :
MSVOA_D
ClientSampleId :
VD0408SBL01

Tgt Ion:114 Resp: 990202
Ion Ratio Lower Upper
114 100
63 18.7 0.0 46.6
88 15.3 0.0 33.2

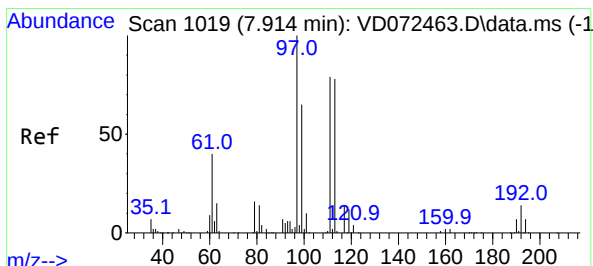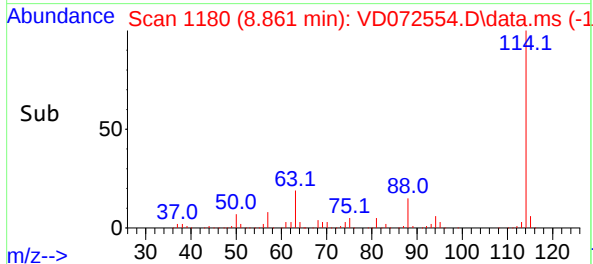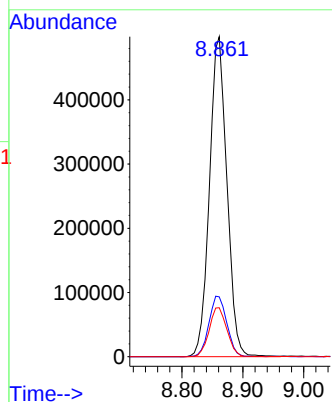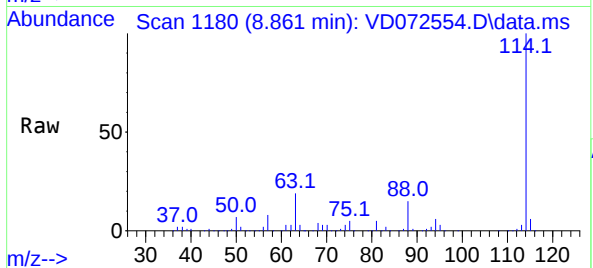

#35
Dibromofluoromethane
Concen: 41.489 ug/l
RT: 7.908 min Scan# 1018
Delta R.T. -0.006 min
Lab File: VD072554.D
Acq: 08 Apr 2022 12:06

Tgt Ion:113 Resp: 319267
Ion Ratio Lower Upper
113 100
111 102.0 83.8 125.6
192 18.3 14.6 21.8


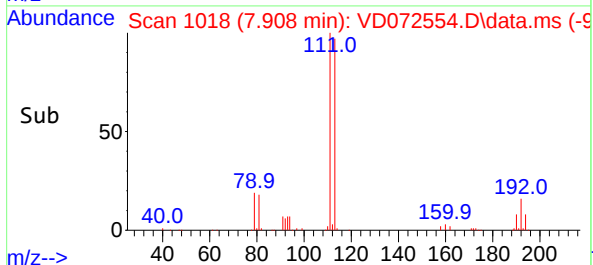
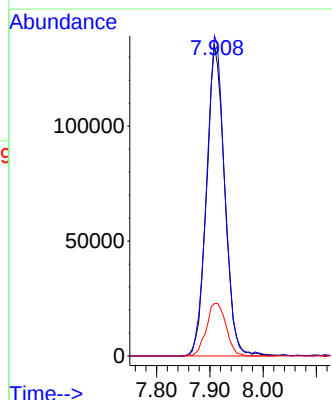
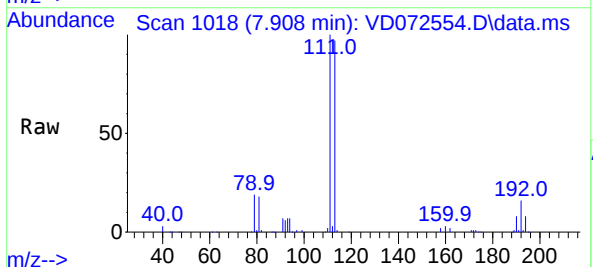




#50
Toluene-d8
Concen: 44.067 ug/l
RT: 10.332 min Scan# 1431
Delta R.T. -0.006 min
Lab File: VD072554.D
Acq: 08 Apr 2022 12:06




Instrument :
MSVOA_D
ClientSampleId :
VD0408SBL01


Tgt Ion: 98 Resp: 1178757
Ion Ratio Lower Upper
98 100
100 66.3 52.4 78.6

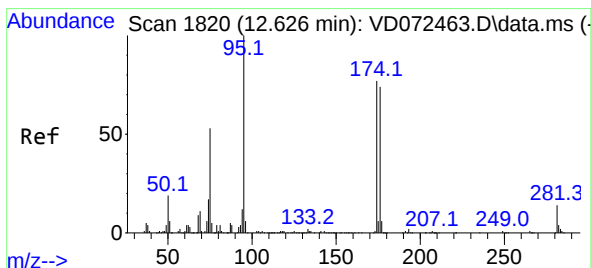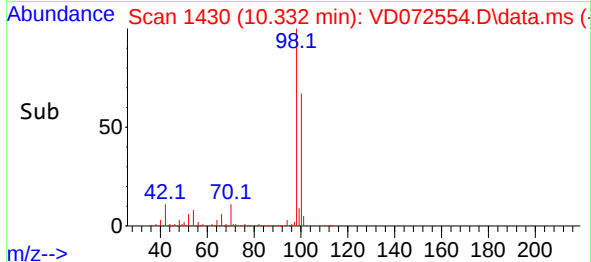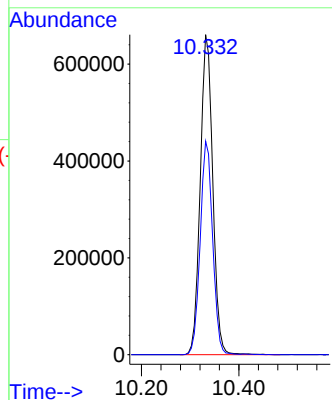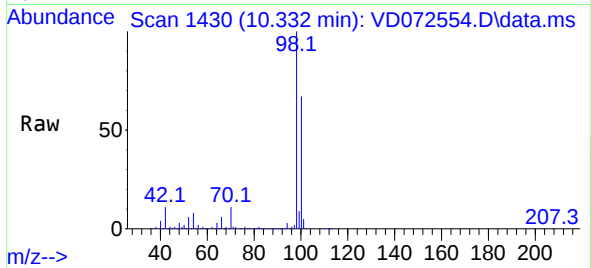

#62
4-Bromofluorobenzene
Concen: 38.629 ug/l
RT: 12.620 min Scan# 1819
Delta R.T. -0.006 min
Lab File: VD072554.D
Acq: 08 Apr 2022 12:06

Tgt Ion: 95 Resp: 403546
Ion Ratio Lower Upper
95 100
174 77.0 0.0 152.8
176 73.8 0.0 145.4


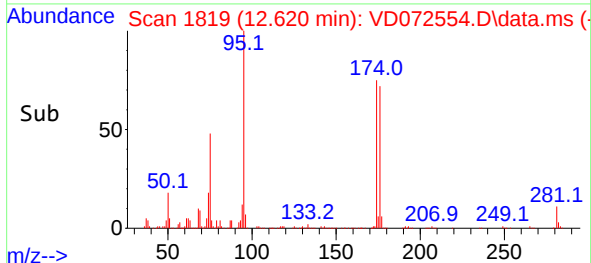
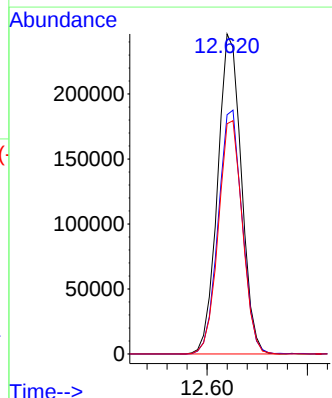
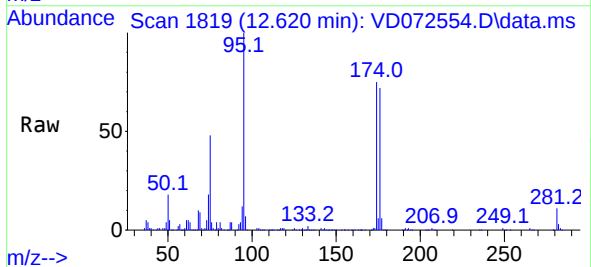


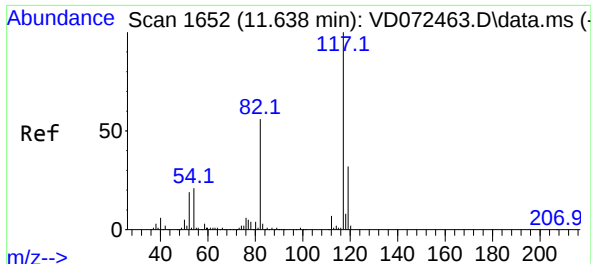

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.638 min Scan# 1179
Delta R.T. -0.000 min
Lab File: VD072554.D
Acq: 08 Apr 2022 12:06

Instrument :
MSVOA_D
ClientSampleId :
VD0408SBL01

Tgt Ion:	117	Resp:	904508
Ion	Ratio	Lower	Upper
117	100		
82	53.7	45.3	67.9
119	31.8	26.6	40.0

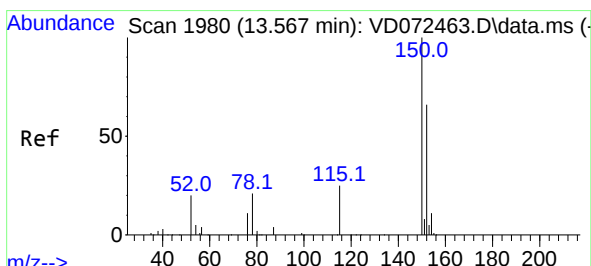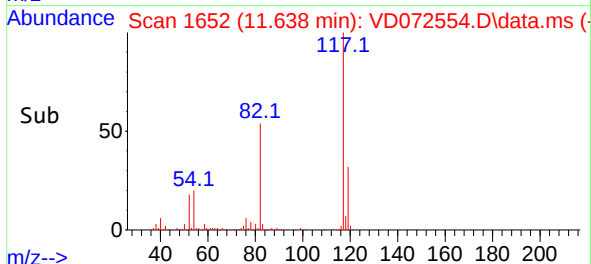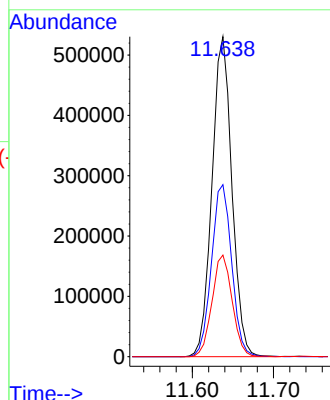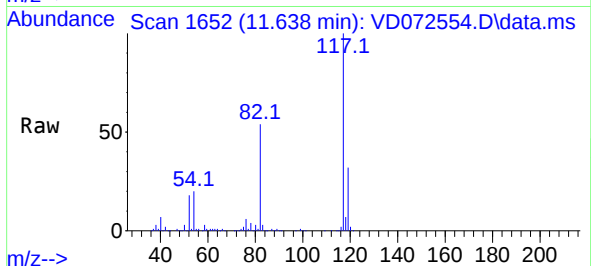

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.561 min Scan# 1979
Delta R.T. -0.006 min
Lab File: VD072554.D
Acq: 08 Apr 2022 12:06

Tgt Ion:	152	Resp:	405970
Ion	Ratio	Lower	Upper
152	100		
115	61.6	31.3	93.8
150	157.0	0.0	348.6

