


Data Path : Z:\voasrv\HPCHEM1\MSVOA D\Data\VD040919\
 Data File : VD061670.D
 Acq On : 9 Apr 2019 12:33
 Operator : VA/AP
 Sample : BFB
 Misc : 5.00µl/5ml/MSVOA D/SOIL
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D040619S.M
 Title : SW846 8260
 Last Update : Mon Apr 08 10:04:03 2019

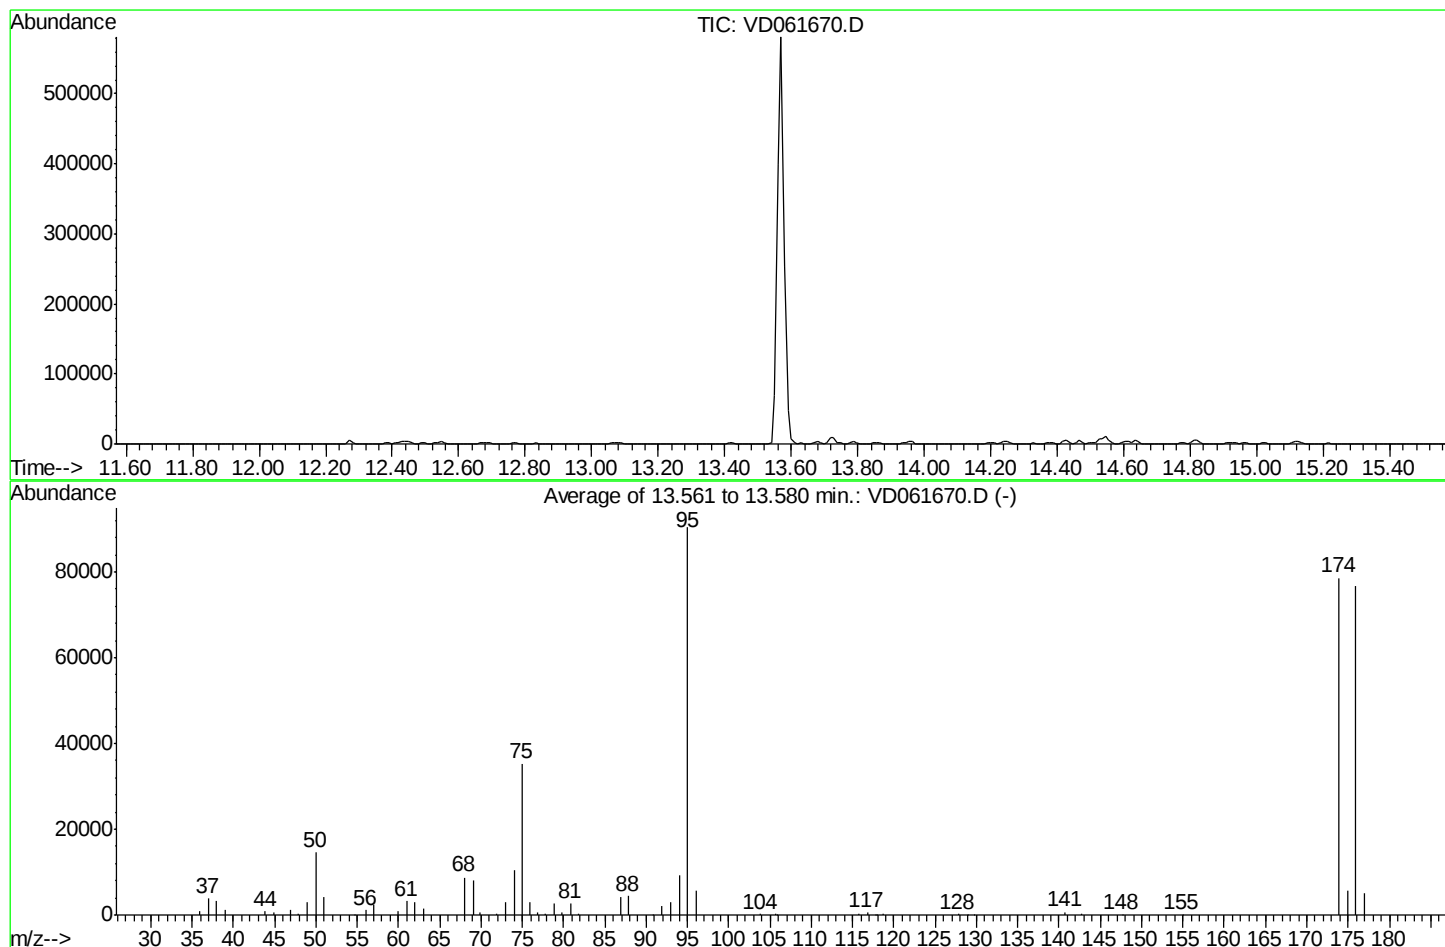

AutoFind: Scans 1233, 1234, 1235; Background Corrected with Scan 1228

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.1	14538	PASS
75	95	30	60	39.1	35336	PASS
95	95	100	100	100.0	90408	PASS
96	95	5	9	6.4	5826	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	86.9	78602	PASS
175	174	5	9	7.3	5724	PASS
176	174	95	101	97.6	76722	PASS
177	176	5	9	6.6	5063	PASS