


Data Path : Z:\voasrv\HPCHEM1\MSVOA D\Data\VD040920\
Data File : VD065605.D
Acq On : 09 Apr 2020 09:35
Operator : VA/SY
Sample : BFB
Misc : 5.00G/5.00ml/MSVOA D/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D040920S.M
Title : SW846 8260
Last Update : Fri Apr 10 01:39:58 2020

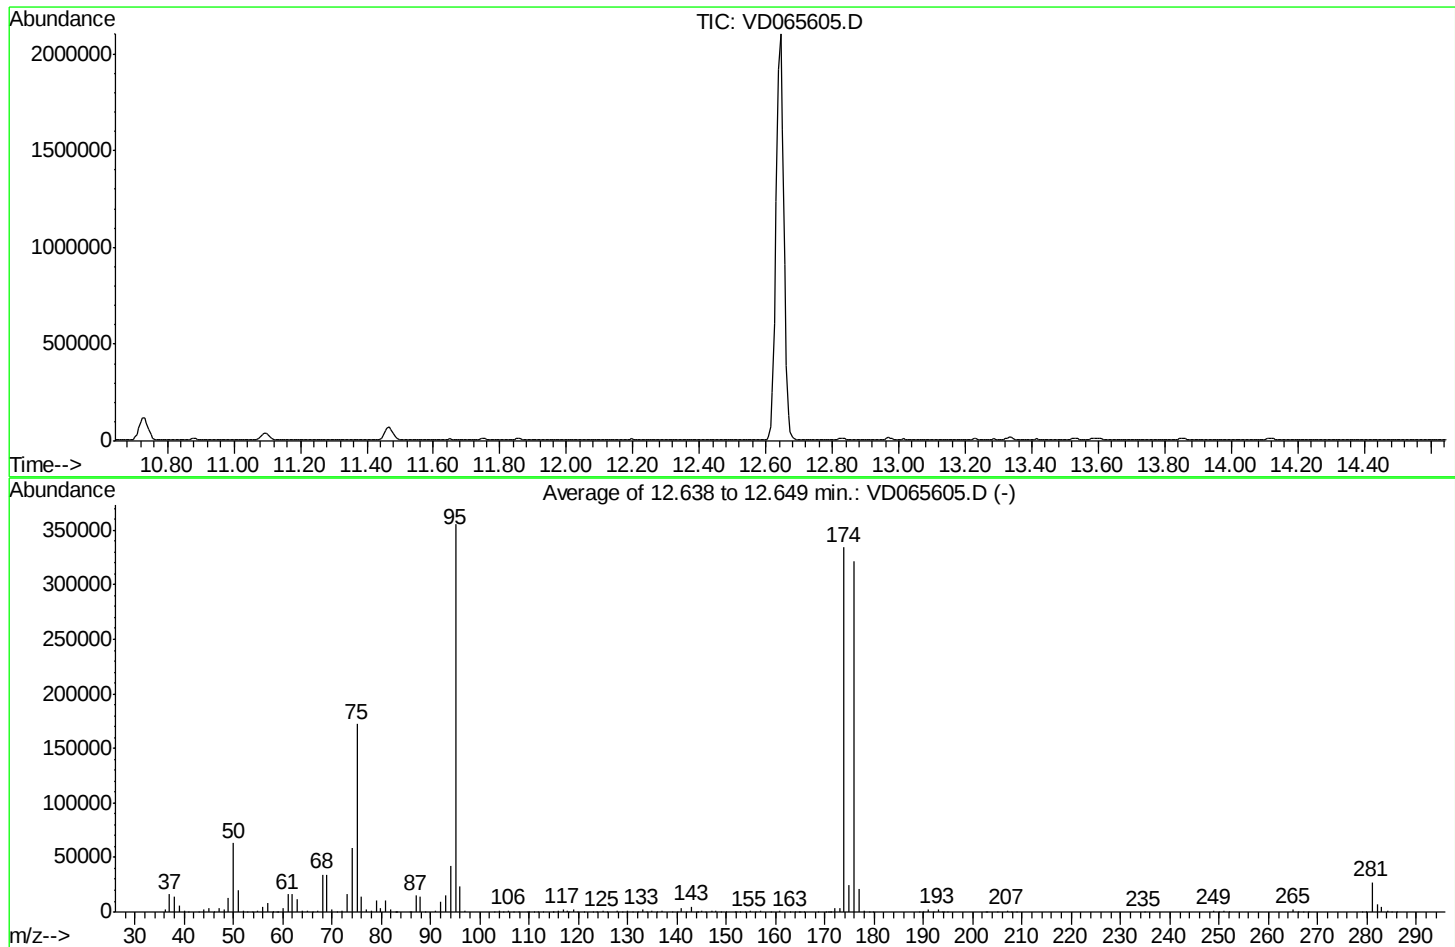

AutoFind: Scans 1822, 1823, 1824; Background Corrected with Scan 1812

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.7	62960	PASS
75	95	30	60	48.4	172053	PASS
95	95	100	100	100.0	355392	PASS
96	95	5	9	6.6	23562	PASS
173	174	0.00	2	1.2	3898	PASS
174	95	50	100	94.0	334122	PASS
175	174	5	9	7.4	24677	PASS
176	174	95	101	96.2	321365	PASS
177	176	5	9	6.6	21253	PASS