
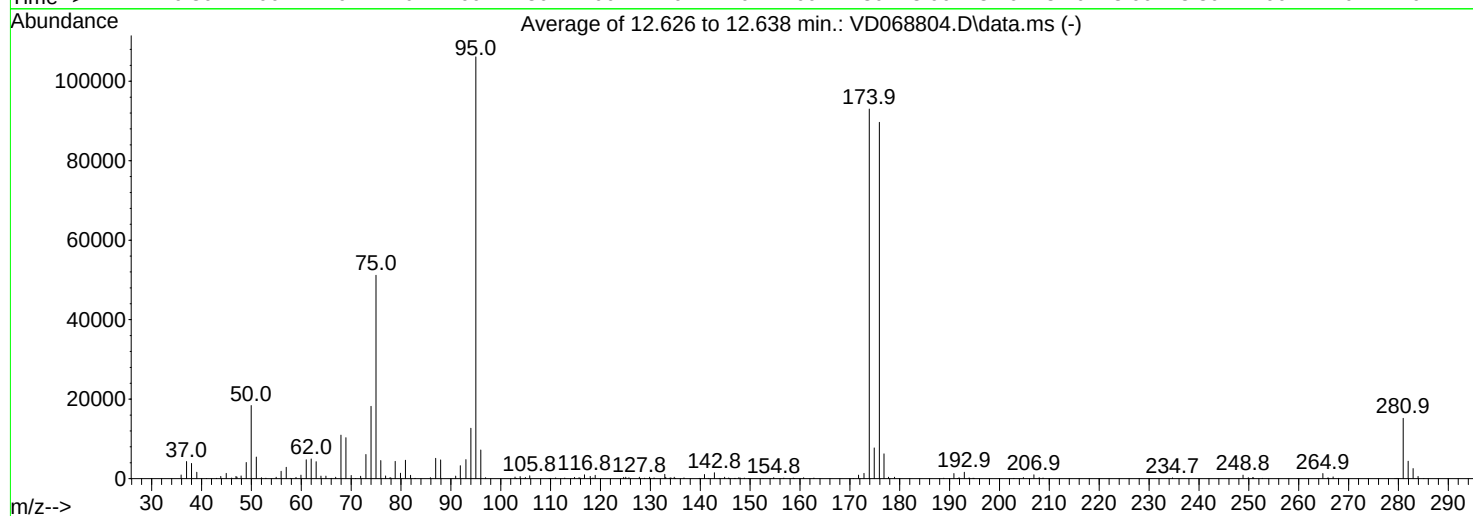


Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD040921\
Data File : VD068804.D
Acq On : 09 Apr 2021 09:28
Operator : VA/SY
Sample : BFB
Misc : 5.00G/5.00ml/MSVOA_D/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D040721S.M
Title : SW846 8260
Last Update : Thu Apr 08 03:50:31 2021

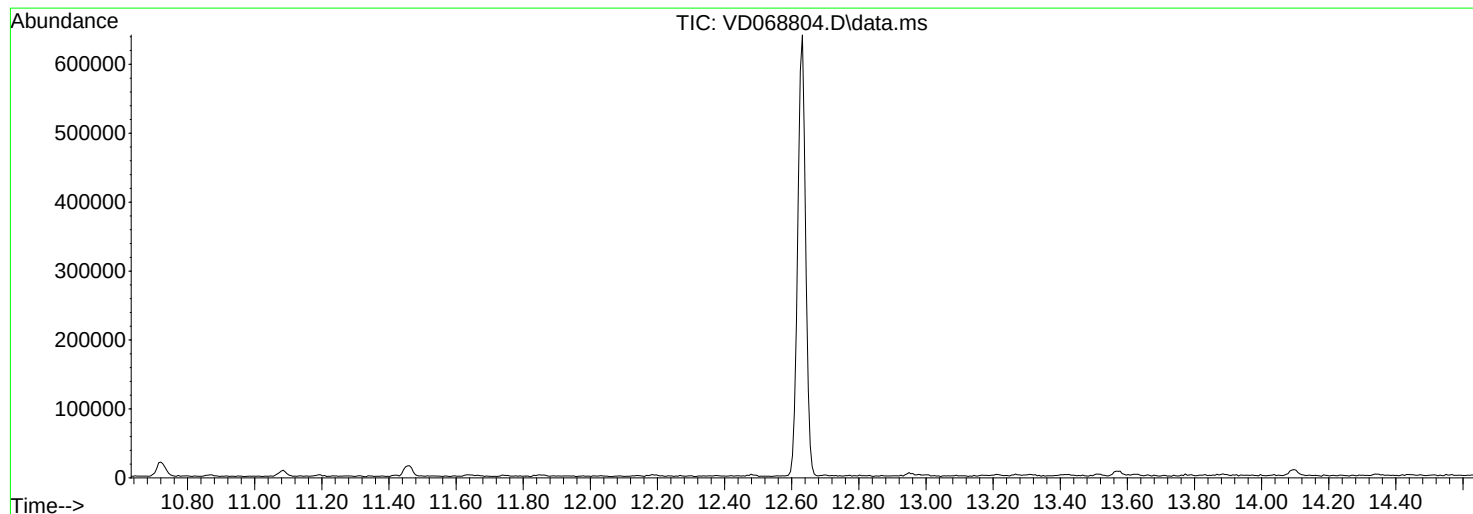

AutoFind: Scans 1820, 1821, 1822; Background Corrected with Scan 1811

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	17.3	18402	PASS
75	95	30	60	48.2	51176	PASS
95	95	100	100	100.0	106136	PASS
96	95	5	9	6.8	7204	PASS
173	174	0.00	2	1.4	1322	PASS
174	95	50	100	87.6	92984	PASS
175	174	5	9	8.3	7739	PASS
176	174	95	101	96.4	89675	PASS
177	176	5	9	7.0	6262	PASS