


Data Path : Z:\voasrv\HPCHEM1\MSVOA D\Data\VD041019\
 Data File : VD061727.D
 Acq On : 10 Apr 2019 22:44
 Operator : VA/AP
 Sample : BFB
 Misc : 5.00µl/5ml/MSVOA D/SOIL
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D040619S.M
 Title : SW846 8260
 Last Update : Mon Apr 08 10:04:03 2019

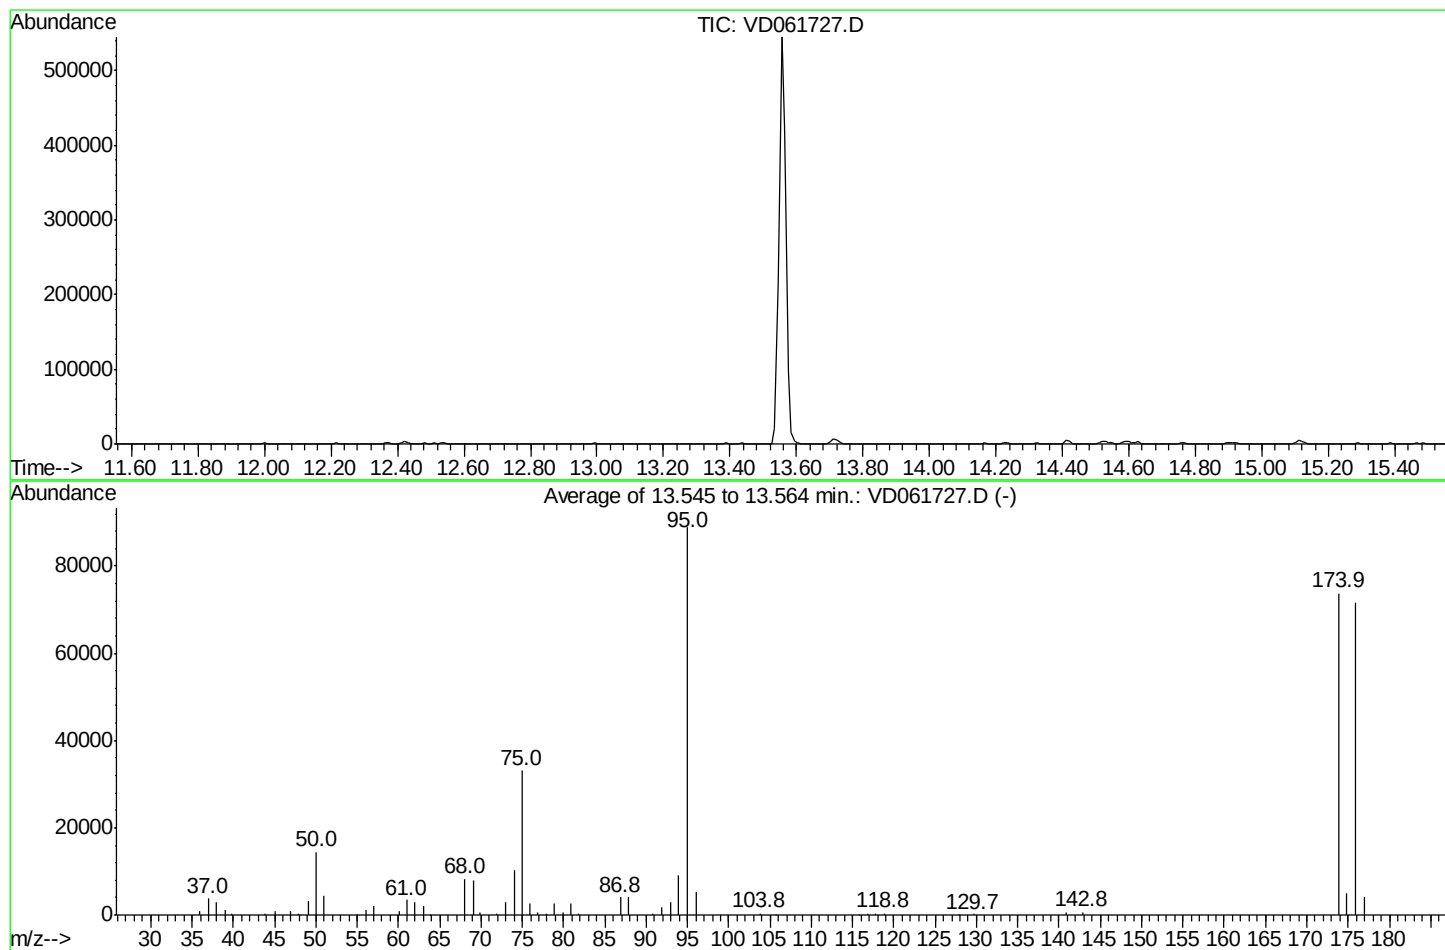

AutoFind: Scans 1231, 1232, 1233; Background Corrected with Scan 1227

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.2	14423	PASS
75	95	30	60	37.3	33144	PASS
95	95	100	100	100.0	88877	PASS
96	95	5	9	6.1	5439	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	82.9	73680	PASS
175	174	5	9	6.9	5107	PASS
176	174	95	101	97.1	71536	PASS
177	176	5	9	5.8	4175	PASS