
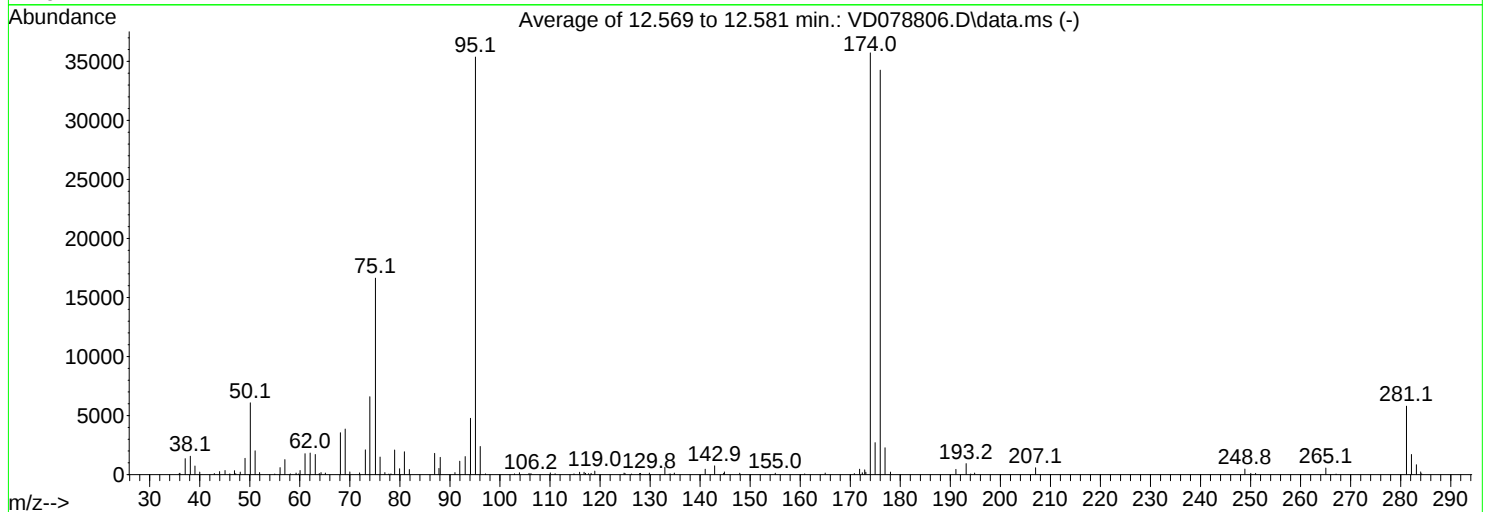


Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD041124\
Data File : VD078806.D
Acq On : 11 Apr 2024 10:41
Operator : RP/MD
Sample : BFB210
Misc : 5.00G/5ml/MSVOA_D/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB210

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\SFAMDLM041124SMA.M
Title : SFAM01.0
Last Update : Fri Apr 12 07:08:03 2024

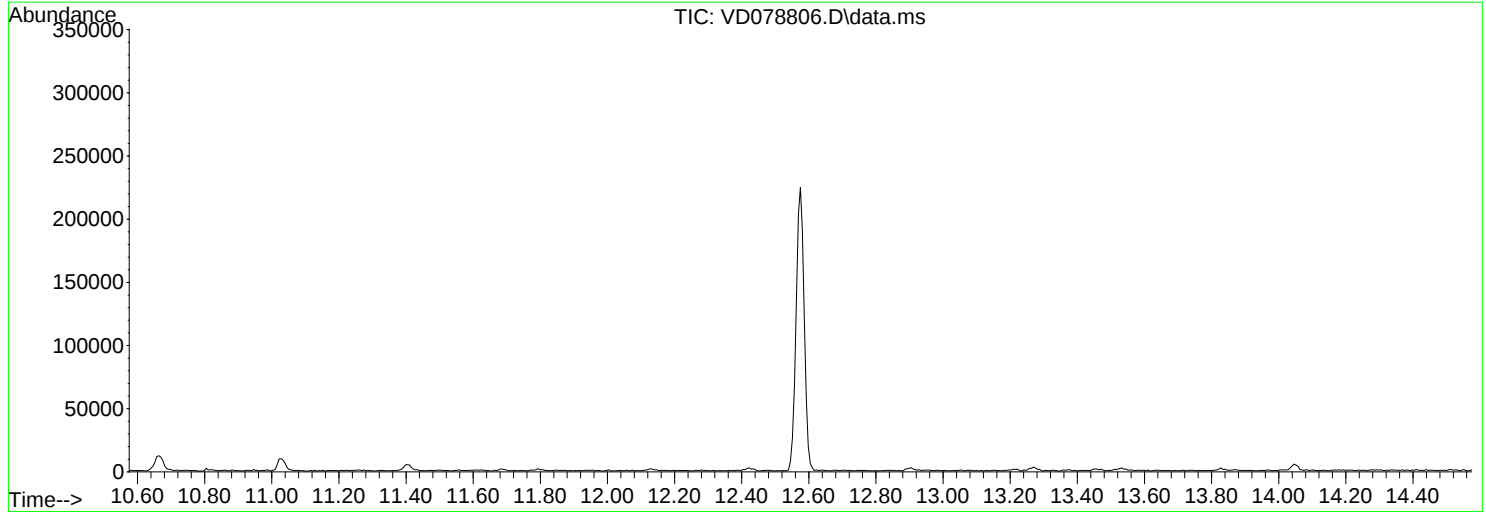

AutoFind: Scans 1867, 1868, 1869; Background Corrected with Scan 1860

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	17.2	6090	PASS
75	95	30	80	47.0	16639	PASS
95	95	100	100	100.0	35368	PASS
96	95	5	9	6.8	2392	PASS
173	174	0.00	2	1.1	404	PASS
174	95	50	120	101.0	35723	PASS
175	174	5	9	7.6	2709	PASS
176	174	95	105	95.9	34256	PASS
177	176	5	10	6.6	2273	PASS

Scan 1860 (12.528 min): VD078806.D\data.ms
BFB210

m/z	Abundance
40.00	674.0
44.10	336.0

Instrument :
MSVOA_D
ClientSampleId :
BFB210

m/z	Abundance
35.90	281.0
37.10	1644.0
38.10	1472.0
39.00	767.0
40.00	899.0
44.00	519.0
45.00	324.0
46.90	585.0
48.10	164.0
49.10	1423.0
50.10	6582.0
51.10	2552.0
51.90	159.0
56.10	621.0
57.00	1235.0
60.00	451.0
61.00	1887.0
62.00	2245.0
63.20	1922.0
63.90	299.0
68.10	3255.0
69.00	4225.0
70.00	255.0
72.00	259.0
73.10	2128.0
74.00	7107.0
75.10	17848.0
76.10	1692.0
78.90	2376.0
80.00	436.0
80.90	2394.0
81.90	472.0
87.00	1688.0
88.10	2239.0
92.00	1028.0
93.00	1413.0
94.10	4916.0
95.10	33800.0
96.10	2245.0
97.10	199.0
103.90	154.0
105.80	334.0
110.00	216.0
111.00	240.0
115.90	182.0
116.80	282.0
117.70	227.0
118.90	332.0
127.90	285.0
129.90	176.0
133.00	590.0
134.80	220.0
141.00	483.0
142.90	867.0
144.70	303.0
148.00	167.0
155.00	194.0
171.80	598.0
172.90	487.0
174.00	34104.0
175.00	2405.0
176.00	33264.0
176.90	2605.0
191.10	617.0
193.10	905.0
194.80	259.0
207.00	347.0
248.90	371.0
251.00	180.0
265.10	599.0
281.10	4856.0
282.10	892.0
283.10	637.0
284.00	218.0

Instrument :
MSVOA_D
ClientSampleId :
BFB210

m/z	Abundance
36.10	176.0
37.10	1437.0
38.10	1536.0
39.10	599.0
40.00	945.0
44.20	406.0
45.00	314.0
46.00	207.0
47.00	447.0
48.20	252.0
49.00	1413.0
50.10	6577.0
51.00	2306.0
52.00	231.0
55.00	158.0
56.00	551.0
57.00	1285.0
58.10	203.0
59.20	188.0
60.10	610.0
61.10	1599.0
62.10	1770.0
63.00	1850.0
64.30	157.0
65.10	391.0
68.10	4001.0
69.10	3941.0
70.00	154.0
71.90	209.0
73.00	2746.0
74.00	6939.0
75.10	17016.0
76.00	1565.0
77.00	320.0
77.80	174.0
79.00	2533.0
80.00	665.0
80.90	1758.0
81.80	475.0
87.00	2471.0
87.80	1589.0
91.00	225.0
91.90	1249.0
93.00	1819.0
94.10	4813.0
95.10	39256.0
96.00	2477.0
102.90	225.0
103.90	332.0
106.20	280.0
110.10	215.0
116.00	249.0
117.10	339.0
118.20	164.0
119.00	350.0
124.80	410.0
126.30	158.0
128.10	317.0
129.80	252.0
133.00	526.0
133.80	155.0
134.90	206.0
141.00	454.0
143.00	764.0
144.90	393.0
155.00	175.0
165.00	258.0
170.80	271.0
171.90	503.0
172.90	726.0
174.00	39000.0
174.90	3309.0
176.00	38184.0
176.90	1921.0
178.10	241.0
191.10	423.0
193.20	769.0
207.00	652.0
248.80	352.0
250.10	154.0
265.00	539.0
281.10	6387.0
282.10	2067.0
283.20	960.0
284.00	462.0

Instrument :
MSVOA_D
ClientSampleId :
BFB210

m/z	Abundance
36.00	203.0
37.10	983.0
38.10	1679.0
39.10	836.0
40.00	833.0
42.90	289.0
43.90	256.0
45.10	436.0
47.20	267.0
48.00	256.0
49.00	1302.0
50.10	5112.0
51.00	1220.0
51.90	158.0
56.00	614.0
57.00	1307.0
59.30	208.0
59.80	215.0
61.00	1830.0
62.10	1457.0
63.10	1342.0
64.20	358.0
68.10	3415.0
69.00	3408.0
70.00	298.0
73.20	1407.0
74.00	5755.0
75.10	15054.0
76.00	1218.0
77.00	201.0
78.20	224.0
78.90	1339.0
79.90	392.0
80.90	1659.0
82.00	367.0
86.80	1266.0
88.00	2154.0
91.00	324.0
92.00	1127.0
93.10	1353.0
94.10	4569.0
95.10	33048.0
96.10	2455.0
114.80	218.0
115.80	169.0
116.80	318.0
118.20	160.0
119.00	230.0
125.00	269.0
132.90	756.0
134.10	150.0
141.00	446.0
142.80	588.0
144.80	310.0
147.80	182.0
160.90	212.0
165.00	154.0
171.90	288.0
172.40	503.0
173.10	601.0
174.00	34064.0
175.00	2412.0
176.00	31320.0
177.00	2292.0
178.00	434.0
191.10	313.0
193.10	1147.0
194.10	159.0
194.90	162.0
207.10	754.0
248.90	690.0
250.00	175.0
251.00	162.0
265.10	513.0
267.10	170.0
281.20	6170.0
282.20	2167.0
283.10	916.0
284.20	196.0

Instrument :
MSVOA_D
ClientSampleId :
BFB210