

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD041221\
 Data File : VD068832.D
 Acq On : 12 Apr 2021 15:12
 Operator : VA/SY
 Sample : M1985-01
 Misc : 4.99G/5.00ml/MSVOA_D/SOIL
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 72-11939-72-11936

Quant Time: Apr 13 01:09:46 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D040721S.M
 Quant Title : SW846 8260
 QLast Update : Thu Apr 08 03:50:31 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	7.979	168	281029	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	8.867	114	491247	50.00	ug/l	0.00
63) Chlorobenzene-d5	11.644	117	526854	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.573	152	266866	50.00	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.332	65	117709	39.63	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	=	79.26%
35) Dibromofluoromethane	7.914	113	132276	41.40	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	=	82.80%
50) Toluene-d8	10.338	98	612909	50.85	ug/l	0.00
Spiked Amount	50.000	Range	49 - 140	Recovery	=	101.70%
62) 4-Bromofluorobenzene	12.632	95	234466	58.57	ug/l	0.00
Spiked Amount	50.000	Range	25 - 144	Recovery	=	117.14%
Target Compounds						
					Qvalue	
86) p-Isopropyltoluene	13.514	119	150710	8.46	ug/l	99
95) Naphthalene	15.391	128	11799	1.36	ug/l #	90


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD041221\
Data File : VD068832.D
Acq On : 12 Apr 2021 15:12
Operator : VA/SY
Sample : M1985-01
Misc : 4.99G/5.00ml/MSVOA_D/SOIL
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
72-11939-72-11936

Quant Time: Apr 13 01:09:46 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D040721S.M
Quant Title : SW846 8260
QLast Update : Thu Apr 08 03:50:31 2021
Response via : Initial Calibration




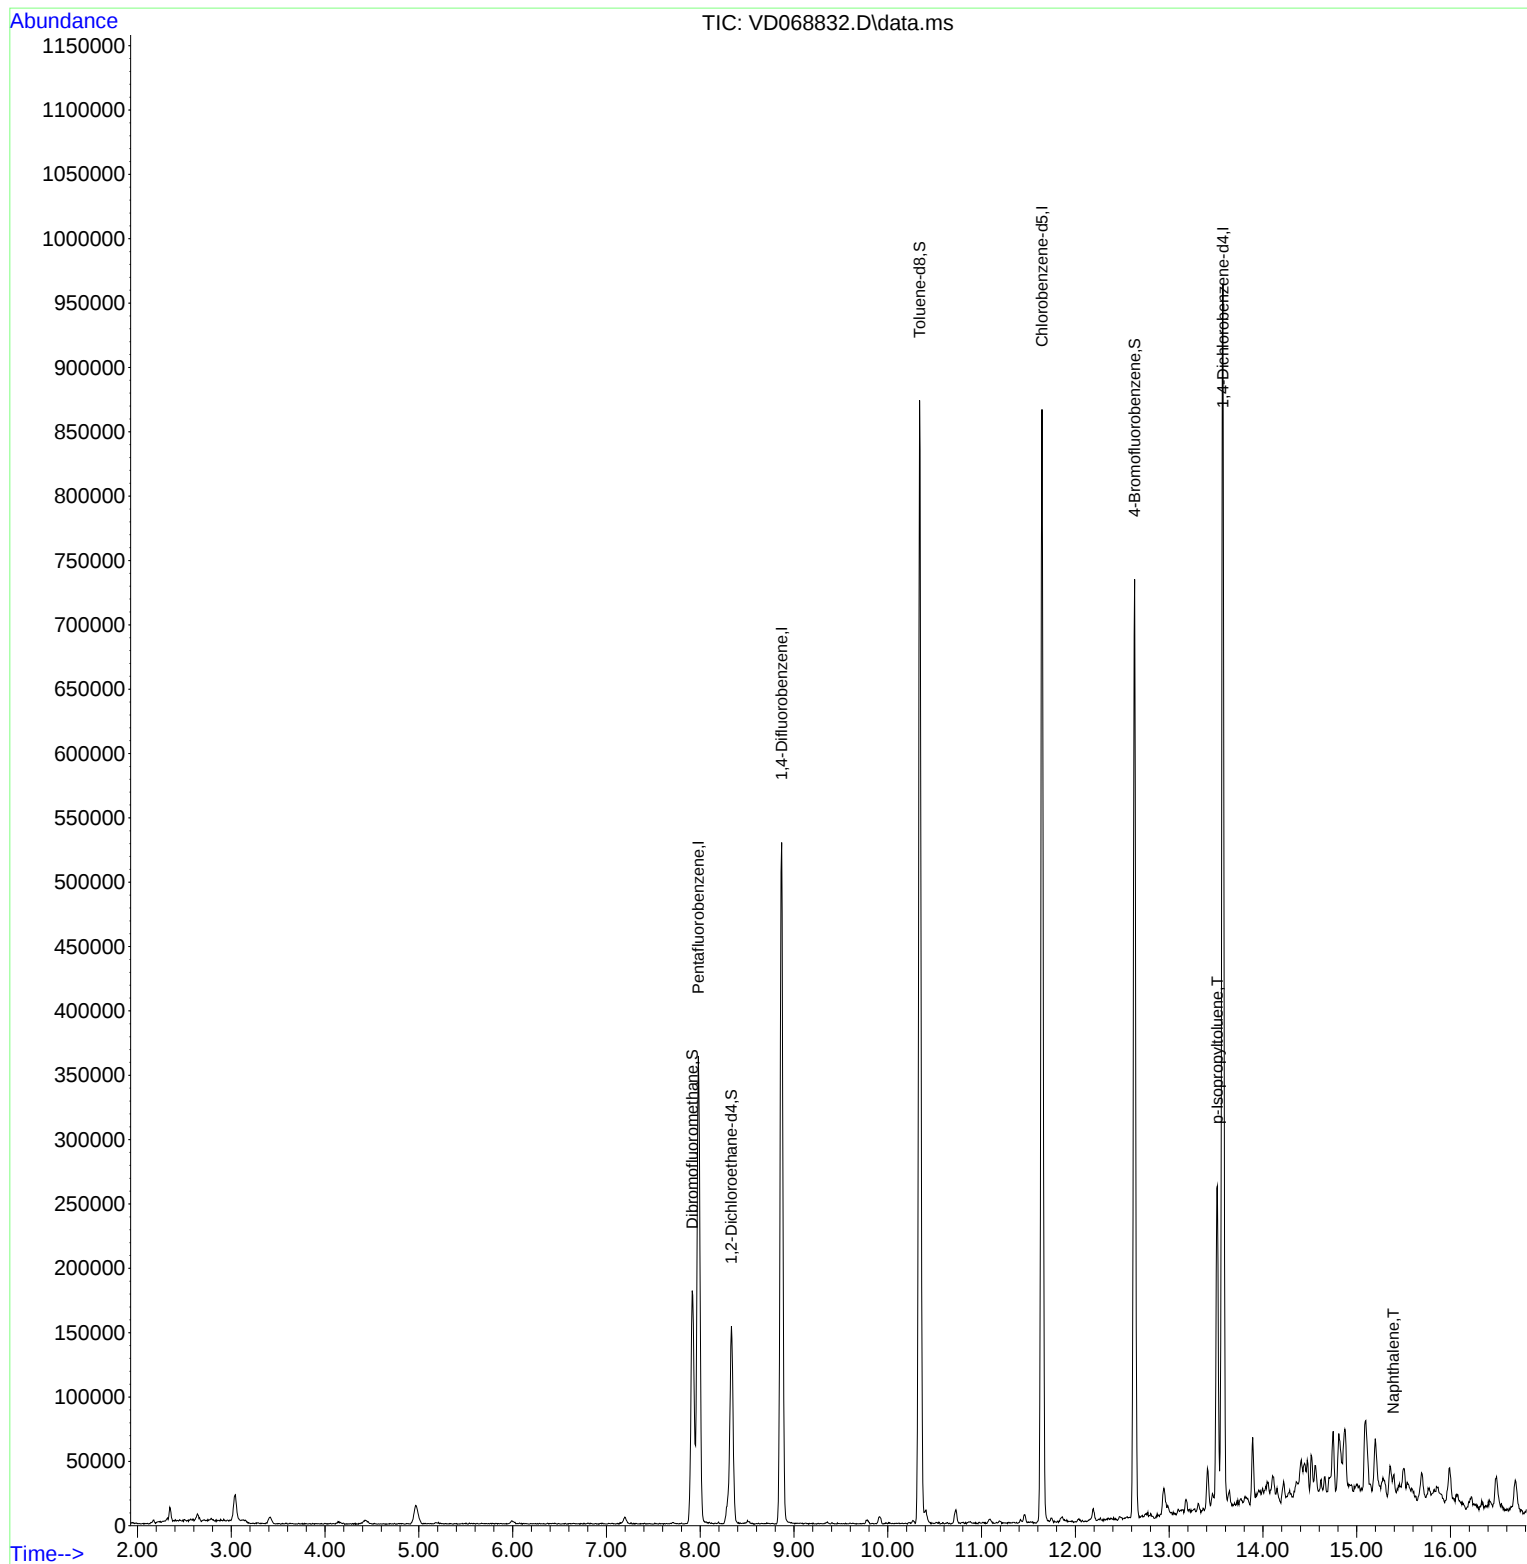


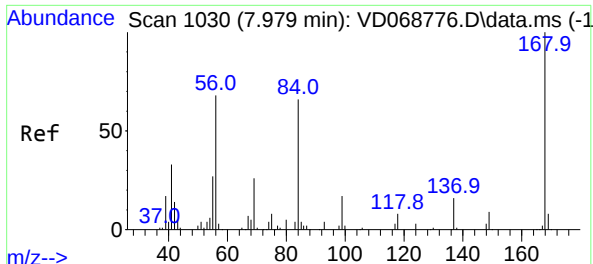

#1
Pentafluorobenzene
Concen: 50.00 ug/l
RT: 7.979 min Scan# 1030
Delta R.T. 0.000 min
Lab File: VD068832.D
Acq: 12 Apr 2021 15:12




Instrument :
MSVOA_D
ClientSampleId :
72-11939-72-11936


Tgt Ion:168 Resp: 281029
Ion Ratio Lower Upper
168 100
99 56.2 46.2 69.2

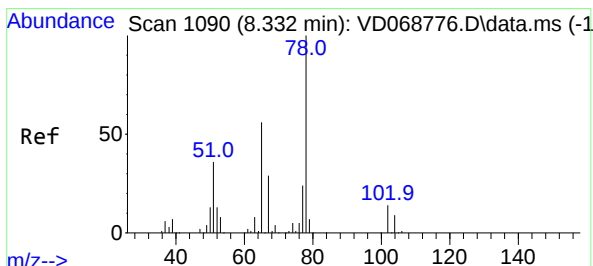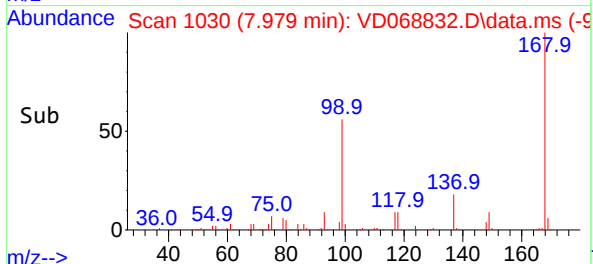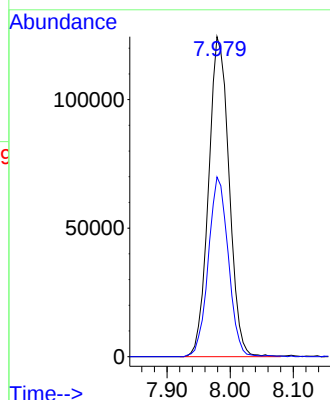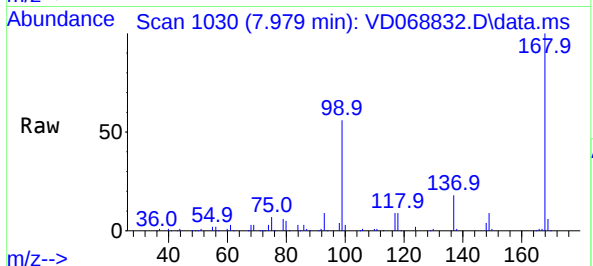

#33
1,2-Dichloroethane-d4
Concen: 39.63 ug/l
RT: 8.332 min Scan# 1090
Delta R.T. 0.000 min
Lab File: VD068832.D
Acq: 12 Apr 2021 15:12

Tgt Ion: 65 Resp: 117709
Ion Ratio Lower Upper
65 100
67 53.0 0.0 106.0


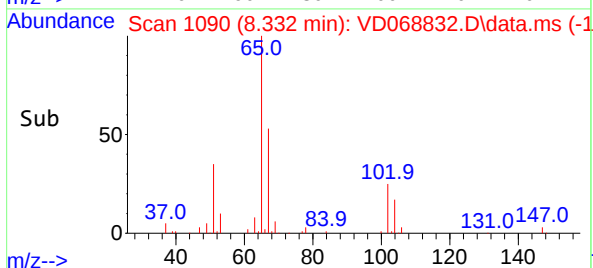
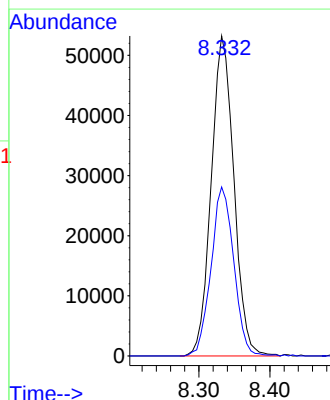
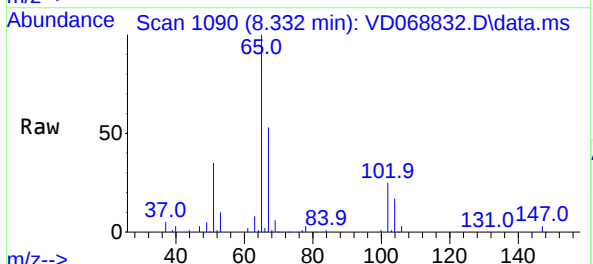


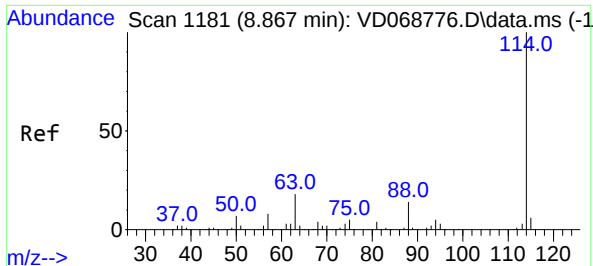

#34
1,4-Difluorobenzene
Concen: 50.00 ug/l
RT: 8.867 min Scan# 1181
Delta R.T. 0.000 min
Lab File: VD068832.D
Acq: 12 Apr 2021 15:12




Instrument :
MSVOA_D
ClientSampleId :
72-11939-72-11936


Tgt Ion:114 Resp: 491247
Ion Ratio Lower Upper
114 100
63 18.5 0.0 38.2
88 14.7 0.0 29.4

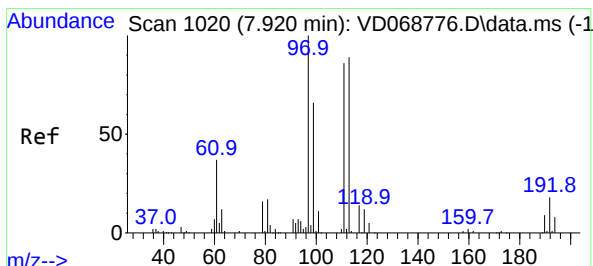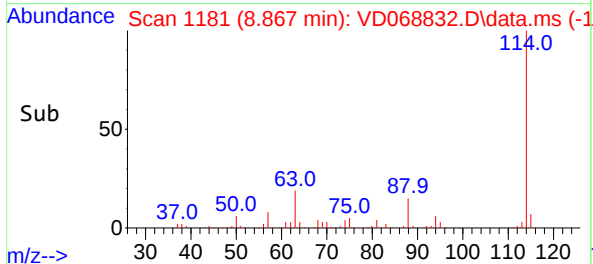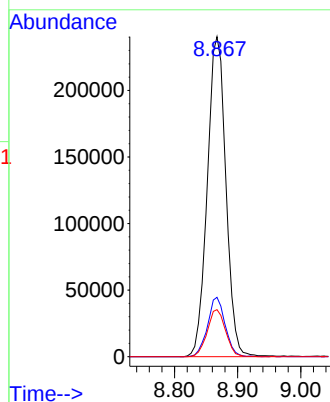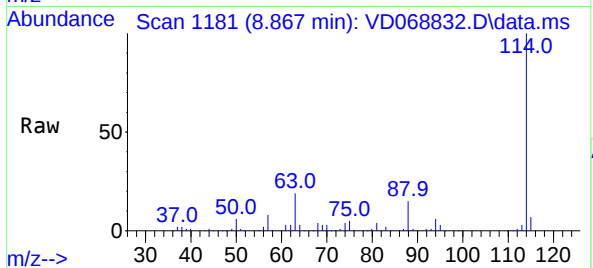

#35
Dibromofluoromethane
Concen: 41.40 ug/l
RT: 7.914 min Scan# 1019
Delta R.T. -0.006 min
Lab File: VD068832.D
Acq: 12 Apr 2021 15:12

Tgt Ion:113 Resp: 132276
Ion Ratio Lower Upper
113 100
111 101.0 82.5 123.7
192 20.0 15.1 22.7


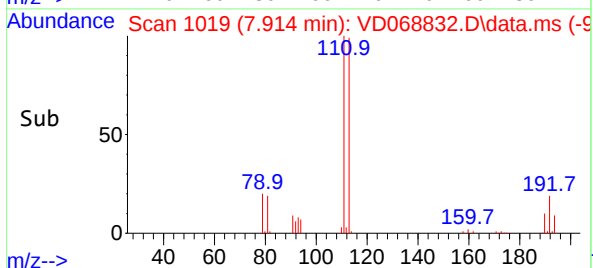
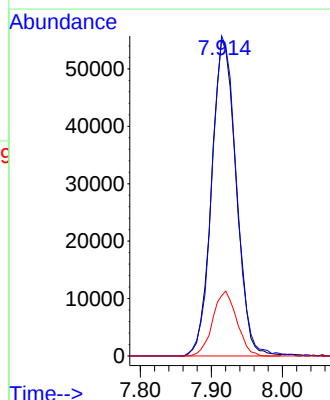
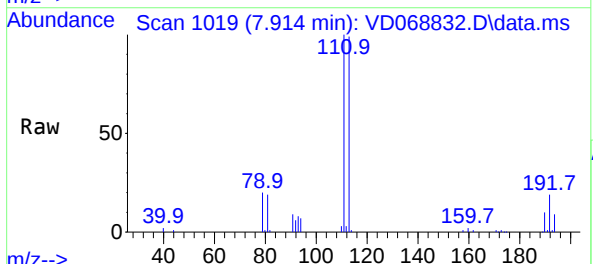


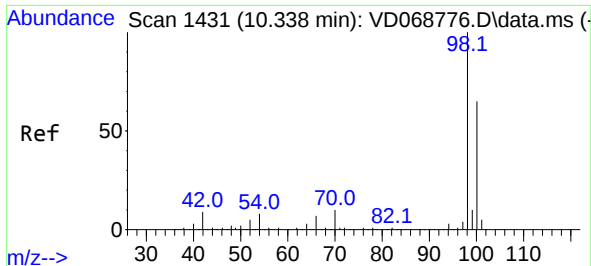

#50
Toluene-d8
Concen: 50.85 ug/l
RT: 10.338 min Scan# 1431
Delta R.T. -0.000 min
Lab File: VD068832.D
Acq: 12 Apr 2021 15:12




Instrument :
MSVOA_D
ClientSampleId :
72-11939-72-11936


Tgt Ion: 98 Resp: 612909
Ion Ratio Lower Upper
98 100
100 64.3 51.8 77.6

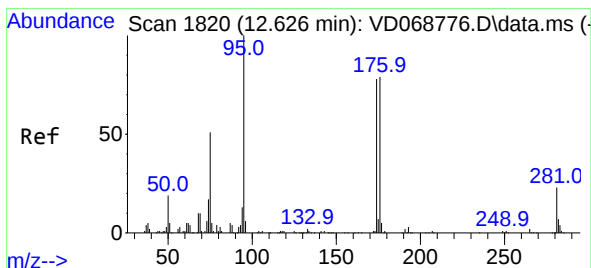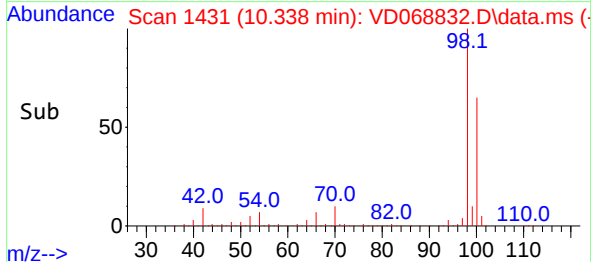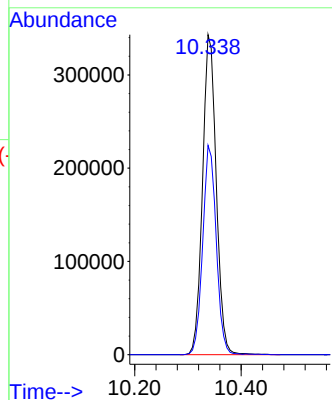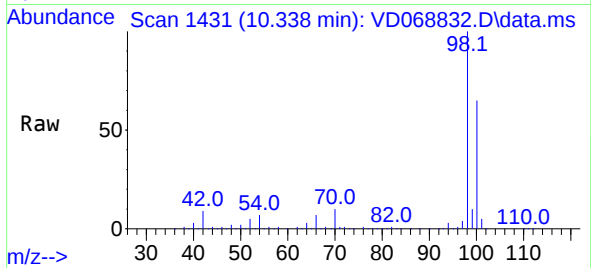

#62
4-Bromofluorobenzene
Concen: 58.57 ug/l
RT: 12.632 min Scan# 1821
Delta R.T. 0.006 min
Lab File: VD068832.D
Acq: 12 Apr 2021 15:12

Tgt Ion: 95 Resp: 234466
Ion Ratio Lower Upper
95 100
174 87.3 0.0 168.0
176 83.7 0.0 160.2


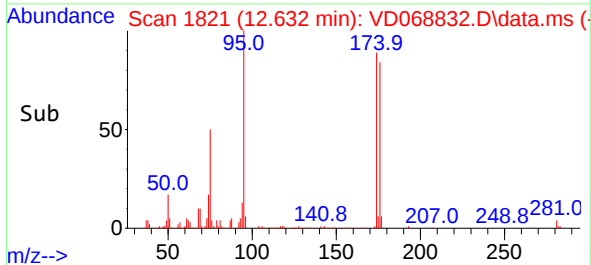
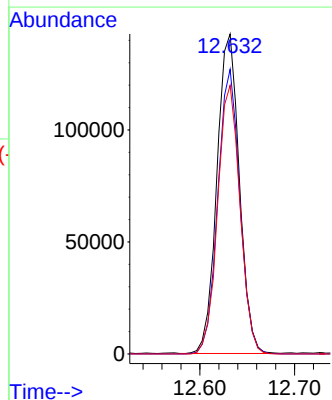
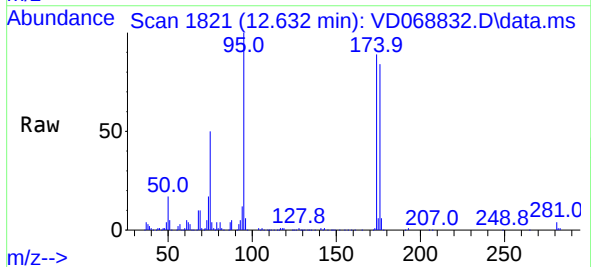


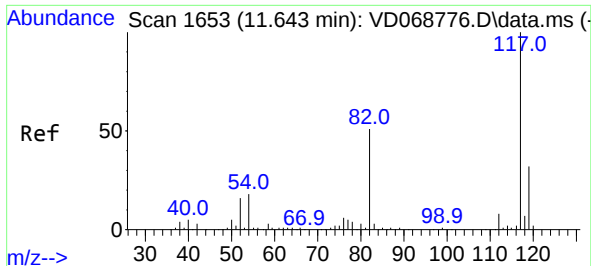

#63
Chlorobenzene-d5
Concen: 50.00 ug/l
RT: 11.644 min Scan# 1653
Delta R.T. 0.001 min
Lab File: VD068832.D
Acq: 12 Apr 2021 15:12




Instrument :
MSVOA_D
ClientSampleId :
72-11939-72-11936


Tgt Ion:117 Resp: 526854
Ion Ratio Lower Upper
117 100
82 50.5 43.5 65.3
119 31.2 26.7 40.1

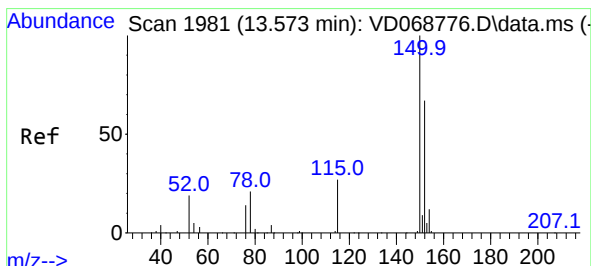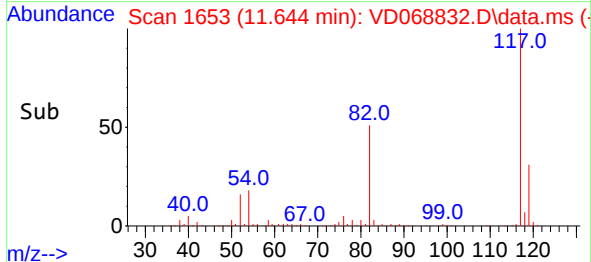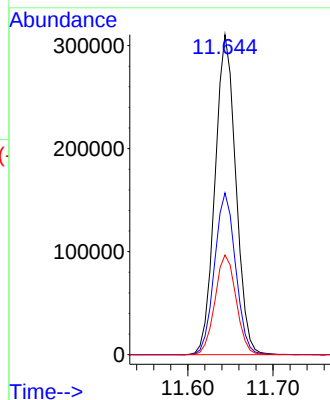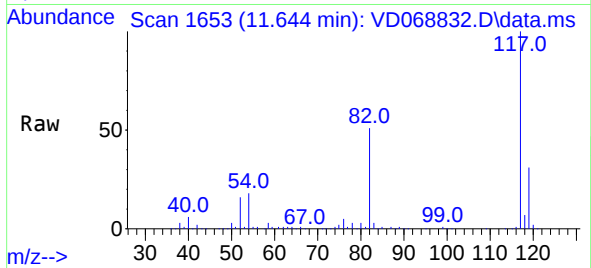

#72
1,4-Dichlorobenzene-d4
Concen: 50.00 ug/l
RT: 13.573 min Scan# 1981
Delta R.T. -0.000 min
Lab File: VD068832.D
Acq: 12 Apr 2021 15:12


Tgt Ion:152 Resp: 266866
Ion Ratio Lower Upper
152 100
115 58.0 29.3 87.8
150 156.7 0.0 347.6

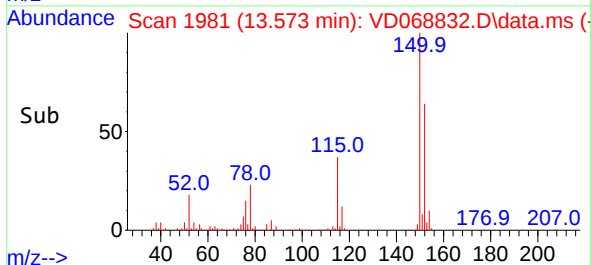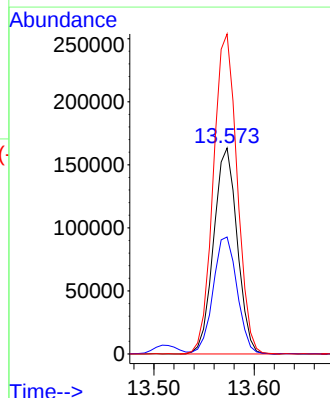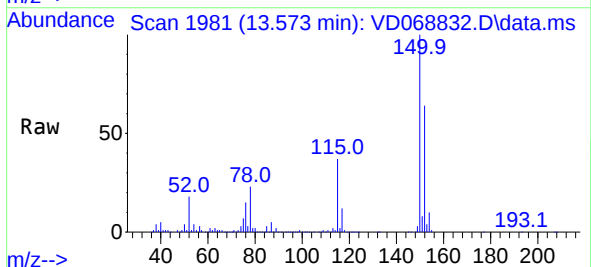



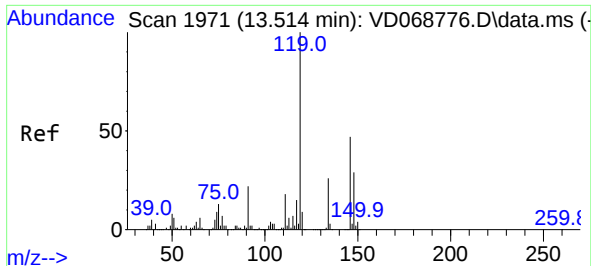


#86
p-Isopropyltoluene
Concen: 8.46 ug/l
RT: 13.514 min Scan# 1971
Delta R.T. 0.000 min
Lab File: VD068832.D
Acq: 12 Apr 2021 15:12

Instrument :
MSVOA_D
ClientSampleId :
72-11939-72-11936

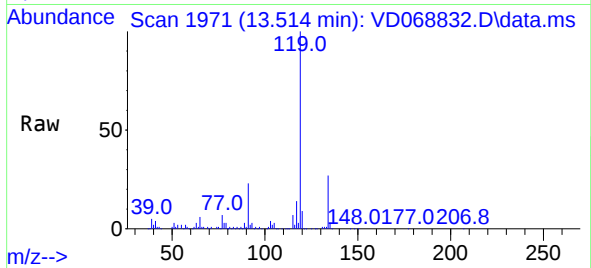

Tgt Ion:119 Resp: 150710
Ion Ratio Lower Upper
119 100
134 26.3 13.3 39.9
91 22.5 11.1 33.1

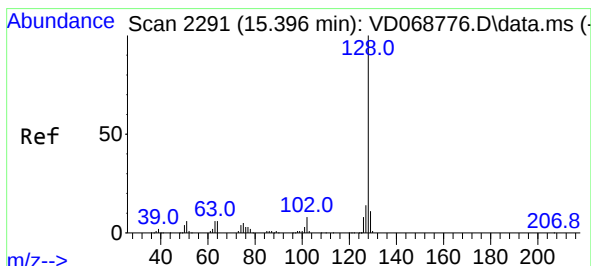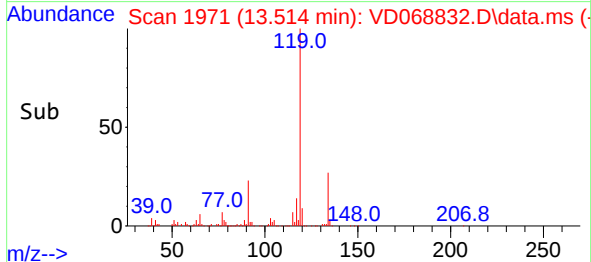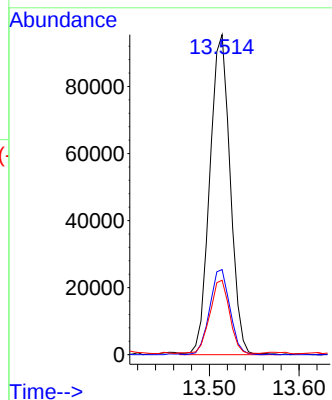

#95
Naphthalene
Concen: 1.36 ug/l
RT: 15.391 min Scan# 2290
Delta R.T. -0.005 min
Lab File: VD068832.D
Acq: 12 Apr 2021 15:12

Tgt Ion:128 Resp: 11799
Ion Ratio Lower Upper
128 100
127 15.7 10.2 15.4#
129 16.3 8.9 13.3#

