



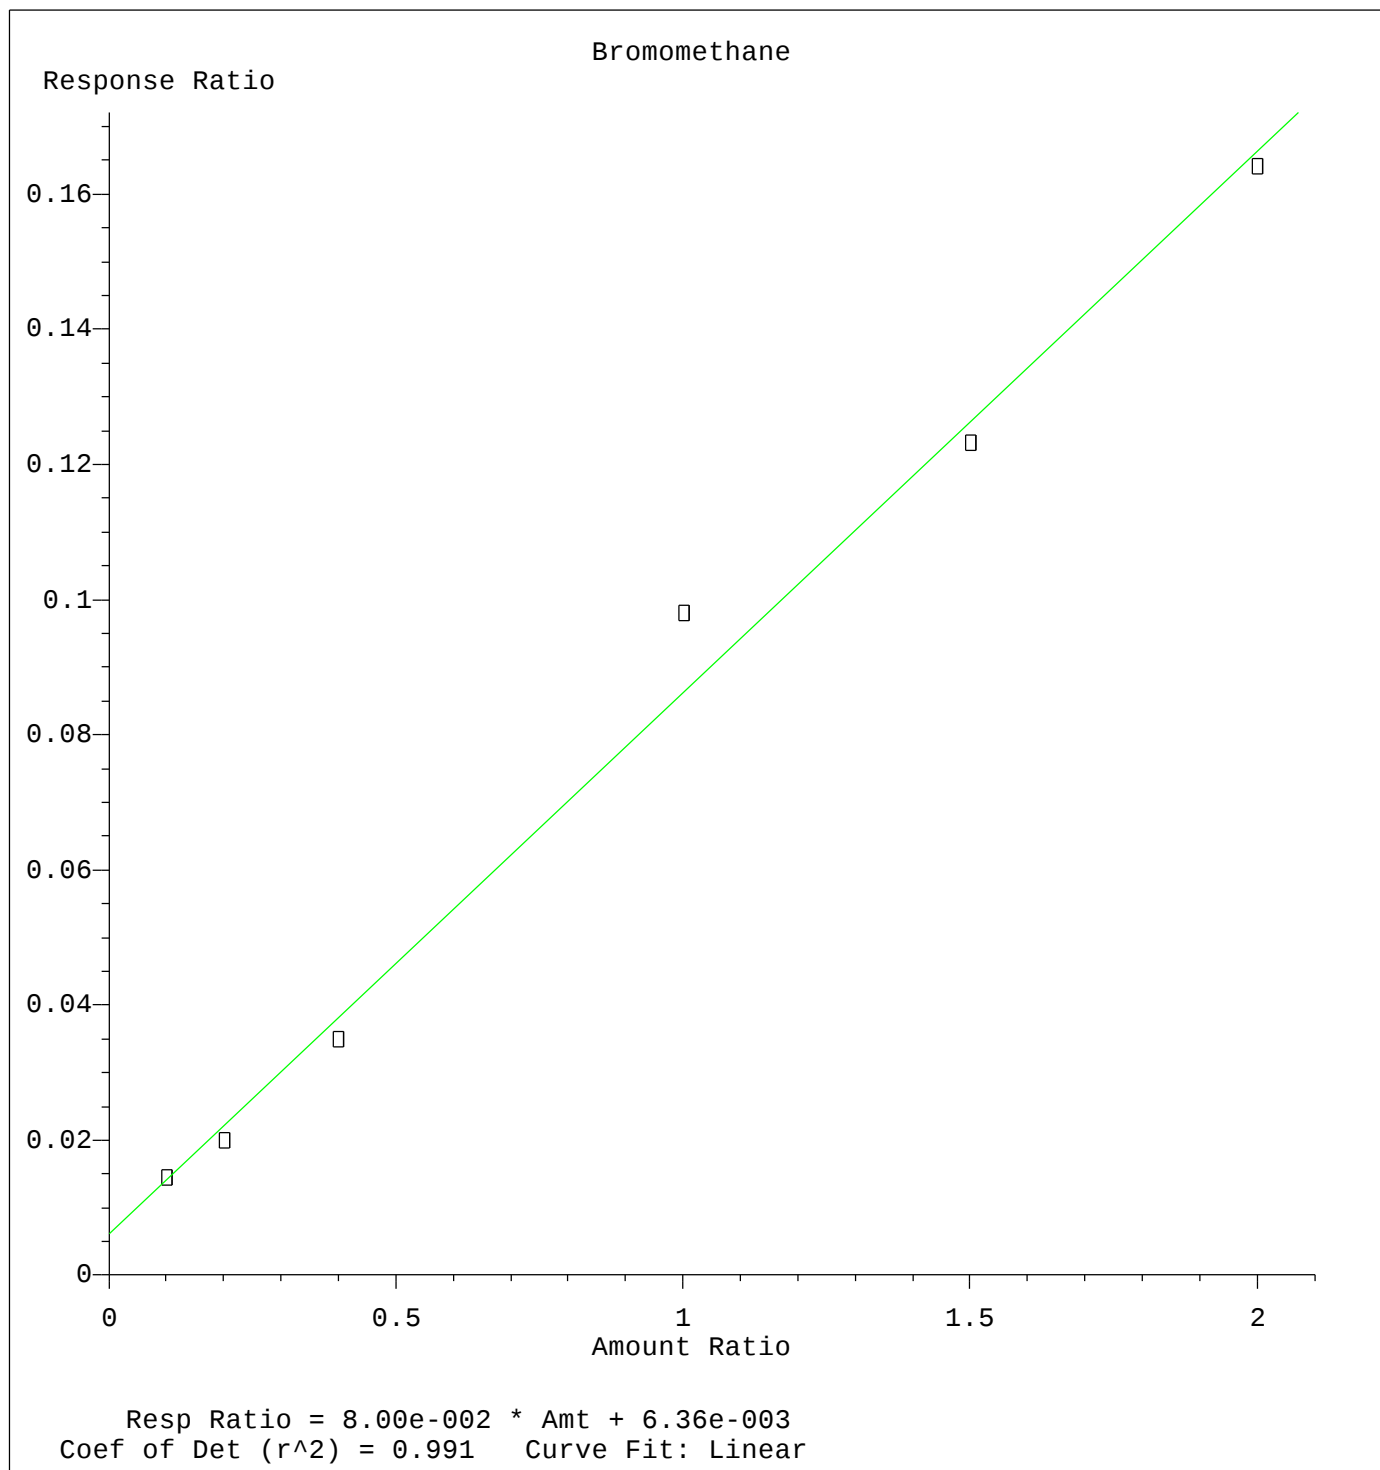


Method Name: Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D041519S.M
Calibration Table Last Updated: Tue Apr 16 08:53:01 2019

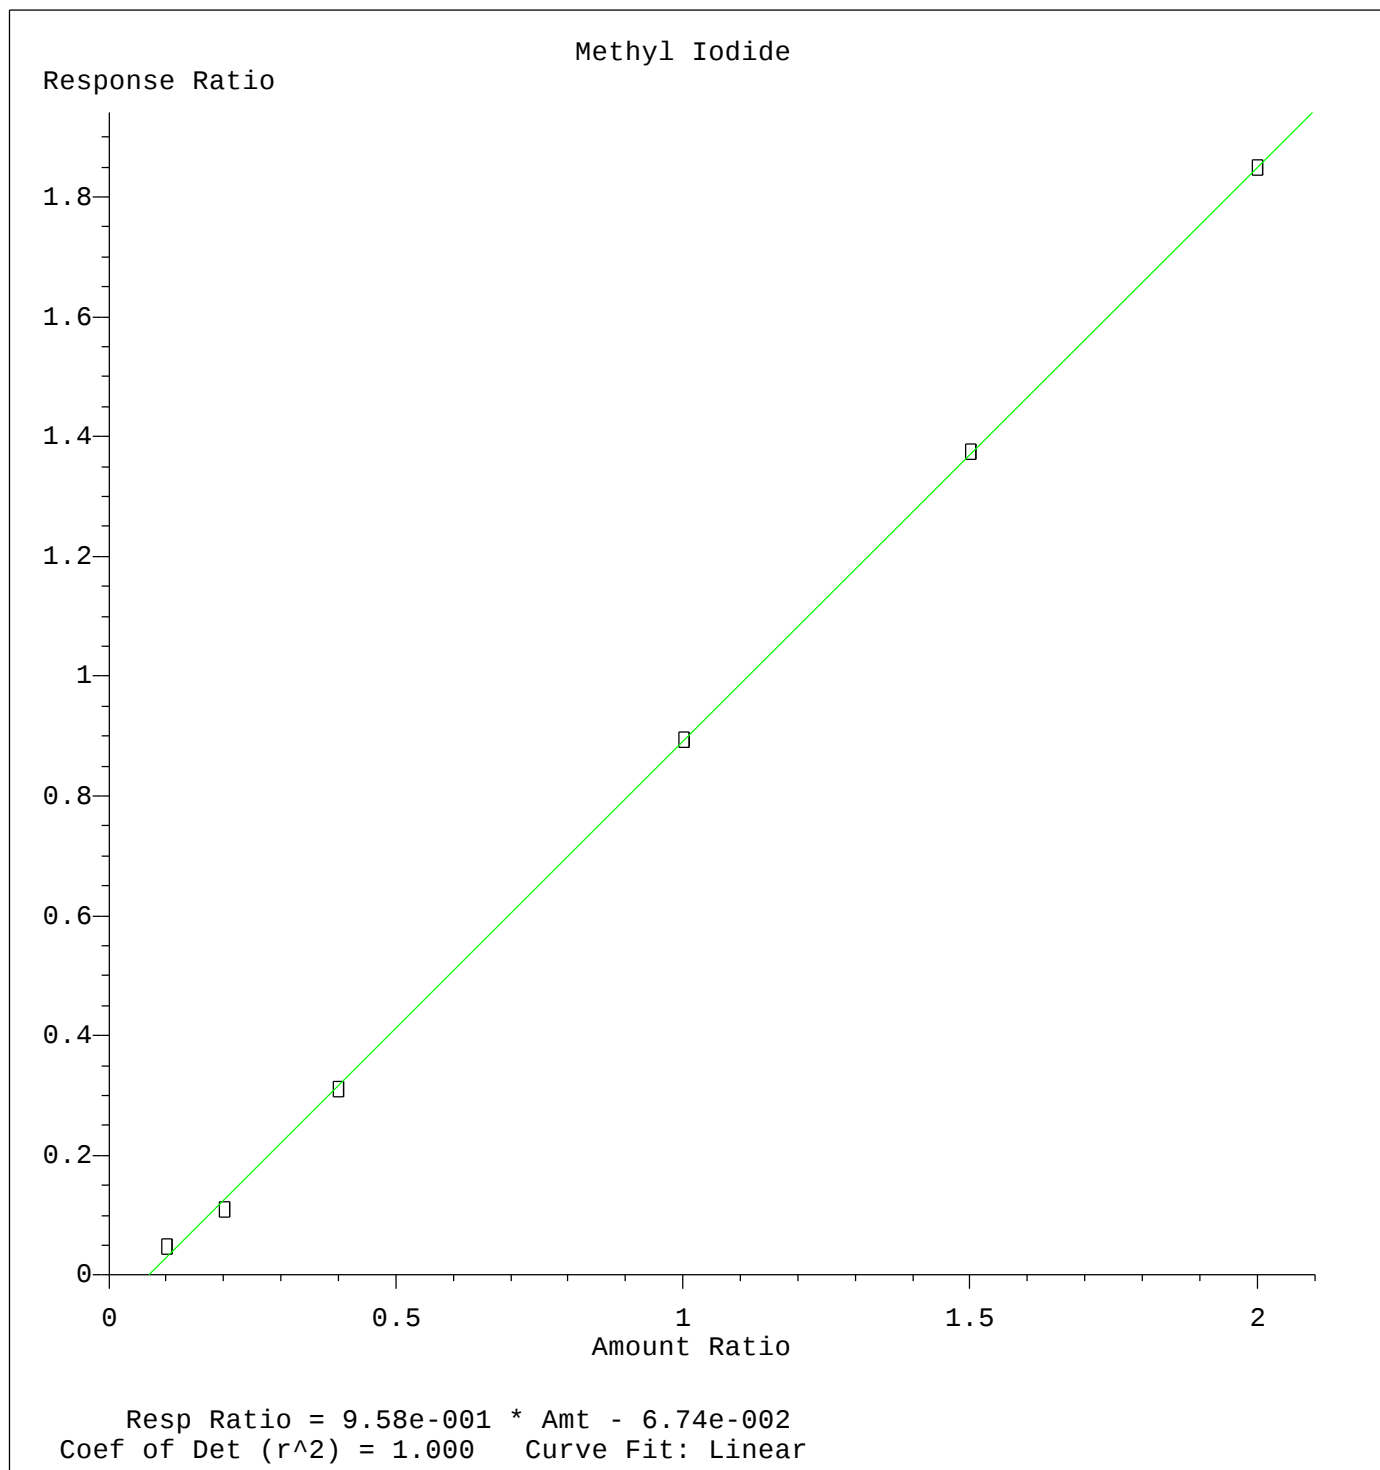

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D041519S.M
Calibration Table Last Updated: Tue Apr 16 08:53:01 2019

Methylene Chloride


Response Ratio

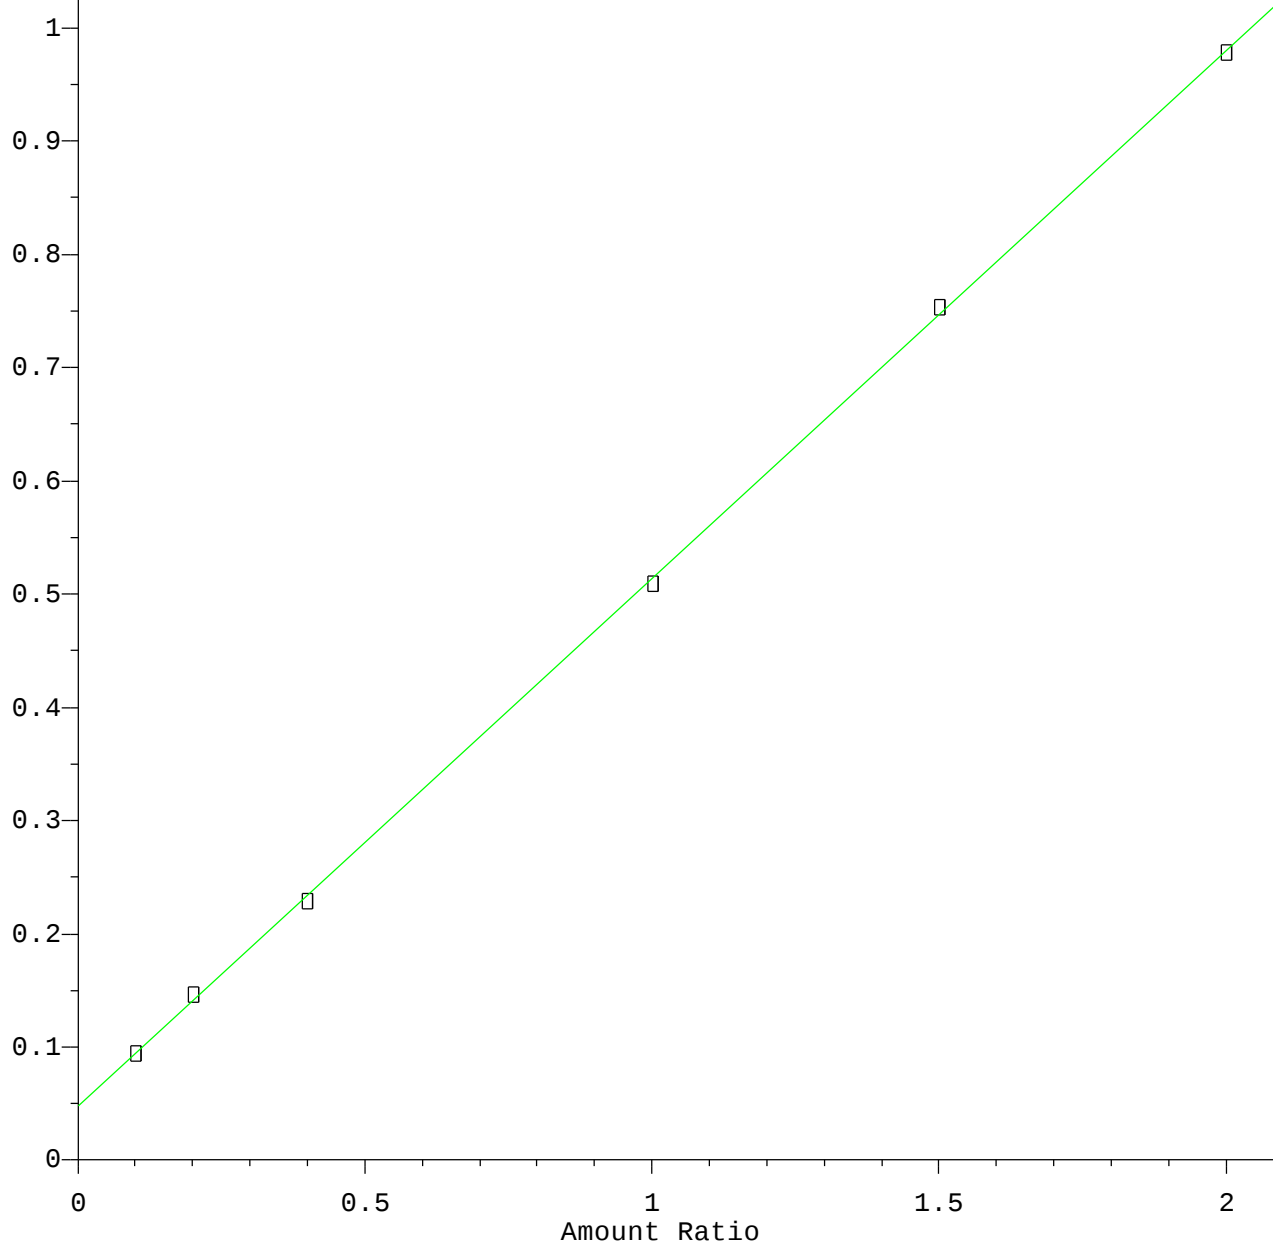

Resp Ratio = $4.66 \times 10^{-1} \times \text{Amt} + 4.71 \times 10^{-2}$
Coef of Det (r^2) = 1.000 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D041519S.M
Calibration Table Last Updated: Tue Apr 16 08:53:01 2019


trans-1,4-Dichloro-2-butene

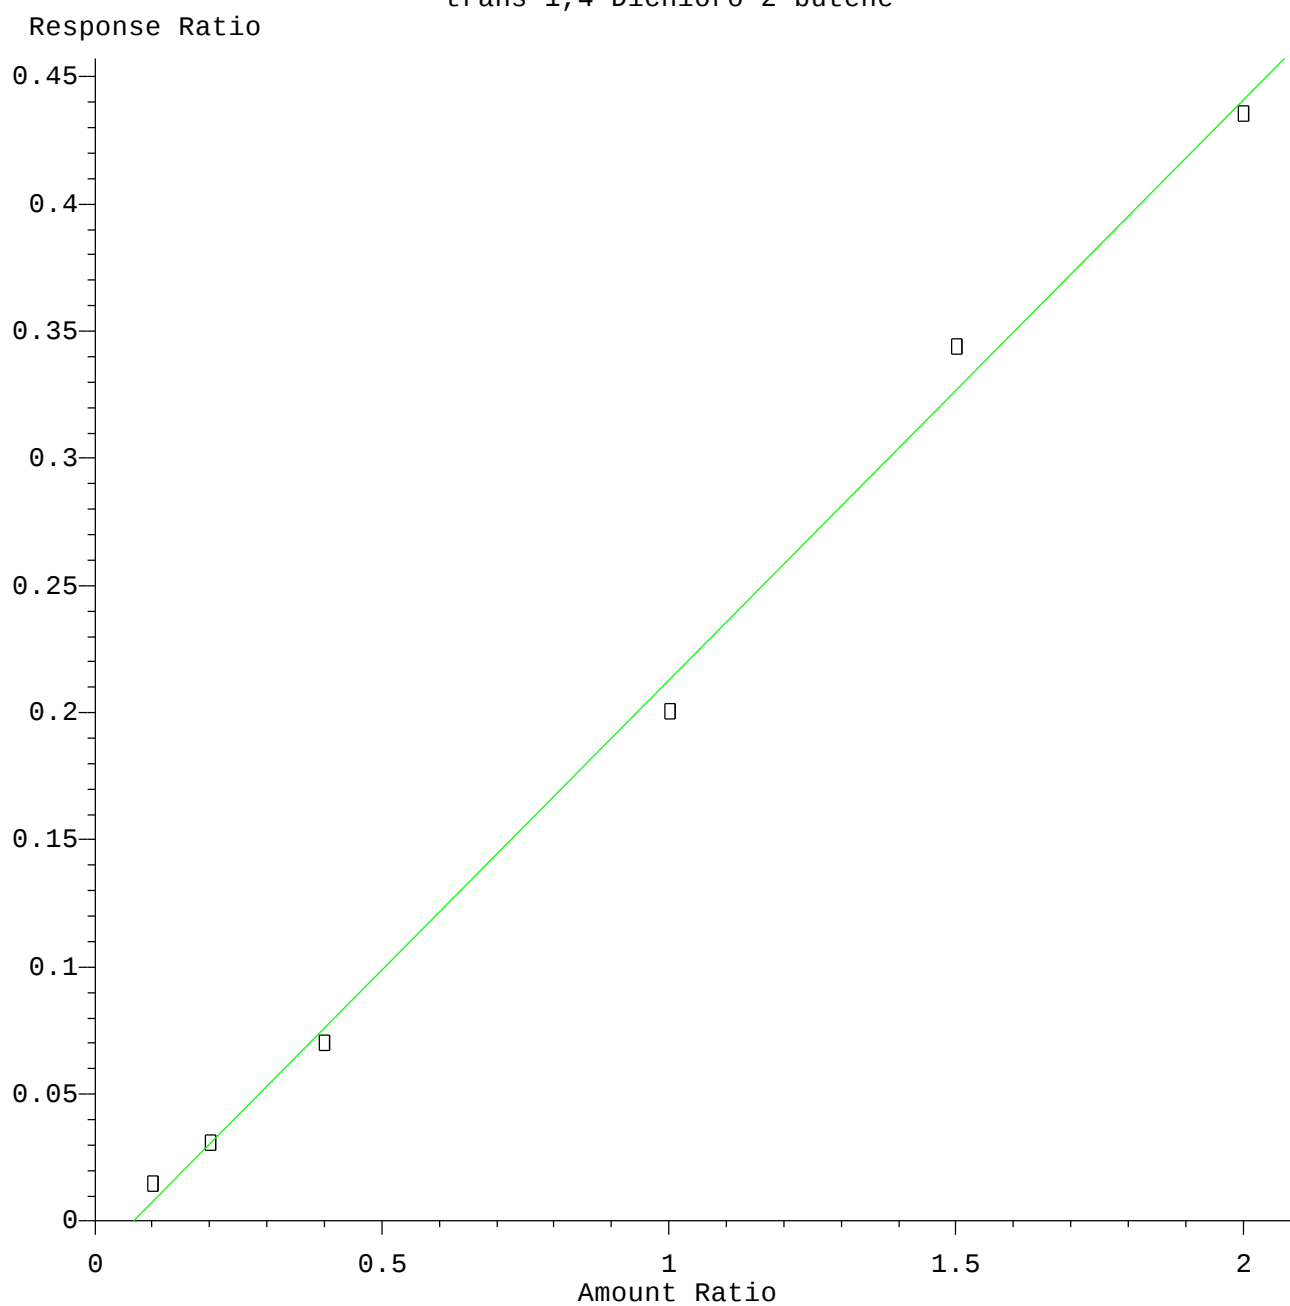

Resp Ratio = $2.28 \times 10^{-1} \times \text{Amt} - 1.51 \times 10^{-2}$
Coef of Det (r^2) = 0.996 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D041519S.M
Calibration Table Last Updated: Tue Apr 16 08:53:01 2019

1,2-Dibromo-3-Chloropropane

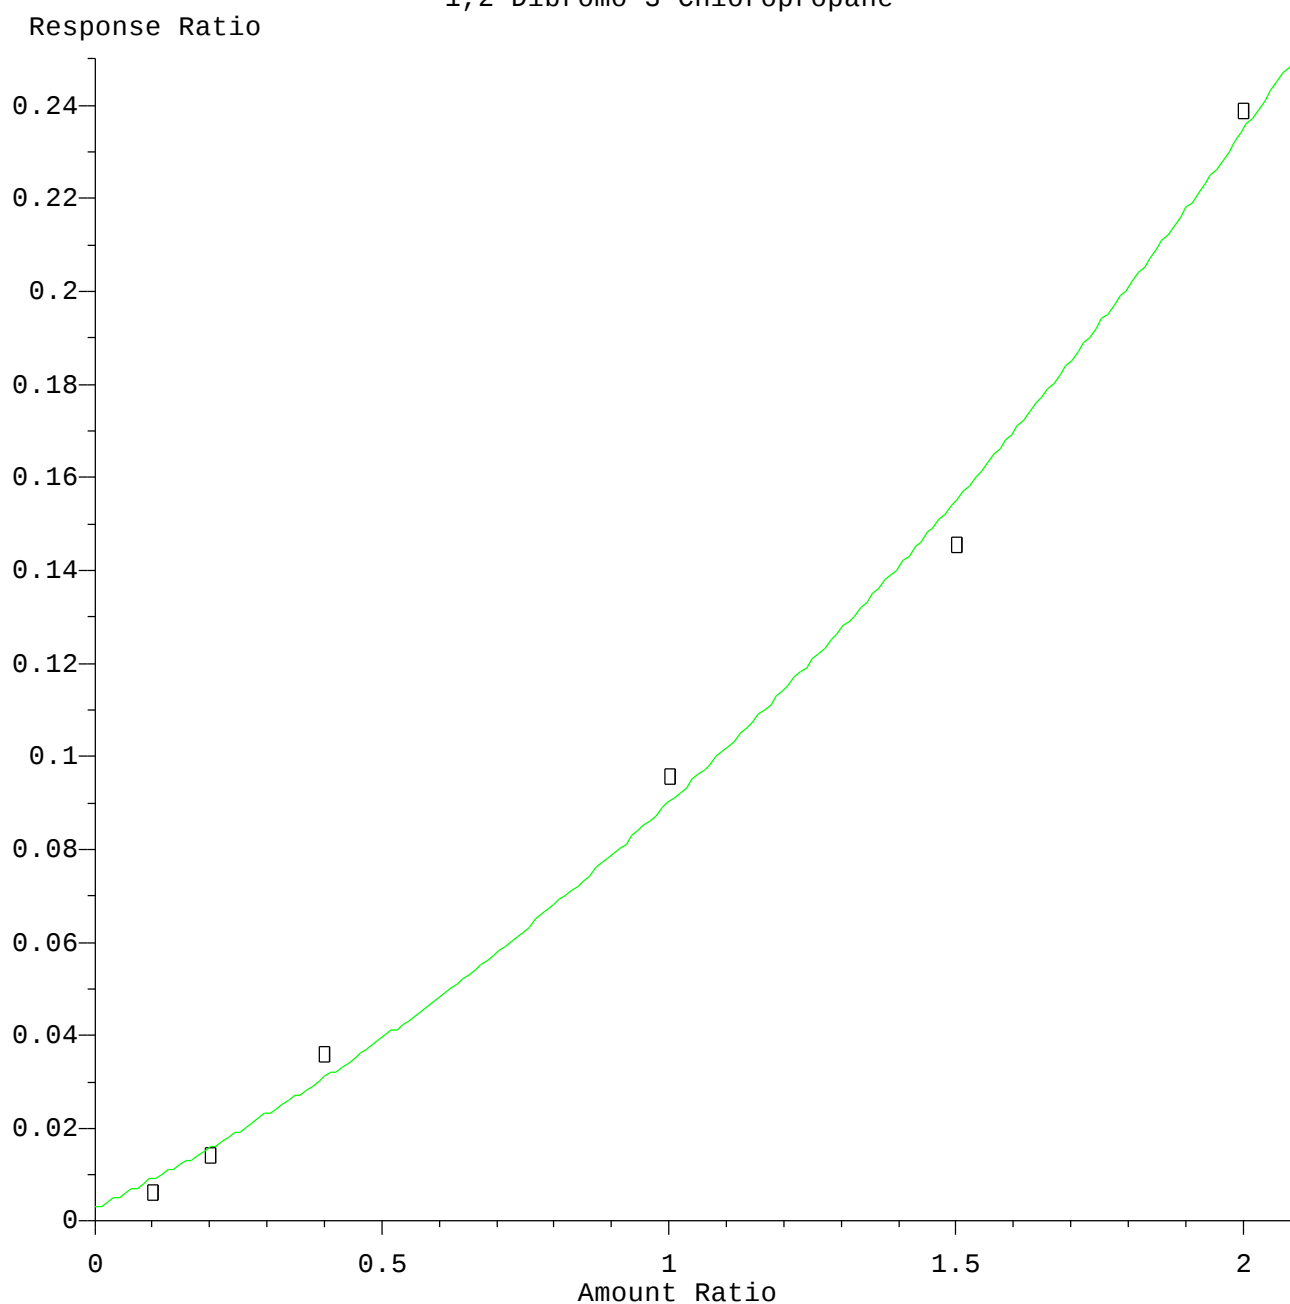

$R = 2.87e-002 A^2 + 5.85e-002 A + 2.83e-003$
Coef of Det (r^2) = 0.996 Curve Fit: Quadratic

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D041519S.M
Calibration Table Last Updated: Tue Apr 16 08:53:01 2019